

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050619\
 Data File : PL048207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2019 11:20
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 00:44:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7) B	delta-BHC	4.501f	0.000	1093151	0	0.077	N.D.	#
12) B	4,4'-DDE	5.432	0.000	12130595	0	0.956	N.D.	#
14) MA	Endrin	5.823	0.000	7157787	0	0.588	N.D.	#
16) A	4,4'-DDD	5.952	0.000	28702952	0	2.949	N.D.	#
17) MA	4,4'-DDT	6.174	0.000	111.1E6	0	11.059	N.D.	#
18) B	Endrin al...	6.253	0.000	103.6E6	0	10.664	N.D.	#
20) A	Methoxychlor	6.742	0.000	238.0E6	0	43.715	N.D.	#
21) B	Endrin ke...	6.948	0.000	46438410	0	3.984	N.D.	#
22)	Mirex	7.115	0.000	17077032	0	1.905	N.D.	#
24)	Chlordane-2	4.679f	0.000	1238404	0	2.394	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050619\
Data File : PL048207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2019 11:20
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 00:44:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

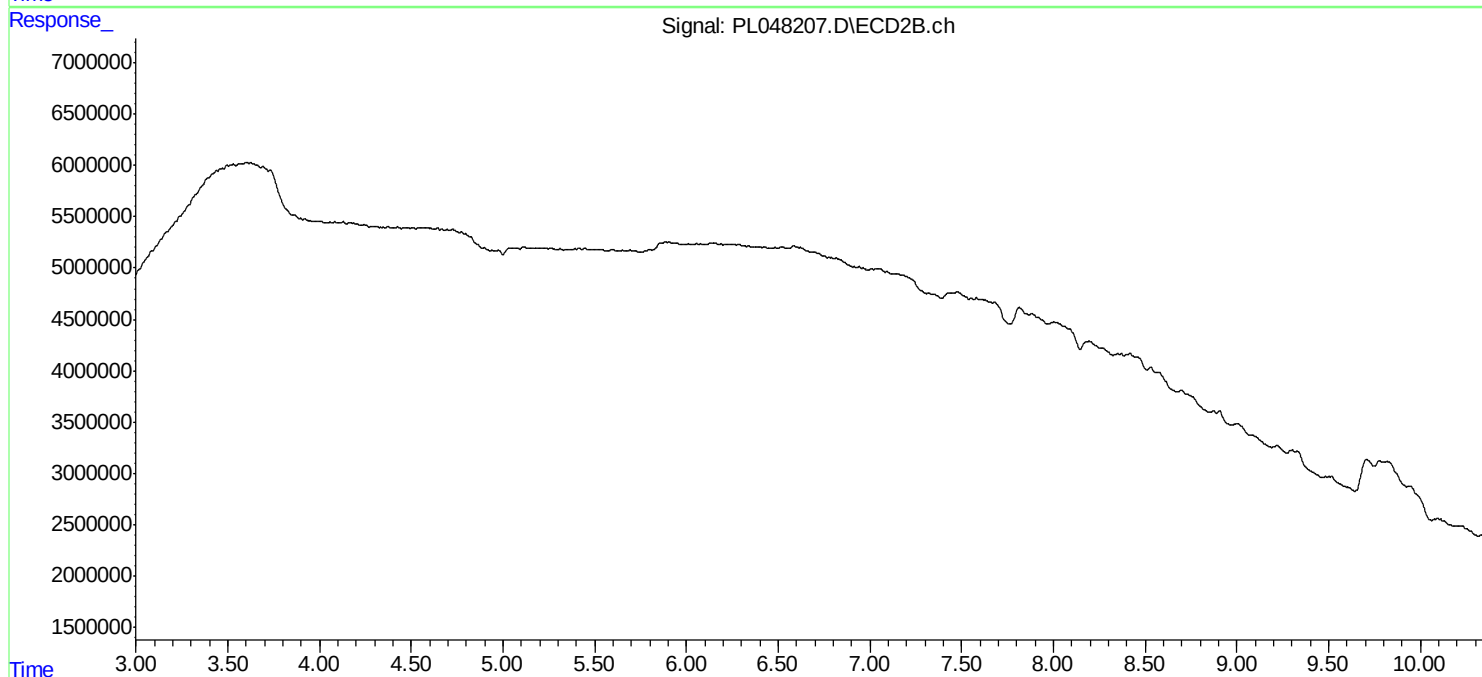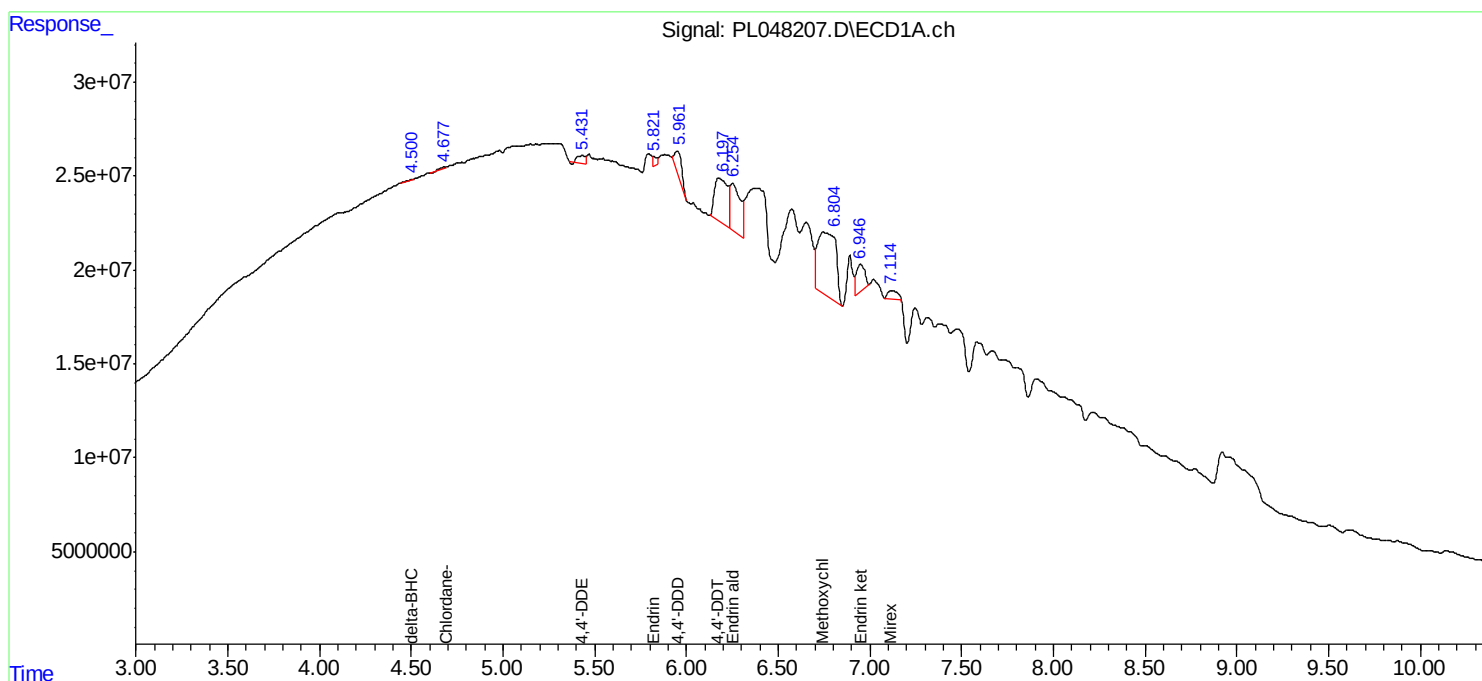


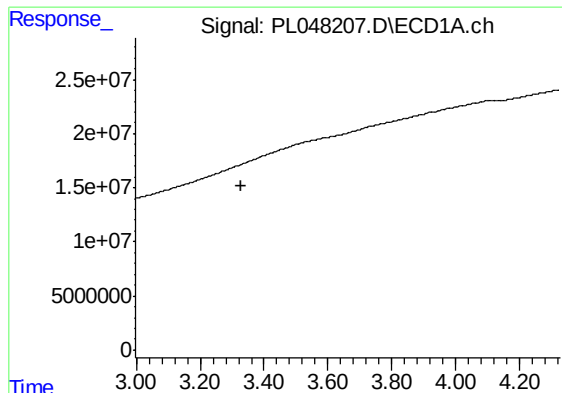

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

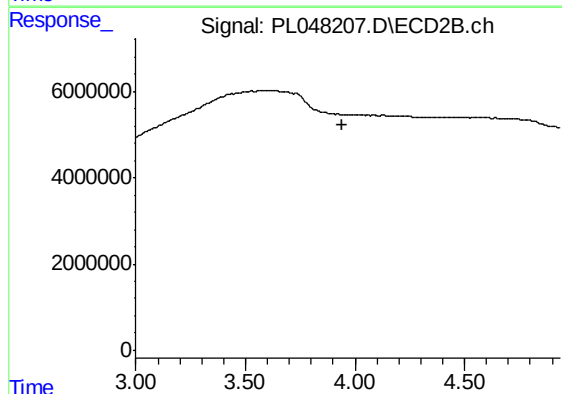


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.940 min
Response: 0
Conc: N.D.

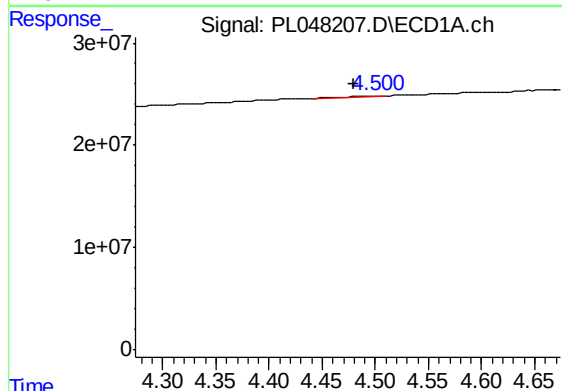


#7 delta-BHC

R.T.: 4.501 min
Delta R.T.: 0.022 min
Response: 1093151
Conc: 0.08 ng/ml

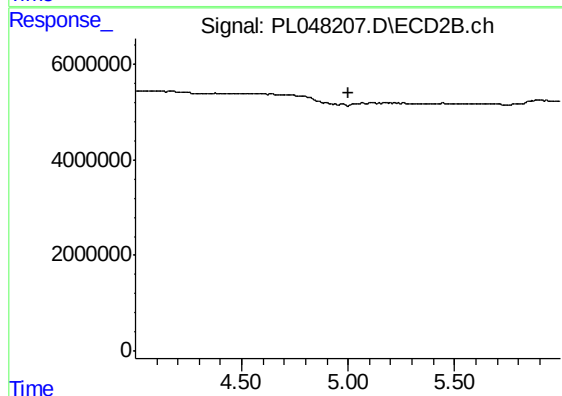

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 5.000 min
Response: 0
Conc: N.D.

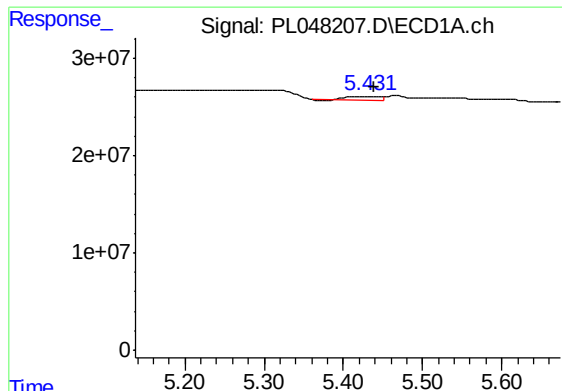

#12 4,4'-DDE


R.T.: 5.432 min
Delta R.T.: -0.006 min
Response: 12130595
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

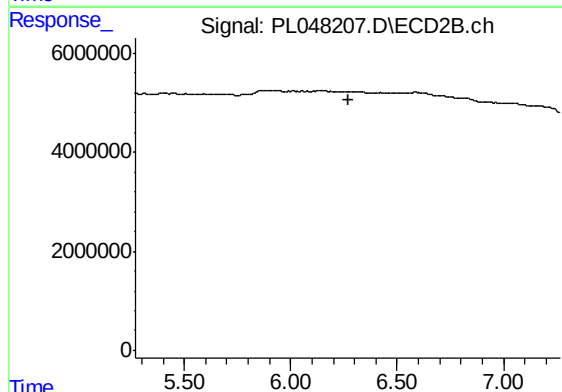


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

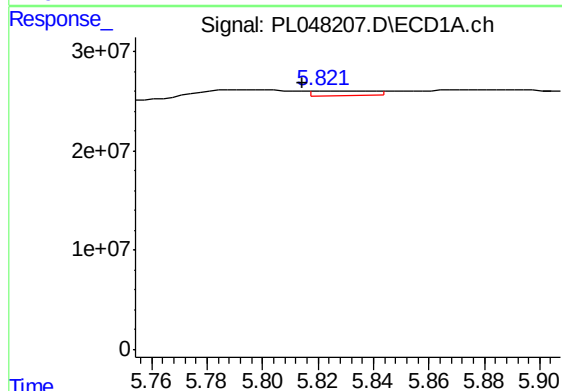


#14 Endrin

R.T.: 5.823 min
Delta R.T.: 0.009 min
Response: 7157787
Conc: 0.59 ng/ml

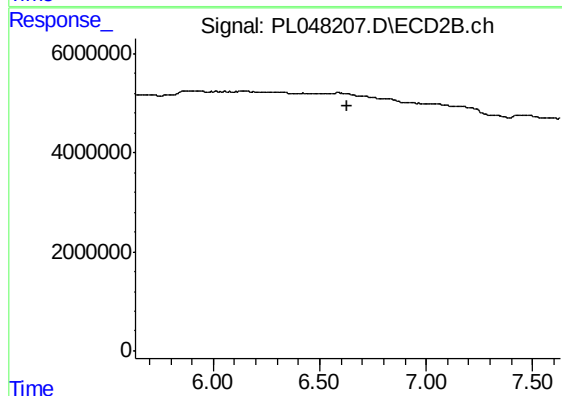

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

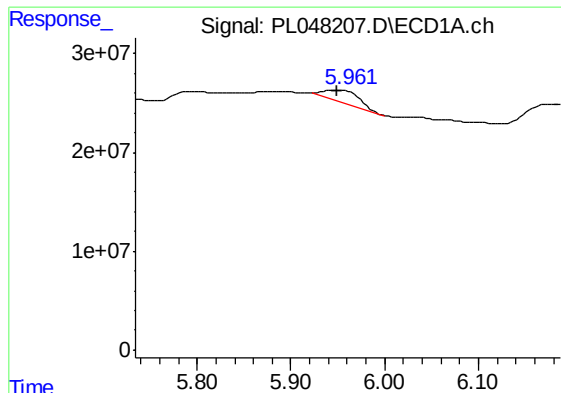

#16 4,4'-DDD


R.T.: 5.952 min
Delta R.T.: 0.003 min
Response: 28702952
Conc: 2.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

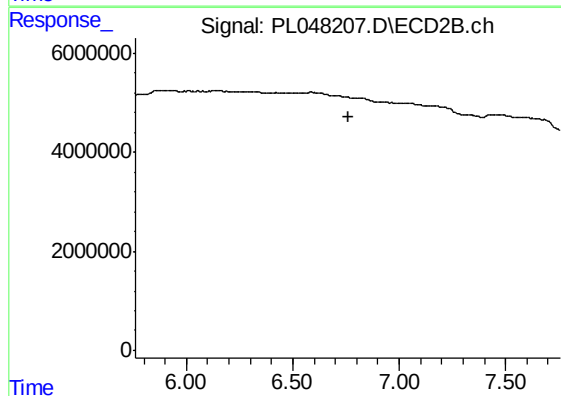


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

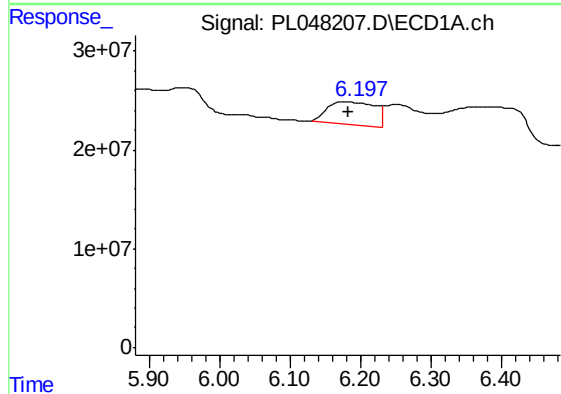


#17 4,4'-DDT

R.T.: 6.174 min
Delta R.T.: -0.010 min
Response: 111102909
Conc: 11.06 ng/ml

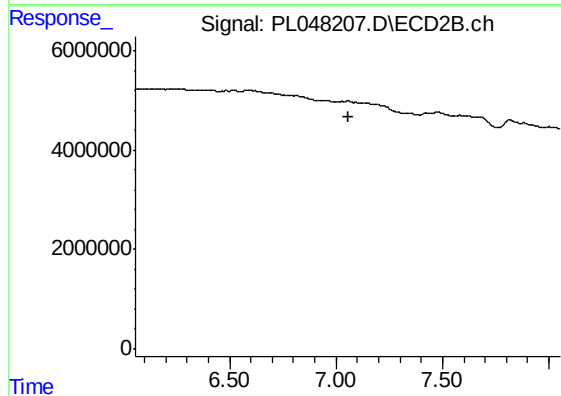

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

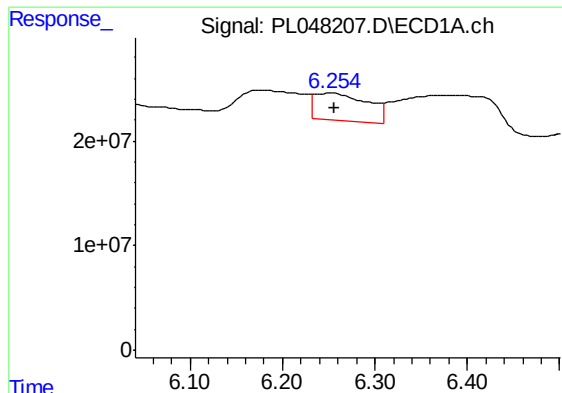

#18 Endrin aldehyde


R.T.: 6.253 min
Delta R.T.: -0.004 min
Response: 103634664
Conc: 10.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

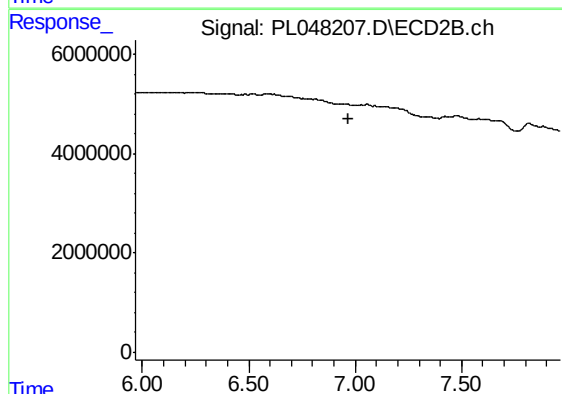


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

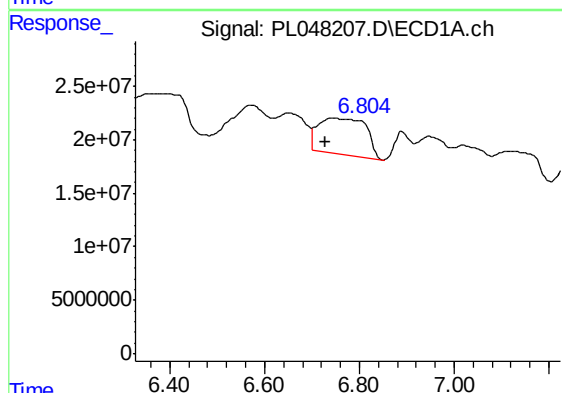


#20 Methoxychlor

R.T.: 6.742 min
Delta R.T.: 0.014 min
Response: 238019127
Conc: 43.72 ng/ml

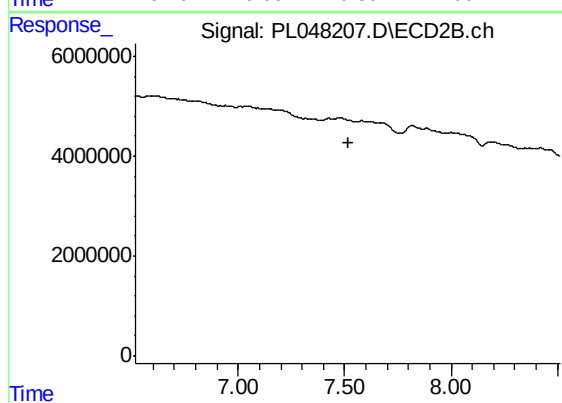

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.

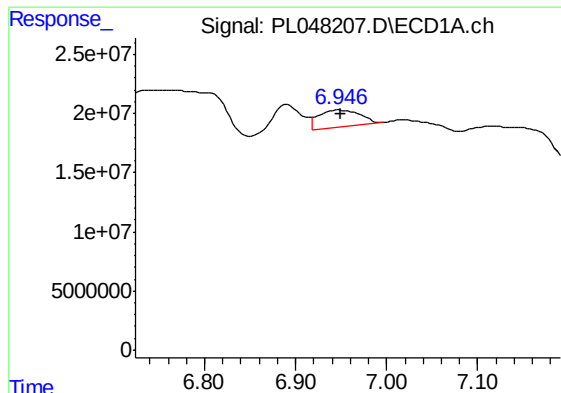

#21 Endrin ketone


R.T.: 6.948 min
Delta R.T.: -0.002 min
Response: 46438410
Conc: 3.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

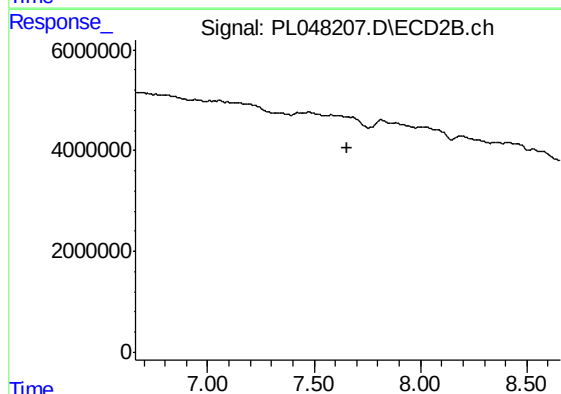


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.658 min
Response: 0
Conc: N.D.

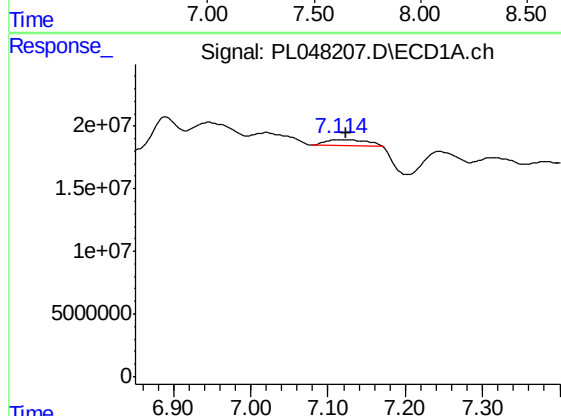


#22 Mirex

R.T.: 7.115 min
Delta R.T.: -0.009 min
Response: 17077032
Conc: 1.91 ng/ml

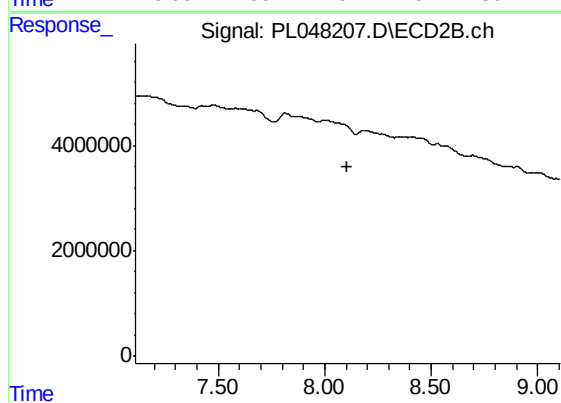

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.109 min
Response: 0
Conc: N.D.

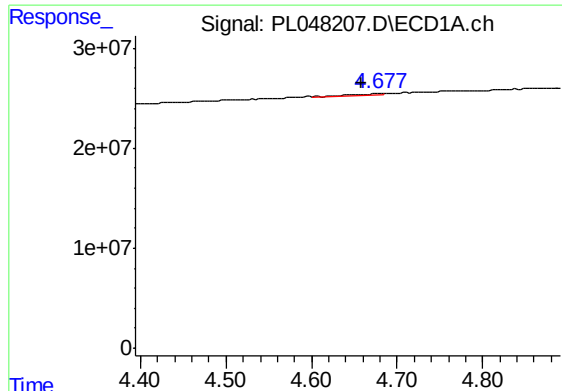

#24 Chlordane-2


R.T.: 4.679 min
Delta R.T.: 0.021 min
Response: 1238404
Conc: 2.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

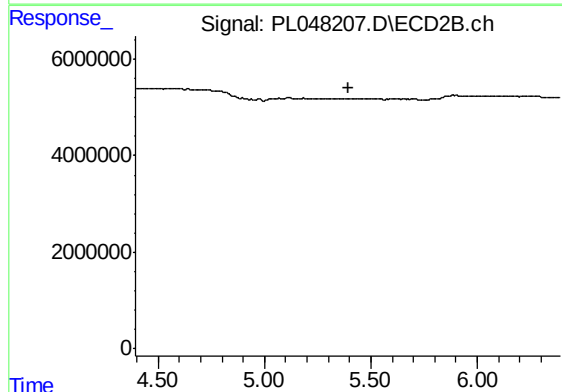


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.394 min
Response: 0
Conc: N.D.

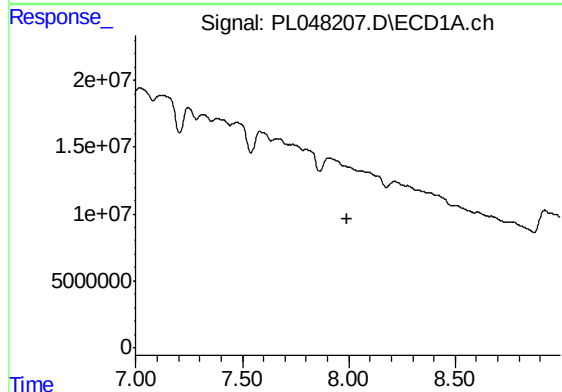

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.996 min
Response: 0
Conc: N.D.

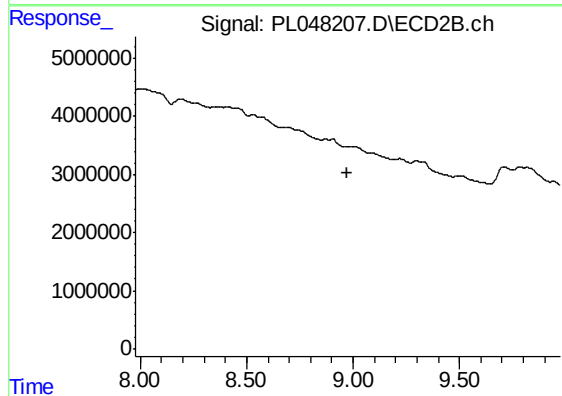

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.975 min
Response: 0
Conc: N.D.