

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050619\
 Data File : PL048226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2019 18:20
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 00:49:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.328	3.940	168.2E6	43696196	17.362	17.542
28) SA Decachlor...	7.997	8.977	168.4E6	46459978	16.752	17.504
Target Compounds						
12) B 4,4'-DDE	5.464f	0.000	1077490	0	0.085	N.D. #
13) MA Dieldrin	5.540f	0.000	4862498	0	0.373	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050619\
Data File : PL048226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2019 18:20
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 00:49:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

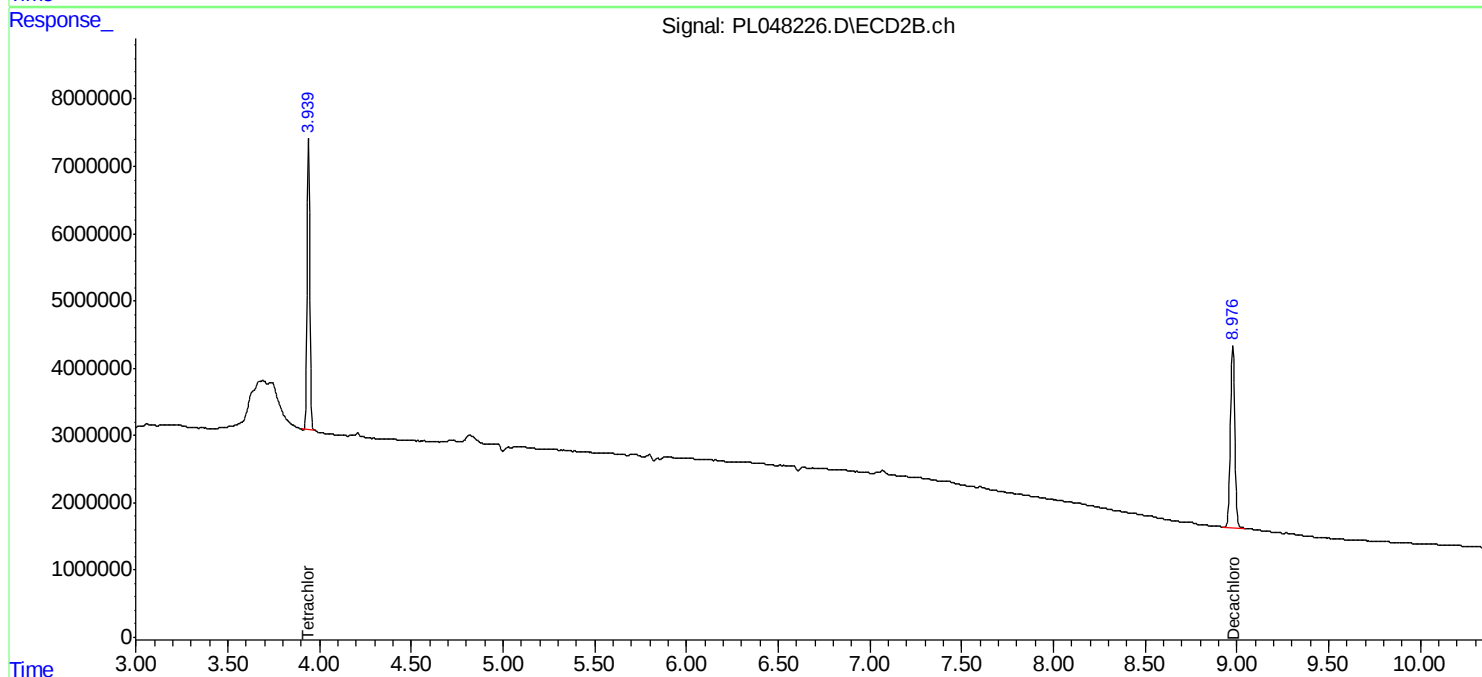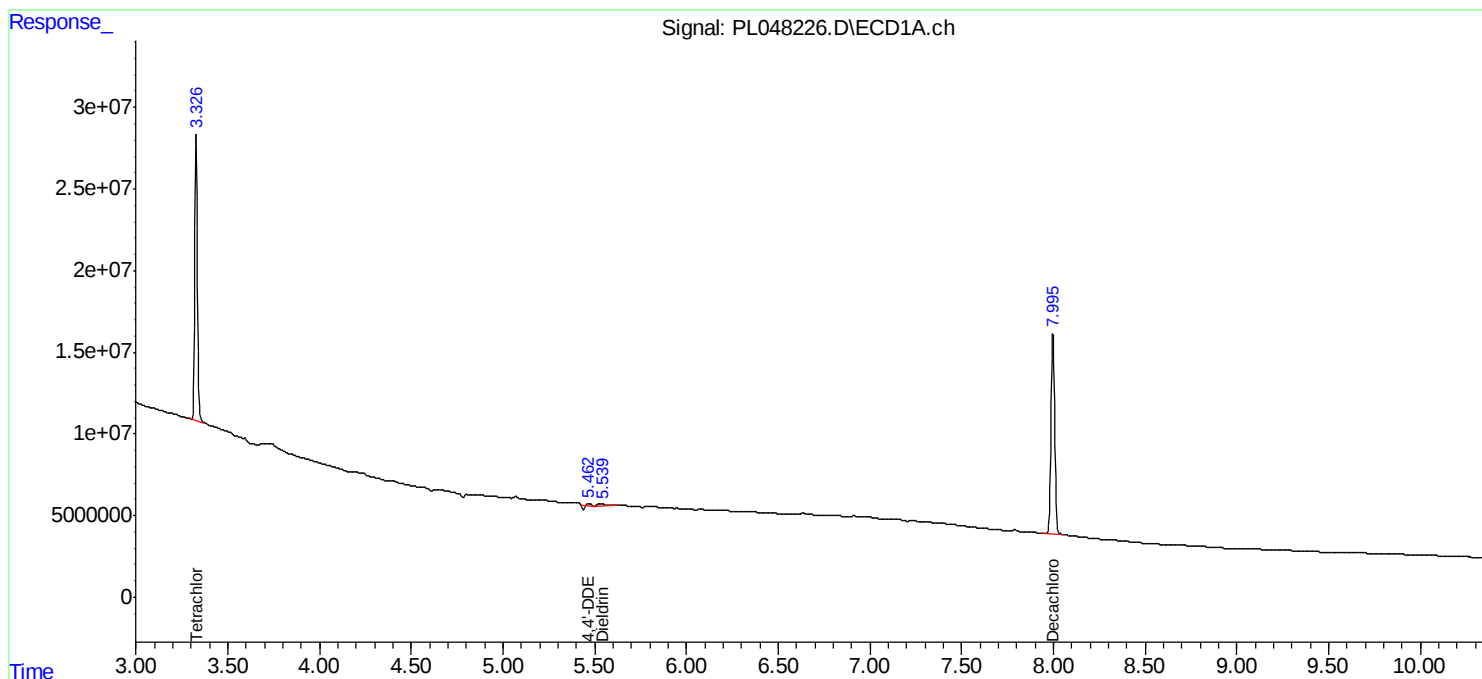


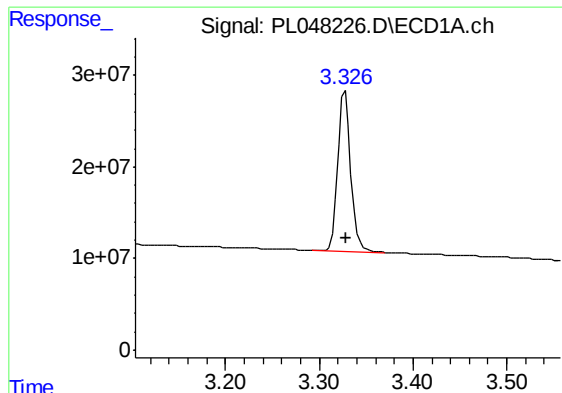

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 168178442
Conc: 17.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

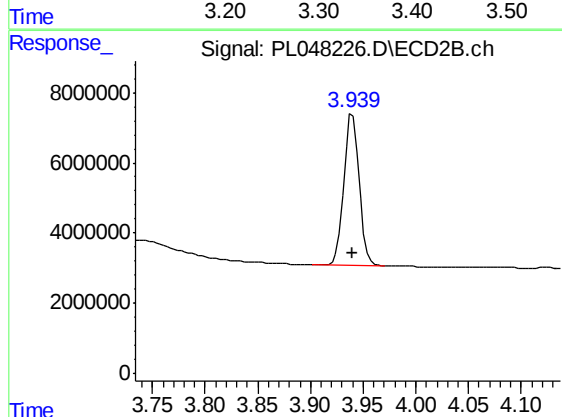


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 43696196
Conc: 17.54 ng/ml

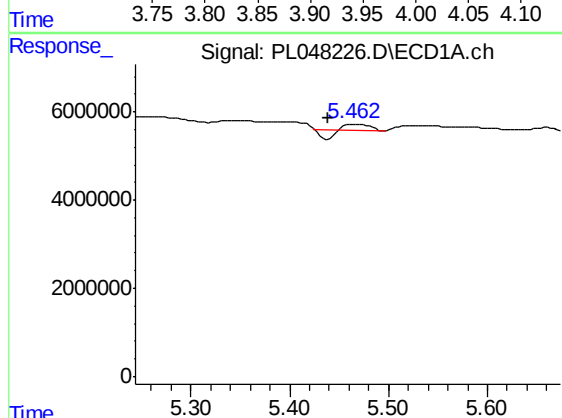


#12 4,4'-DDE

R.T.: 5.464 min
Delta R.T.: 0.025 min
Response: 1077490
Conc: 0.08 ng/ml

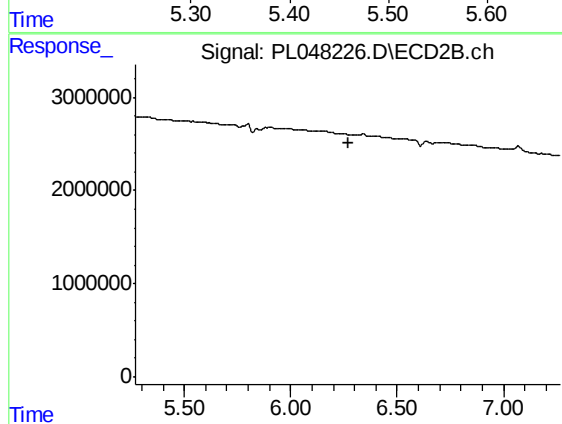

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

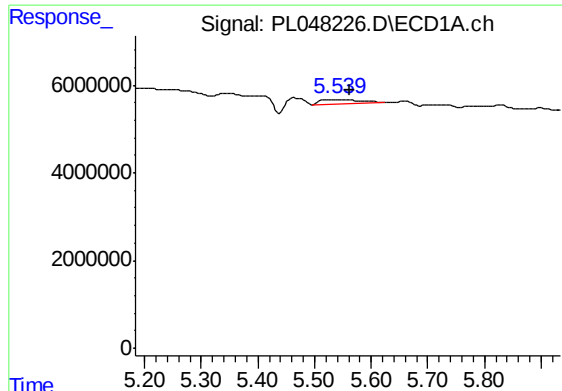

#13 Dielddrin


R.T.: 5.540 min
Delta R.T.: -0.022 min
Response: 4862498
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

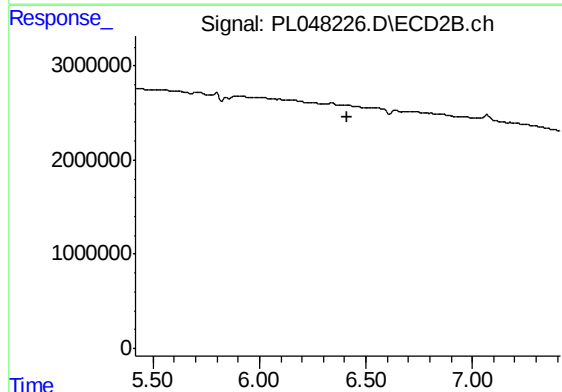


#13 Dielddrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

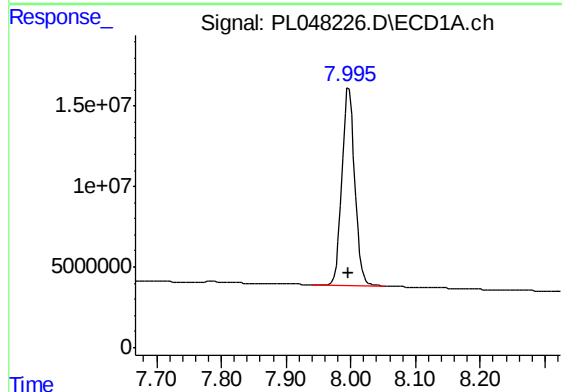

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: 0.001 min
Response: 168426625
Conc: 16.75 ng/ml

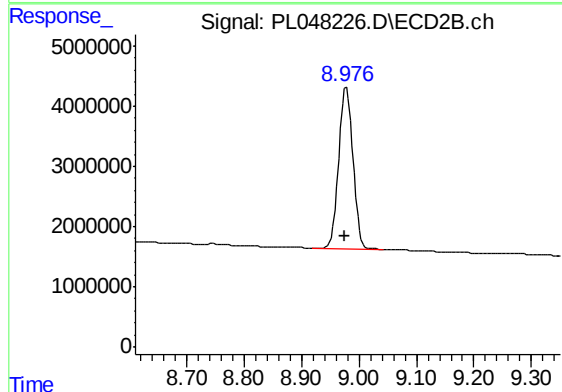

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.002 min
Response: 46459978
Conc: 17.50 ng/ml