

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050619\
 Data File : PL048231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2019 19:35
 Operator : AJ\SJ
 Sample : K2674-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SV28545L

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 00:50:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	142.2E6	36386662	14.683	14.608
28)	SA Decachlor...	7.997	8.978	131.2E6	39900376	13.047	15.032
Target Compounds							
3)	MA gamma-BHC...	4.040	0.000	52500157	0	3.695	N.D. #
4)	MA Heptachlor	4.332f	0.000	4495025	0	0.306	N.D. #
6)	B beta-BHC	4.288	0.000	3887800	0	0.659	N.D. #
7)	B delta-BHC	0.000	4.972f	0	6452647	N.D.	2.282 #
10)	B gamma-Chl...	5.209	0.000	7198039	0	0.539	N.D. #
11)	B alpha-Chl...	5.274	0.000	14487750	0	1.108	N.D. #
13)	MA Dieldrin	5.559	0.000	7719052	0	0.593	N.D. #
14)	MA Endrin	5.838f	0.000	9245007	0	0.759	N.D. #
23)	Chlordane-1	0.000	4.900f	0	6607126	N.D.	54.091 #
25)	Chlordane-3	5.209	0.000	7198039	0	4.571	N.D. #
26)	Chlordane-4	5.274	0.000	14487750	0	9.979	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050619\
Data File : PL048231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2019 19:35
Operator : AJ\SJ
Sample : K2674-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
SV28545L

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 00:50:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

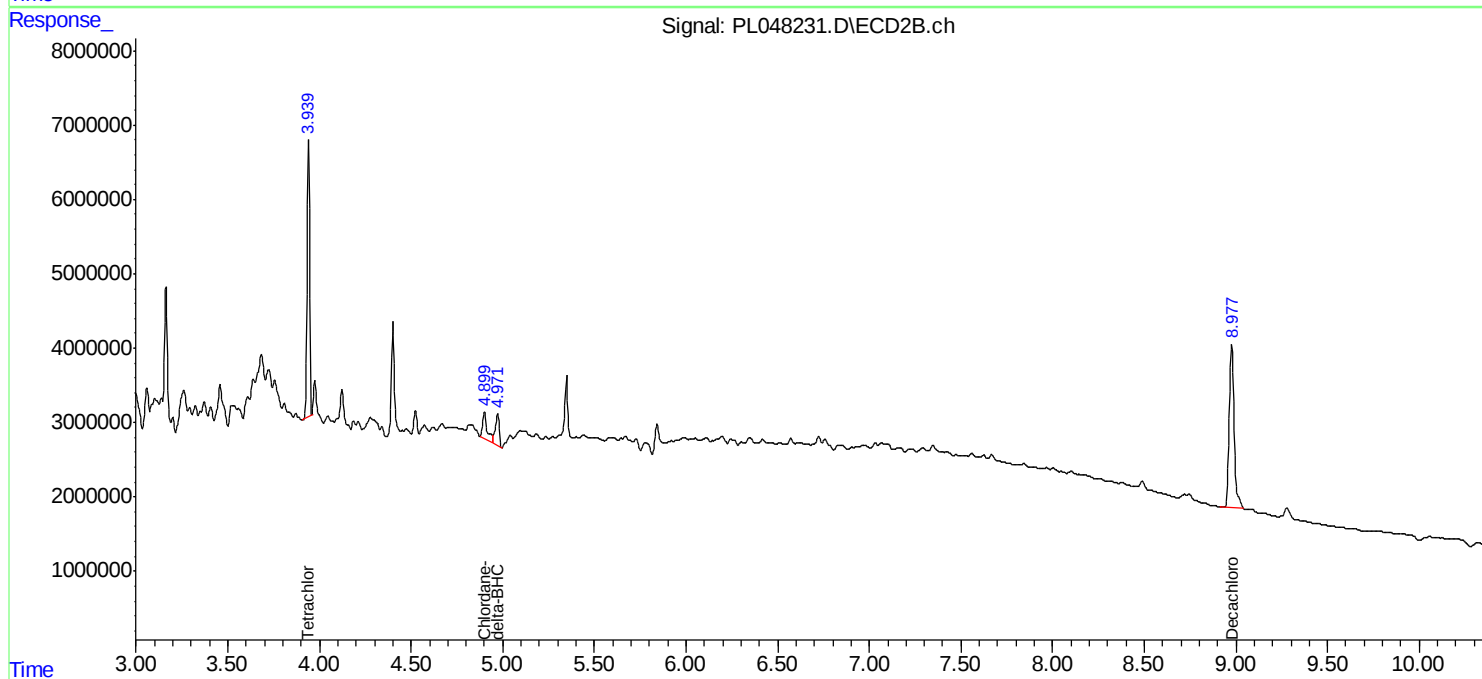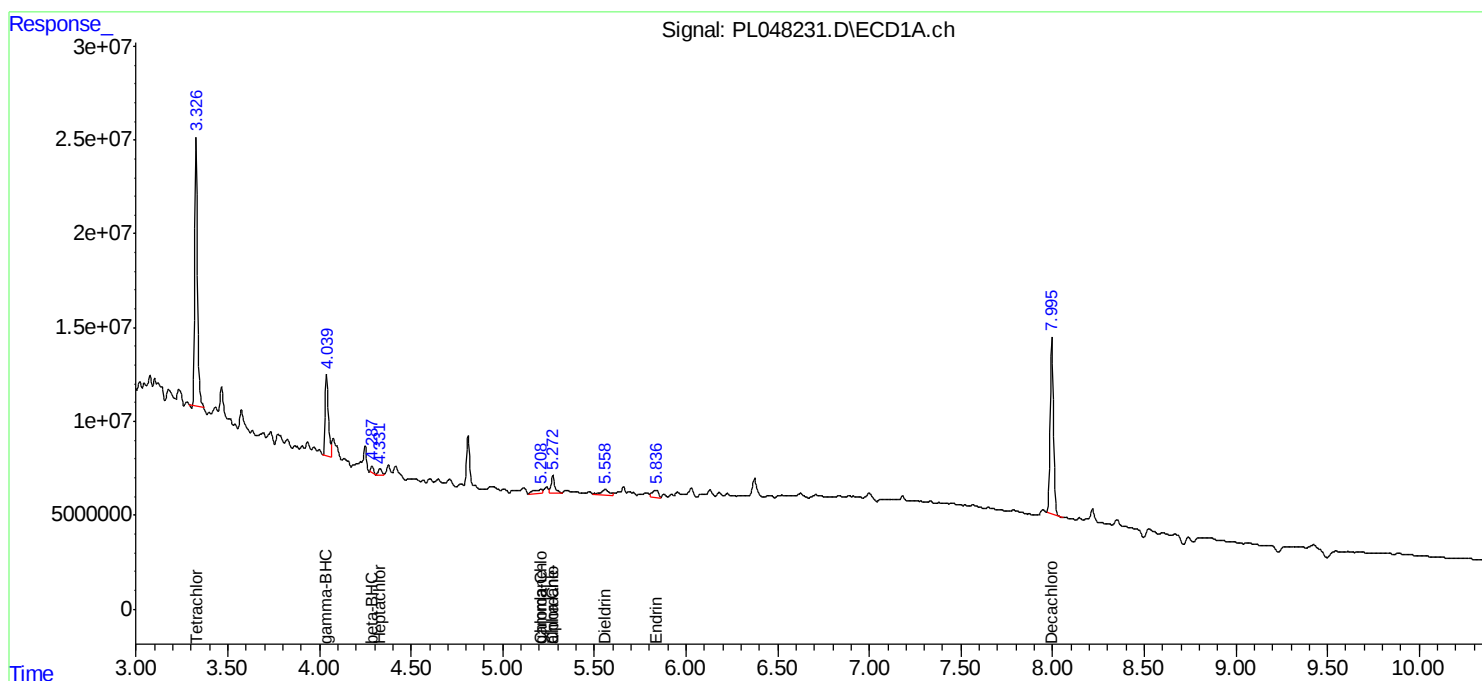


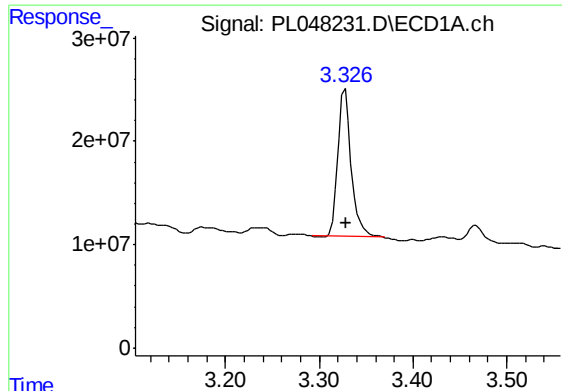

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 142227434
Conc: 14.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV28545L

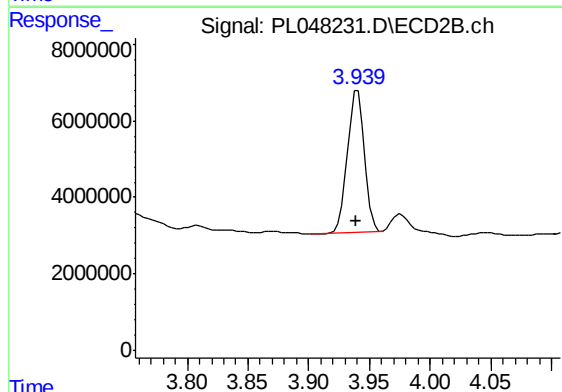


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 36386662
Conc: 14.61 ng/ml

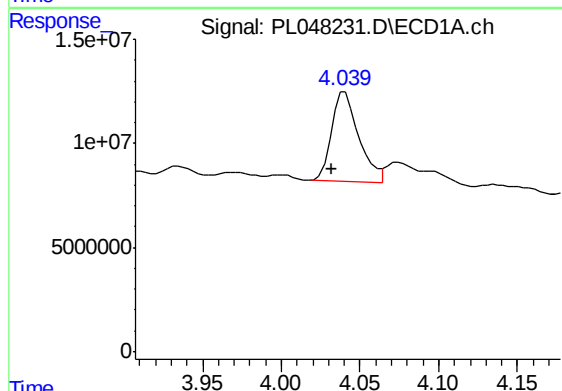


#3 gamma-BHC (Lindane)

R.T.: 4.040 min
Delta R.T.: 0.008 min
Response: 52500157
Conc: 3.69 ng/ml

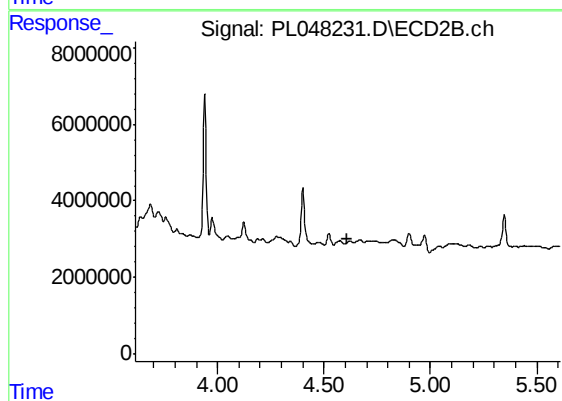

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

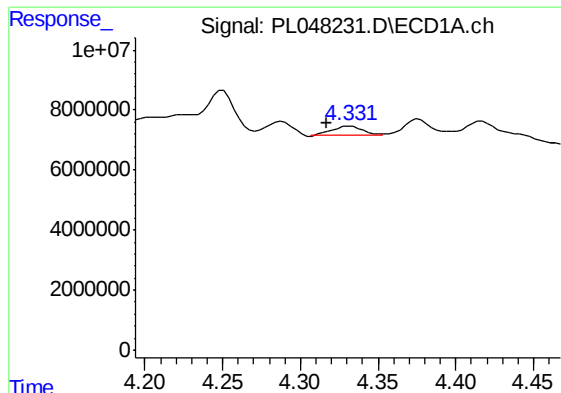

#4 Heptachlor


R.T.: 4.332 min
Delta R.T.: 0.015 min
Response: 4495025
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV28545L

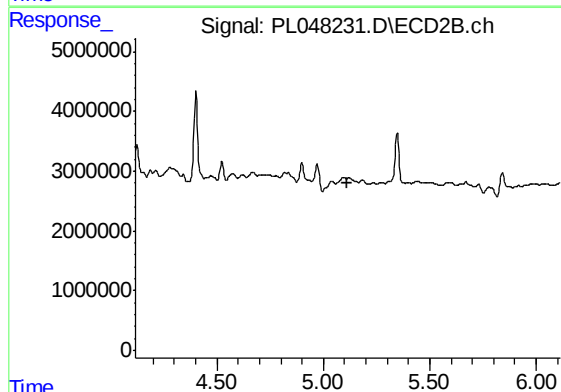


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.116 min
Response: 0
Conc: N.D.

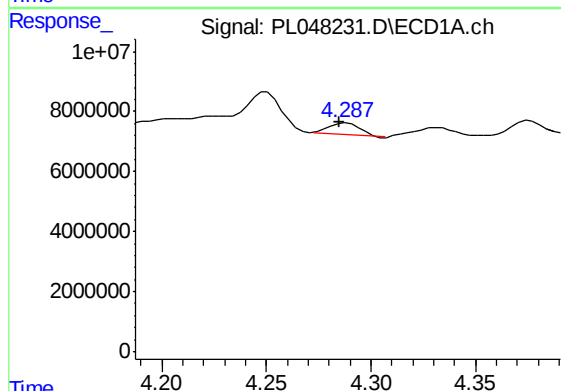


#6 beta-BHC

R.T.: 4.288 min
Delta R.T.: 0.003 min
Response: 3887800
Conc: 0.66 ng/ml

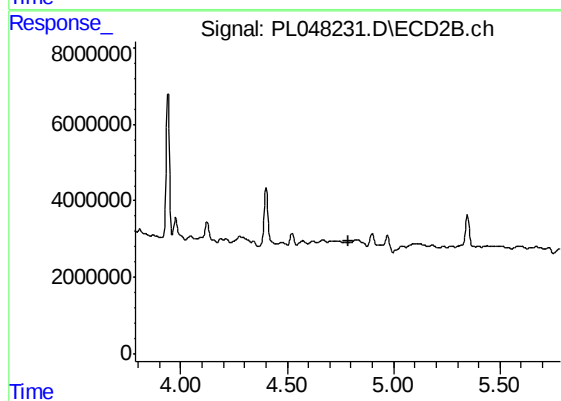

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.786 min
Response: 0
Conc: N.D.

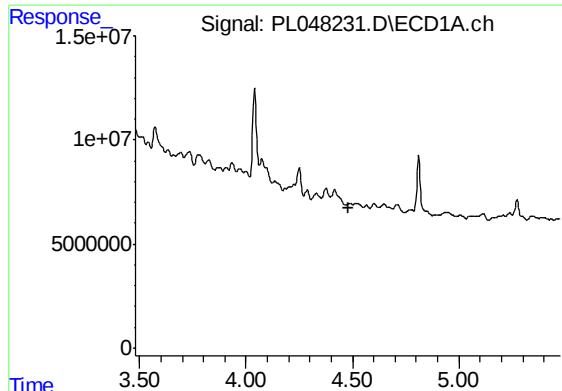

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SV28545L

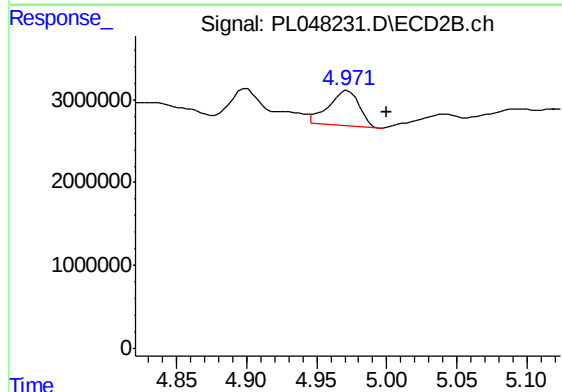


#7 delta-BHC

R.T.: 4.972 min
Delta R.T.: -0.028 min
Response: 6452647
Conc: 2.28 ng/ml

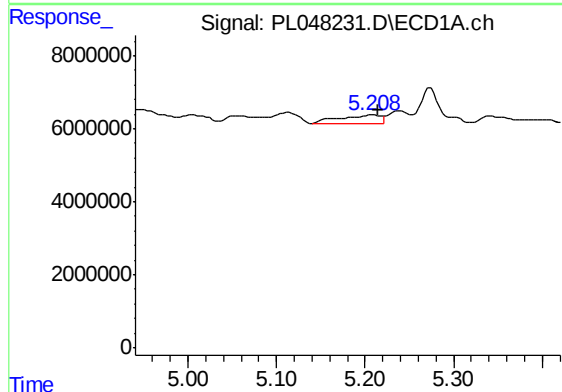


#10 gamma-Chlordane

R.T.: 5.209 min
Delta R.T.: -0.006 min
Response: 7198039
Conc: 0.54 ng/ml

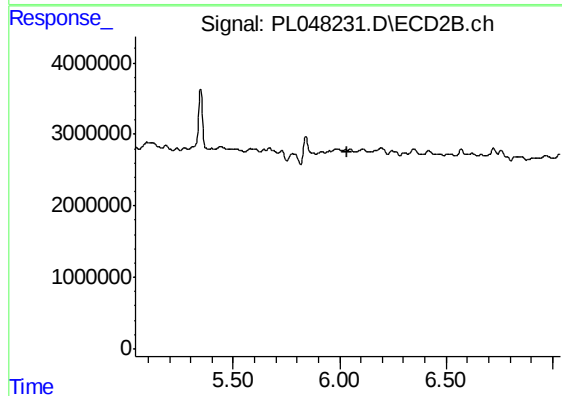

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.038 min
Response: 0
Conc: N.D.

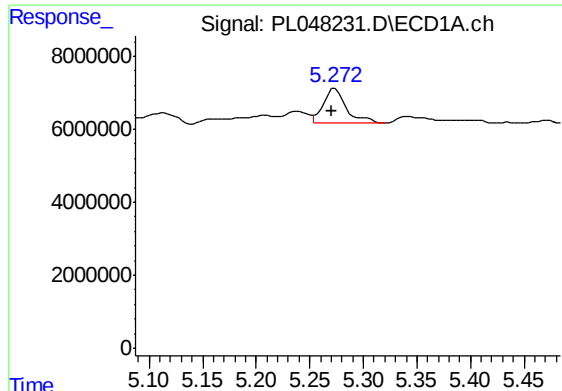

#11 alpha-Chlordane


R.T.: 5.274 min
Delta R.T.: 0.003 min
Response: 14487750
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV28545L

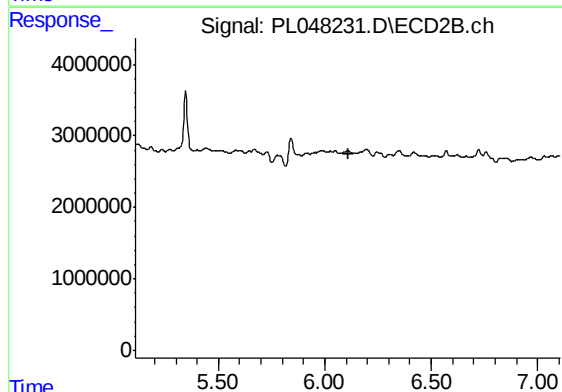


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

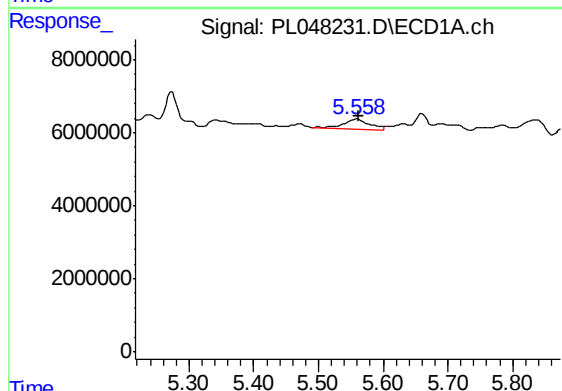


#13 Dieldrin

R.T.: 5.559 min
Delta R.T.: -0.003 min
Response: 7719052
Conc: 0.59 ng/ml

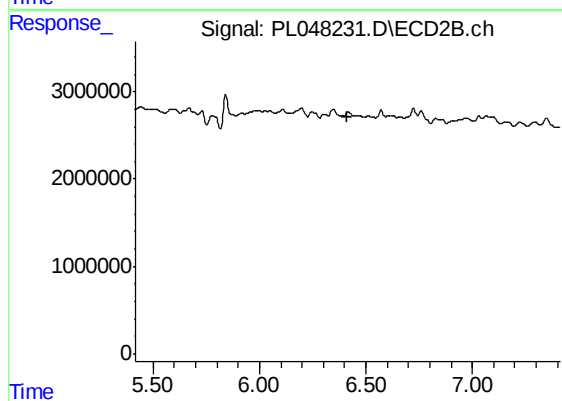

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

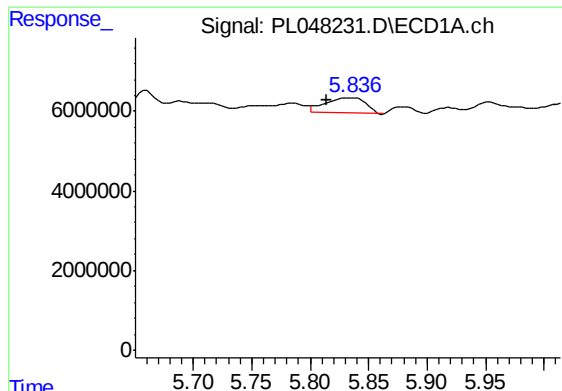

#14 Endrin


R.T.: 5.838 min
Delta R.T.: 0.023 min
Response: 9245007
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV28545L

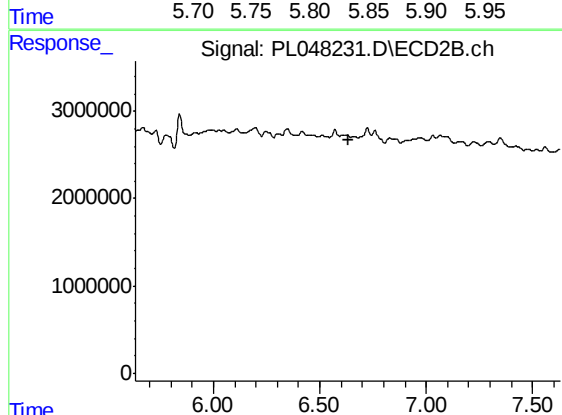


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

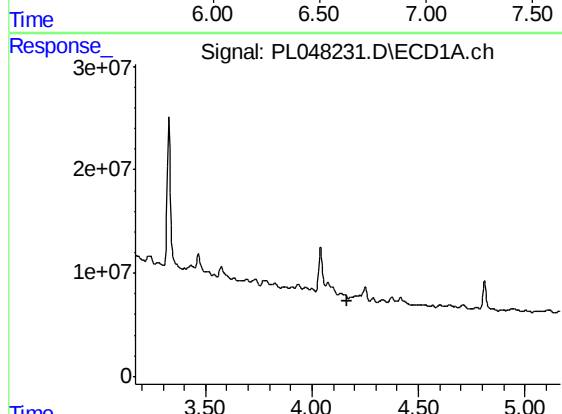


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.168 min
Response: 0
Conc: N.D.

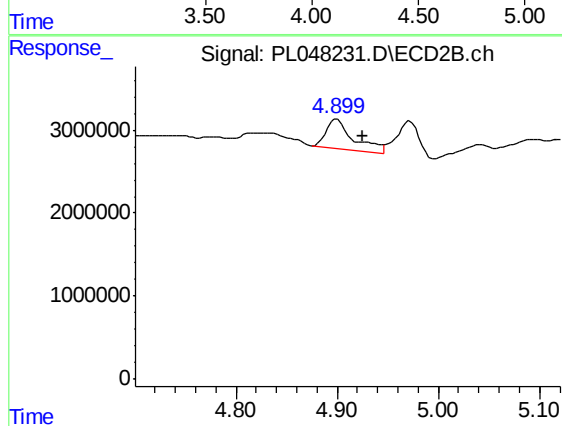

#23 Chlordane-1


R.T.: 4.900 min
Delta R.T.: -0.025 min
Response: 6607126
Conc: 54.09 ng/ml

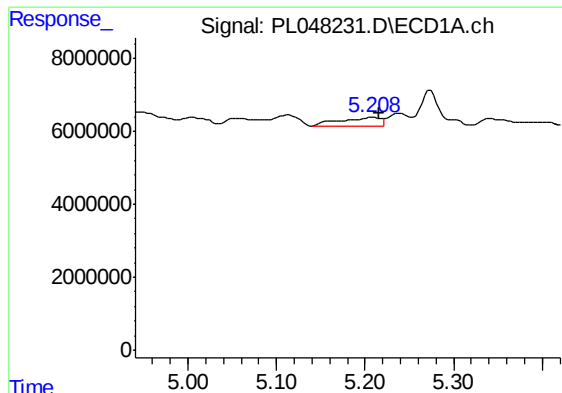

#25 Chlordane-3


R.T.: 5.209 min
Delta R.T.: -0.006 min
Response: 7198039
Conc: 4.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV28545L

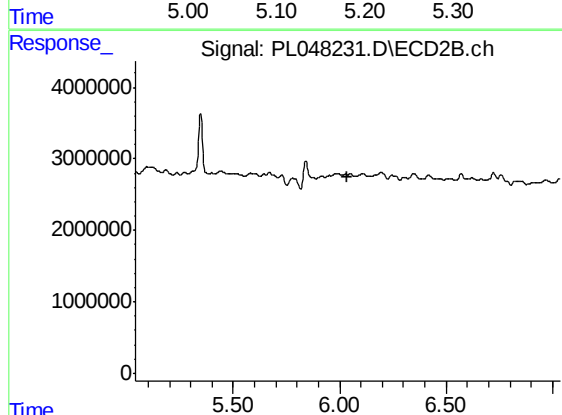


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

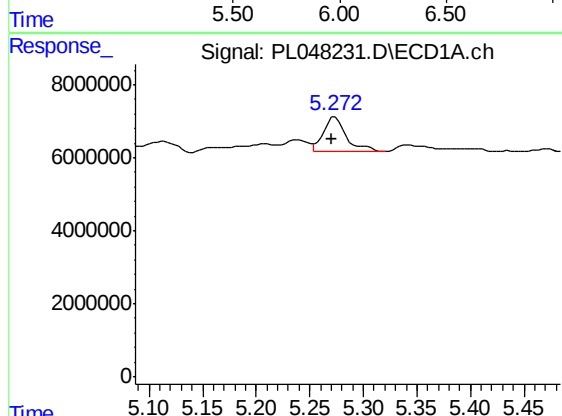


#26 Chlordane-4

R.T.: 5.274 min
Delta R.T.: 0.003 min
Response: 14487750
Conc: 9.98 ng/ml

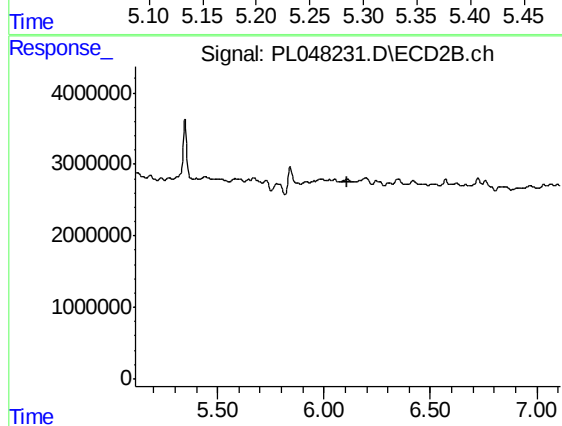

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

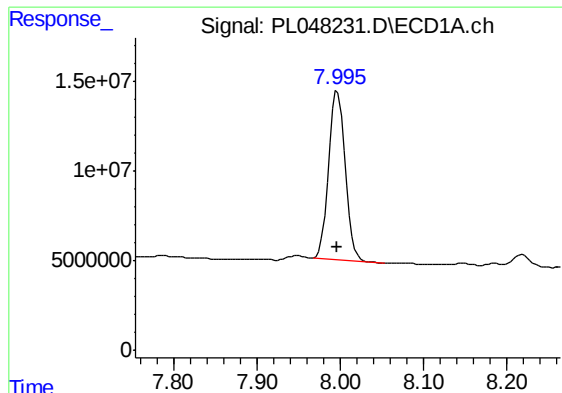

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: 0.000 min
Response: 131178619
Conc: 13.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV28545L

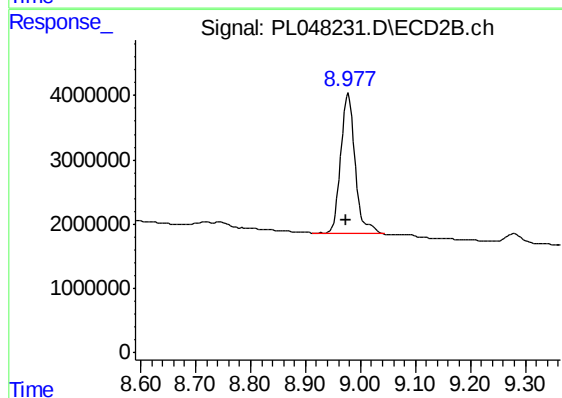

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: 0.003 min
Response: 39900376
Conc: 15.03 ng/ml