

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050620\
 Data File : PL058547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2020 14:17
 Operator : AJ\MA
 Sample : L2491-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 6FT-TP-9

Manual Integrations
 APPROVED

mohammad
 5/8/2020 12:58:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 01:08:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 29 00:55:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.453	3.954	272.6E6	45735164	25.620m	21.160
28)	SA Decachlor...	8.199	8.974	157.1E6	32303030	14.528	14.559

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050620\
Data File : PL058547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2020 14:17
Operator : AJ\MA
Sample : L2491-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
6FT-TP-9


Manual Integrations
APPROVED

mohammad
5/8/2020 12:58:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 01:08:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
Quant Title : GC Extractables
QLast Update : Wed Apr 29 00:55:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

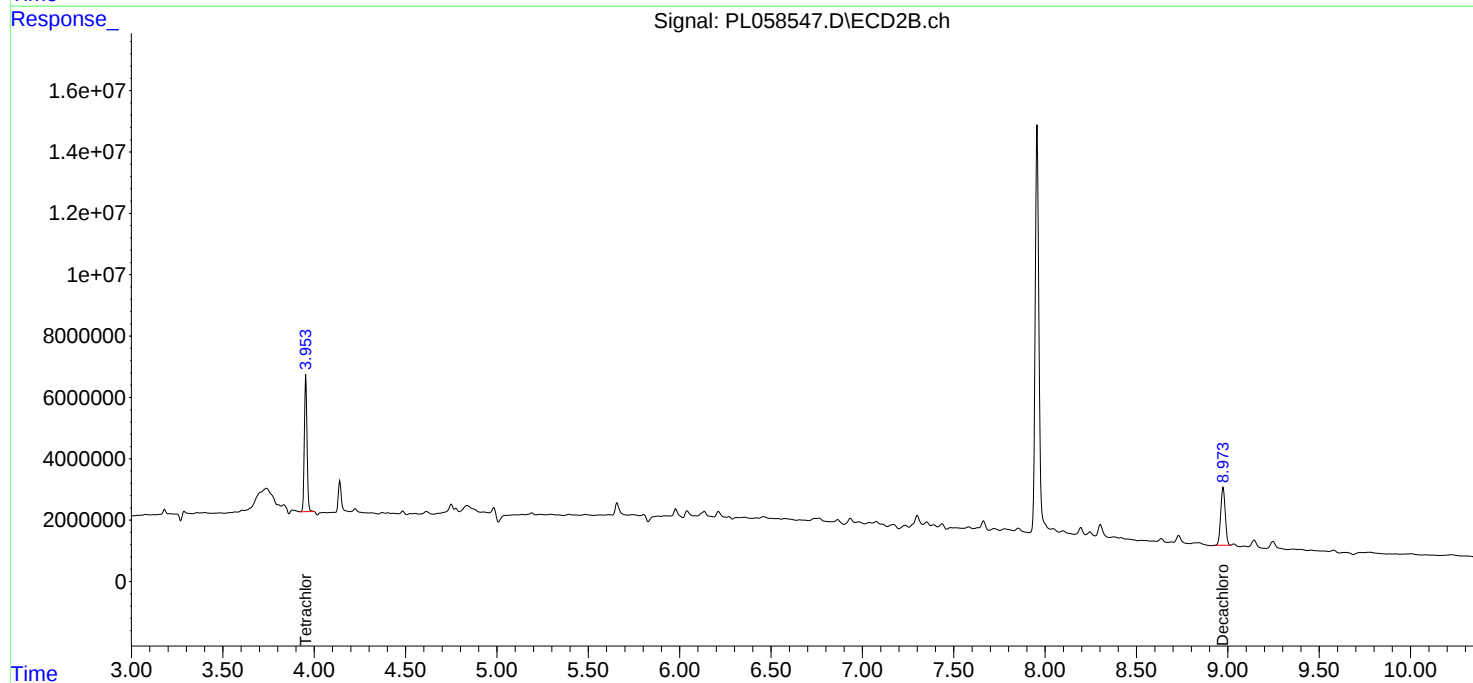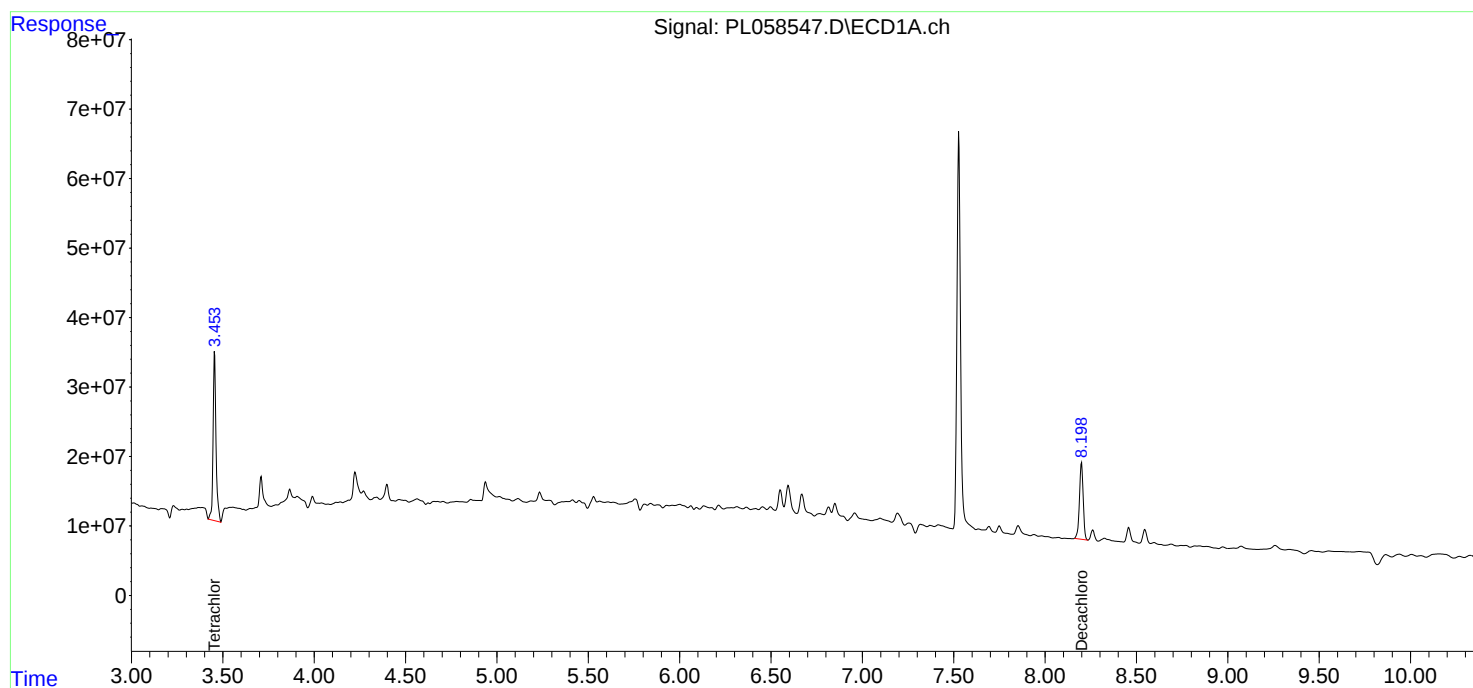

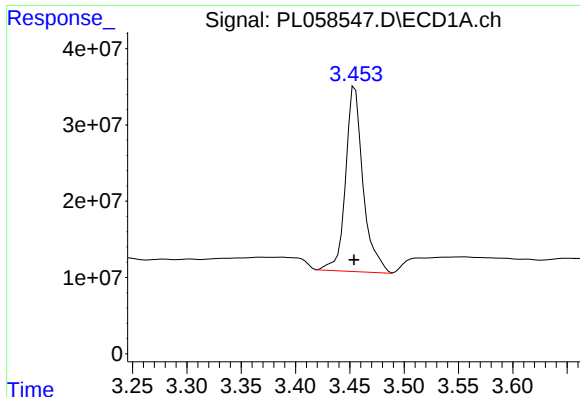


#1 Tetrachloro-m-xylene

R.T.: 3.453 min
Delta R.T.: 0.000 min
Response: 272649316
Conc: 25.62 ng/ml m

Instrument :
ECD_L
ClientSampleId :
6FT-TP-9


Manual Integrations
APPROVED

mohammad
5/8/2020 12:58:11 PM

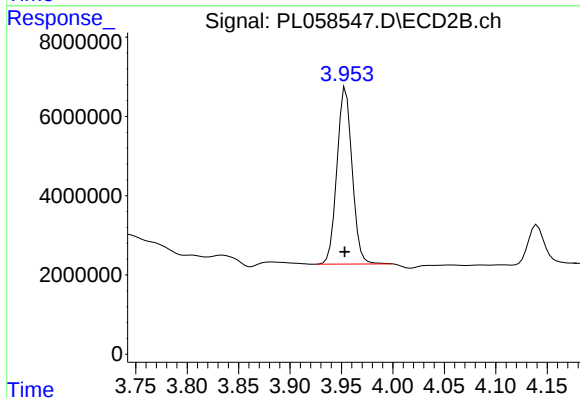


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: 0.001 min
Response: 45735164
Conc: 21.16 ng/ml

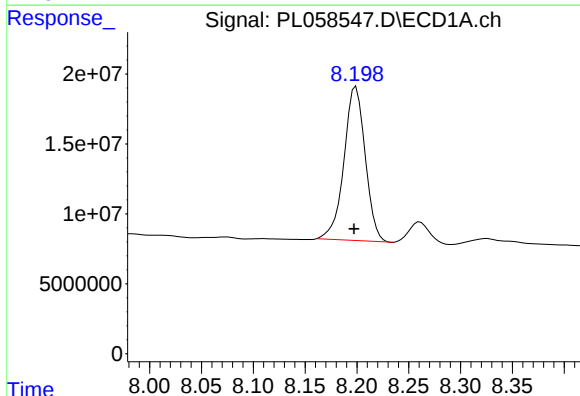

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.002 min
Response: 157113667
Conc: 14.53 ng/ml

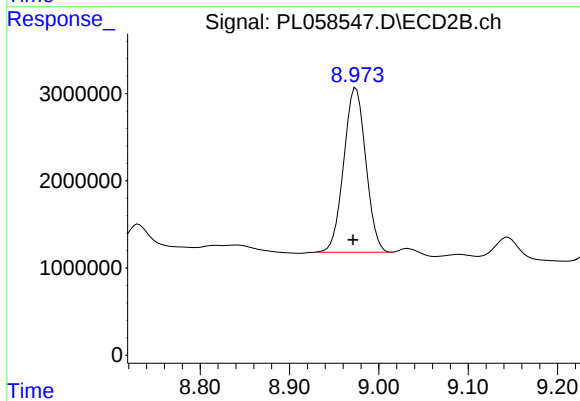

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: 0.003 min
Response: 32303030
Conc: 14.56 ng/ml