

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050620\
 Data File : PL058553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2020 15:43
 Operator : AJ\MA
 Sample : L2513-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BU-03-050520

Manual Integrations
 APPROVED

mohammad
 5/8/2020 12:58:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 01:10:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 29 00:55:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.454	3.954	160.0E6	29557034	15.038	13.675
28)	SA Decachlor...	8.199	8.975	138.1E6	30193190	12.769	13.608
Target Compounds							
12)	B 4,4'-DDE	5.612	6.273	8354700	2499281	0.553m	0.819 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050620\
Data File : PL058553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2020 15:43
Operator : AJ\MA
Sample : L2513-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BU-03-050520


Manual Integrations
APPROVED

mohammad
5/8/2020 12:58:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 01:10:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
Quant Title : GC Extractables
QLast Update : Wed Apr 29 00:55:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

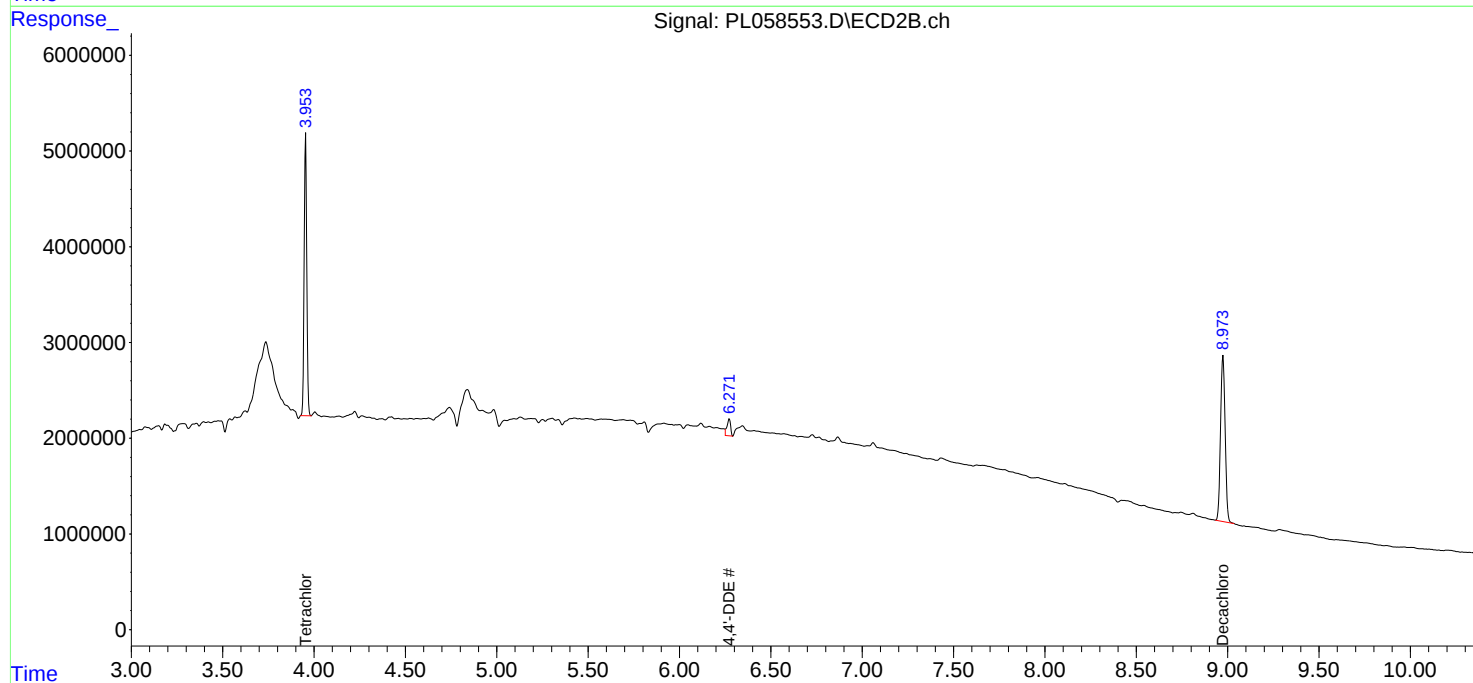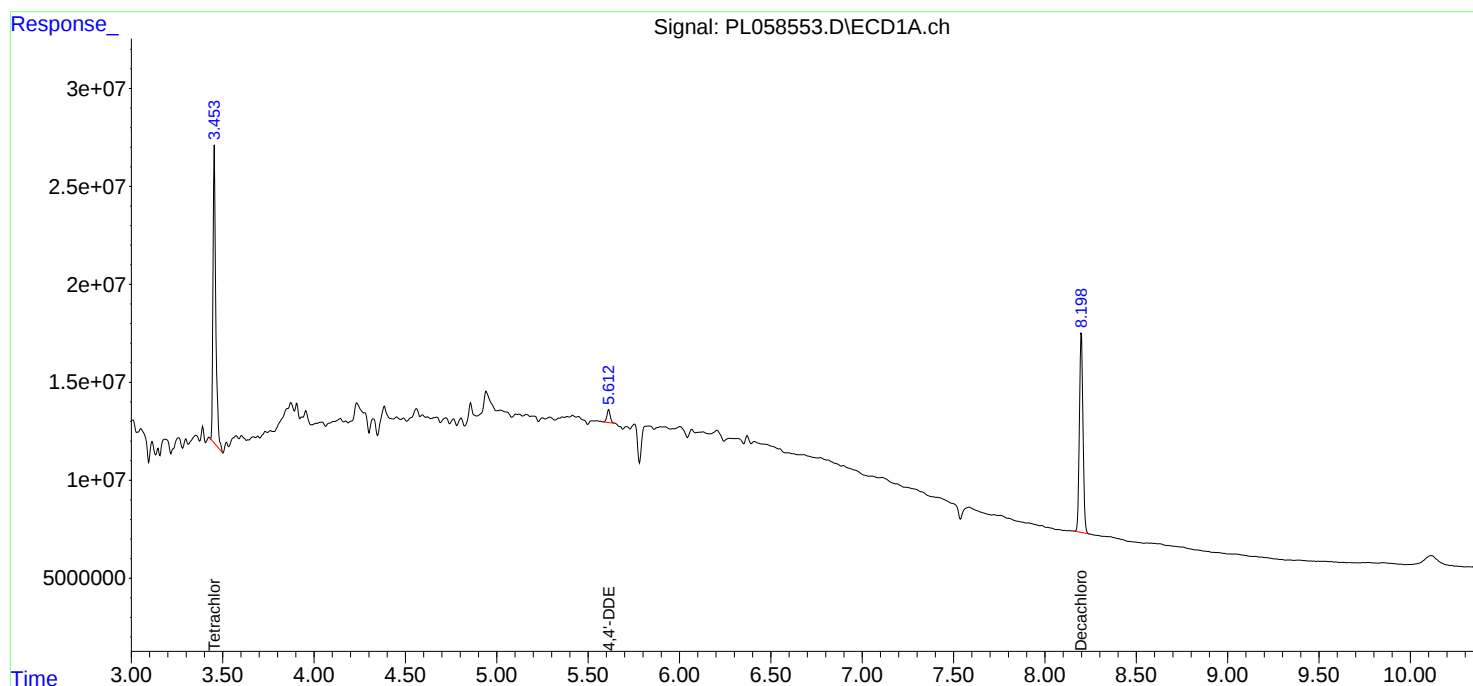

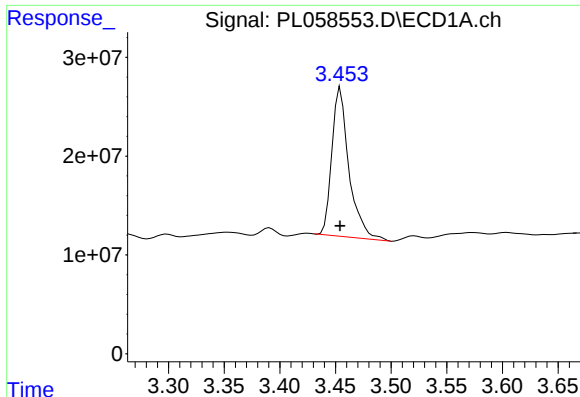


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: 0.000 min
Response: 160039940
Conc: 15.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-03-050520


Manual Integrations
APPROVED

mohammad
5/8/2020 12:58:24 PM

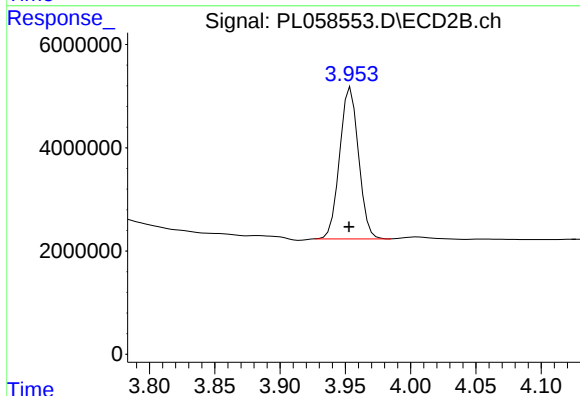


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: 0.001 min
Response: 29557034
Conc: 13.67 ng/ml

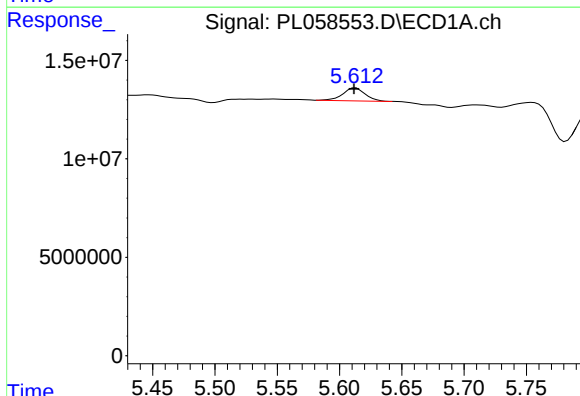


#12 4,4'-DDE

R.T.: 5.612 min
Delta R.T.: 0.000 min
Response: 8354700
Conc: 0.55 ng/ml m

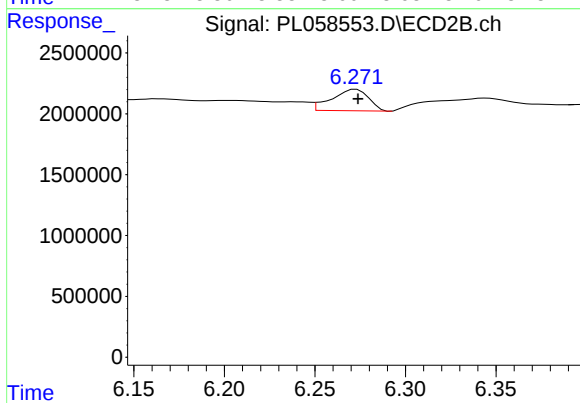

#12 4,4'-DDE

R.T.: 6.273 min
Delta R.T.: -0.001 min
Response: 2499281
Conc: 0.82 ng/ml

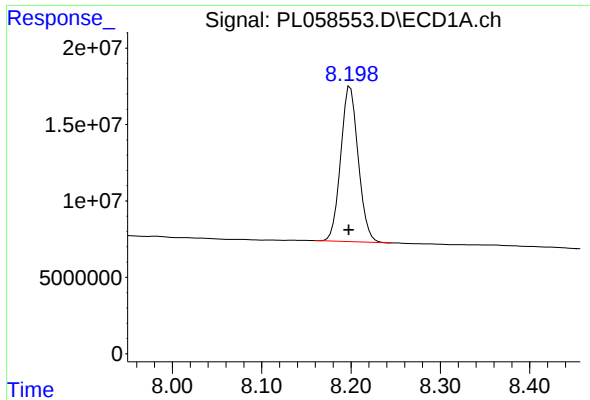


#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.002 min
Response: 138088256
Conc: 12.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-03-050520

Manual Integrations
APPROVED

mohammad
5/8/2020 12:58:24 PM

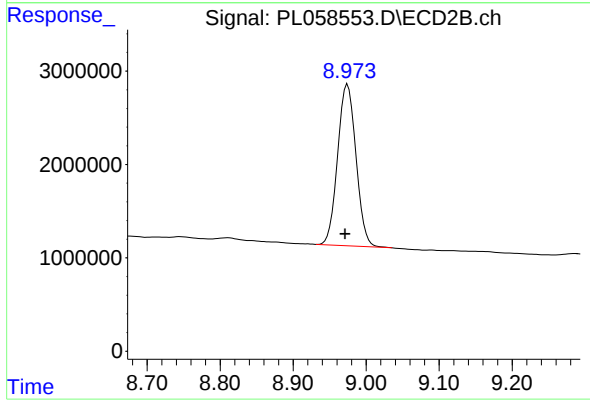

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.003 min
Response: 30193190
Conc: 13.61 ng/ml