

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050621\
 Data File : PL066731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2021 12:09
 Operator : AR\AJ
 Sample : M2280-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-072

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 05:09:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.425	4.151	44762795	45705484	11.880	13.014
28)	SA Decachlor...	8.144	9.346	40400740	33364366	10.537	10.785
Target Compounds							
11)	B alpha-Chl...	5.397	6.380	4580334	8555375	0.930m	2.062 #
12)	B 4,4'-DDE	5.564	6.536	2069042	2636379	0.453m	0.695 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050621\
Data File : PL066731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2021 12:09
Operator : AR\AJ
Sample : M2280-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-072

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 05:09:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

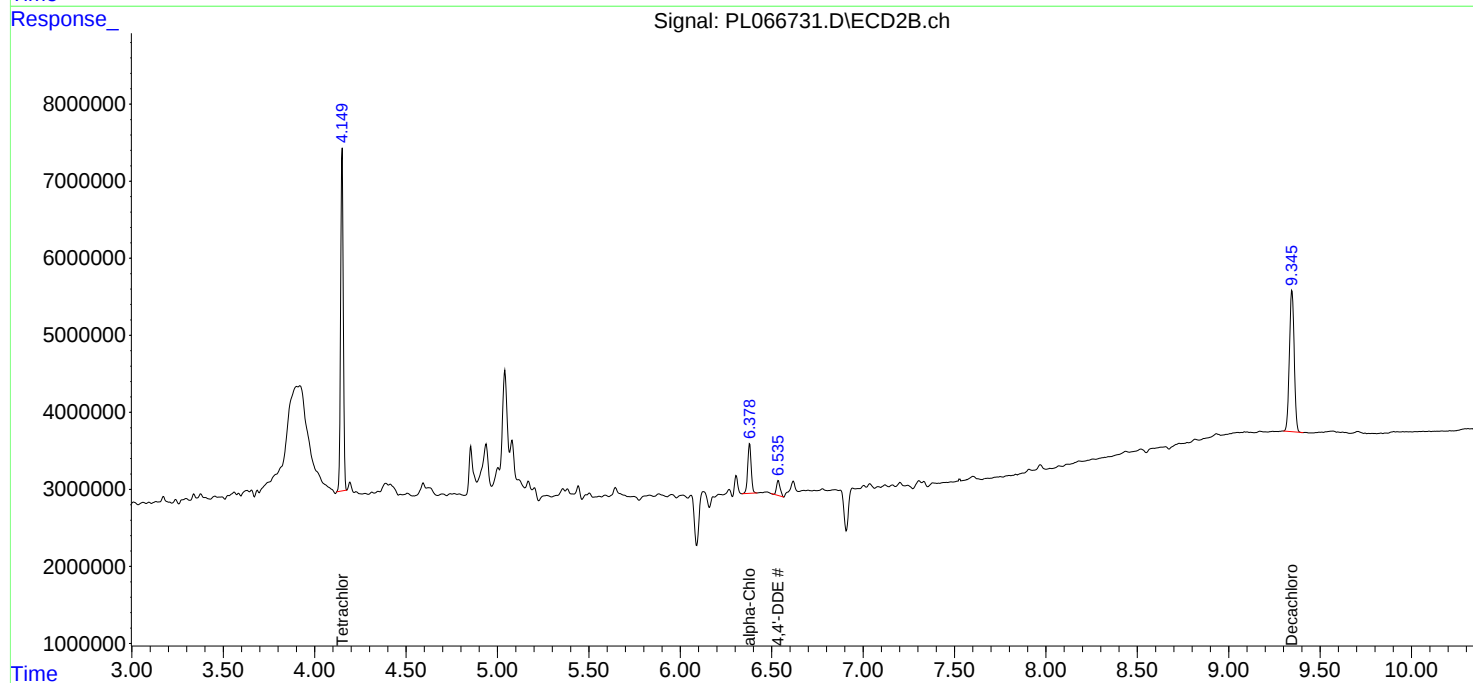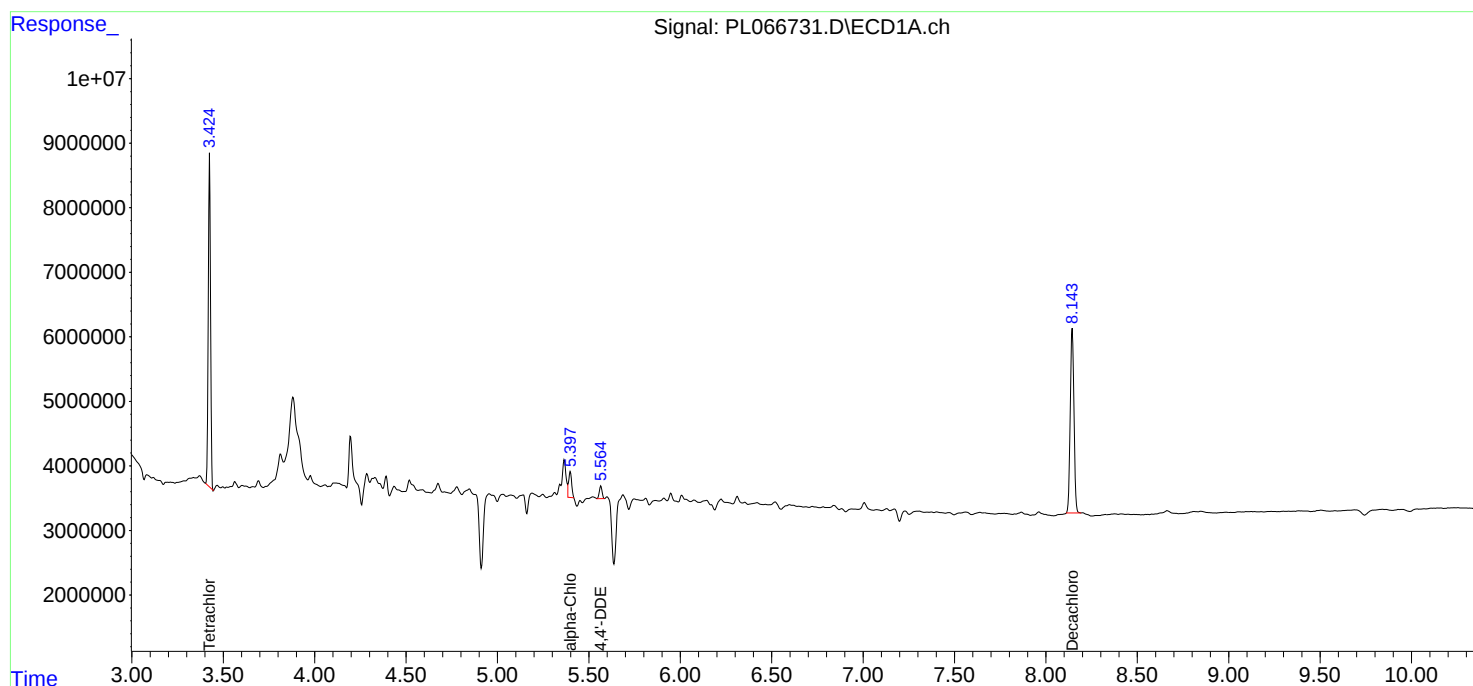


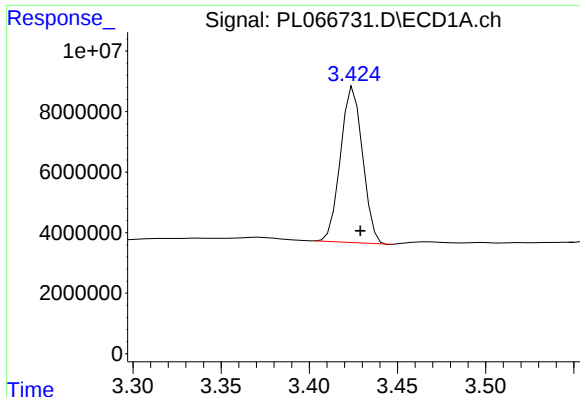

#1 Tetrachloro-m-xylene


R.T.: 3.425 min
Delta R.T.: -0.004 min
Response: 44762795
Conc: 11.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-072

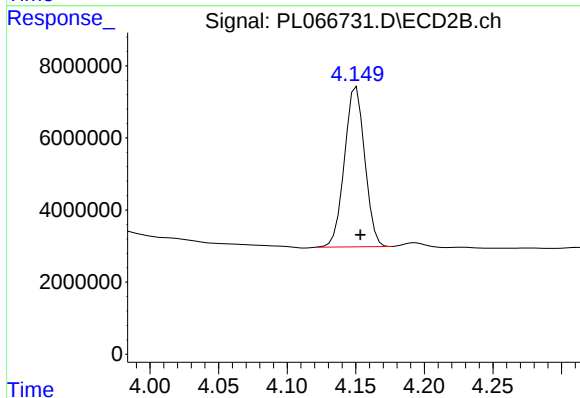


#1 Tetrachloro-m-xylene

R.T.: 4.151 min
Delta R.T.: -0.003 min
Response: 45705484
Conc: 13.01 ng/ml

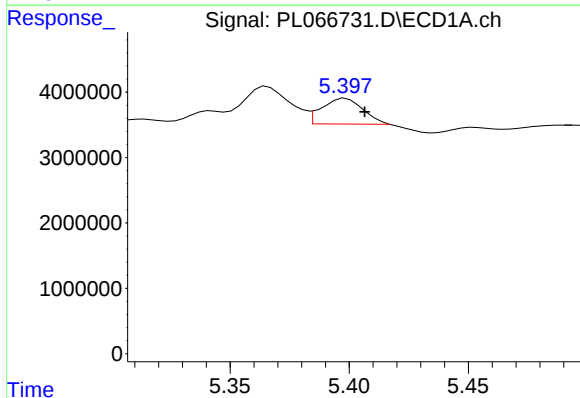


#11 alpha-Chlordane

R.T.: 5.397 min
Delta R.T.: -0.009 min
Response: 4580334
Conc: 0.93 ng/ml m

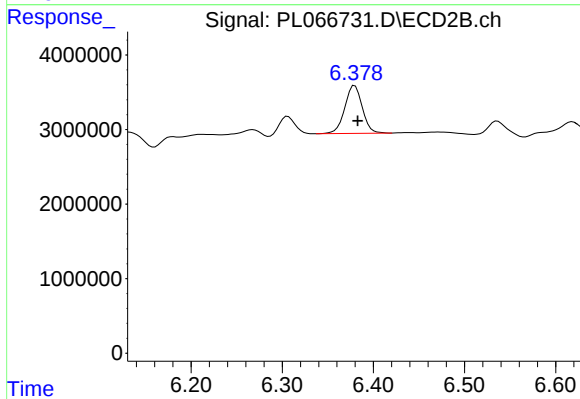

#11 alpha-Chlordane


R.T.: 6.380 min
Delta R.T.: -0.003 min
Response: 8555375
Conc: 2.06 ng/ml

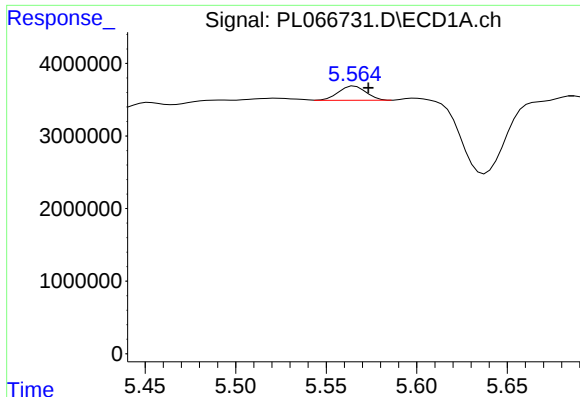

#12 4,4'-DDE


R.T.: 5.564 min
Delta R.T.: -0.009 min
Response: 2069042
Conc: 0.45 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-072

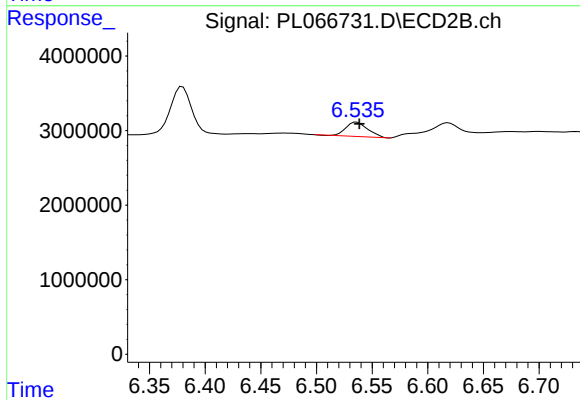


#12 4,4'-DDE

R.T.: 6.536 min
Delta R.T.: -0.002 min
Response: 2636379
Conc: 0.69 ng/ml

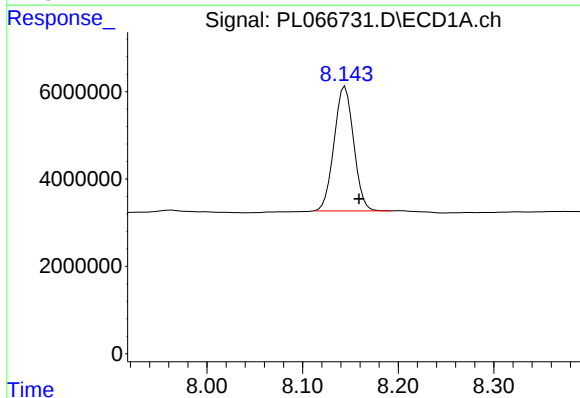

#28 Decachlorobiphenyl

R.T.: 8.144 min
Delta R.T.: -0.015 min
Response: 40400740
Conc: 10.54 ng/ml

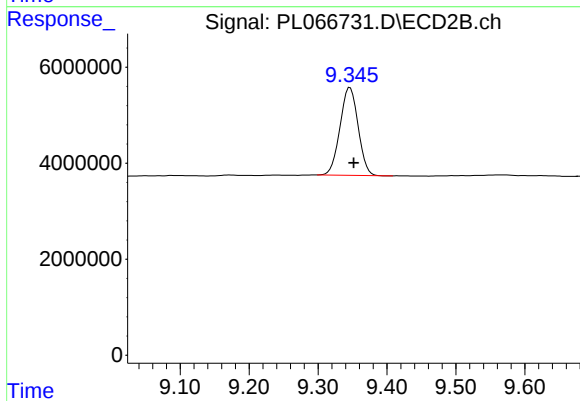

#28 Decachlorobiphenyl

R.T.: 9.346 min
Delta R.T.: -0.005 min
Response: 33364366
Conc: 10.79 ng/ml