

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050624\
 Data File : PL089375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2024 15:06
 Operator : AR\AJ
 Sample : P2378-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-05032024

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/07/2024
 Supervised By :Ankita Jodhani 05/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 10:56:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 26 19:27:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.796	22218450	13188206	11.034	10.279
2) SA Decachlor...	9.066	7.948	12668517	10815845	9.055	8.040
Target Compounds						
17) MA 4,4'-DDT	7.030	6.065	1482981	887231	0.806m	0.656

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050624\
Data File : PL089375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2024 15:06
Operator : AR\AJ
Sample : P2378-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-02-05032024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/07/2024
Supervised By : Ankita Jodhani 05/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 10:56:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
Quant Title : GC Extractables
QLast Update : Fri Apr 26 19:27:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

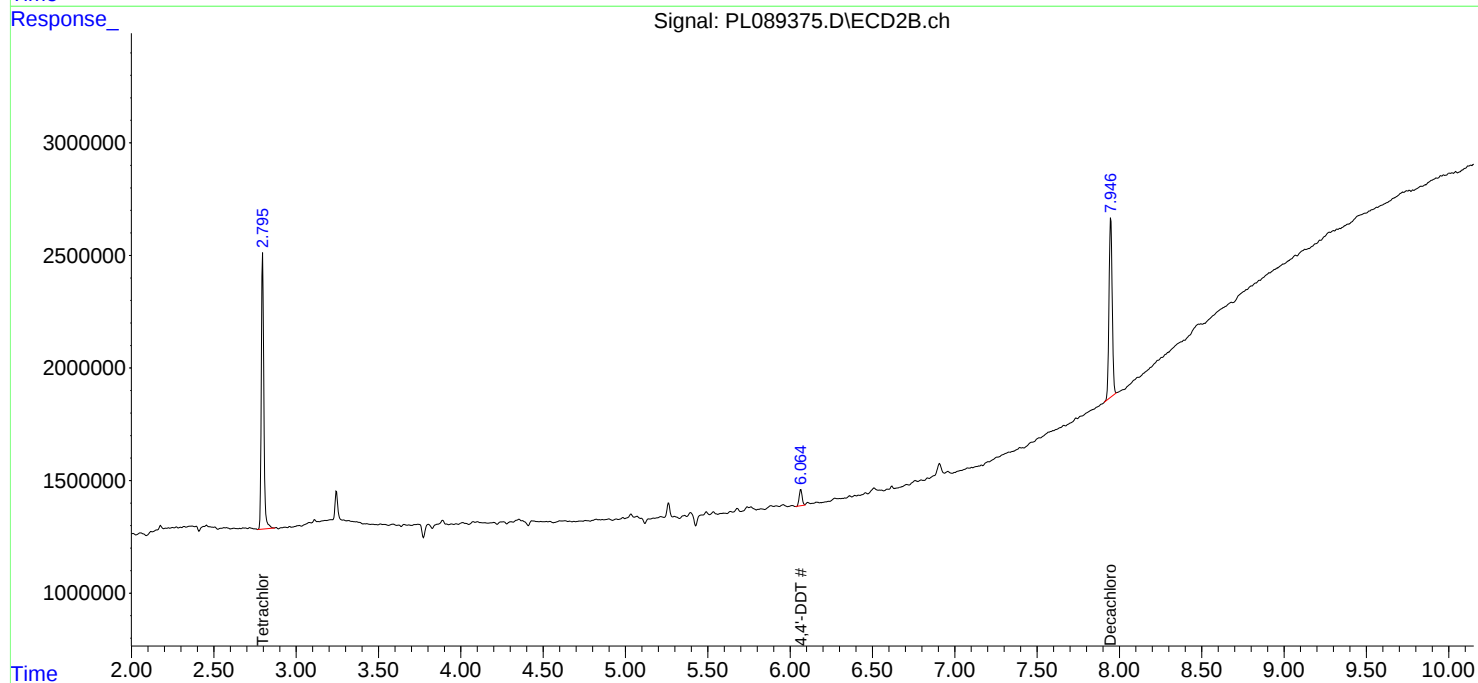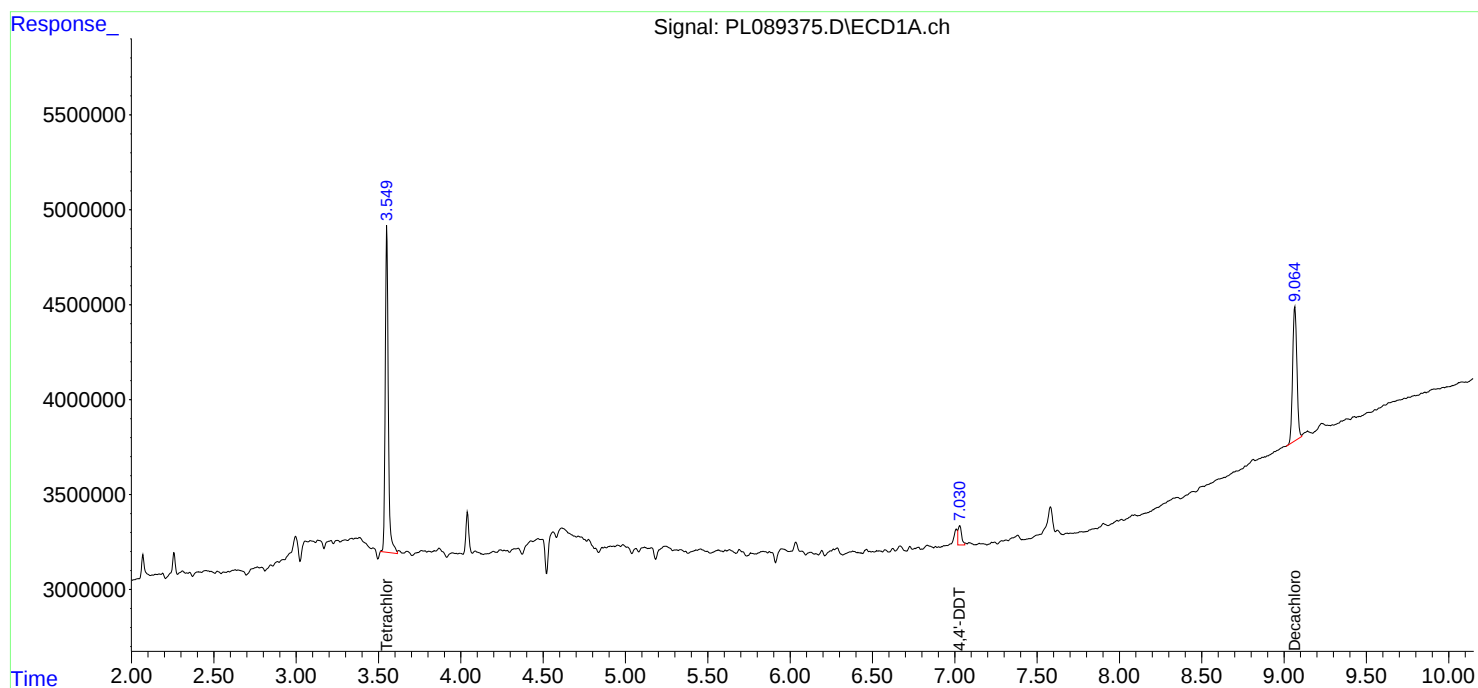

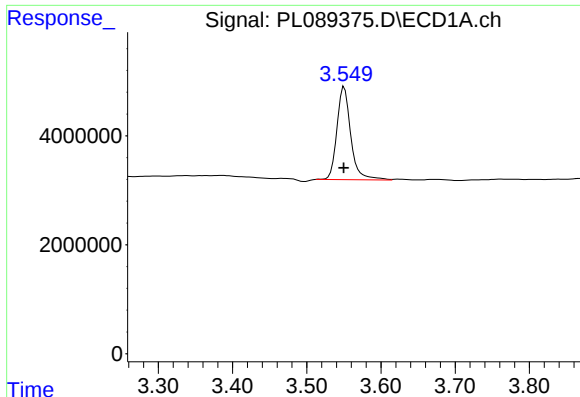


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 22218450
Conc: 11.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-05032024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/07/2024
Supervised By :Ankita Jodhani 05/07/2024

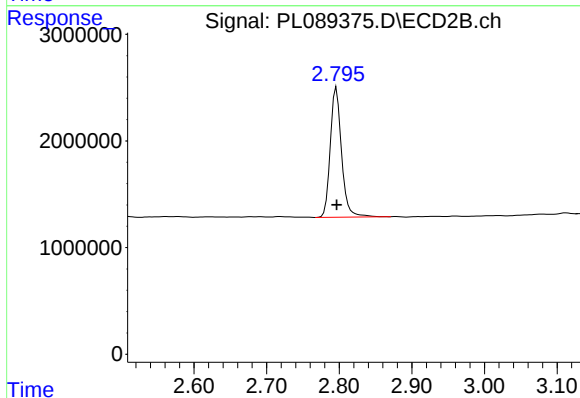


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 13188206
Conc: 10.28 ng/ml

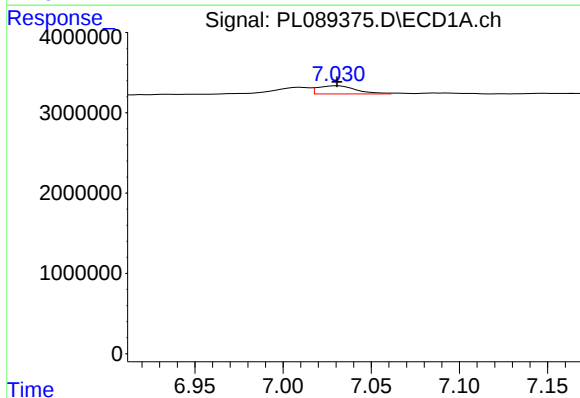


#17 4,4'-DDT

R.T.: 7.030 min
Delta R.T.: 0.000 min
Response: 1482981
Conc: 0.81 ng/ml m

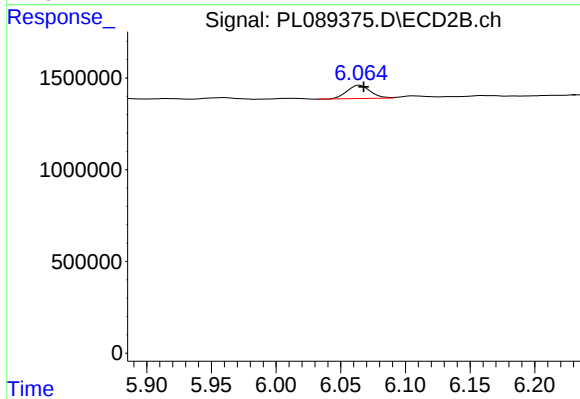

#17 4,4'-DDT

R.T.: 6.065 min
Delta R.T.: -0.003 min
Response: 887231
Conc: 0.66 ng/ml

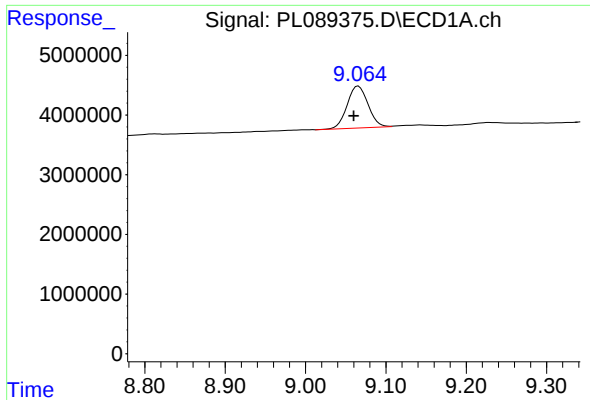


#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.006 min
Response: 12668517
Conc: 9.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-05032024

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/07/2024
Supervised By :Ankita Jodhani 05/07/2024

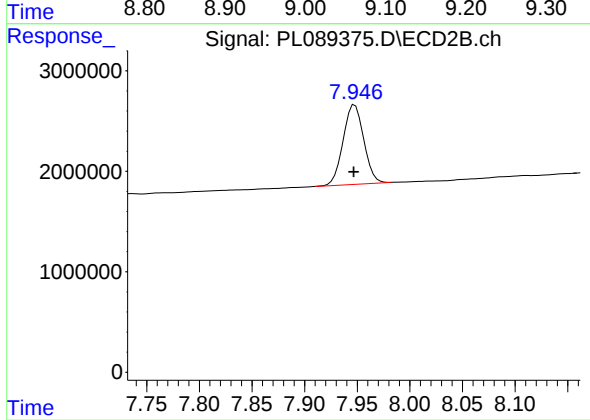

#28 Decachlorobiphenyl

R.T.: 7.948 min
Delta R.T.: 0.001 min
Response: 10815845
Conc: 8.04 ng/ml