

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050625\
Data File : PL095528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2025 08:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 01:37:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.595	2.912	56860627	68798591	17.417	21.636
28) SA Decachlor...	9.120	8.090	54048671	61070371	19.506	20.637
Target Compounds						
6) B beta-BHC	0.000	4.019f	0	4805873	N.D.	2.315 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050625\
Data File : PL095528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 May 2025 08:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 01:37:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

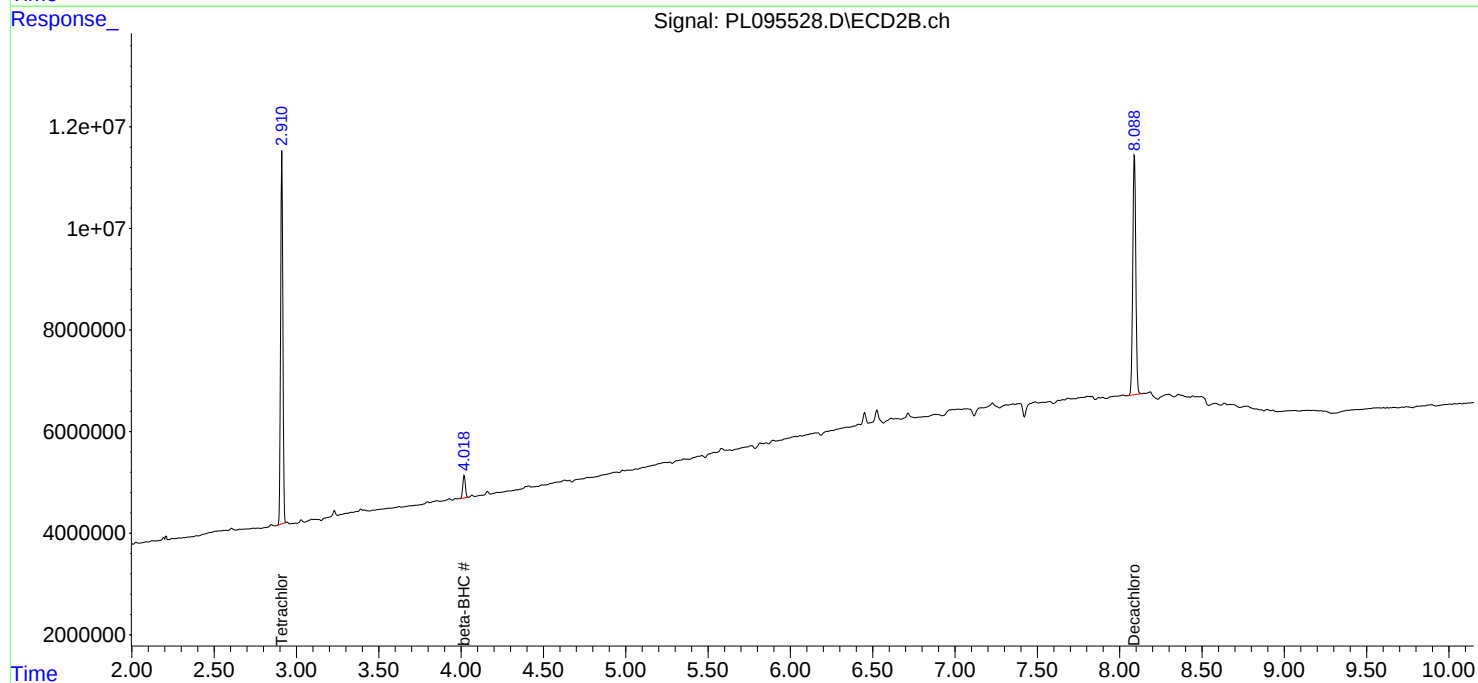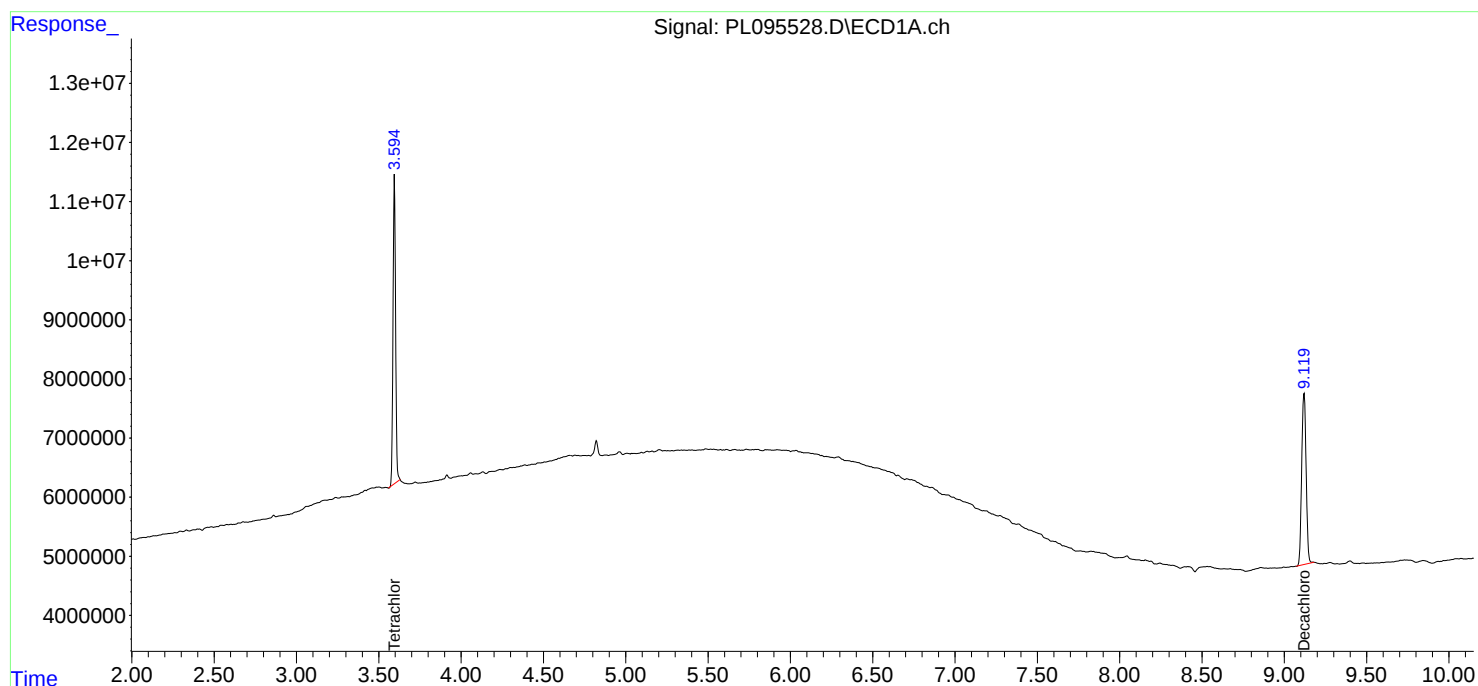


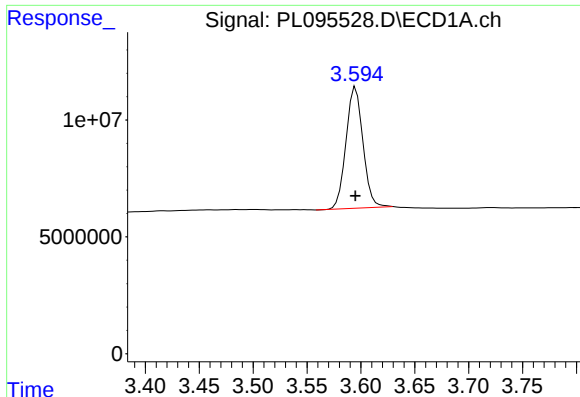

#1 Tetrachloro-m-xylene


R.T.: 3.595 min
Delta R.T.: 0.000 min
Response: 56860627
Conc: 17.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

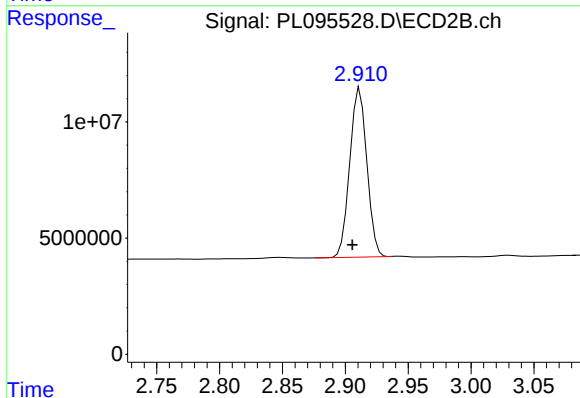


#1 Tetrachloro-m-xylene

R.T.: 2.912 min
Delta R.T.: 0.006 min
Response: 68798591
Conc: 21.64 ng/ml

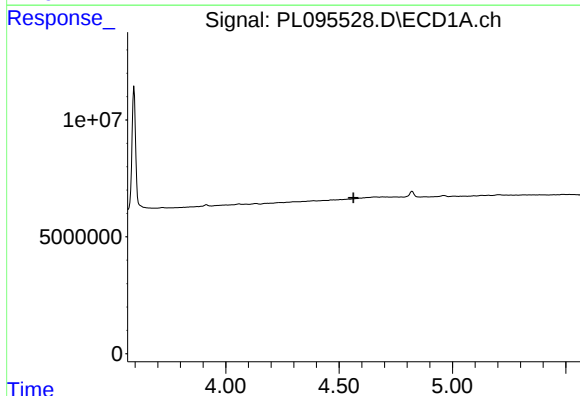


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.564 min
Response: 0
Conc: N.D.

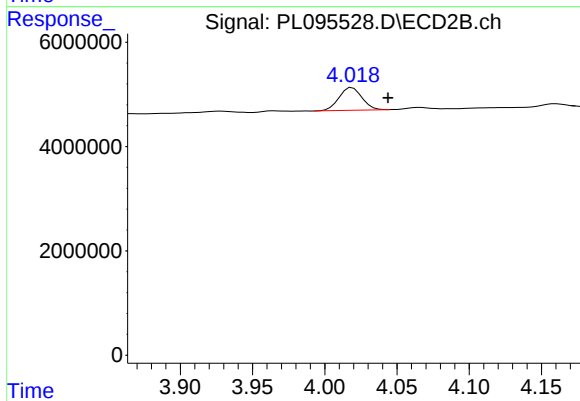

#6 beta-BHC


R.T.: 4.019 min
Delta R.T.: -0.025 min
Response: 4805873
Conc: 2.32 ng/ml

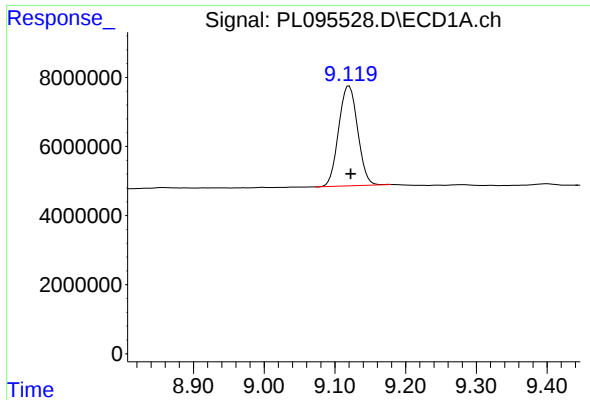

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: -0.002 min
Response: 54048671
Conc: 19.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

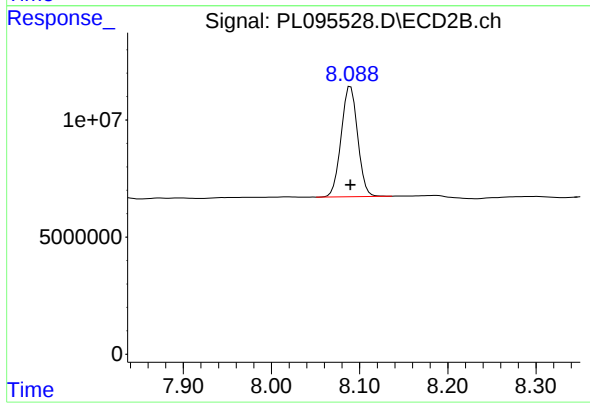

#28 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 61070371
Conc: 20.64 ng/ml