

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050721\
 Data File : PL066759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 11:04
 Operator : AR\AJ
 Sample : PB136205BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB136205BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 17:15:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.151	71166934	70236431	18.887	19.999
28)	SA Decachlor...	8.147	9.349	70559675	57783093	18.403	18.678
Target Compounds							
15)	B Endosulfa...	0.000	7.122	0	2037788	N.D.	0.617 #
23)	Chlordane-1	4.311f	0.000	2777022	0	16.429	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050721\
Data File : PL066759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 11:04
Operator : AR\AJ
Sample : PB136205BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB136205BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 17:15:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

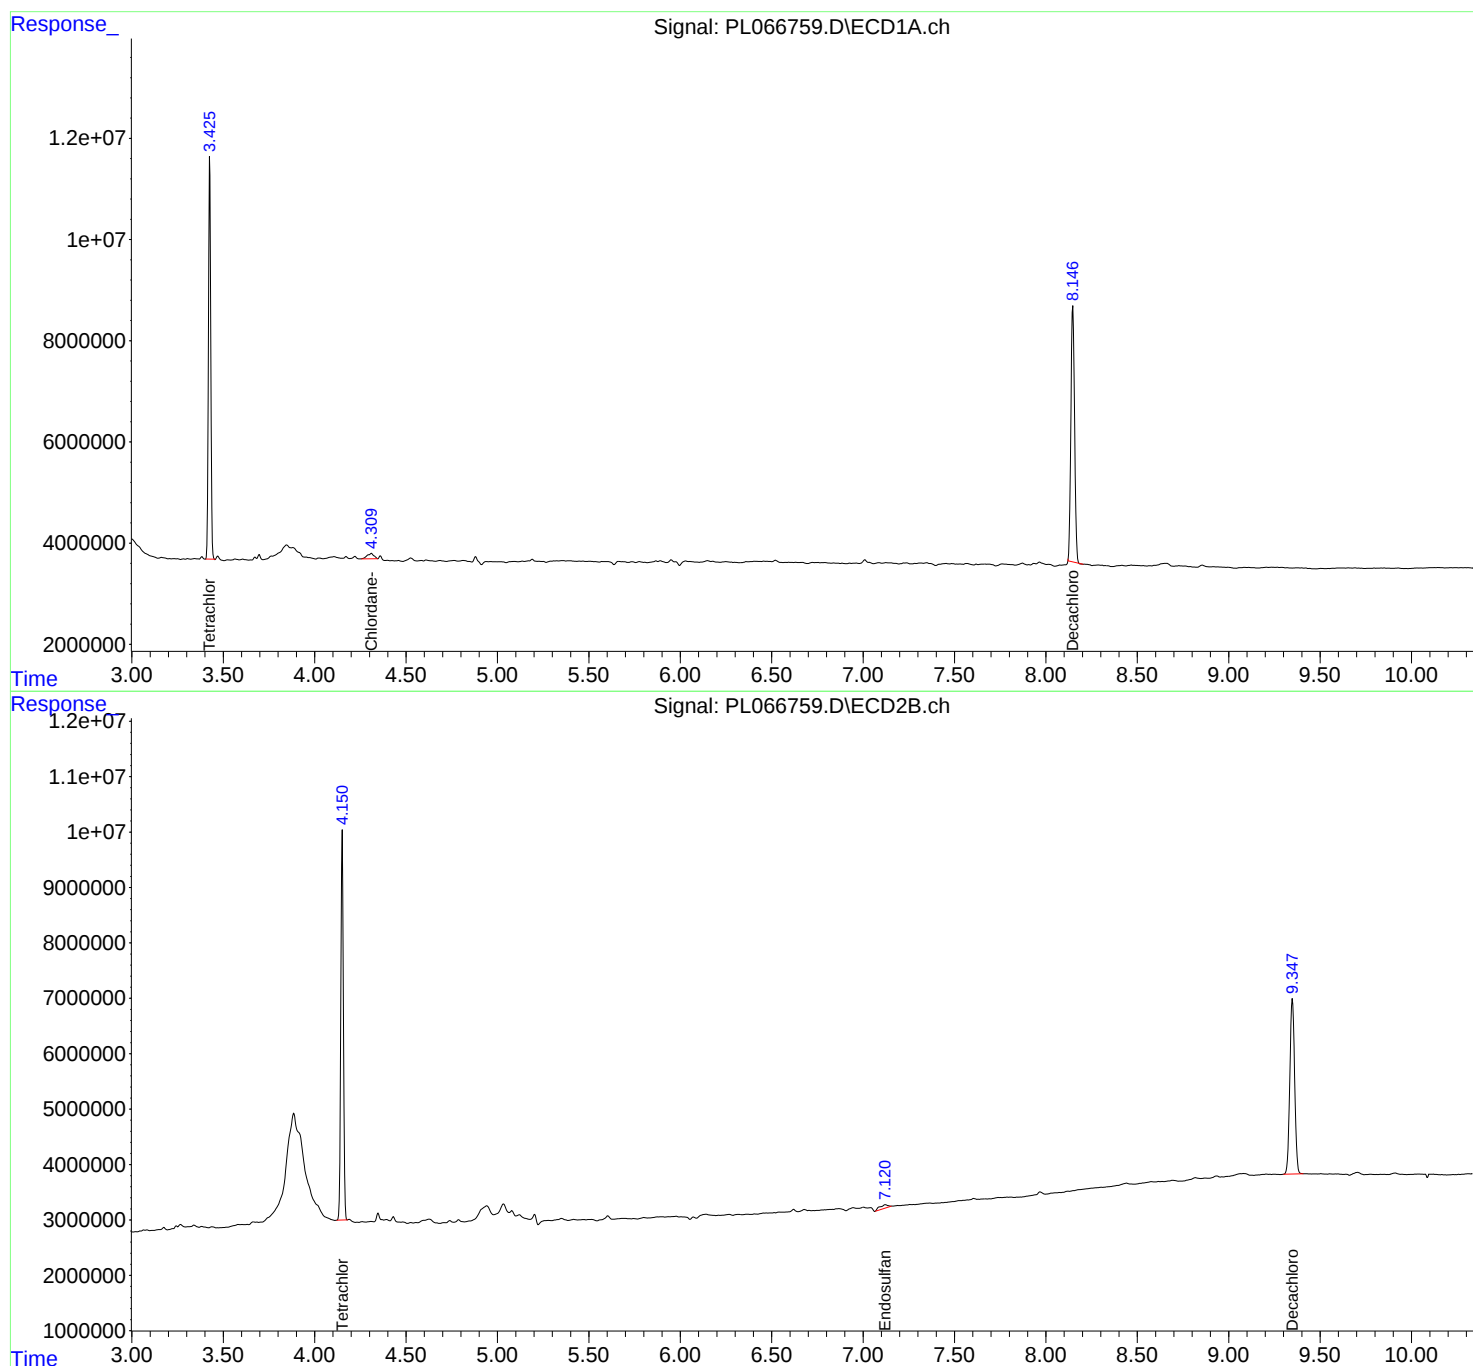


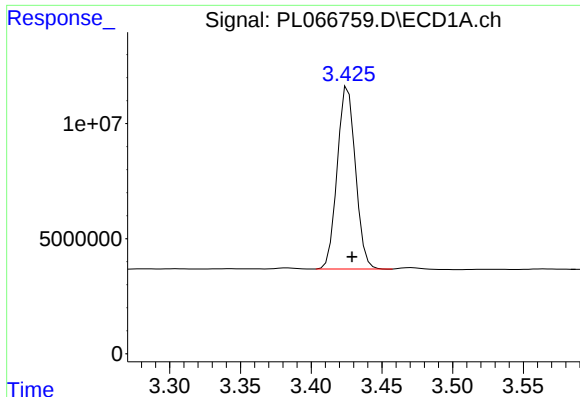

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: -0.003 min
Response: 71166934
Conc: 18.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136205BL

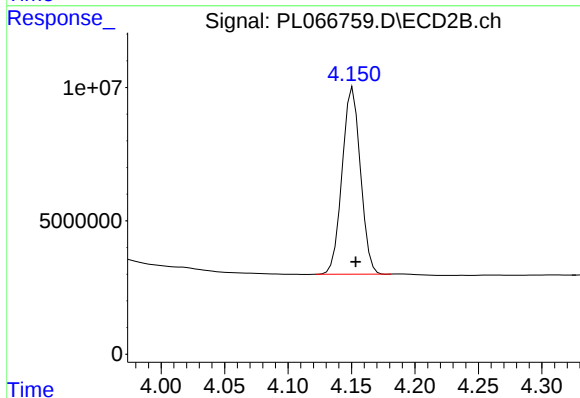


#1 Tetrachloro-m-xylene

R.T.: 4.151 min
Delta R.T.: -0.002 min
Response: 70236431
Conc: 20.00 ng/ml

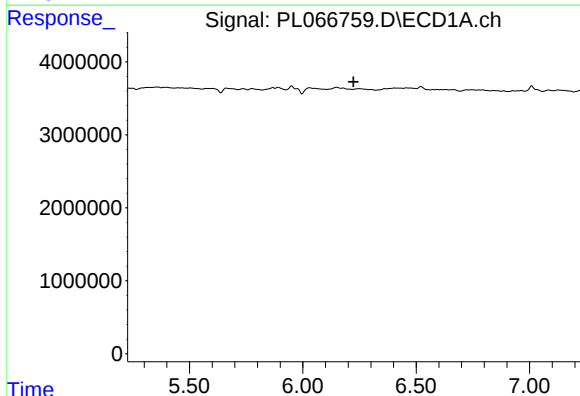


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.224 min
Response: 0
Conc: N.D.

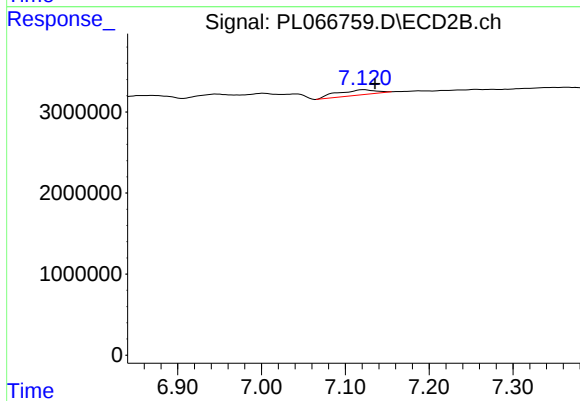

#15 Endosulfan II


R.T.: 7.122 min
Delta R.T.: -0.013 min
Response: 2037788
Conc: 0.62 ng/ml

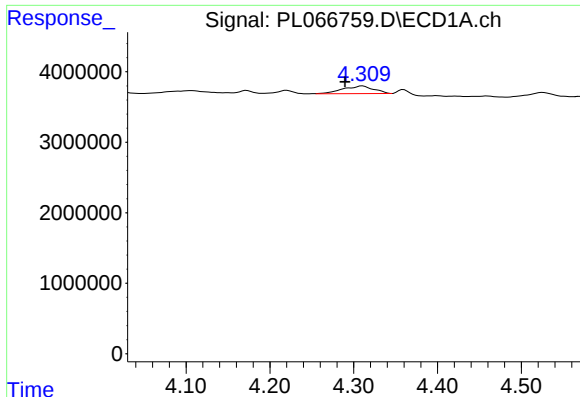

#23 Chlordane-1


R.T.: 4.311 min
Delta R.T.: 0.021 min
Response: 2777022
Conc: 16.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB136205BL

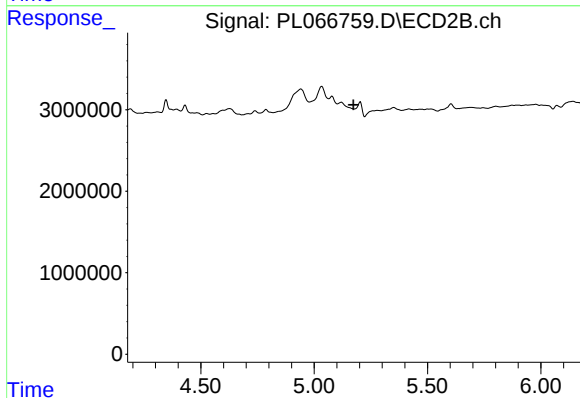


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.174 min
Response: 0
Conc: N.D.

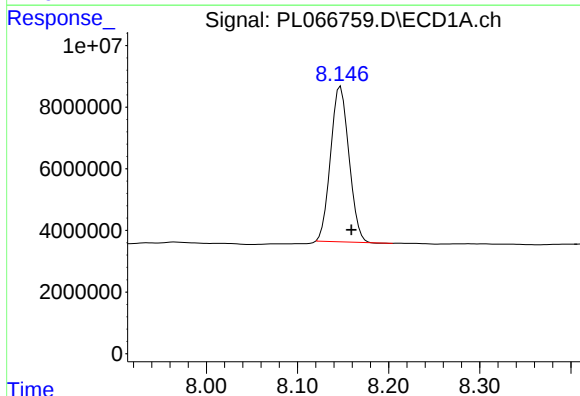

#28 Decachlorobiphenyl

R.T.: 8.147 min
Delta R.T.: -0.012 min
Response: 70559675
Conc: 18.40 ng/ml

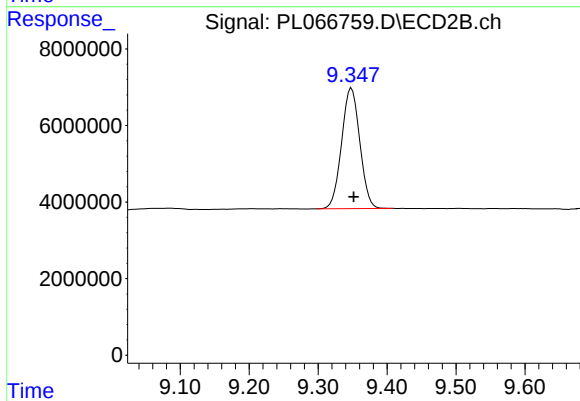

#28 Decachlorobiphenyl

R.T.: 9.349 min
Delta R.T.: -0.003 min
Response: 57783093
Conc: 18.68 ng/ml