

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050721\
 Data File : PL066767.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2021 14:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 13:55:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 28 08:49:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.425	4.151	78369726	80259428	20.798	22.853
28)	SA Decachlor...	8.145	9.345	79076362	64241646	20.624	20.766
Target Compounds							
2)	A alpha-BHC	3.881f	0.000	8315679	0	1.336	N.D. #
6)	B beta-BHC	4.398	5.041	1569632	17321866	0.593	4.669 #
15)	B Endosulfa...	0.000	7.123	0	4838922	N.D.	1.465 #
23)	Chlordane-1	4.311f	0.000	2139599	0	12.658	N.D. #
27)	Chlordane-5	0.000	7.207	0	1110891	N.D.	9.460 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050721\
Data File : PL066767.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2021 14:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 13:55:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042621.M
Quant Title : GC Extractables
QLast Update : Wed Apr 28 08:49:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

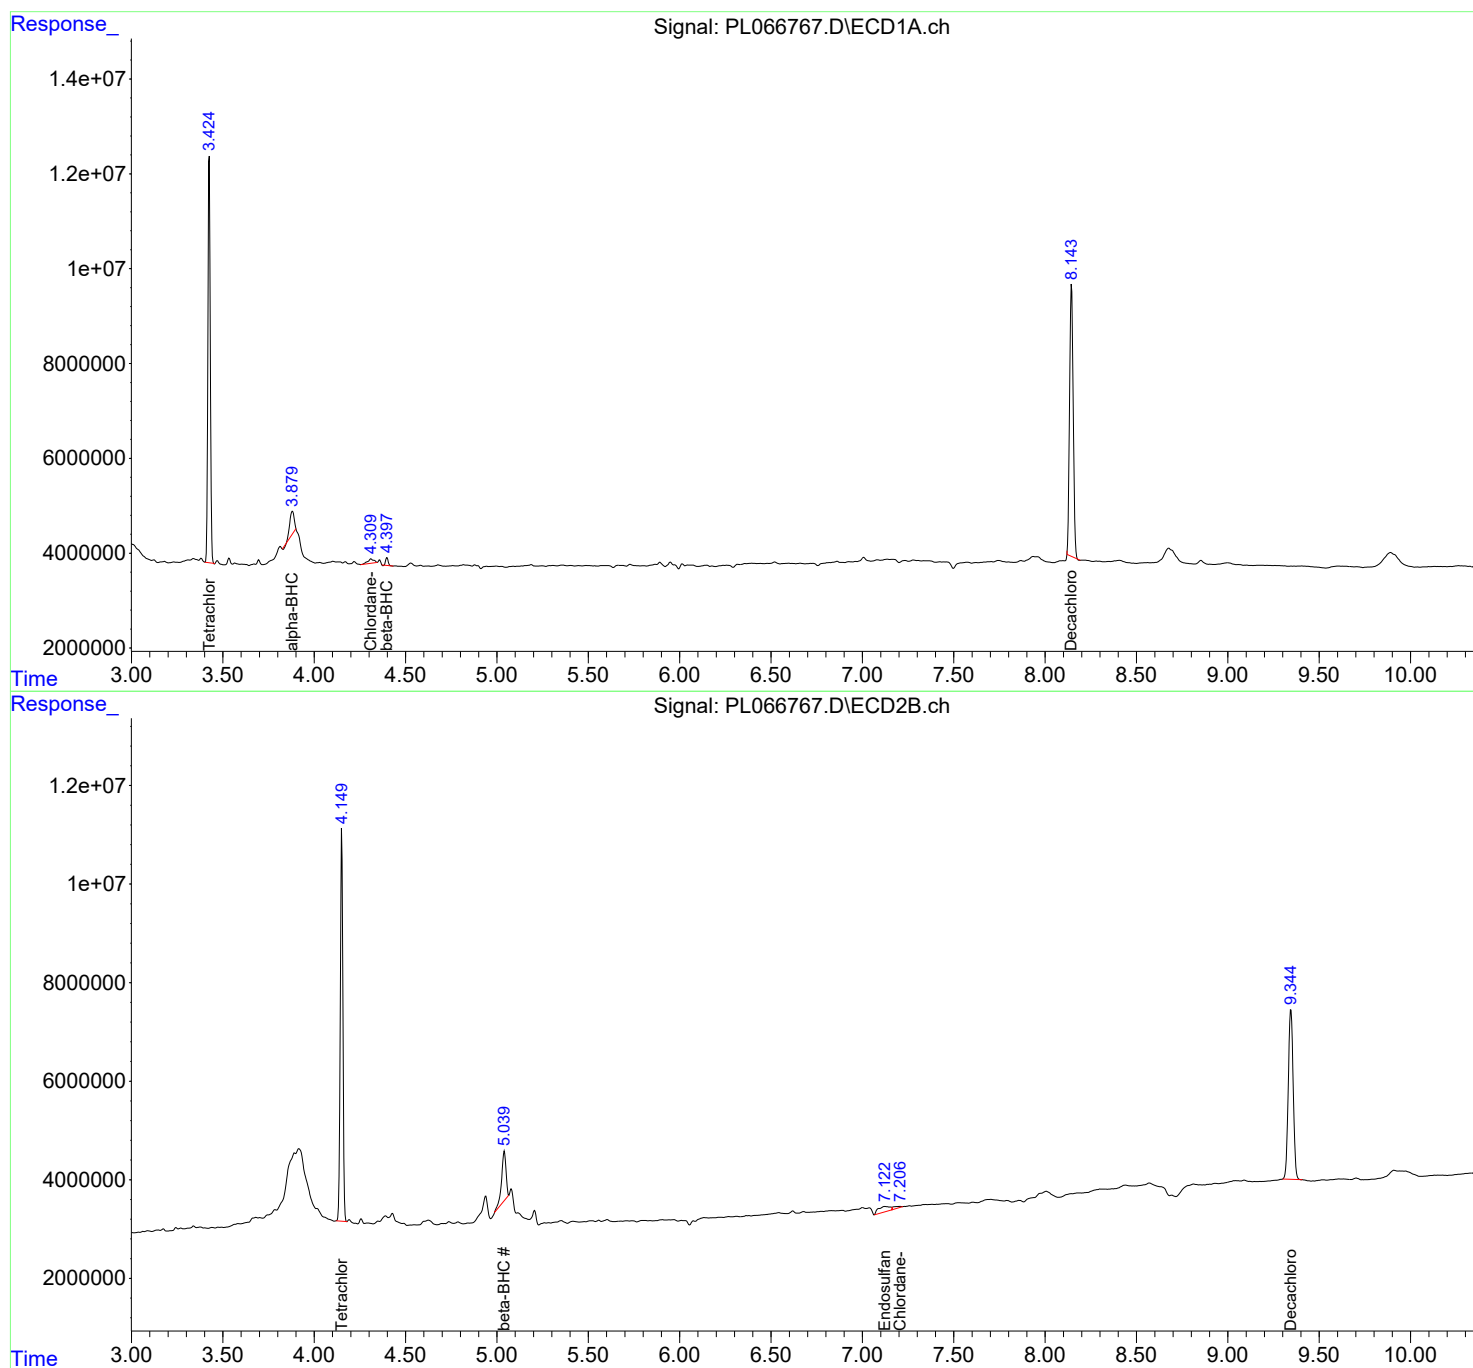


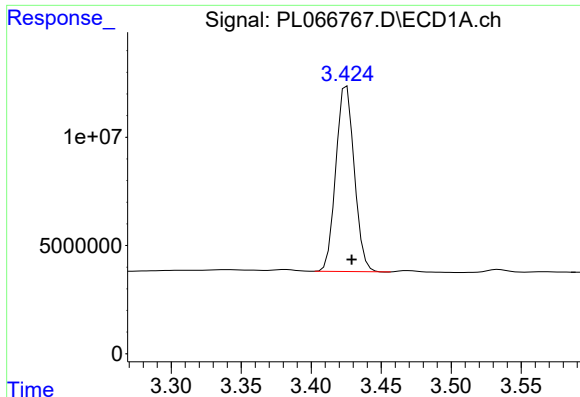

#1 Tetrachloro-m-xylene


R.T.: 3.425 min
Delta R.T.: -0.004 min
Response: 78369726
Conc: 20.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

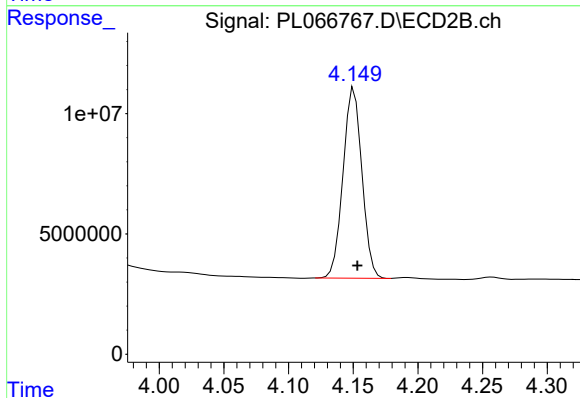


#1 Tetrachloro-m-xylene

R.T.: 4.151 min
Delta R.T.: -0.002 min
Response: 80259428
Conc: 22.85 ng/ml

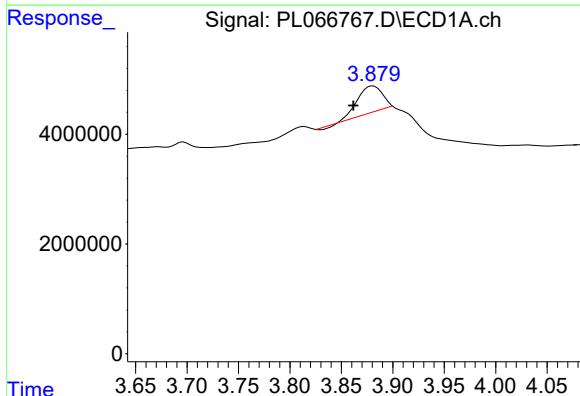


#2 alpha-BHC

R.T.: 3.881 min
Delta R.T.: 0.019 min
Response: 8315679
Conc: 1.34 ng/ml

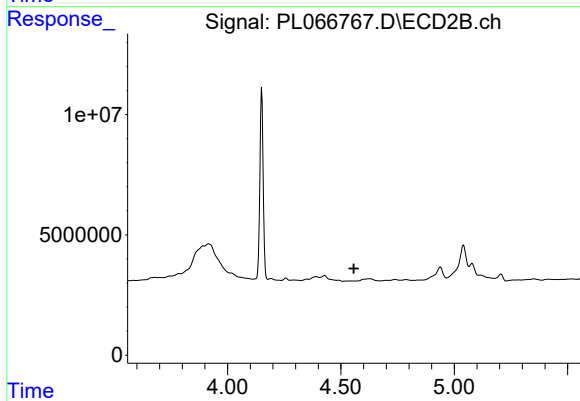

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.557 min
Response: 0
Conc: N.D.

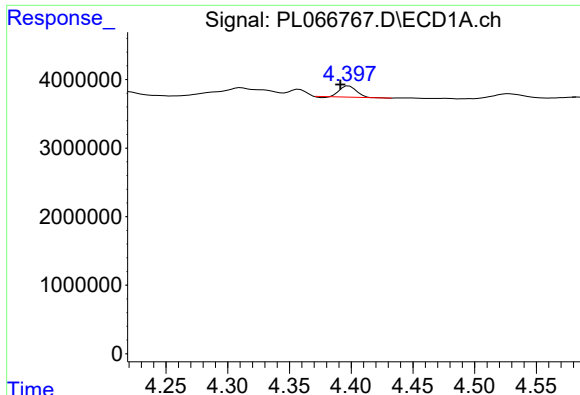

#6 beta-BHC


R.T.: 4.398 min
Delta R.T.: 0.007 min
Response: 1569632
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

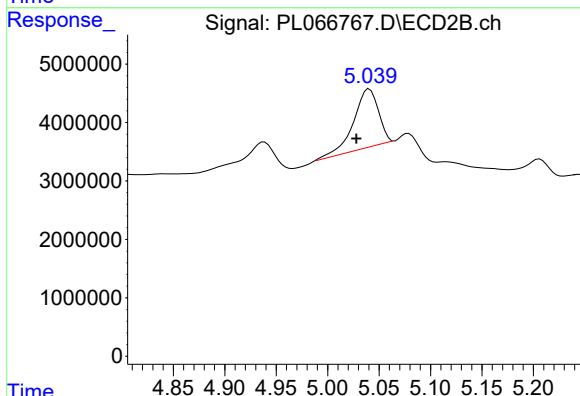


#6 beta-BHC

R.T.: 5.041 min
Delta R.T.: 0.013 min
Response: 17321866
Conc: 4.67 ng/ml

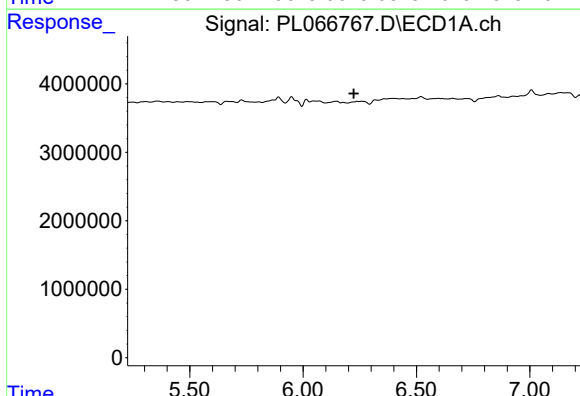


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.224 min
Response: 0
Conc: N.D.

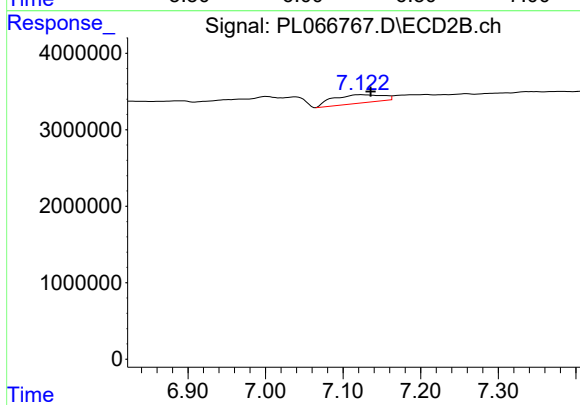

#15 Endosulfan II


R.T.: 7.123 min
Delta R.T.: -0.012 min
Response: 4838922
Conc: 1.47 ng/ml

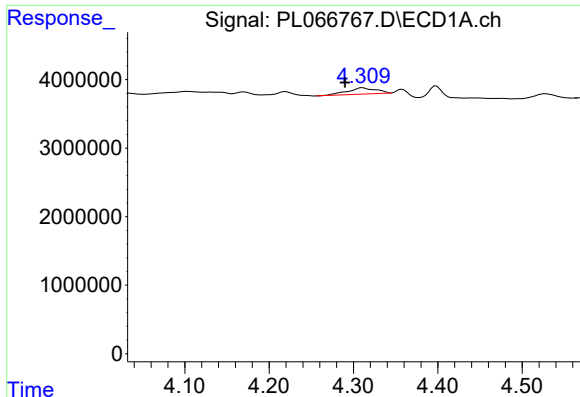

#23 Chlordane-1


R.T.: 4.311 min
Delta R.T.: 0.021 min
Response: 2139599
Conc: 12.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

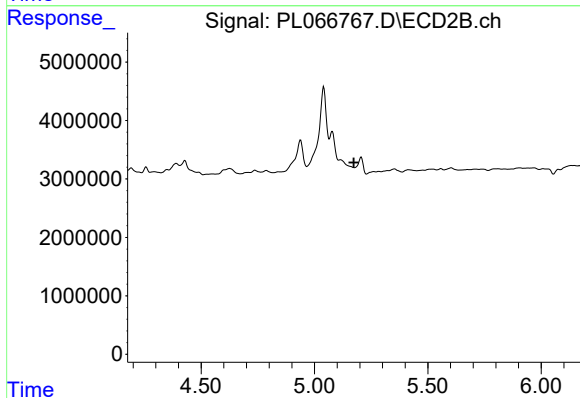


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

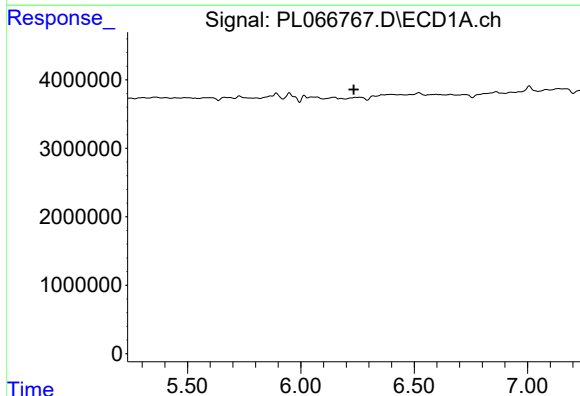


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

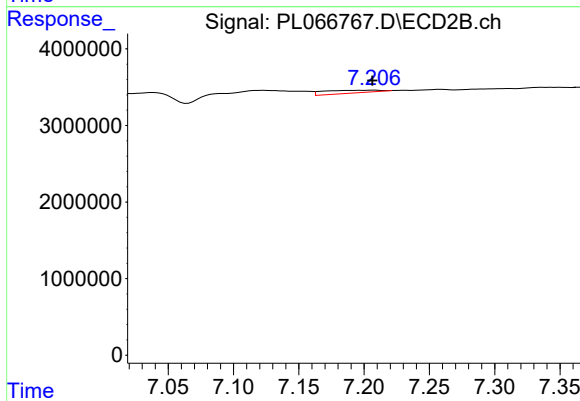

#27 Chlordane-5


R.T.: 7.207 min
Delta R.T.: 0.001 min
Response: 1110891
Conc: 9.46 ng/ml

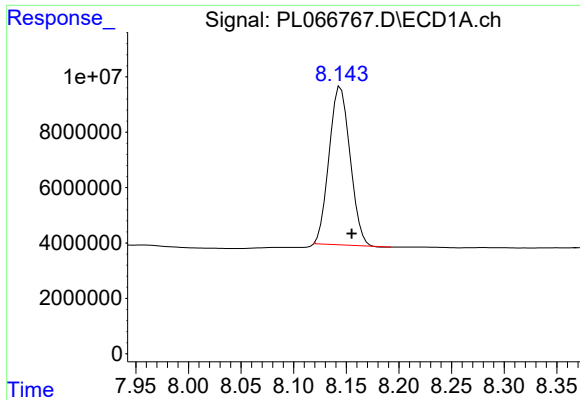

#28 Decachlorobiphenyl

R.T.: 8.145 min
Delta R.T.: -0.010 min
Response: 79076362
Conc: 20.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

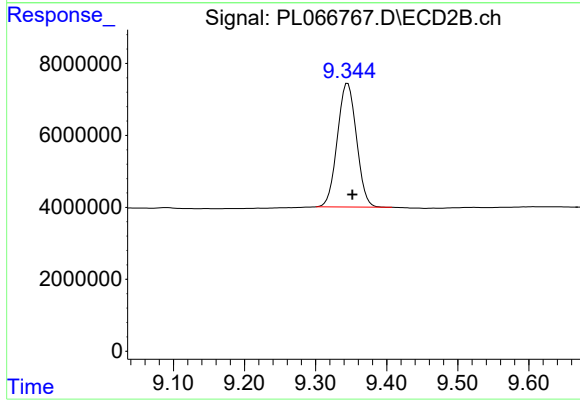

#28 Decachlorobiphenyl

R.T.: 9.345 min
Delta R.T.: -0.007 min
Response: 64241646
Conc: 20.77 ng/ml