

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050724\
 Data File : PL089390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 May 2024 13:15
 Operator : AR\AJ
 Sample : P2395-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-DRIVEWAY

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/08/2024
 Supervised By :Ankita Jodhani 05/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 07 22:11:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 26 19:27:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.558	2.797	47642381	30295631	23.659	23.612
28) SA Decachlor...	9.076	7.951	25946771	23906685	18.546	17.772
Target Compounds						
13) MA Dieldrin	6.361	5.397	729059	730879	0.326m	0.454 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050724\
Data File : PL089390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 May 2024 13:15
Operator : AR\AJ
Sample : P2395-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP-DRIVEWAY


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/08/2024
Supervised By : Ankita Jodhani 05/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 07 22:11:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042624.M
Quant Title : GC Extractables
QLast Update : Fri Apr 26 19:27:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

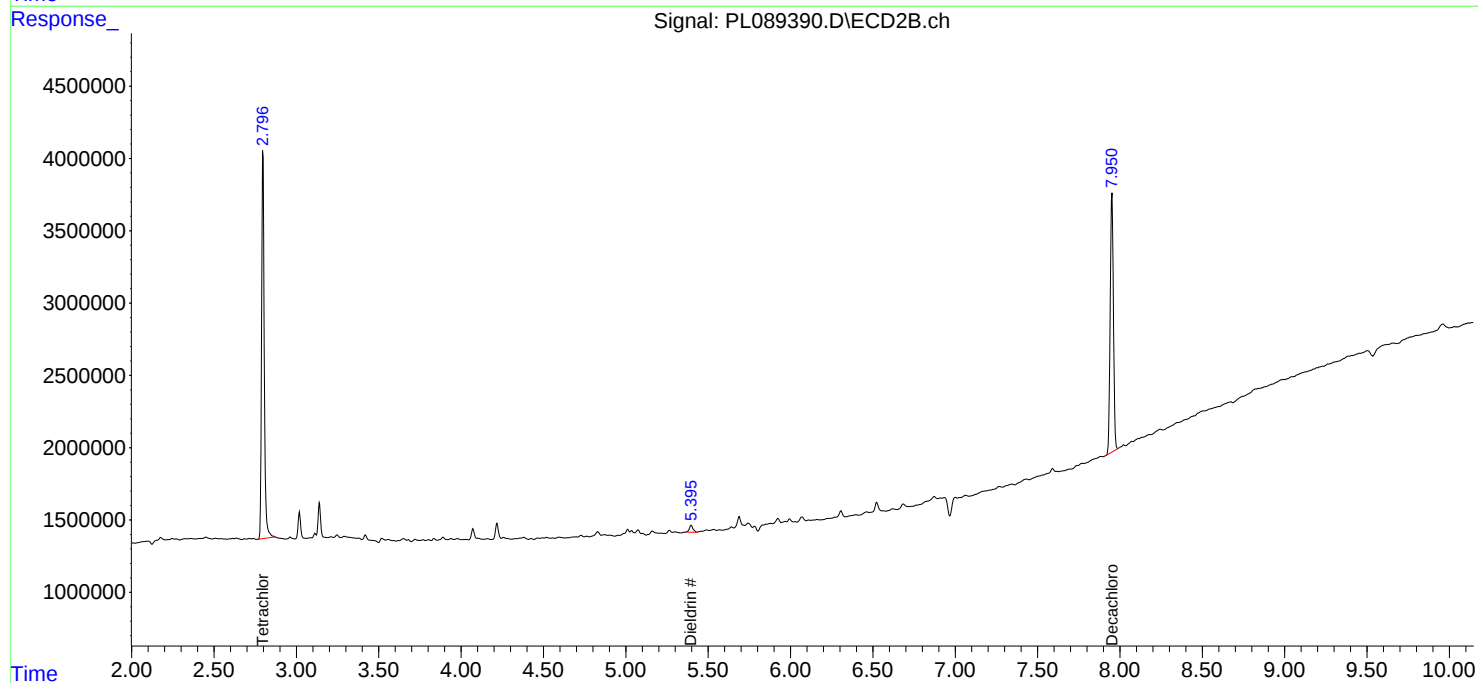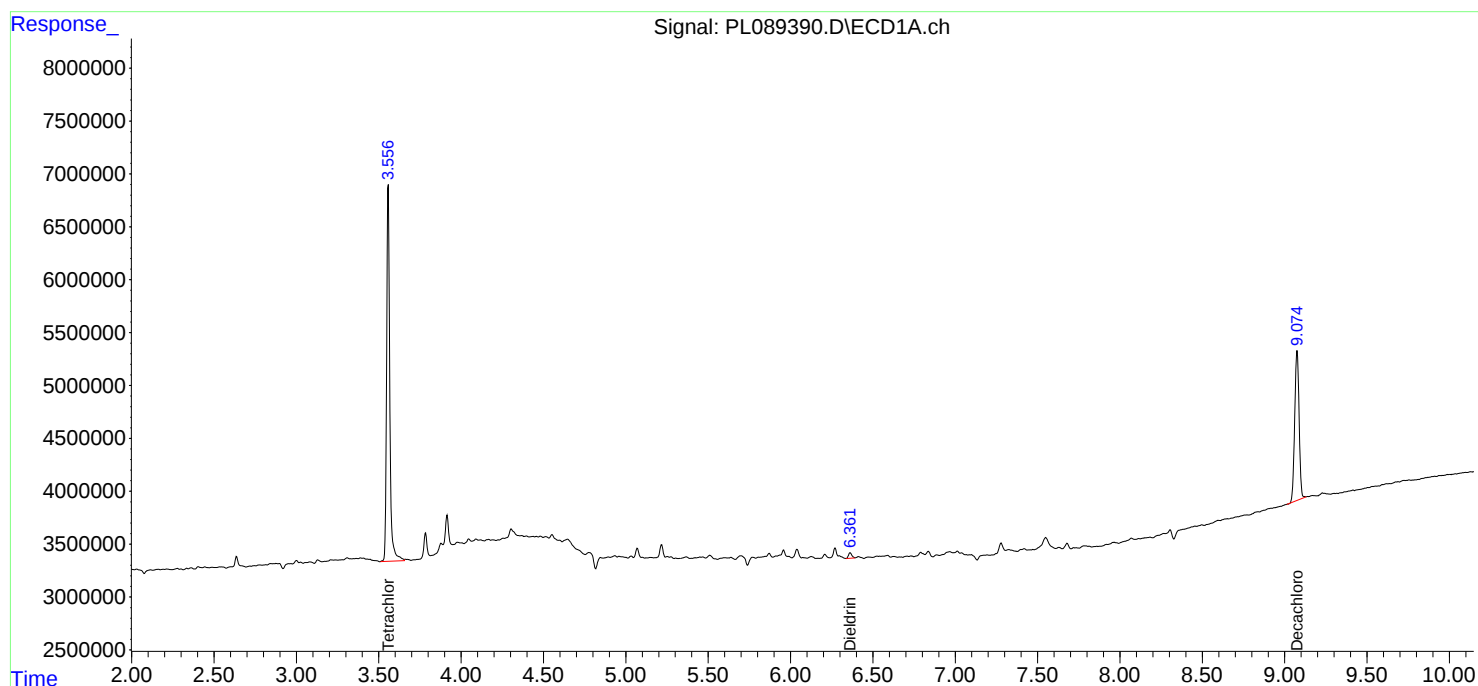

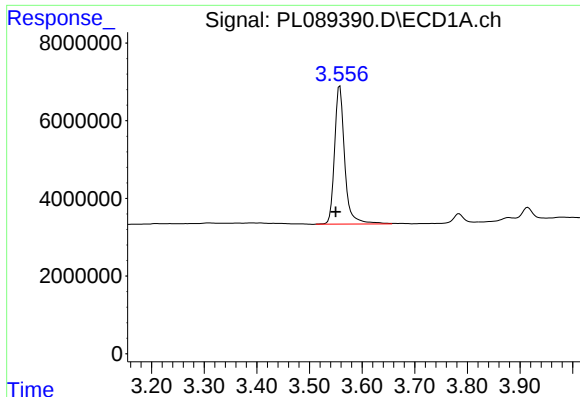


#1 Tetrachloro-m-xylene

R.T.: 3.558 min
Delta R.T.: 0.008 min
Response: 47642381
Conc: 23.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-DRIVEWAY


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/08/2024
Supervised By :Ankita Jodhani 05/08/2024

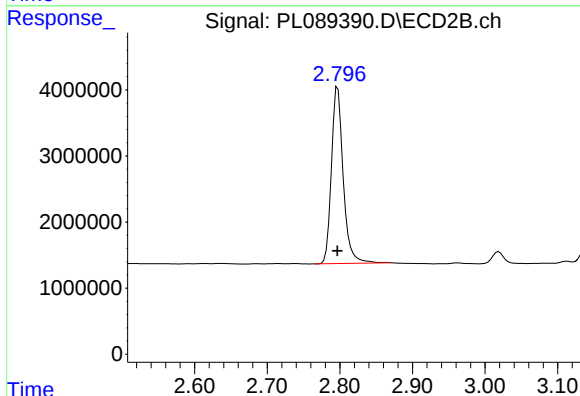


#1 Tetrachloro-m-xylene

R.T.: 2.797 min
Delta R.T.: 0.000 min
Response: 30295631
Conc: 23.61 ng/ml

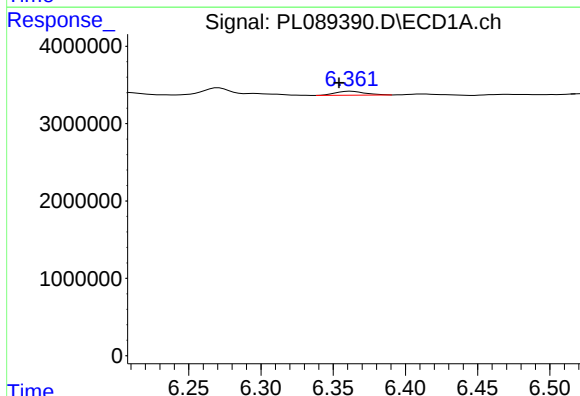


#13 Dieldrin

R.T.: 6.361 min
Delta R.T.: 0.007 min
Response: 729059
Conc: 0.33 ng/ml m

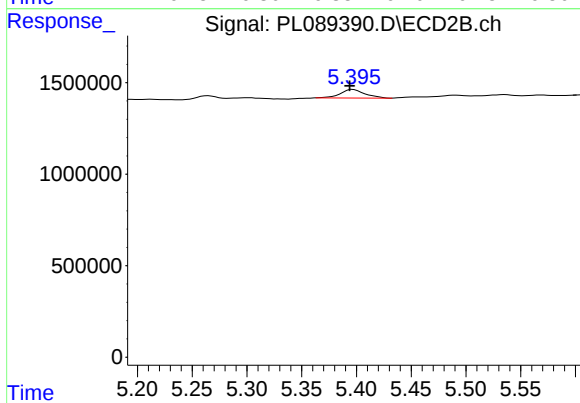

#13 Dieldrin

R.T.: 5.397 min
Delta R.T.: 0.003 min
Response: 730879
Conc: 0.45 ng/ml

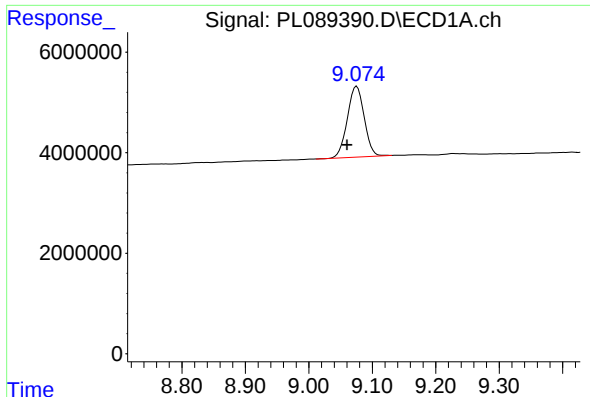


#28 Decachlorobiphenyl

R.T.: 9.076 min
Delta R.T.: 0.015 min
Response: 25946771
Conc: 18.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-DRIVEWAY

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/08/2024
Supervised By :Ankita Jodhani 05/08/2024

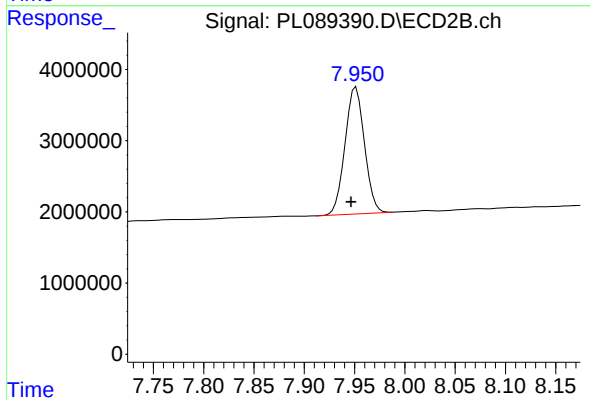

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.005 min
Response: 23906685
Conc: 17.77 ng/ml