

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050819\
 Data File : PL048256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2019 15:11
 Operator : AJ\SJ
 Sample : K2641-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-050719-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 00:59:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.939	93183836	26408122	9.620	10.602
28)	SA Decachlor...	7.994	8.974	102.7E6	28129010	10.215	10.598
Target Compounds							
4)	MA Heptachlor	4.292f	0.000	19281096	0	1.311	N.D. #
6)	B beta-BHC	4.292	0.000	19281096	0	3.267	N.D. #
10)	B gamma-Chl...	5.232f	0.000	19013728	0	1.424	N.D. #
13)	MA Dieldrin	5.558	0.000	19821589	0	1.522	N.D. #
17)	MA 4,4'-DDT	6.176	0.000	11296953	0	1.124	N.D. #
23)	Chlordane-1	4.171	0.000	9755319	0	21.731	N.D. #
25)	Chlordane-3	5.232f	0.000	19013728	0	12.076	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050819\
Data File : PL048256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2019 15:11
Operator : AJ\SJ
Sample : K2641-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
CL-02-050719-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 00:59:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

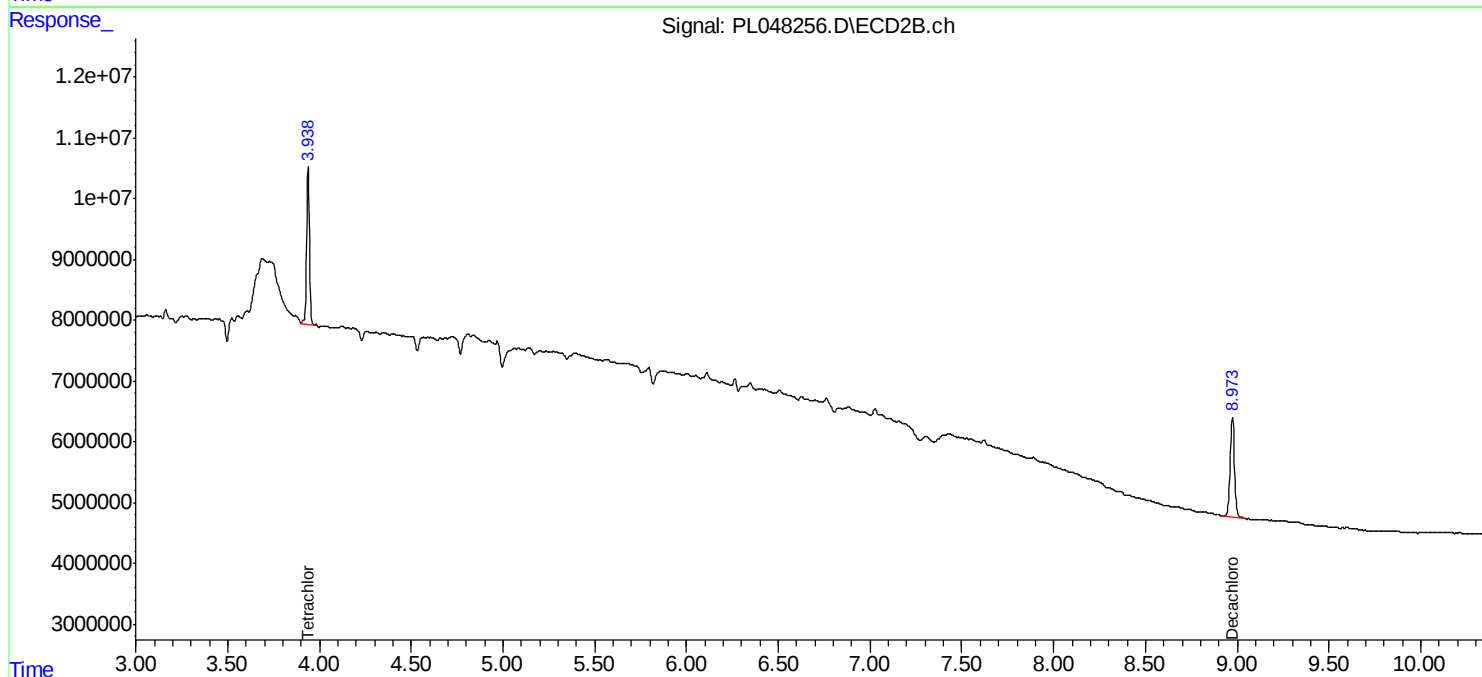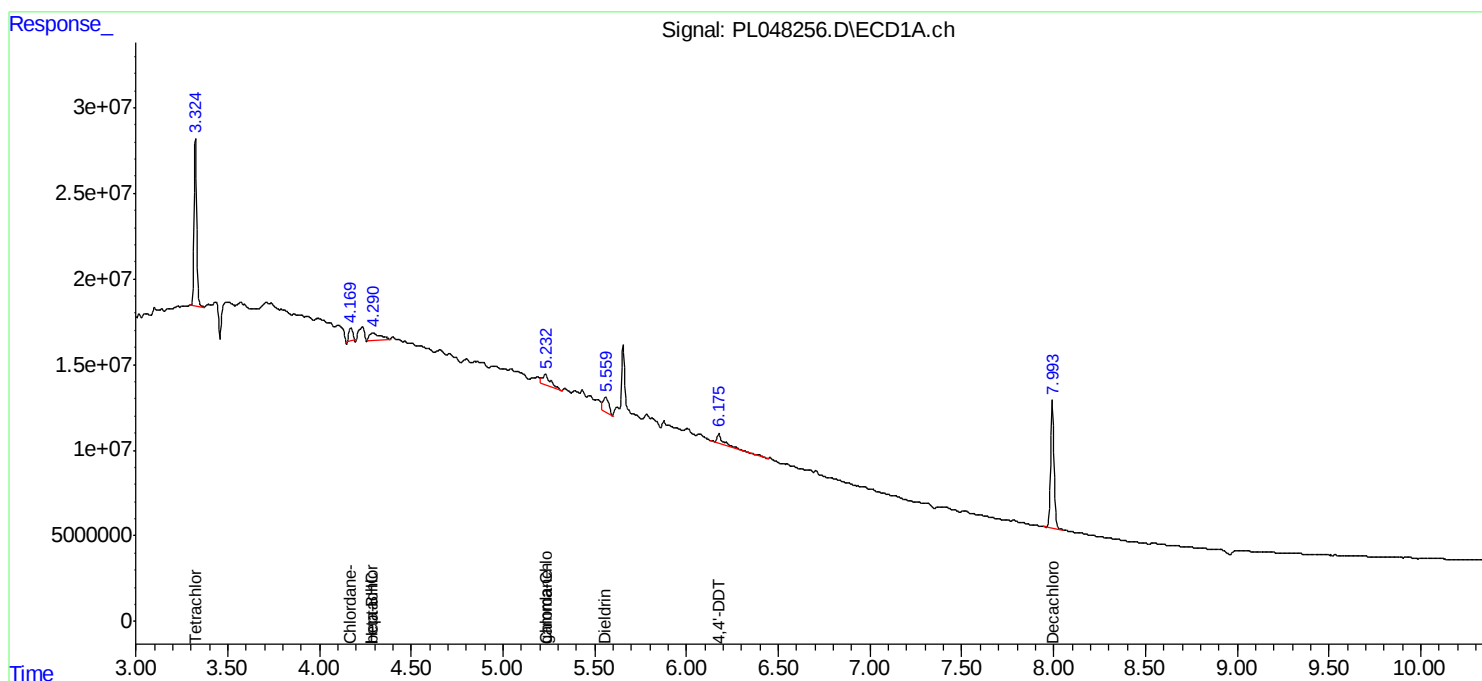


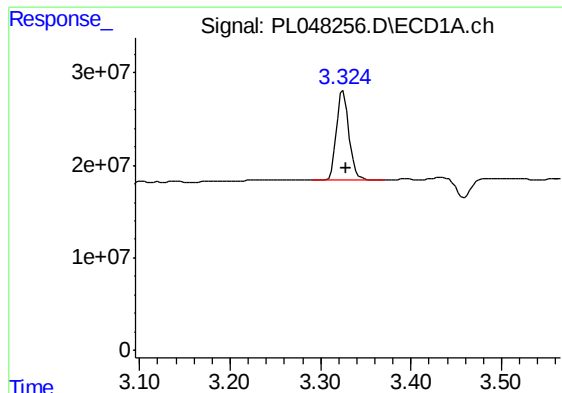

#1 Tetrachloro-m-xylene


R.T.: 3.325 min
Delta R.T.: -0.003 min
Response: 93183836
Conc: 9.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-B

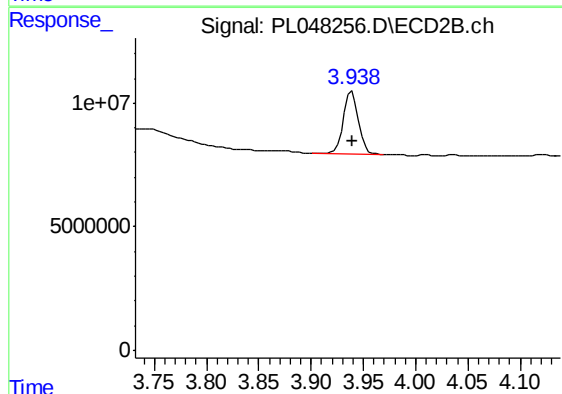


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 26408122
Conc: 10.60 ng/ml

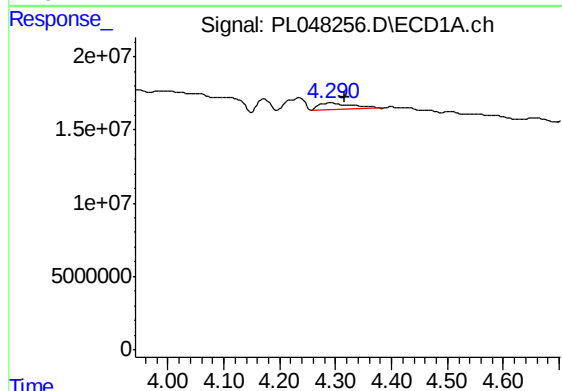


#4 Heptachlor

R.T.: 4.292 min
Delta R.T.: -0.025 min
Response: 19281096
Conc: 1.31 ng/ml

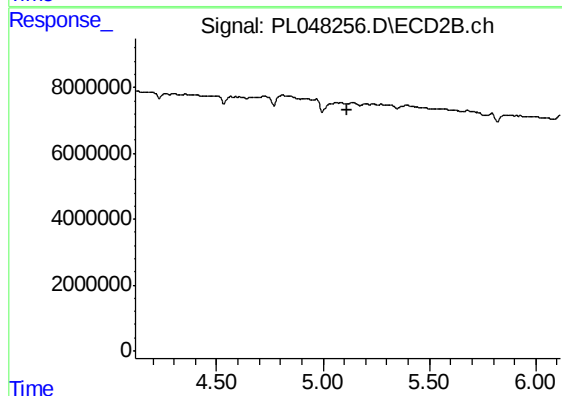

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.116 min
Response: 0
Conc: N.D.

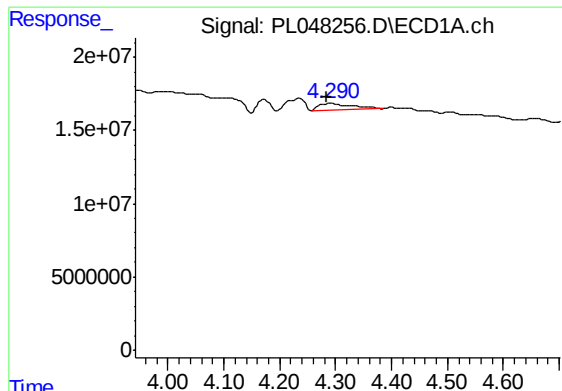

#6 beta-BHC


R.T.: 4.292 min
Delta R.T.: 0.007 min
Response: 19281096
Conc: 3.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-B

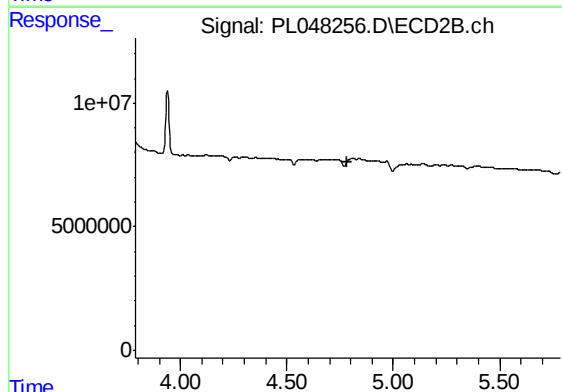


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.786 min
Response: 0
Conc: N.D.

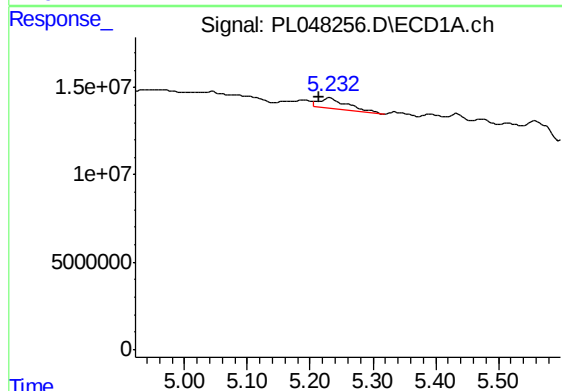


#10 gamma-Chlordane

R.T.: 5.232 min
Delta R.T.: 0.017 min
Response: 19013728
Conc: 1.42 ng/ml

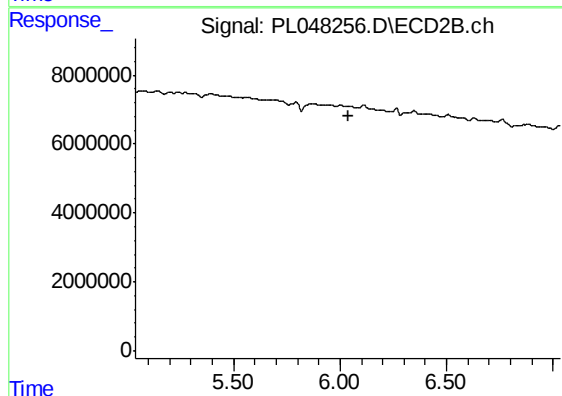

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

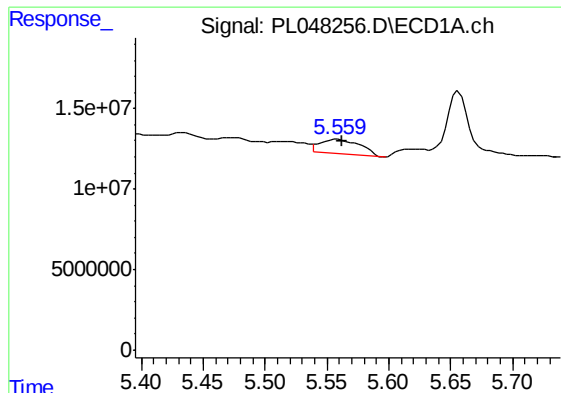

#13 Dielddrin


R.T.: 5.558 min
Delta R.T.: -0.004 min
Response: 19821589
Conc: 1.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-B

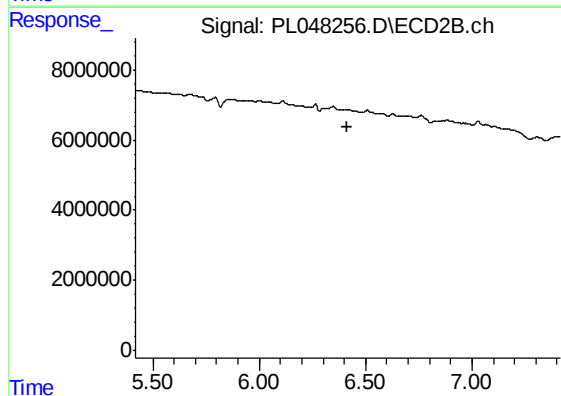


#13 Dielddrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

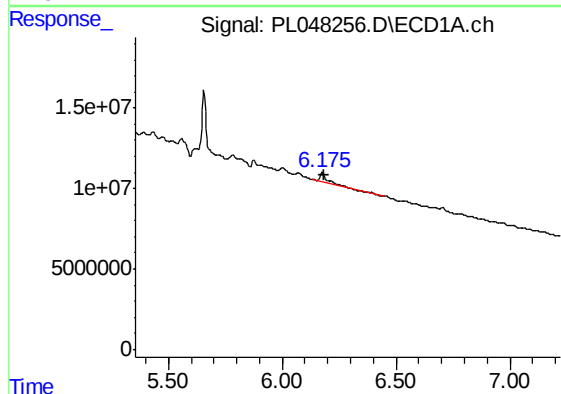


#17 4,4'-DDT

R.T.: 6.176 min
Delta R.T.: -0.008 min
Response: 11296953
Conc: 1.12 ng/ml

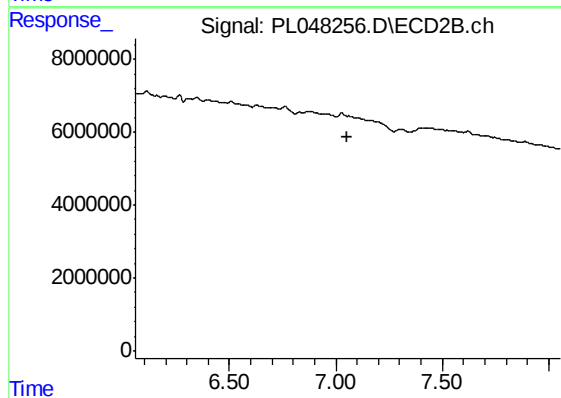

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

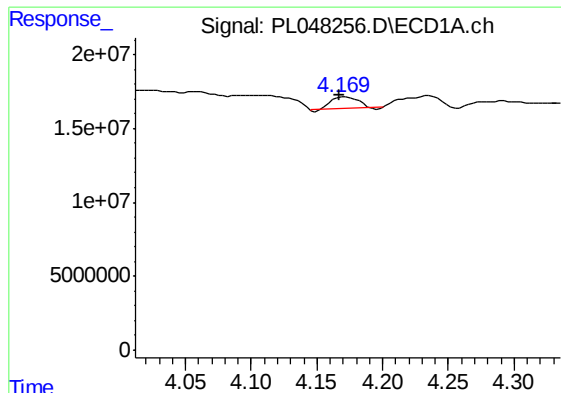

#23 Chlordane-1


R.T.: 4.171 min
Delta R.T.: 0.003 min
Response: 9755319
Conc: 21.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-B

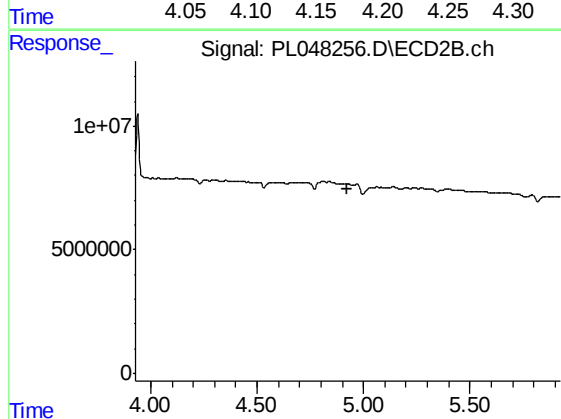


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

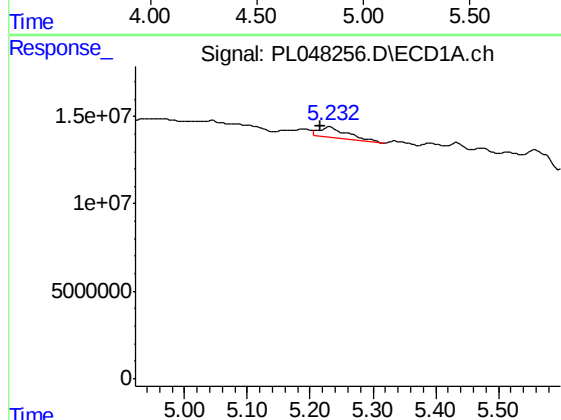


#25 Chlordane-3

R.T.: 5.232 min
Delta R.T.: 0.017 min
Response: 19013728
Conc: 12.08 ng/ml

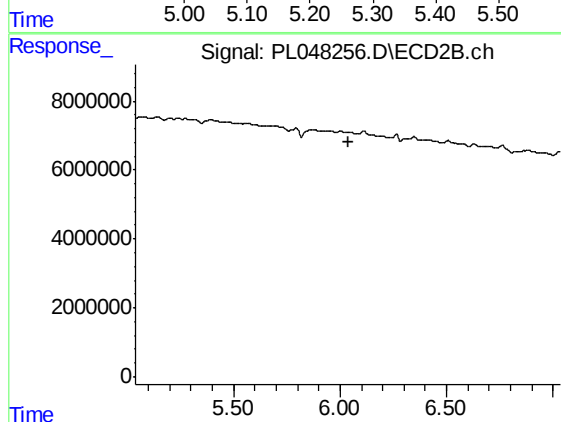

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

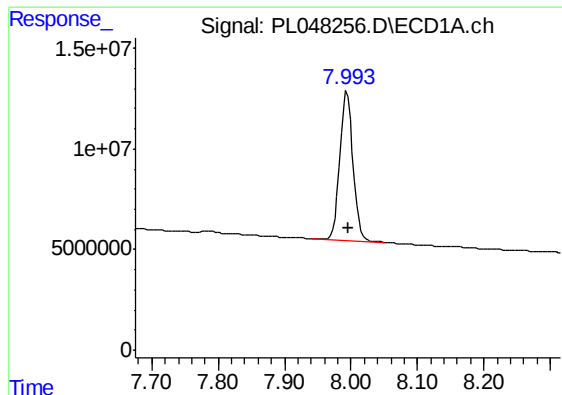

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: -0.002 min
Response: 102700437
Conc: 10.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-B

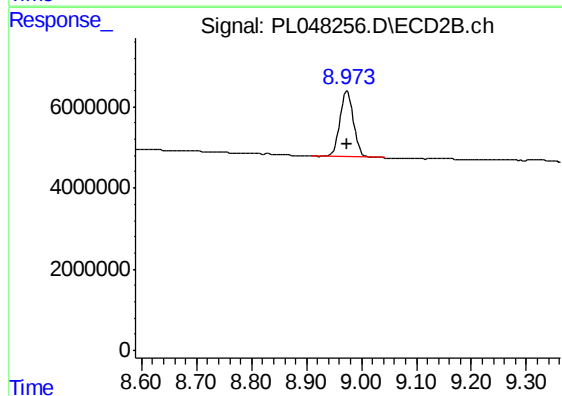

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: 0.000 min
Response: 28129010
Conc: 10.60 ng/ml