

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050819\
 Data File : PL048268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2019 18:12
 Operator : AJ\SJ
 Sample : K2728-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P-3A-OW(0-10)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 01:03:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.940	73920461	20350115	7.631	8.170
28)	SA Decachlor...	7.996	8.976	74995011	24920006	7.459	9.389 #
Target Compounds							
10)	B gamma-Chl...	5.218	6.013f	23041829	651884	1.726	0.212 #
12)	B 4,4'-DDE	5.438	6.270	641.5E6	156.1E6	50.572	56.551
17)	MA 4,4'-DDT	6.178	0.000	4554661	0	0.453	N.D. #
19)	B Endosulfa...	6.459	0.000	7743978	0	0.722	N.D. #
20)	A Methoxychlor	6.707f	0.000	9741851	0	1.789	N.D. #
23)	Chlordane-1	4.172	0.000	1575611	0	3.510	N.D. #
25)	Chlordane-3	5.218	6.013f	23041829	651884	14.634	1.488 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050819\
Data File : PL048268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2019 18:12
Operator : AJ\SJ
Sample : K2728-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
P-3A-OW(0-10)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 01:03:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

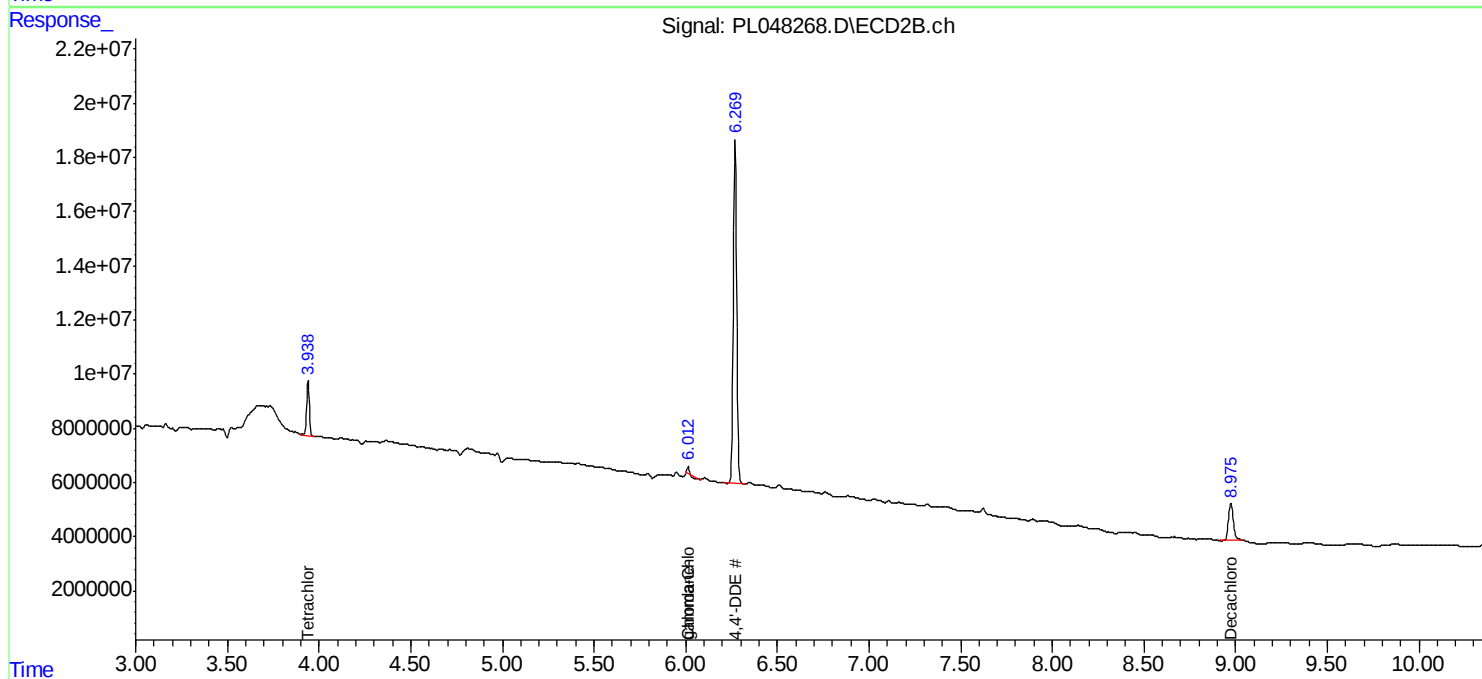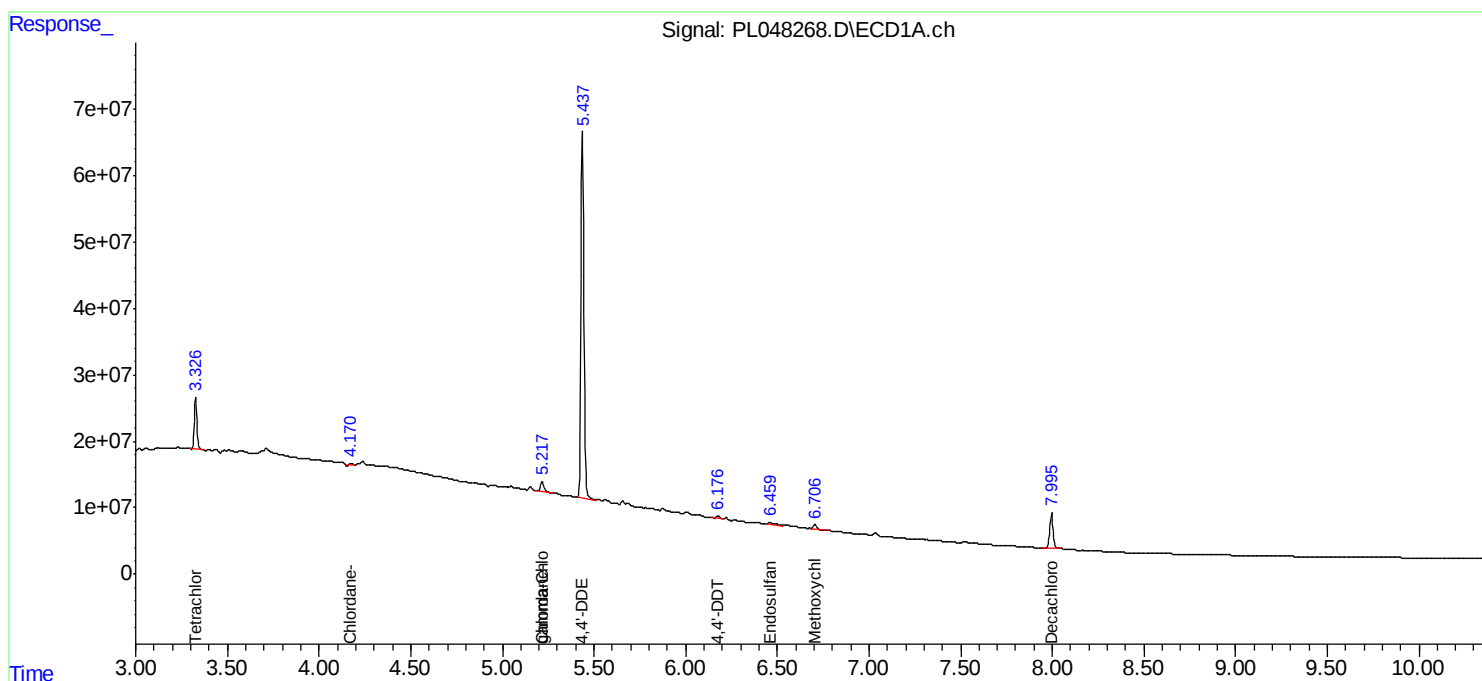


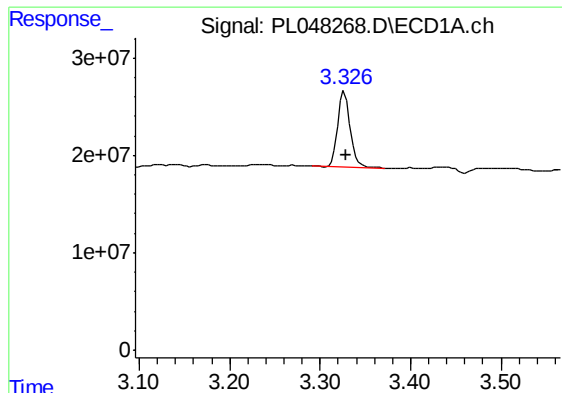

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 73920461
Conc: 7.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-3A-OW(0-10)

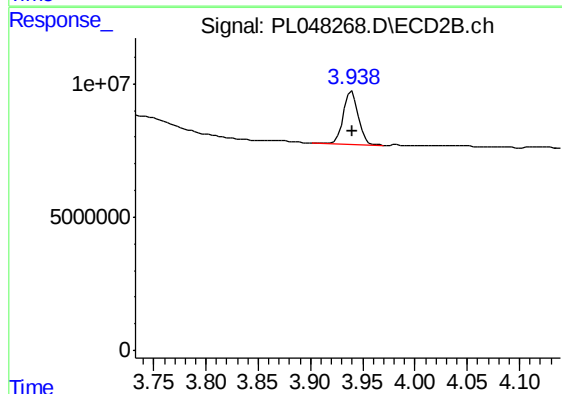


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 20350115
Conc: 8.17 ng/ml

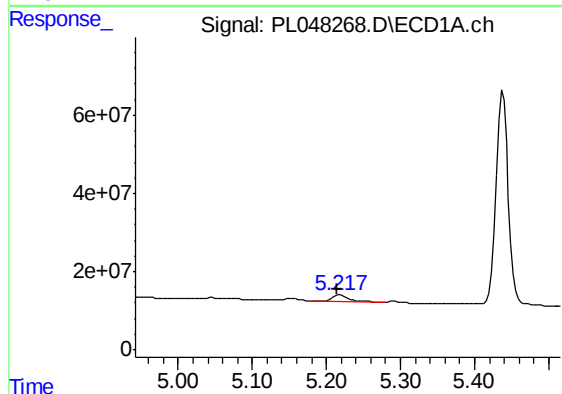


#10 gamma-Chlordane

R.T.: 5.218 min
Delta R.T.: 0.003 min
Response: 23041829
Conc: 1.73 ng/ml

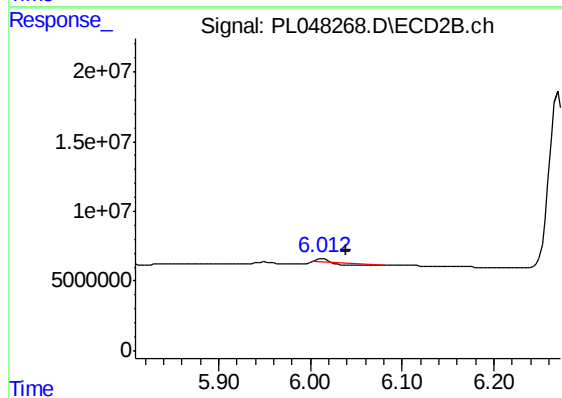

#10 gamma-Chlordane


R.T.: 6.013 min
Delta R.T.: -0.025 min
Response: 651884
Conc: 0.21 ng/ml

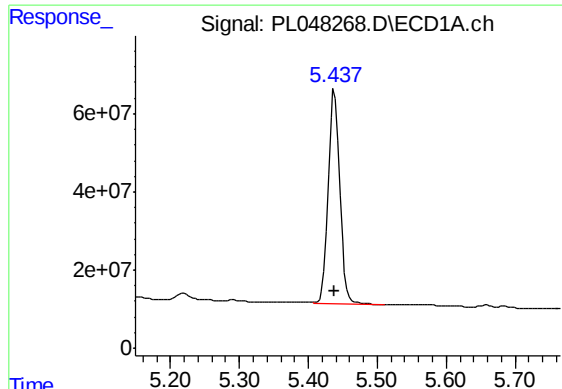

#12 4,4'-DDE


R.T.: 5.438 min
Delta R.T.: 0.000 min
Response: 641520978
Conc: 50.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-3A-OW(0-10)

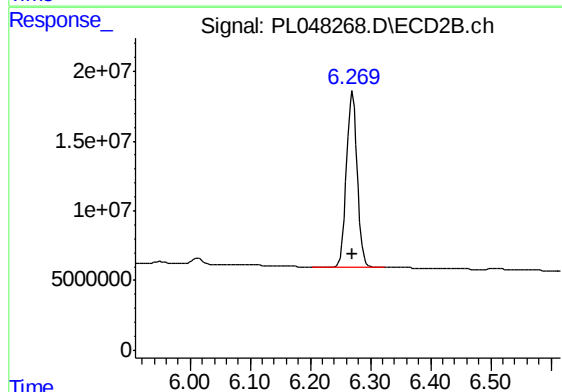


#12 4,4'-DDE

R.T.: 6.270 min
Delta R.T.: 0.000 min
Response: 156132644
Conc: 56.55 ng/ml

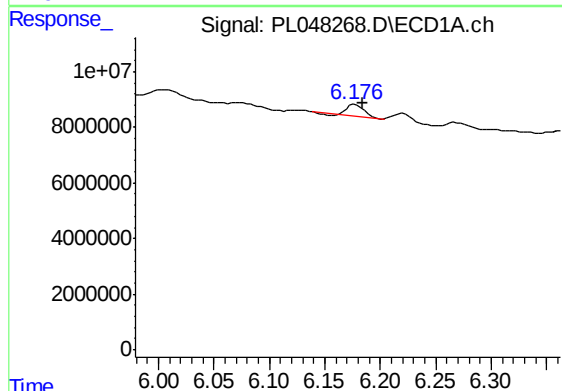


#17 4,4'-DDT

R.T.: 6.178 min
Delta R.T.: -0.006 min
Response: 4554661
Conc: 0.45 ng/ml

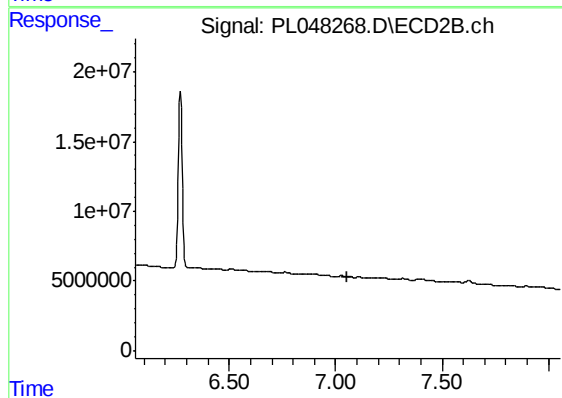

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

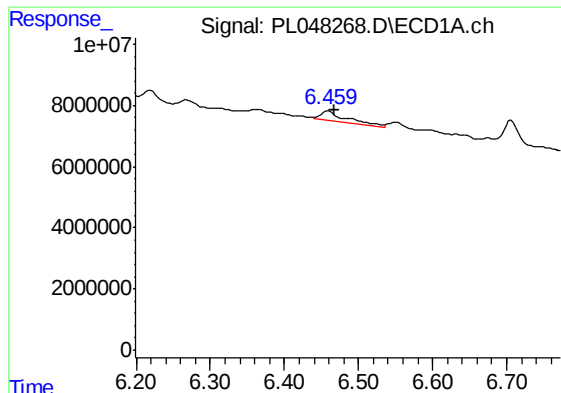

#19 Endosulfan Sulfate


R.T.: 6.459 min
Delta R.T.: -0.008 min
Response: 7743978
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-3A-OW(0-10)

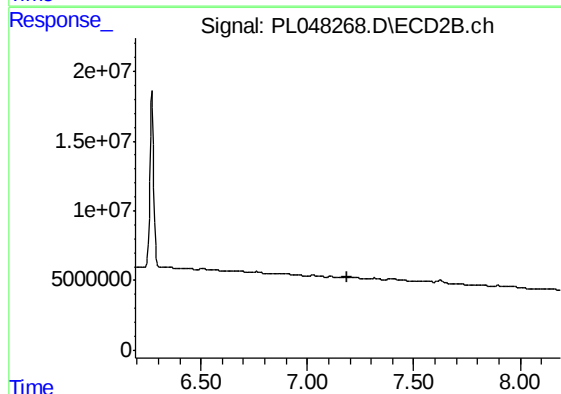


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.190 min
Response: 0
Conc: N.D.

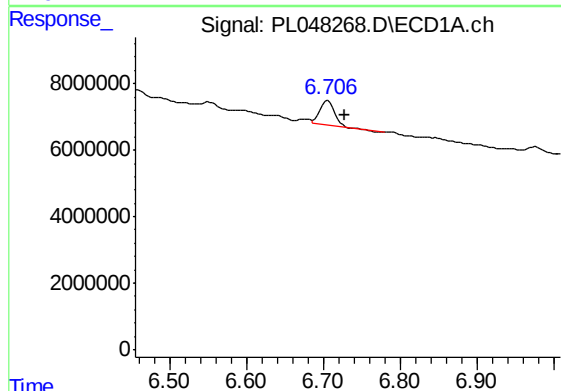


#20 Methoxychlor

R.T.: 6.707 min
Delta R.T.: -0.022 min
Response: 9741851
Conc: 1.79 ng/ml

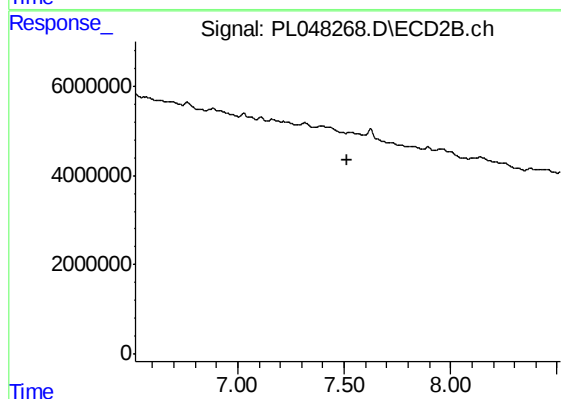

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.

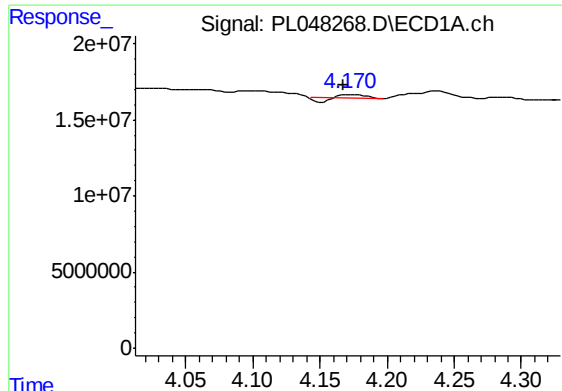

#23 Chlordane-1


R.T.: 4.172 min
Delta R.T.: 0.004 min
Response: 1575611
Conc: 3.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-3A-OW(0-10)

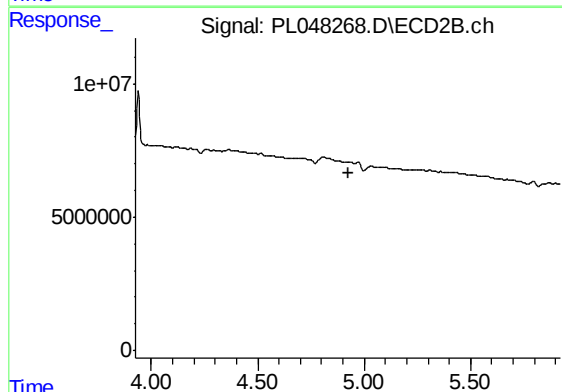


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

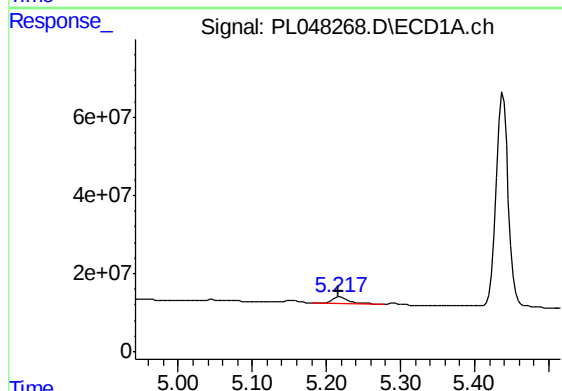


#25 Chlordane-3

R.T.: 5.218 min
Delta R.T.: 0.003 min
Response: 23041829
Conc: 14.63 ng/ml

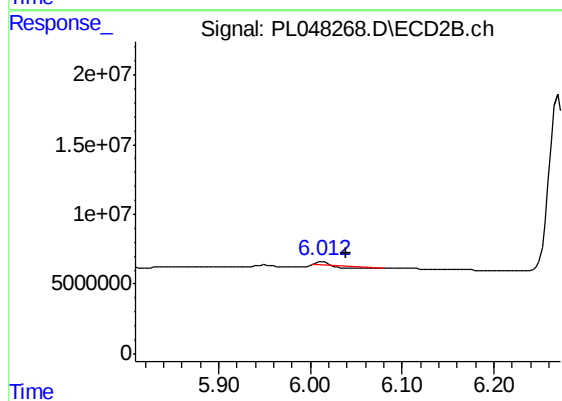

#25 Chlordane-3


R.T.: 6.013 min
Delta R.T.: -0.025 min
Response: 651884
Conc: 1.49 ng/ml

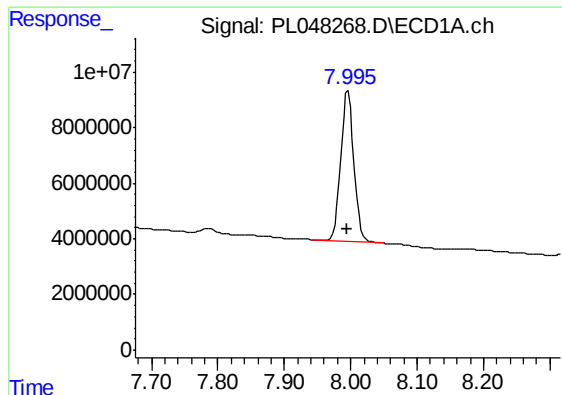

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 74995011
Conc: 7.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
P-3A-OW(0-10)

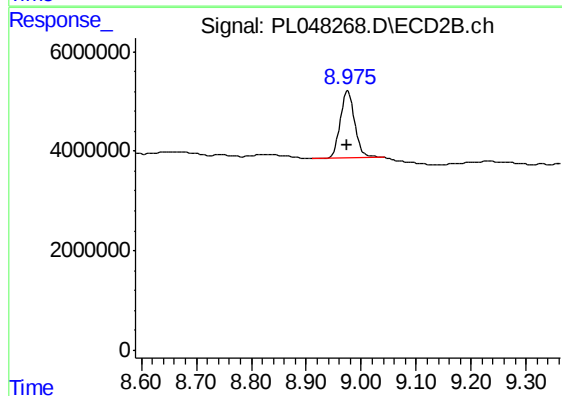

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.001 min
Response: 24920006
Conc: 9.39 ng/ml