

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050819\
 Data File : PL048276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2019 20:12
 Operator : AJ\SJ
 Sample : K2641-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-050719-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 01:05:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	156.1E6	42479776	16.117	17.054
28)	SA Decachlor...	7.995	8.976	139.1E6	39368696	13.838	14.832
Target Compounds							
2)	A alpha-BHC	3.727f	0.000	523122	0	0.034	N.D. #
3)	MA gamma-BHC...	4.053f	0.000	20437487	0	1.438	N.D. #
4)	MA Heptachlor	0.000	5.097f	0	16311333	N.D.	4.712 #
5)	MB Aldrin	4.556	0.000	6655745	0	0.486	N.D. #
7)	B delta-BHC	4.475	4.975f	-1360874	21903844	N.D.	7.746
10)	B gamma-Chl...	5.199f	0.000	30826688	0	2.309	N.D. #
23)	Chlordane-1	4.164	0.000	4717840	0	10.510	N.D. #
25)	Chlordane-3	5.199f	0.000	30826688	0	19.578	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050819\
Data File : PL048276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2019 20:12
Operator : AJ\SJ
Sample : K2641-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 01:05:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

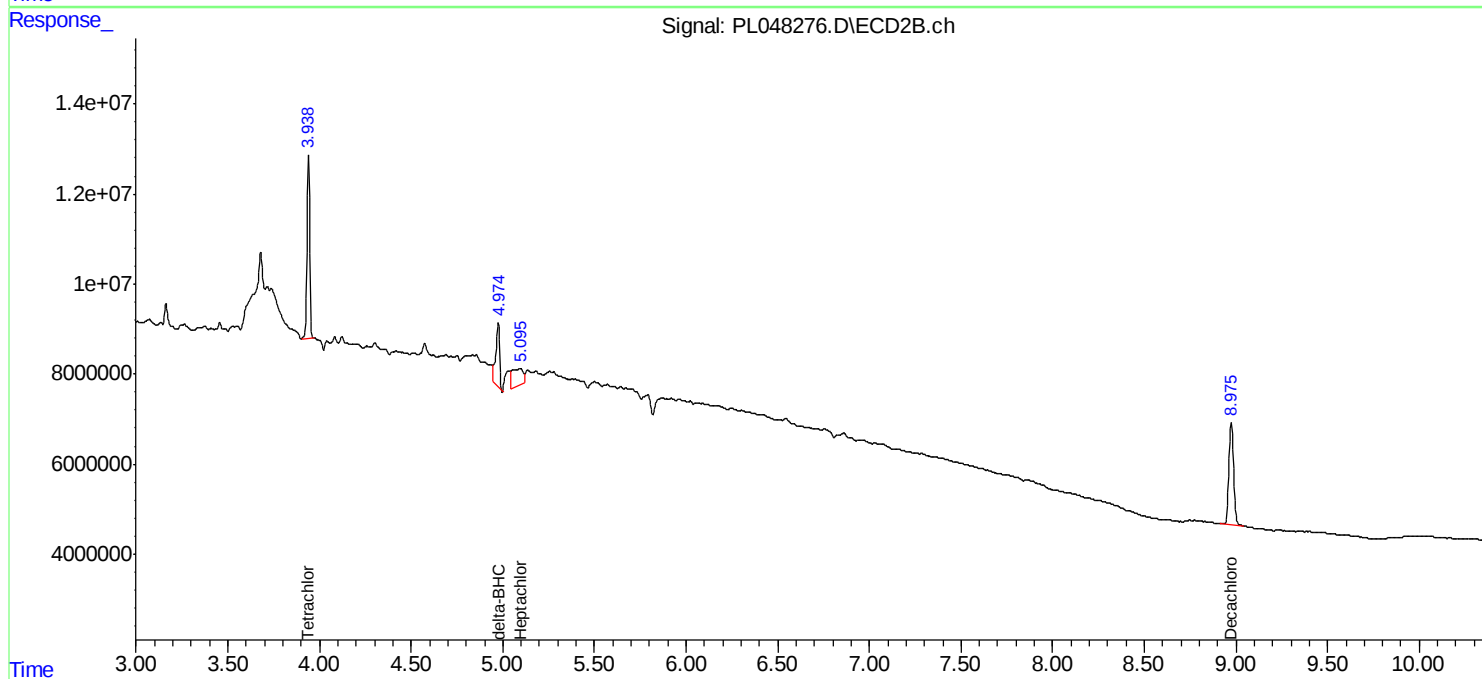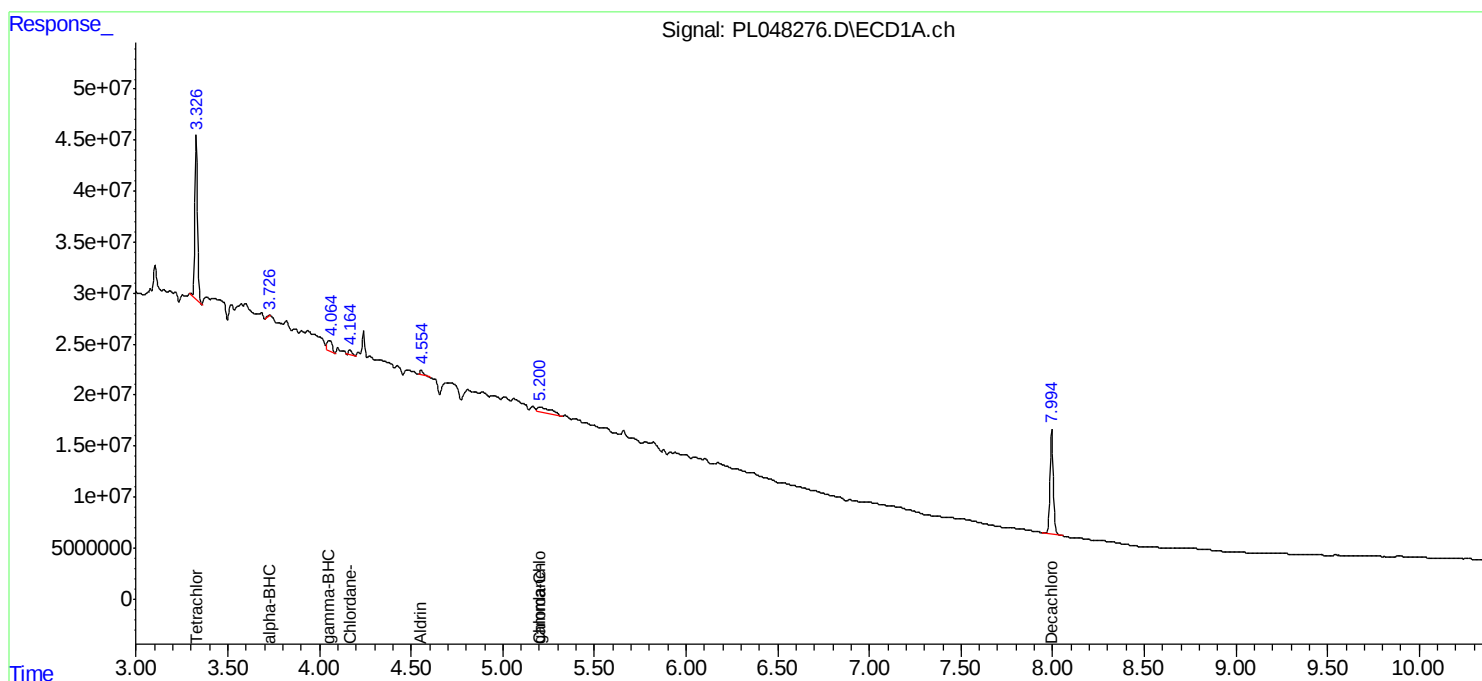


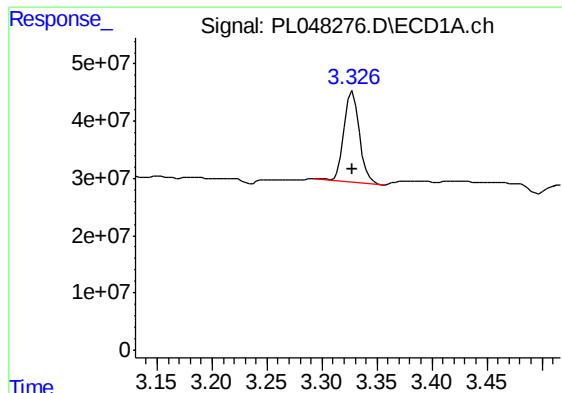

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 156121411
Conc: 16.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-C

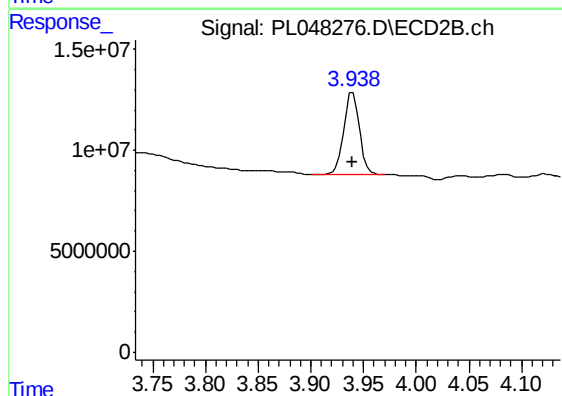


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 42479776
Conc: 17.05 ng/ml

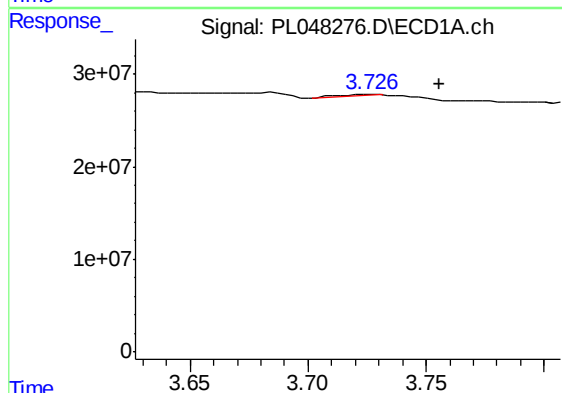


#2 alpha-BHC

R.T.: 3.727 min
Delta R.T.: -0.029 min
Response: 523122
Conc: 0.03 ng/ml

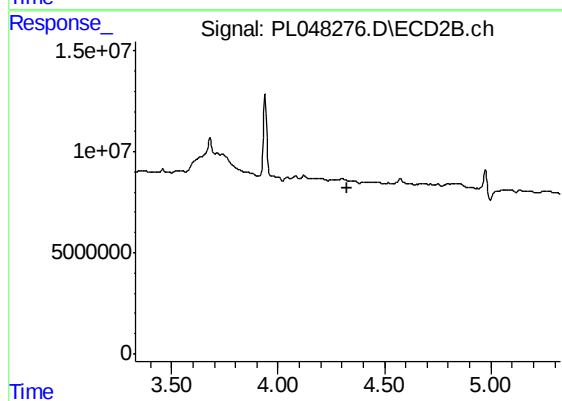

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.328 min
Response: 0
Conc: N.D.

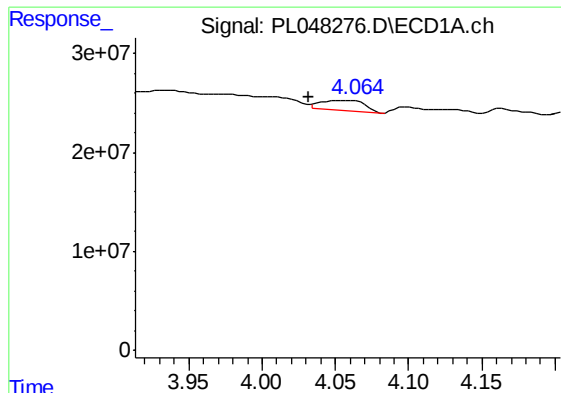

#3 gamma-BHC (Lindane)


R.T.: 4.053 min
Delta R.T.: 0.021 min
Response: 20437487
Conc: 1.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-C

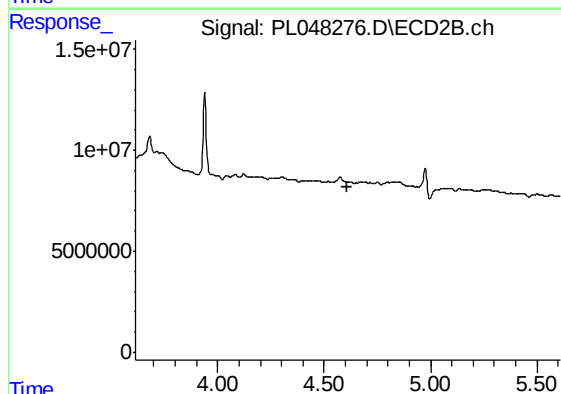


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

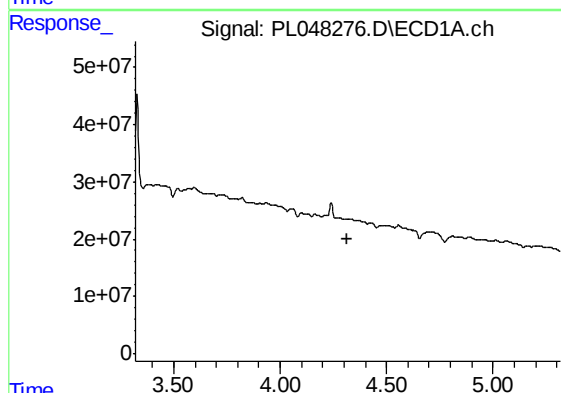


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

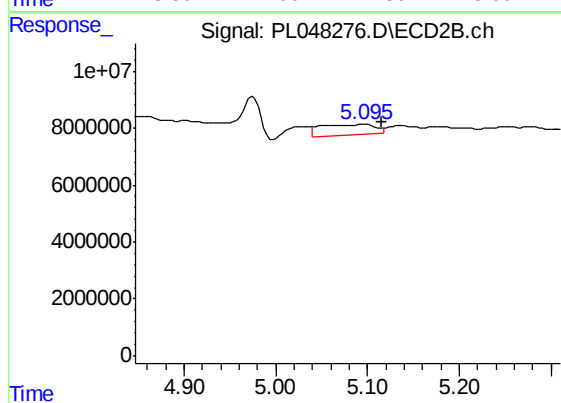

#4 Heptachlor


R.T.: 5.097 min
Delta R.T.: -0.019 min
Response: 16311333
Conc: 4.71 ng/ml

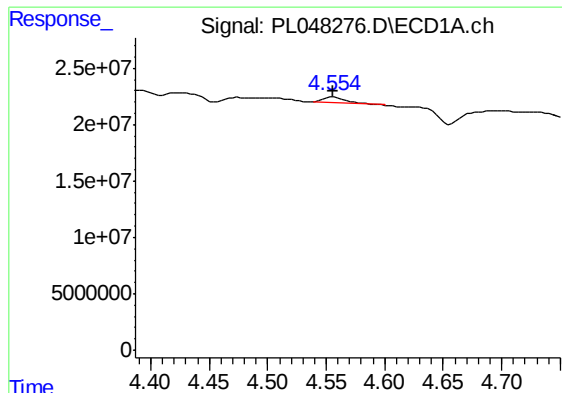

#5 Aldrin


R.T.: 4.556 min
Delta R.T.: 0.000 min
Response: 6655745
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-C

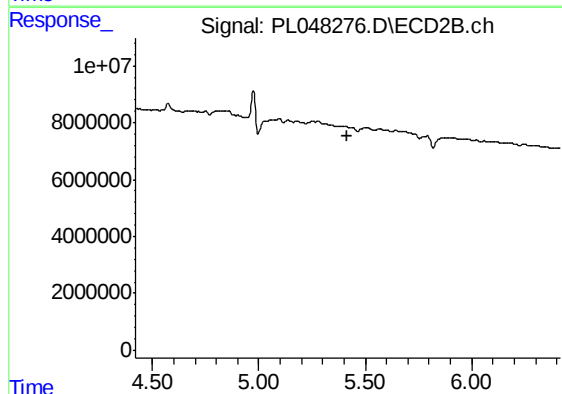


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.418 min
Response: 0
Conc: N.D.

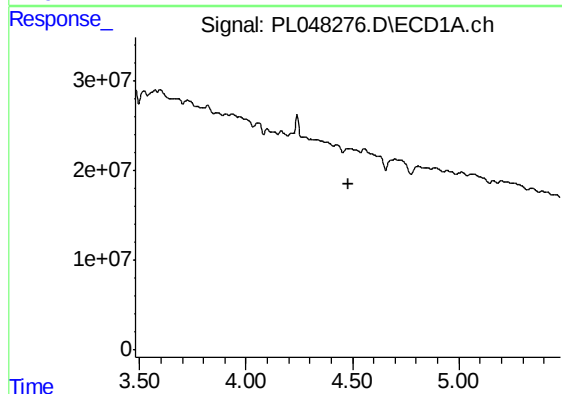


#7 delta-BHC

R.T.: 4.475 min
Delta R.T.: -0.004 min
Response: -1360874
Conc: N.D.

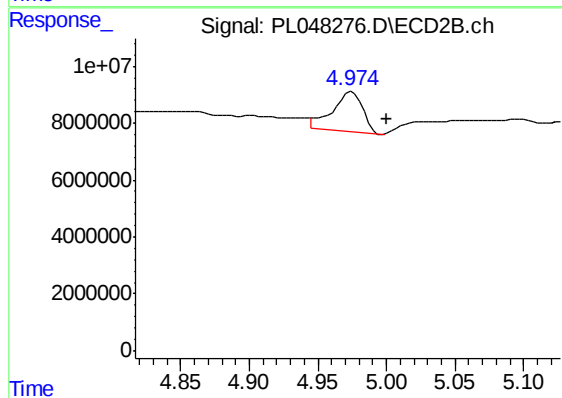

#7 delta-BHC


R.T.: 4.975 min
Delta R.T.: -0.025 min
Response: 21903844
Conc: 7.75 ng/ml

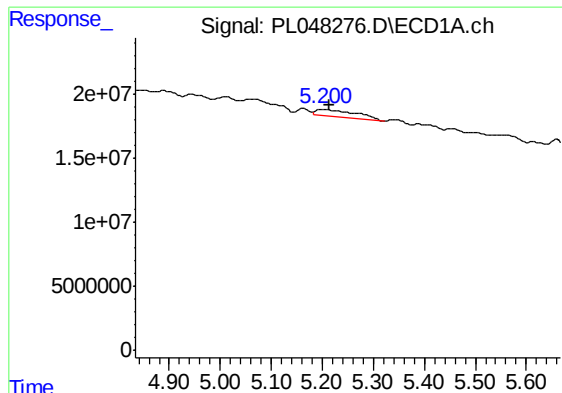

#10 gamma-Chlordane


R.T.: 5.199 min
Delta R.T.: -0.016 min
Response: 30826688
Conc: 2.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-C

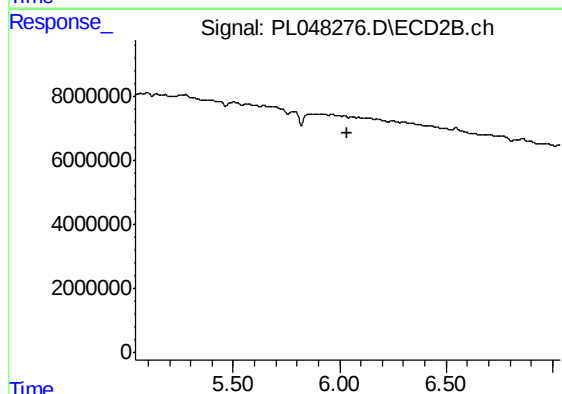


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

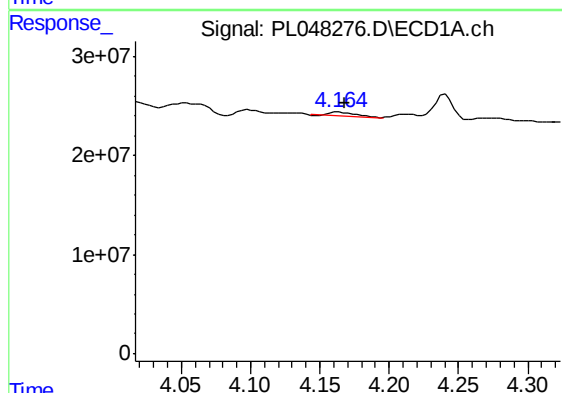


#23 Chlordane-1

R.T.: 4.164 min
Delta R.T.: -0.004 min
Response: 4717840
Conc: 10.51 ng/ml

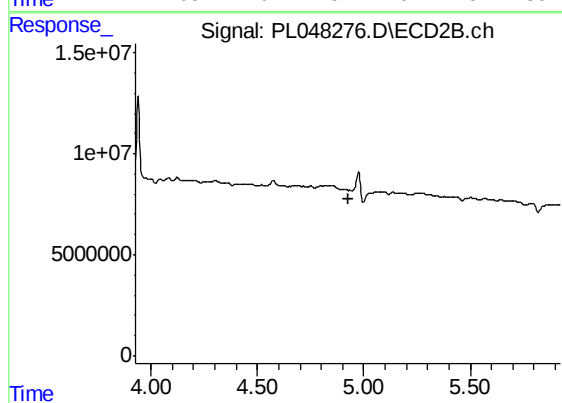

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

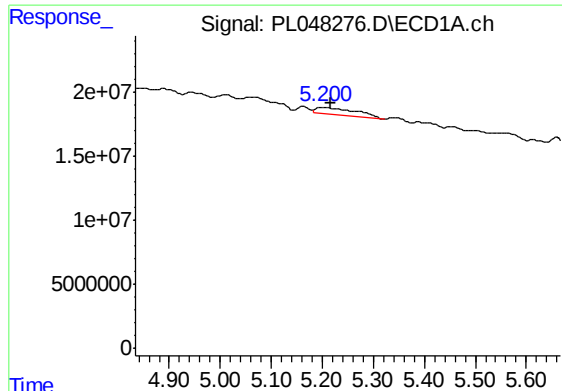

#25 Chlordane-3


R.T.: 5.199 min
Delta R.T.: -0.016 min
Response: 30826688
Conc: 19.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-C

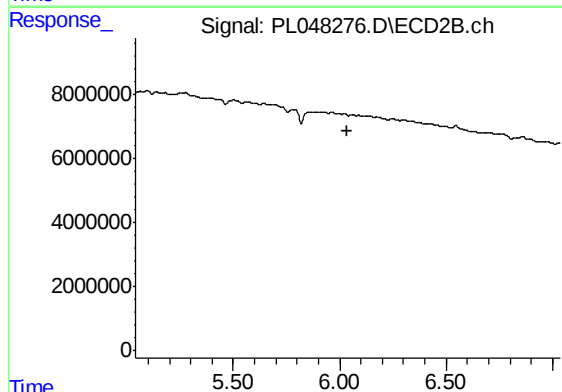


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

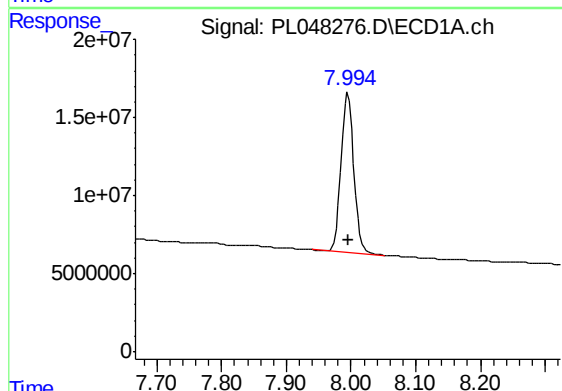

#28 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 139130949
Conc: 13.84 ng/ml

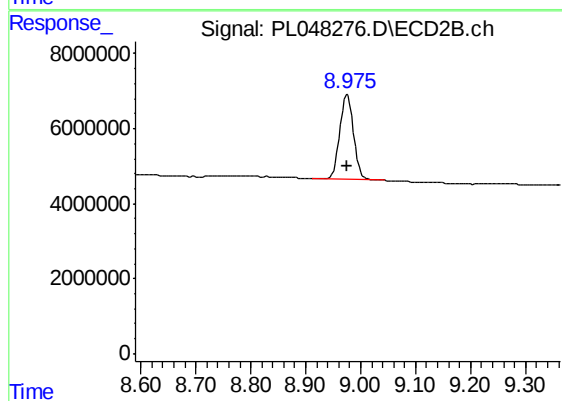

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.001 min
Response: 39368696
Conc: 14.83 ng/ml