

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050819\
 Data File : PL048280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2019 21:13
 Operator : AJ\SJ
 Sample : K2641-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-050719-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 01:06:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.939	174.3E6	47564199	17.994	19.095
28)	SA Decachlor...	7.995	8.976	135.4E6	37685438	13.464	14.198
Target Compounds							
4)	MA Heptachlor	0.000	5.135f	0	4361871	N.D.	1.260 #
7)	B delta-BHC	4.477	4.975f	-4466609	16690361	N.D.	5.902
9)	A Endosulfan I	5.348f	0.000	1758639	0	0.146	N.D. #
10)	B gamma-Chl...	5.203	0.000	6715535	0	0.503	N.D. #
23)	Chlordane-1	4.178	0.000	7868583	0	17.528	N.D. #
25)	Chlordane-3	5.203	0.000	6715535	0	4.265	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050819\
Data File : PL048280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2019 21:13
Operator : AJ\SJ
Sample : K2641-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
CL-02-050719-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 01:06:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

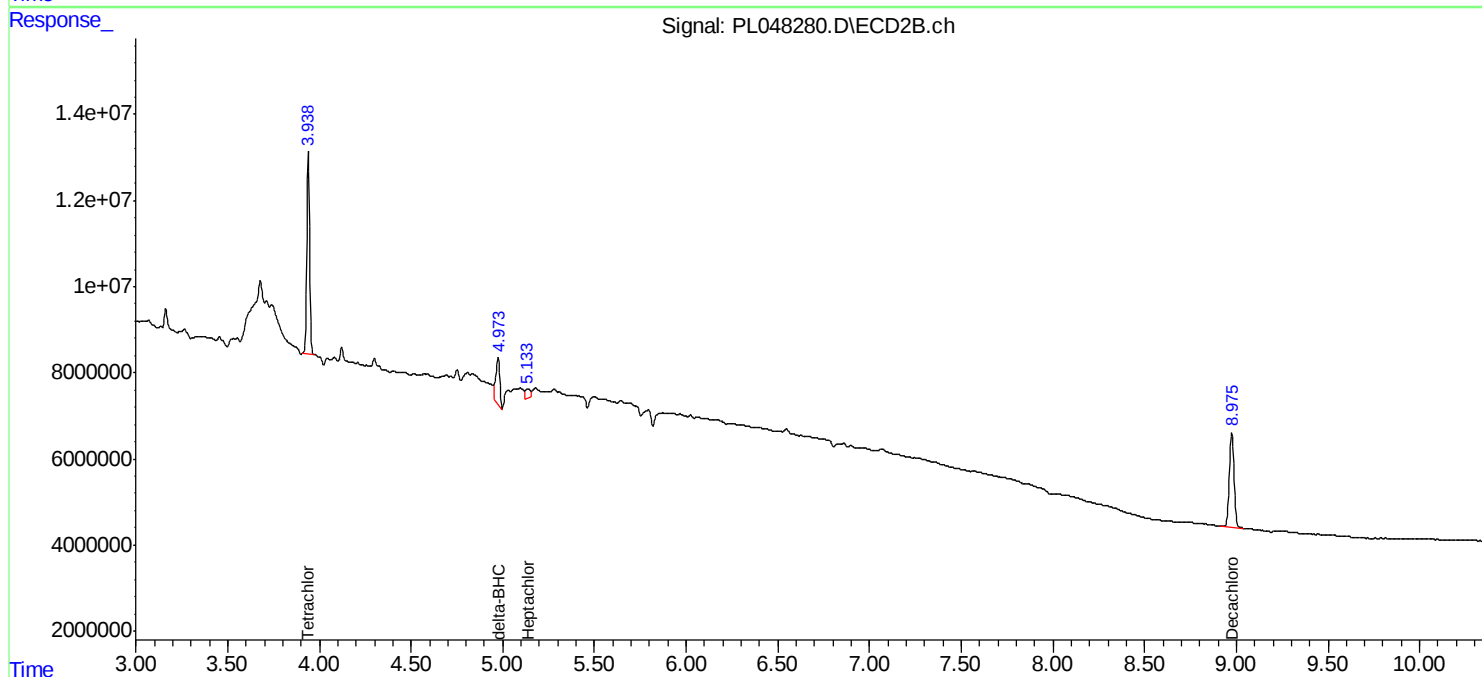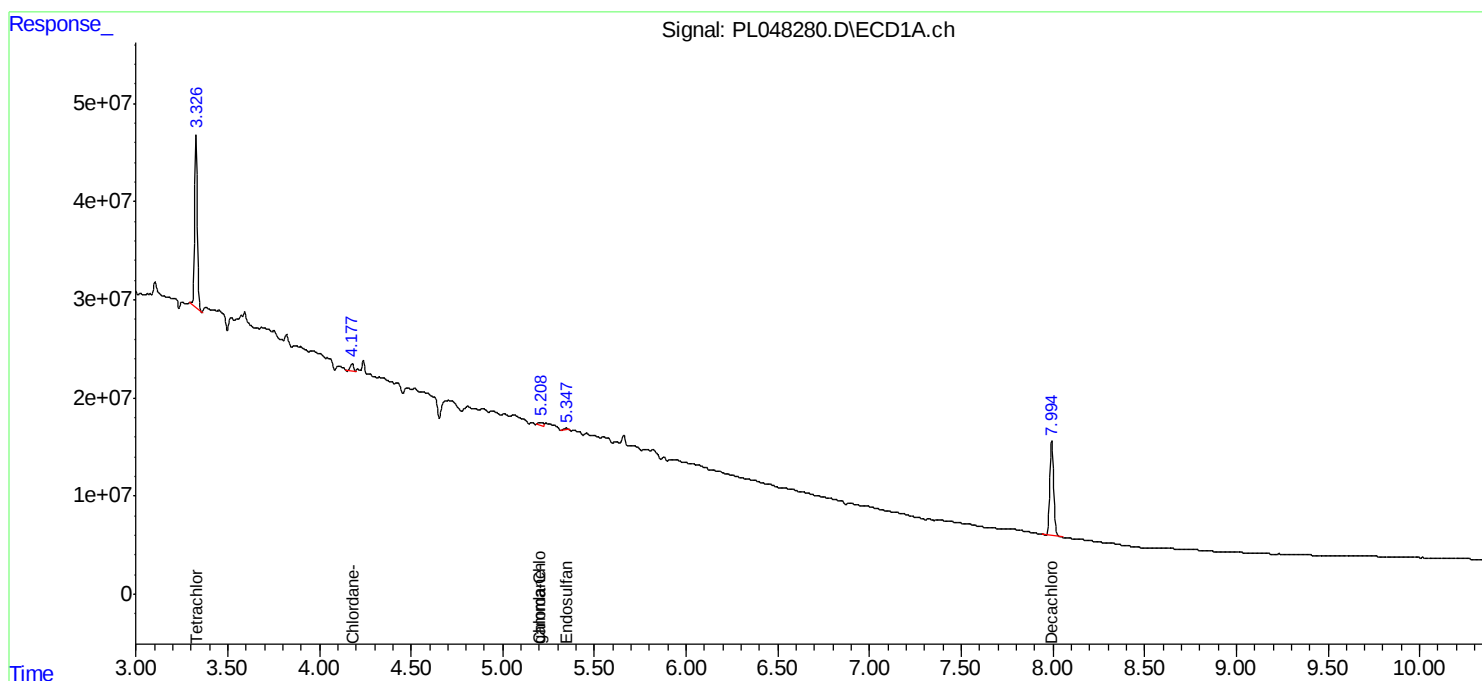


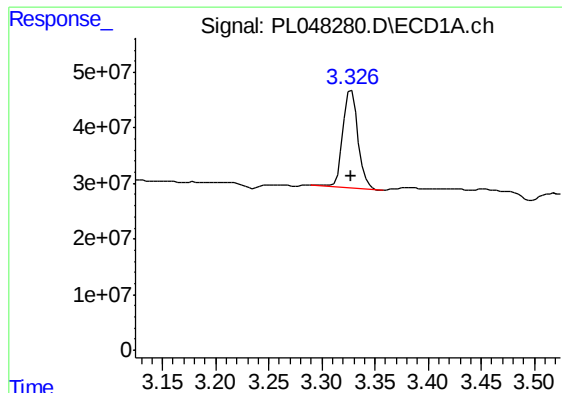

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 174305439
Conc: 17.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-D

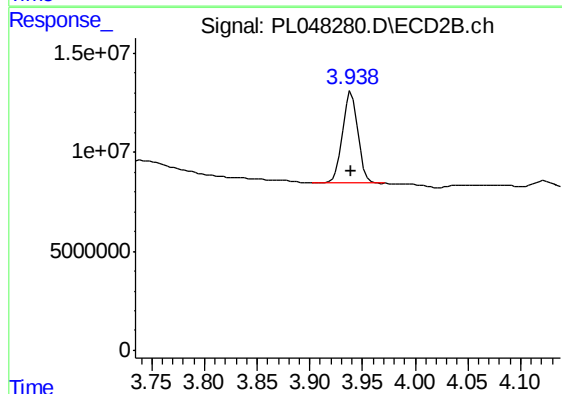


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 47564199
Conc: 19.10 ng/ml

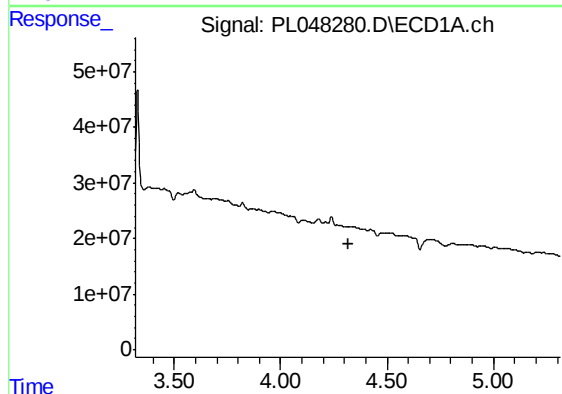


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

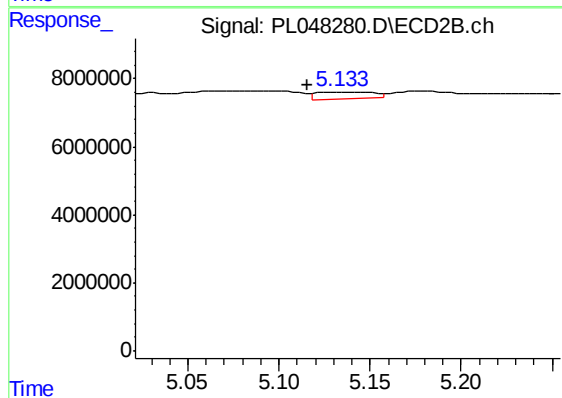

#4 Heptachlor


R.T.: 5.135 min
Delta R.T.: 0.019 min
Response: 4361871
Conc: 1.26 ng/ml

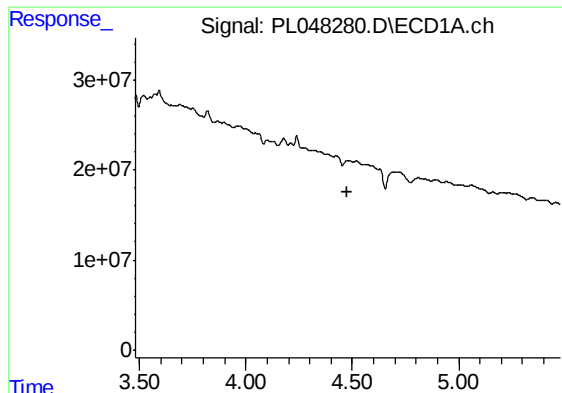

#7 delta-BHC


R.T.: 4.477 min
Delta R.T.: -0.003 min
Response: -4466609
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-D

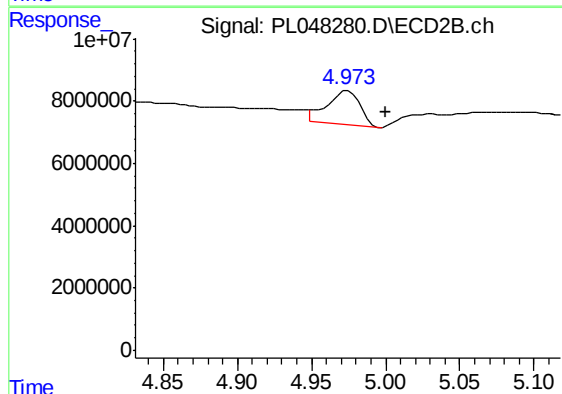


#7 delta-BHC

R.T.: 4.975 min
Delta R.T.: -0.025 min
Response: 16690361
Conc: 5.90 ng/ml

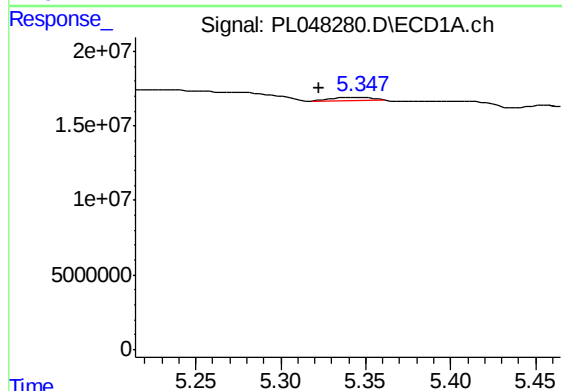


#9 Endosulfan I

R.T.: 5.348 min
Delta R.T.: 0.026 min
Response: 1758639
Conc: 0.15 ng/ml

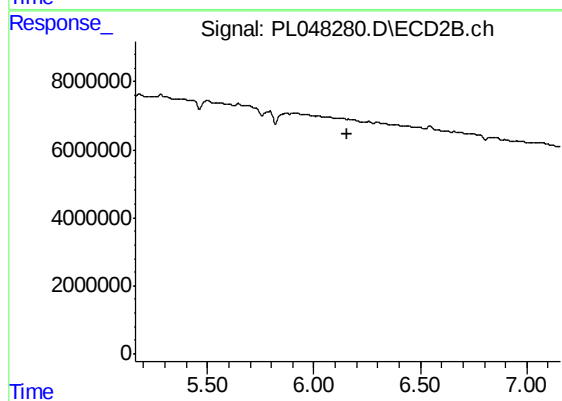

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.159 min
Response: 0
Conc: N.D.

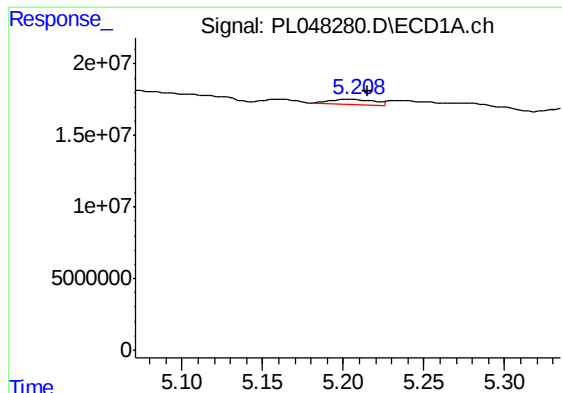

#10 gamma-Chlordane


R.T.: 5.203 min
Delta R.T.: -0.012 min
Response: 6715535
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-D

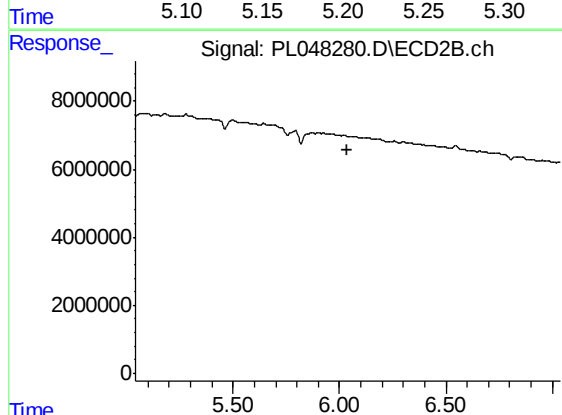


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

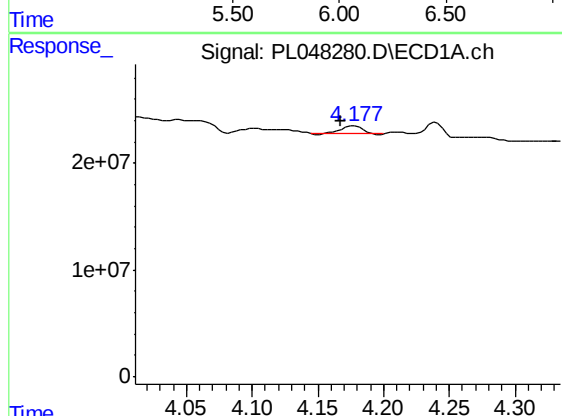


#23 Chlordane-1

R.T.: 4.178 min
Delta R.T.: 0.011 min
Response: 7868583
Conc: 17.53 ng/ml

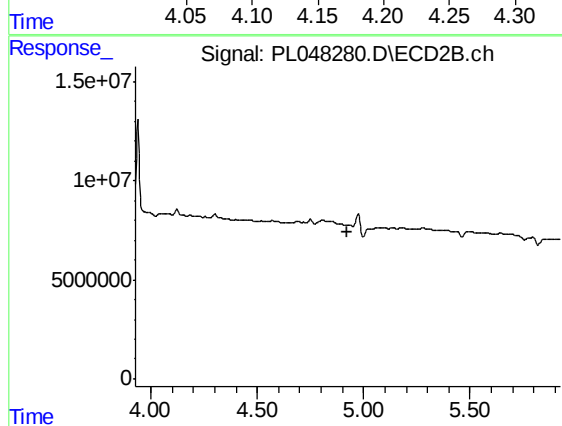

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

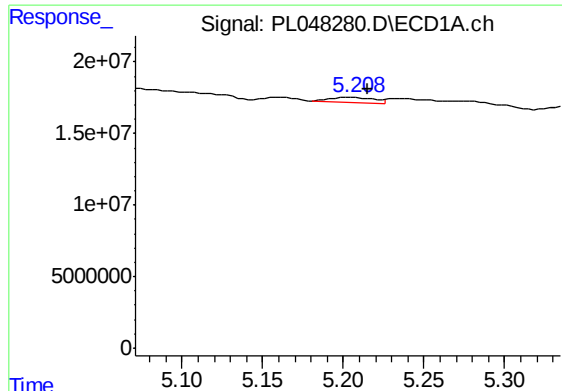

#25 Chlordane-3


R.T.: 5.203 min
Delta R.T.: -0.013 min
Response: 6715535
Conc: 4.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-050719-D

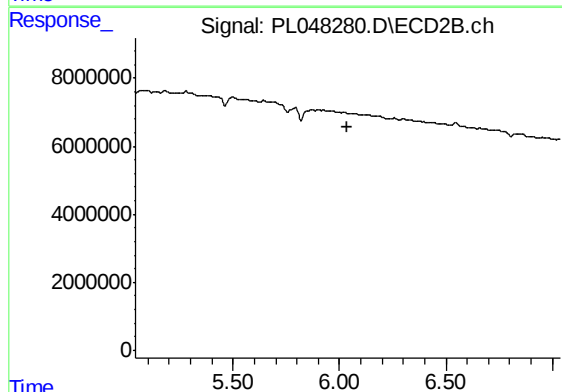


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

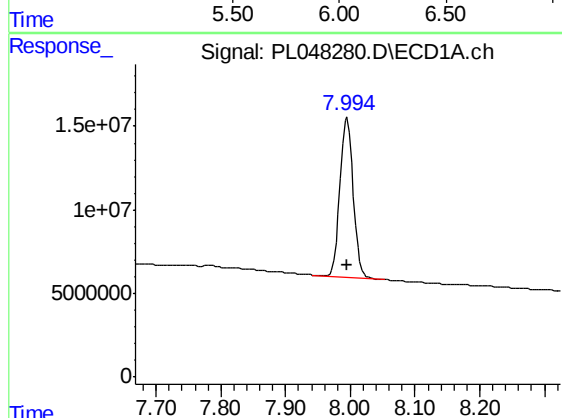

#28 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 135368527
Conc: 13.46 ng/ml

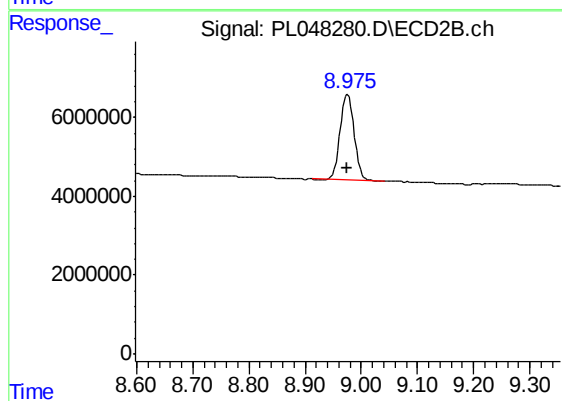

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.000 min
Response: 37685438
Conc: 14.20 ng/ml