

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050819\
 Data File : PL048288.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2019 23:13
 Operator : AJ\SJ
 Sample : K2645-10
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PL-02-050719-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 01:08:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	218.2E6	62829008	22.528	25.224
28)	SA Decachlor...	7.995	8.975	205.9E6	56510257	20.480	21.290
Target Compounds							
2)	A alpha-BHC	0.000	4.301f	0	3739049	N.D.	1.065 #
4)	MA Heptachlor	0.000	5.128	0	1548523	N.D.	0.447 #
7)	B delta-BHC	4.488	4.974f	-2504671	11400151	N.D.	4.031
9)	A Endosulfan I	5.351f	0.000	2344792	0	0.195	N.D. #
10)	B gamma-Chl...	5.195f	0.000	9274751	0	0.695	N.D. #
13)	MA Dieldrin	5.551	0.000	9856337	0	0.757	N.D. #
23)	Chlordane-1	4.178	0.000	1584778	0	3.530	N.D. #
25)	Chlordane-3	5.195f	0.000	9274751	0	5.890	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050819\
Data File : PL048288.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2019 23:13
Operator : AJ\SJ
Sample : K2645-10
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PL-02-050719-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 01:08:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

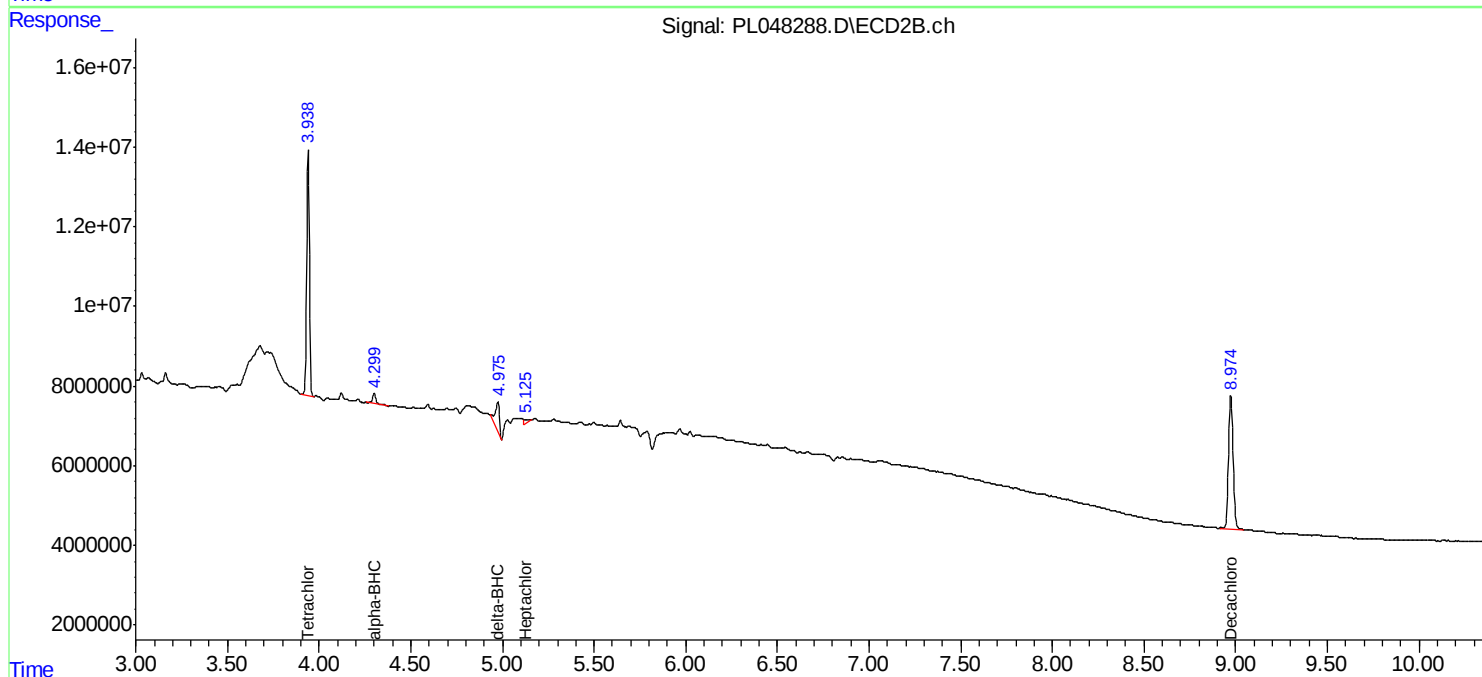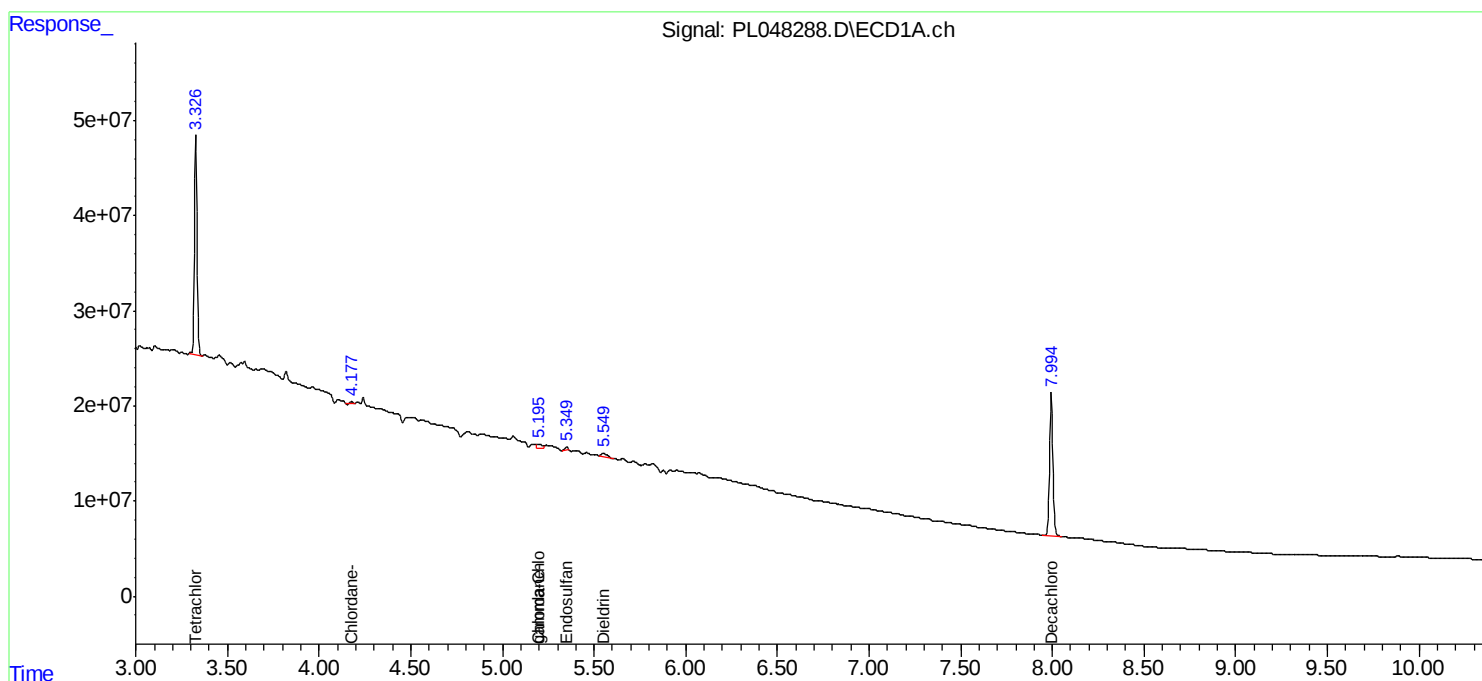


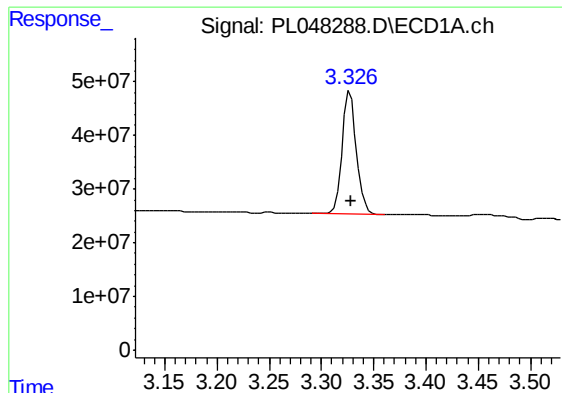

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 218228589
Conc: 22.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-050719-E

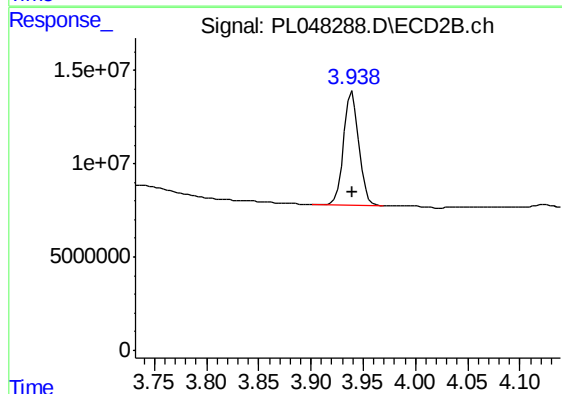


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 62829008
Conc: 25.22 ng/ml

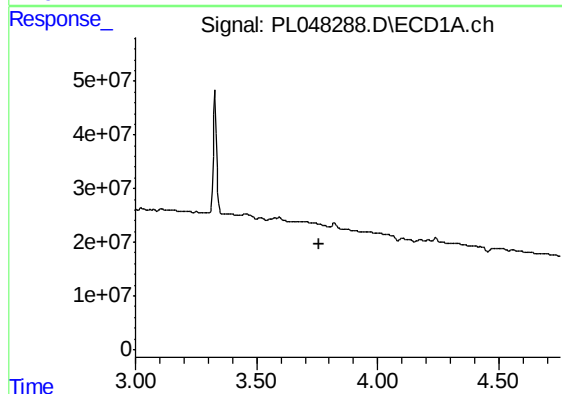


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.756 min
Response: 0
Conc: N.D.

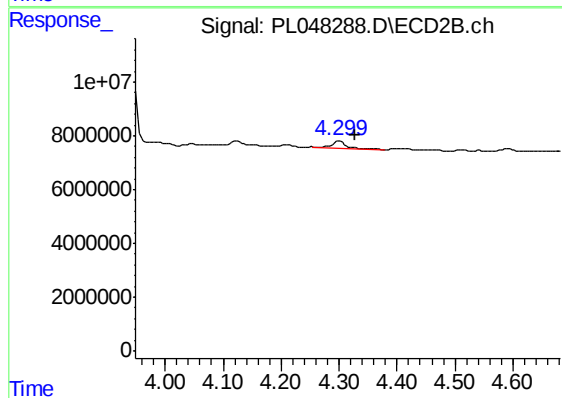

#2 alpha-BHC


R.T.: 4.301 min
Delta R.T.: -0.028 min
Response: 3739049
Conc: 1.06 ng/ml

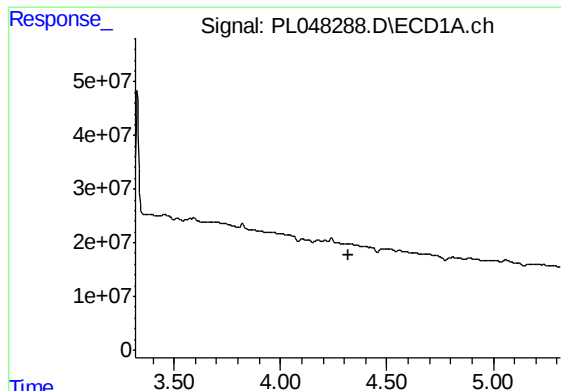

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PL-02-050719-E

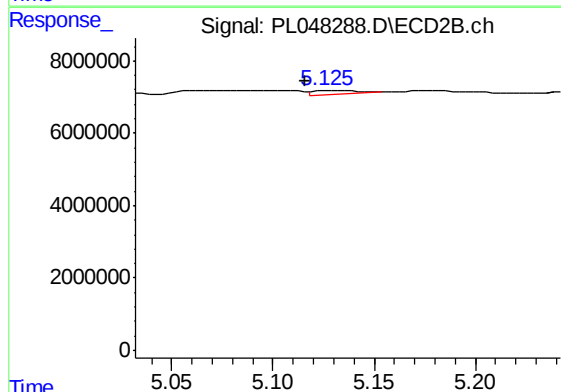


#4 Heptachlor

R.T.: 5.128 min
Delta R.T.: 0.013 min
Response: 1548523
Conc: 0.45 ng/ml

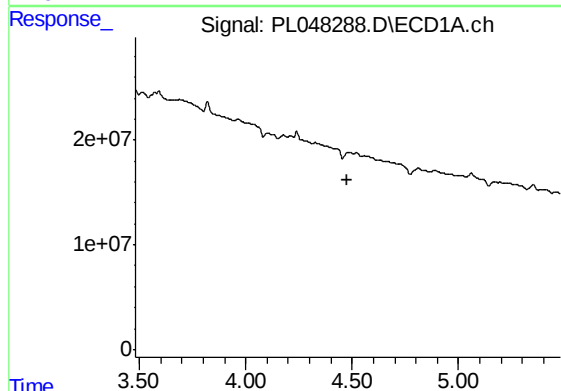


#7 delta-BHC

R.T.: 4.488 min
Delta R.T.: 0.008 min
Response: -2504671
Conc: N.D.

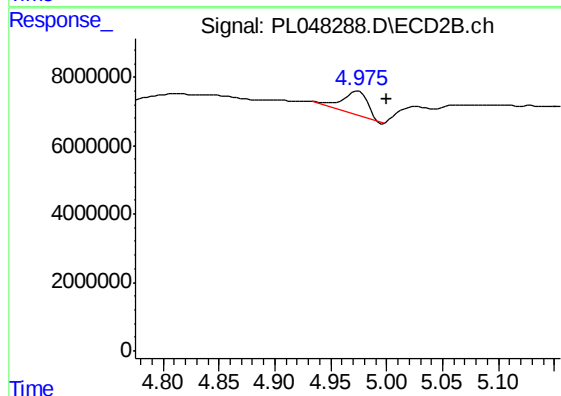

#7 delta-BHC


R.T.: 4.974 min
Delta R.T.: -0.026 min
Response: 11400151
Conc: 4.03 ng/ml

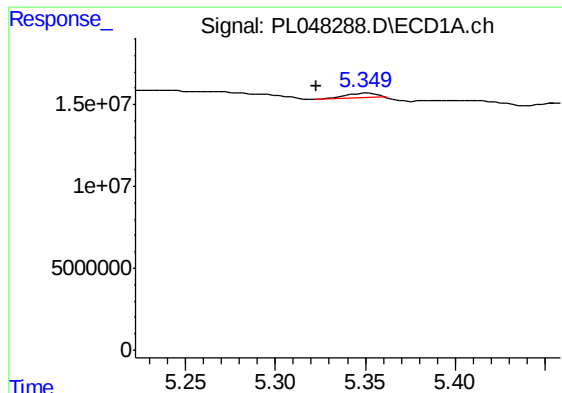

#9 Endosulfan I


R.T.: 5.351 min
Delta R.T.: 0.028 min
Response: 2344792
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-050719-E

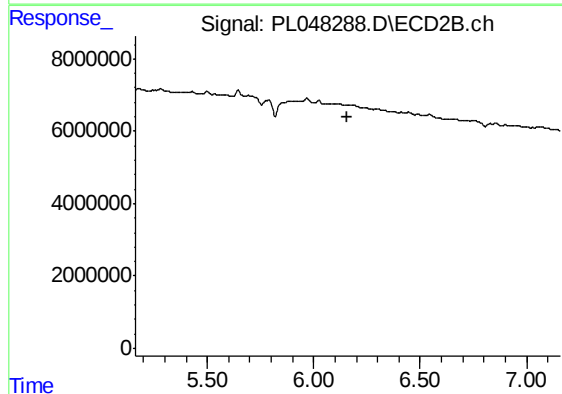


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.159 min
Response: 0
Conc: N.D.

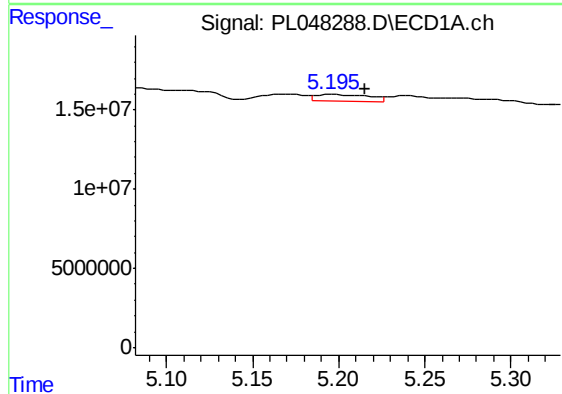


#10 gamma-Chlordane

R.T.: 5.195 min
Delta R.T.: -0.020 min
Response: 9274751
Conc: 0.69 ng/ml

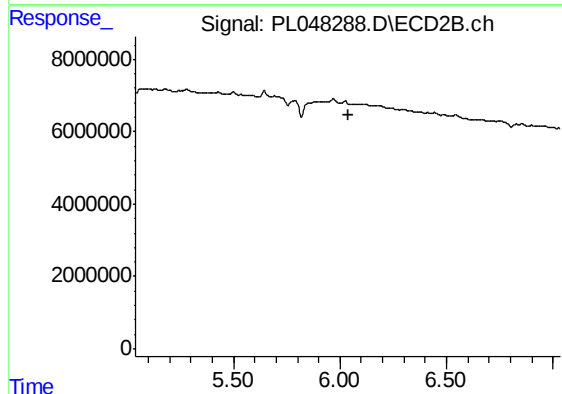

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

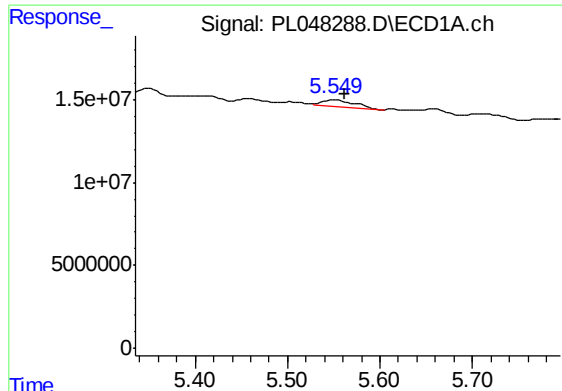

#13 Dieldrin


R.T.: 5.551 min
Delta R.T.: -0.011 min
Response: 9856337
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-050719-E

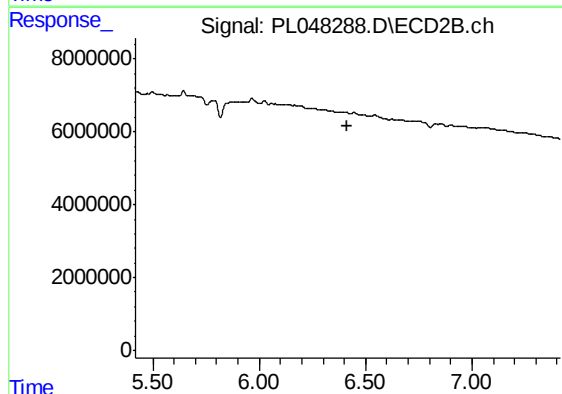


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

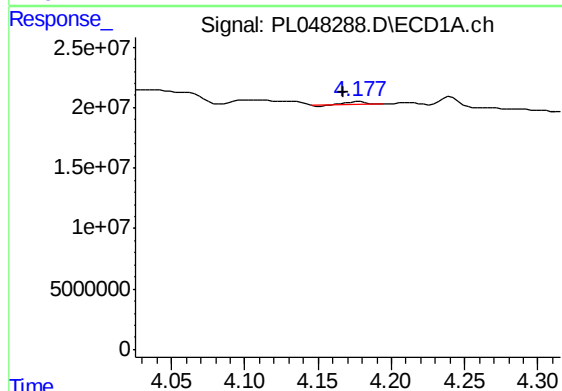


#23 Chlordane-1

R.T.: 4.178 min
Delta R.T.: 0.011 min
Response: 1584778
Conc: 3.53 ng/ml

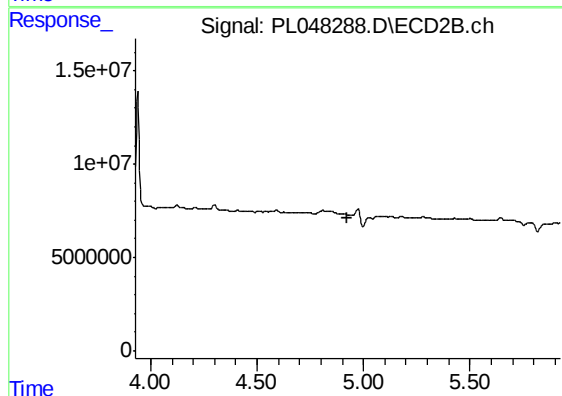

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

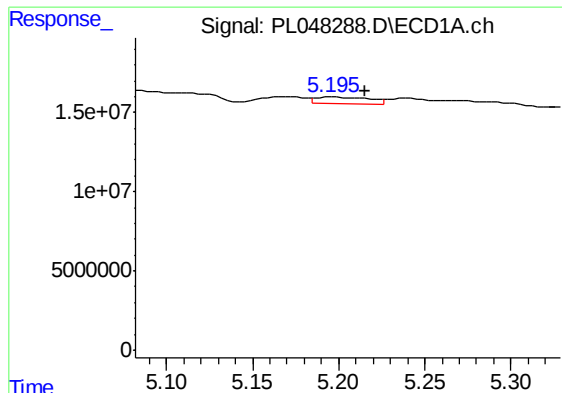

#25 Chlordane-3


R.T.: 5.195 min
Delta R.T.: -0.020 min
Response: 9274751
Conc: 5.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-050719-E

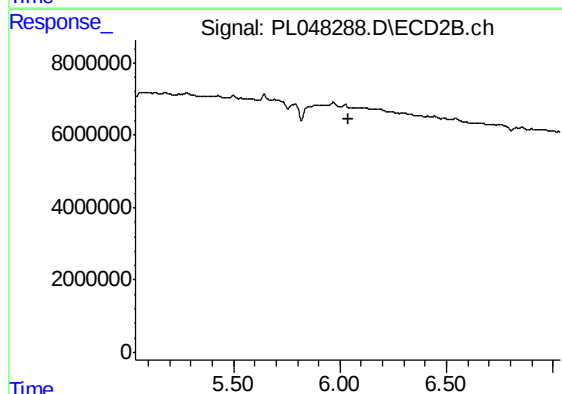


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

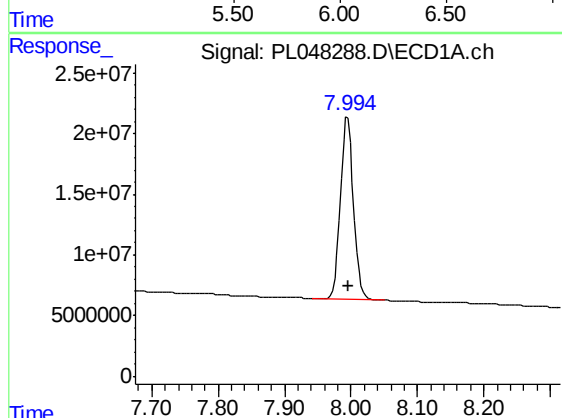

#28 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 205911218
Conc: 20.48 ng/ml

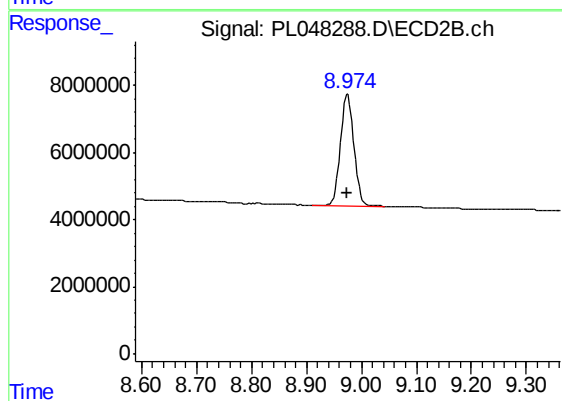

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 56510257
Conc: 21.29 ng/ml