

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050820\
 Data File : PL058624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2020 21:21
 Operator : AJ\MA
 Sample : L2557-08
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-13A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 00:32:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 29 00:55:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.455	3.954	225.7E6	49577716	21.207	22.938
28)	SA Decachlor...	8.201	8.976	209.3E6	43939726	19.351	19.803
Target Compounds							
2)	A alpha-BHC	3.894	0.000	5476243	0	0.299	N.D. #
4)	MA Heptachlor	0.000	5.135	0	657864	N.D.	0.190 #
5)	MB Aldrin	4.724	0.000	1807083	0	0.109	N.D. #
7)	B delta-BHC	4.642	4.986f	906427	1505846	0.053	0.599 #
8)	B Heptachlo...	5.156	5.812	11469396	1851493	0.755	0.578
9)	A Endosulfan I	5.514	0.000	695287	0	0.049	N.D. #
10)	B gamma-Chl...	5.362f	6.039	8988091	2114408	0.584	0.626
11)	B alpha-Chl...	5.445	0.000	7209766	0	0.475	N.D. #
19)	B Endosulfa...	6.671f	0.000	357935	0	0.031	N.D. #
24)	Chlordane-2	4.819	0.000	2582402	0	6.218	N.D. #
25)	Chlordane-3	5.362f	6.039	8988091	2114408	6.843	5.287
26)	Chlordane-4	5.445	0.000	7209766	0	6.569	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050820\
Data File : PL058624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2020 21:21
Operator : AJ\MA
Sample : L2557-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-13A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 00:32:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042820.M
Quant Title : GC Extractables
QLast Update : Wed Apr 29 00:55:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

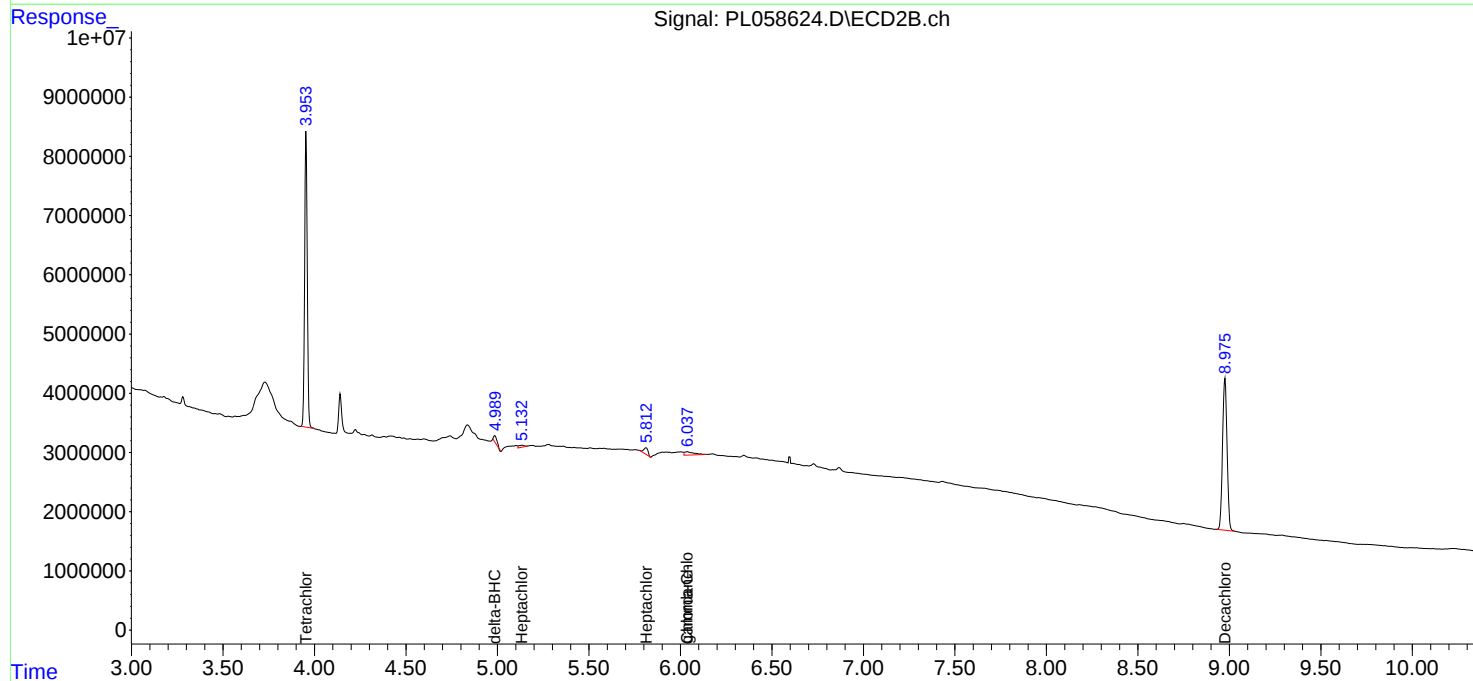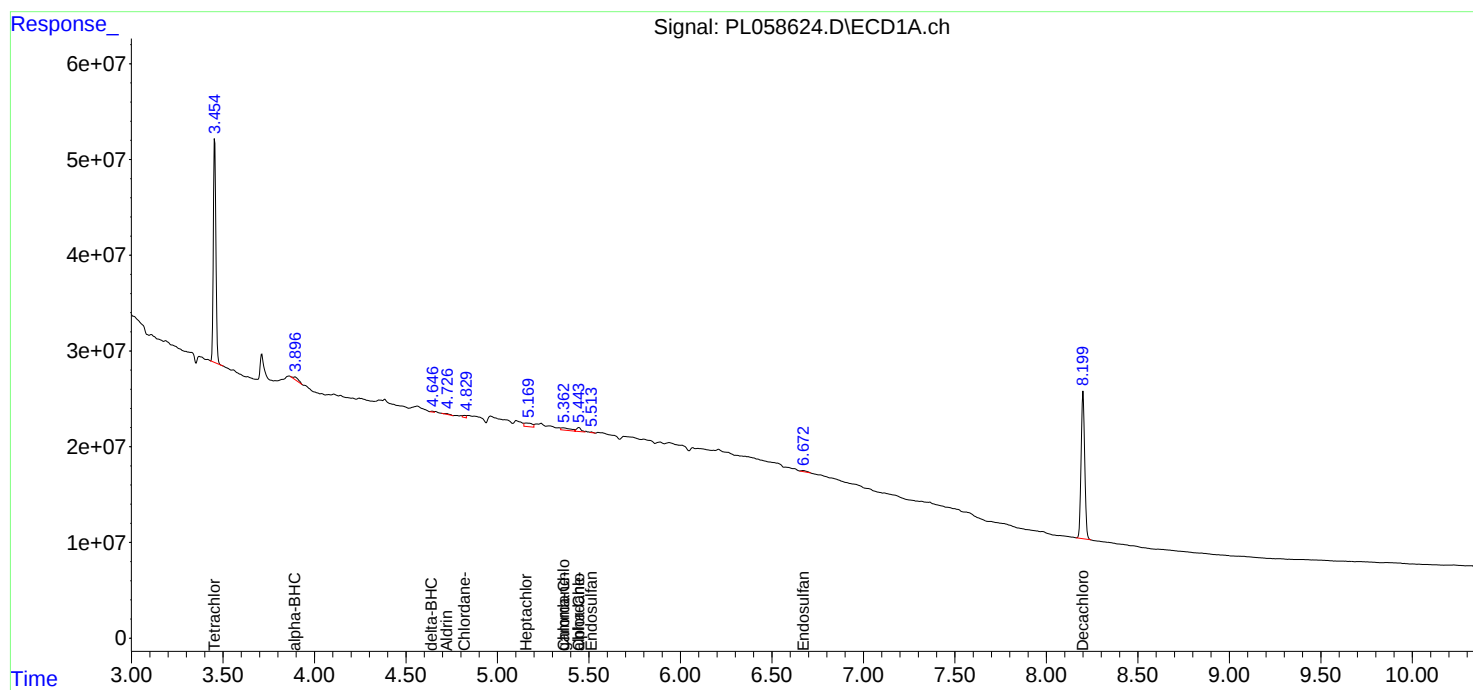


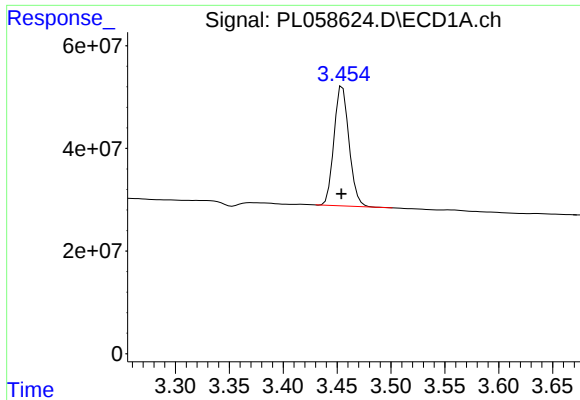

#1 Tetrachloro-m-xylene


R.T.: 3.455 min
Delta R.T.: 0.001 min
Response: 225684742
Conc: 21.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13A

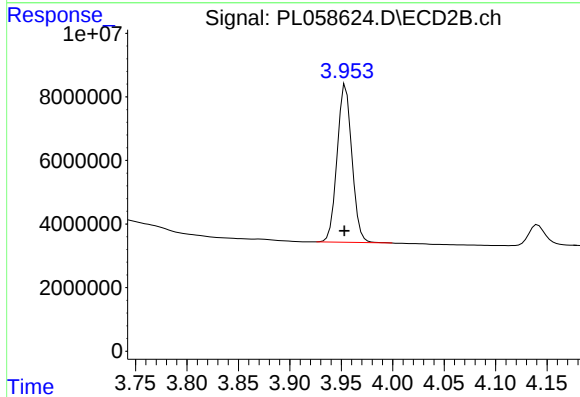


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: 0.001 min
Response: 49577716
Conc: 22.94 ng/ml

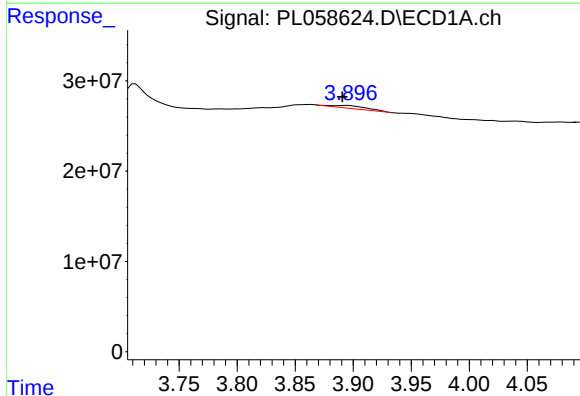


#2 alpha-BHC

R.T.: 3.894 min
Delta R.T.: 0.004 min
Response: 5476243
Conc: 0.30 ng/ml

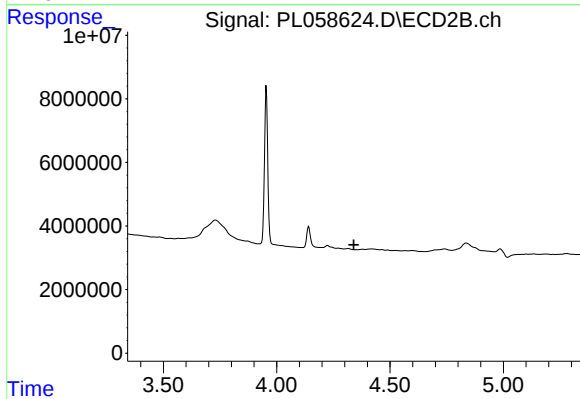

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.340 min
Response: 0
Conc: N.D.

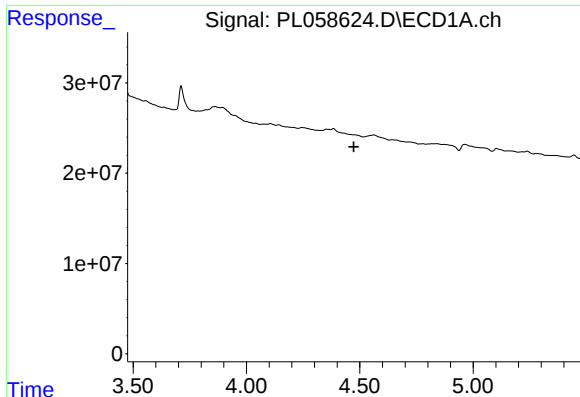

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-13A

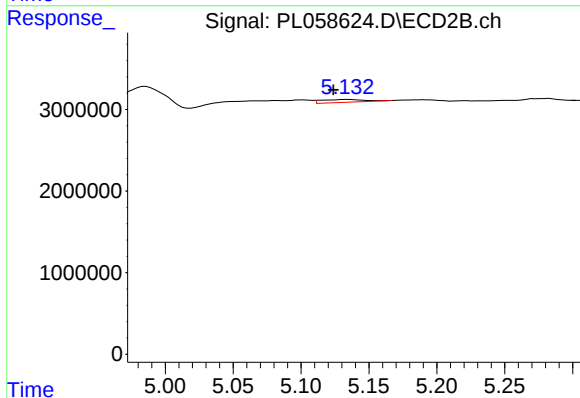


#4 Heptachlor

R.T.: 5.135 min
Delta R.T.: 0.011 min
Response: 657864
Conc: 0.19 ng/ml

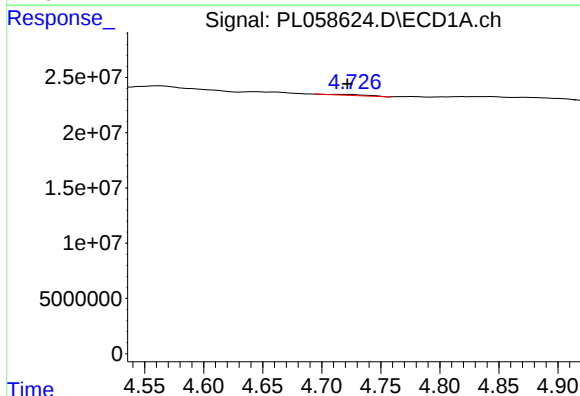


#5 Aldrin

R.T.: 4.724 min
Delta R.T.: 0.002 min
Response: 1807083
Conc: 0.11 ng/ml

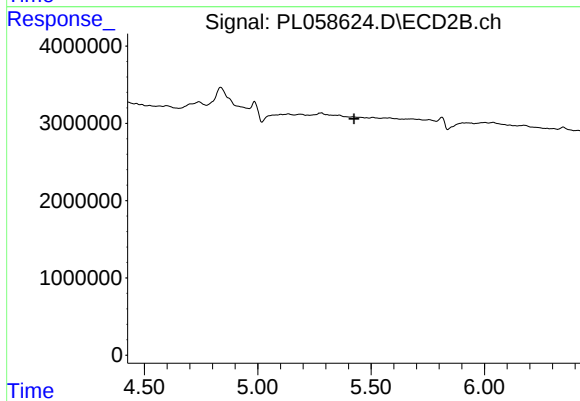

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.425 min
Response: 0
Conc: N.D.

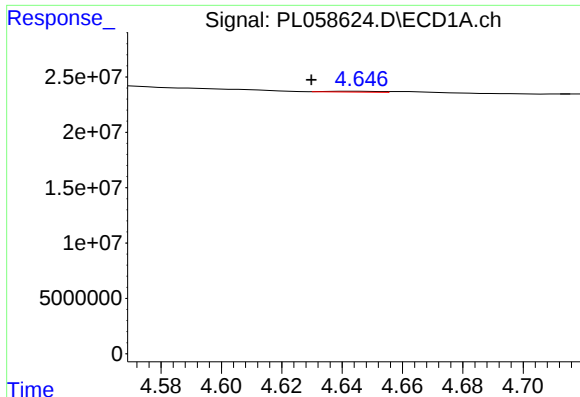

#7 delta-BHC


R.T.: 4.642 min
Delta R.T.: 0.012 min
Response: 906427
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13A

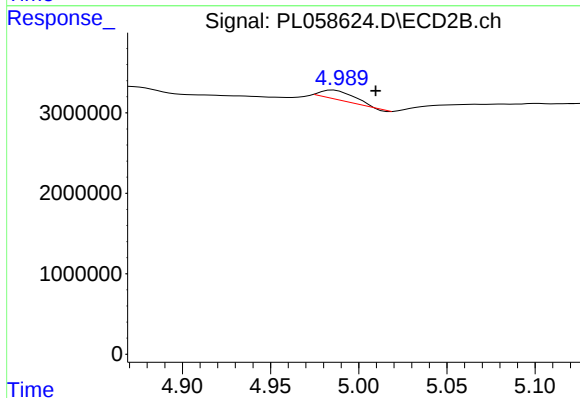


#7 delta-BHC

R.T.: 4.986 min
Delta R.T.: -0.024 min
Response: 1505846
Conc: 0.60 ng/ml

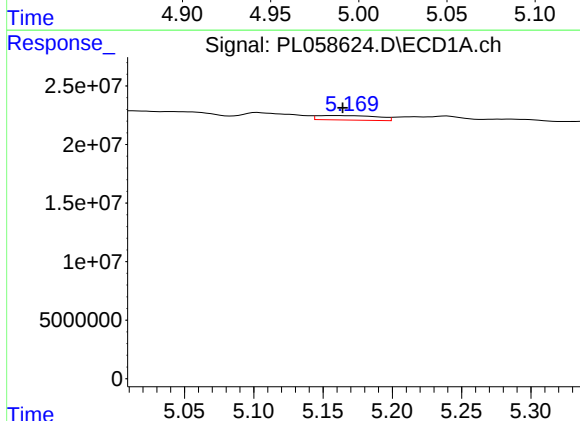


#8 Heptachlor epoxide

R.T.: 5.156 min
Delta R.T.: -0.008 min
Response: 11469396
Conc: 0.76 ng/ml

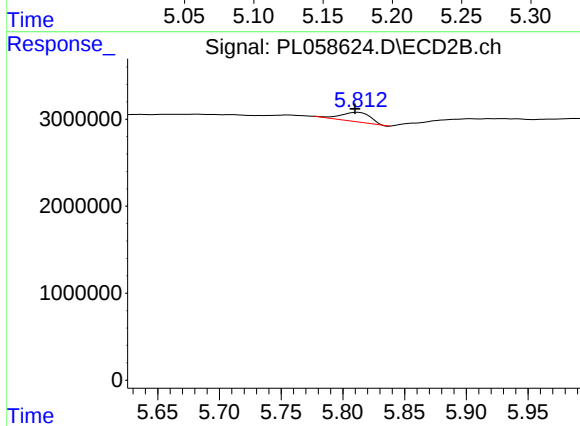

#8 Heptachlor epoxide


R.T.: 5.812 min
Delta R.T.: 0.002 min
Response: 1851493
Conc: 0.58 ng/ml

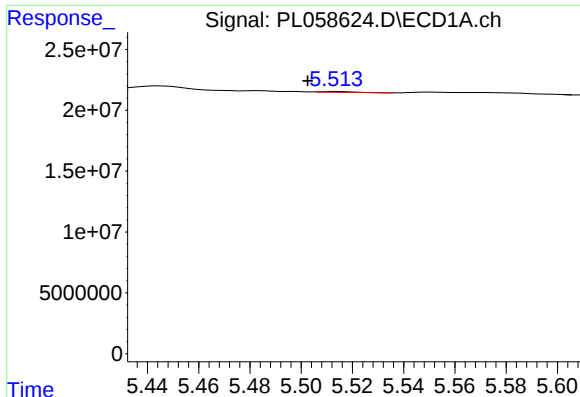

#9 Endosulfan I


R.T.: 5.514 min
Delta R.T.: 0.012 min
Response: 695287
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13A

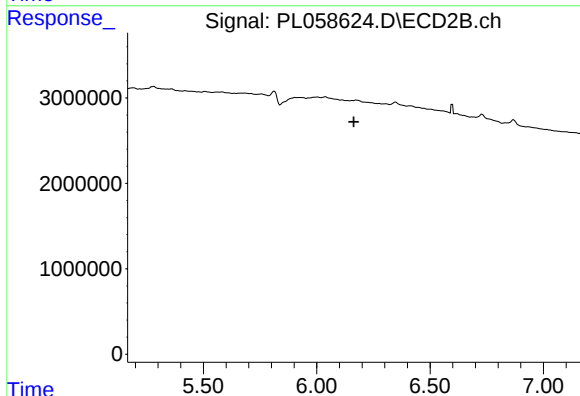


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

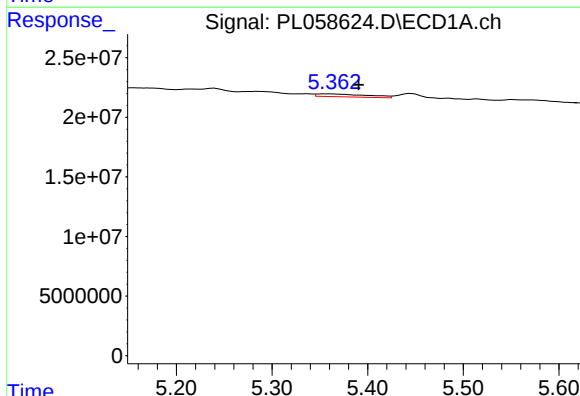


#10 gamma-Chlordane

R.T.: 5.362 min
Delta R.T.: -0.029 min
Response: 8988091
Conc: 0.58 ng/ml

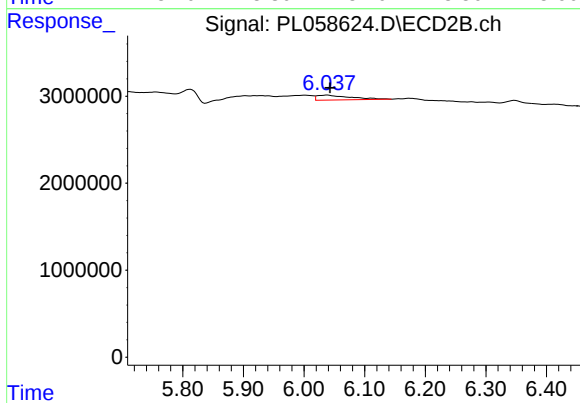

#10 gamma-Chlordane


R.T.: 6.039 min
Delta R.T.: -0.004 min
Response: 2114408
Conc: 0.63 ng/ml

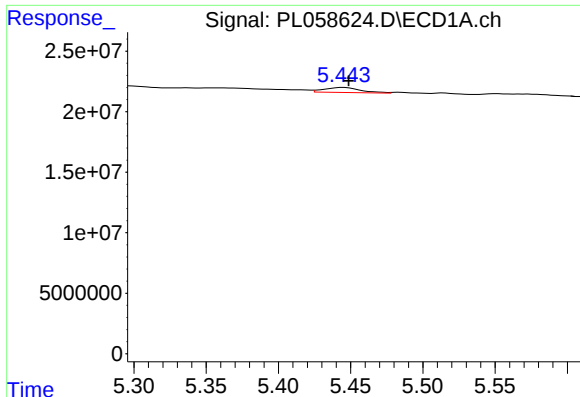

#11 alpha-Chlordane


R.T.: 5.445 min
Delta R.T.: -0.004 min
Response: 7209766
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13A

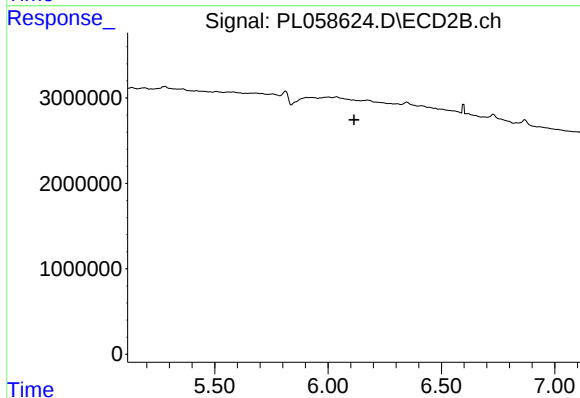


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

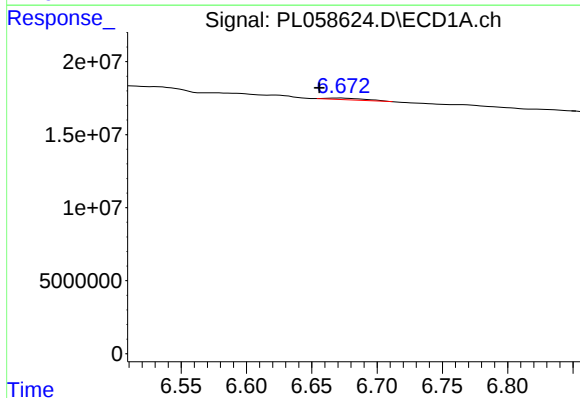


#19 Endosulfan Sulfate

R.T.: 6.671 min
Delta R.T.: 0.015 min
Response: 357935
Conc: 0.03 ng/ml

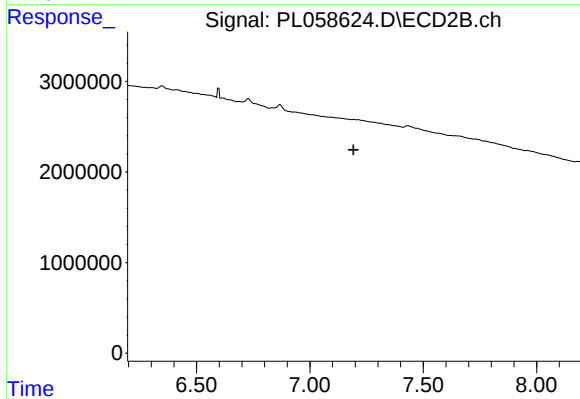

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

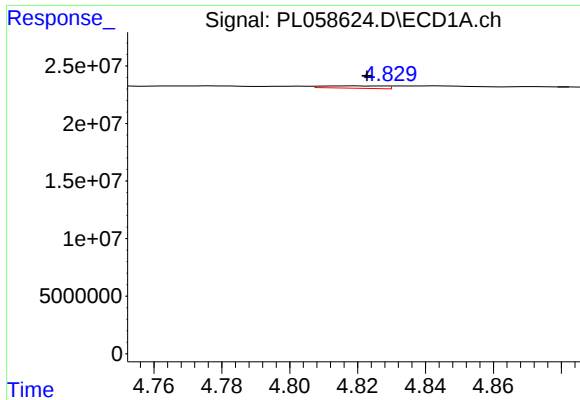

#24 Chlordane-2


R.T.: 4.819 min
Delta R.T.: -0.004 min
Response: 2582402
Conc: 6.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13A

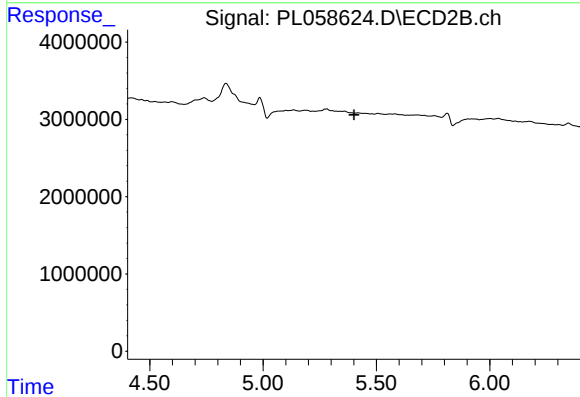


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

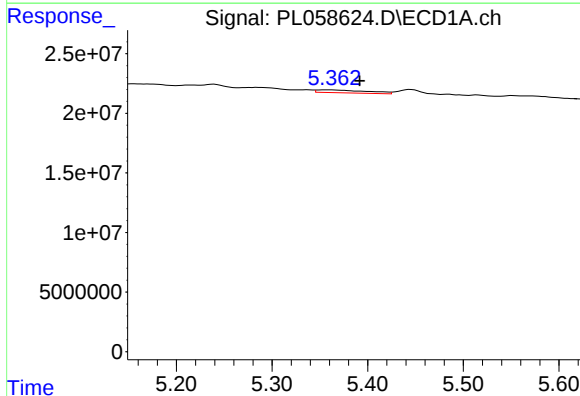


#25 Chlordane-3

R.T.: 5.362 min
Delta R.T.: -0.030 min
Response: 8988091
Conc: 6.84 ng/ml

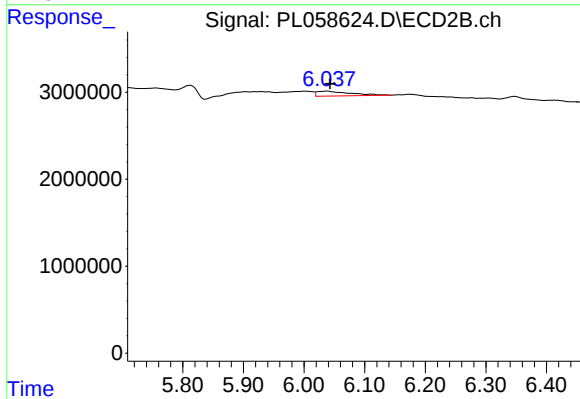

#25 Chlordane-3


R.T.: 6.039 min
Delta R.T.: -0.004 min
Response: 2114408
Conc: 5.29 ng/ml

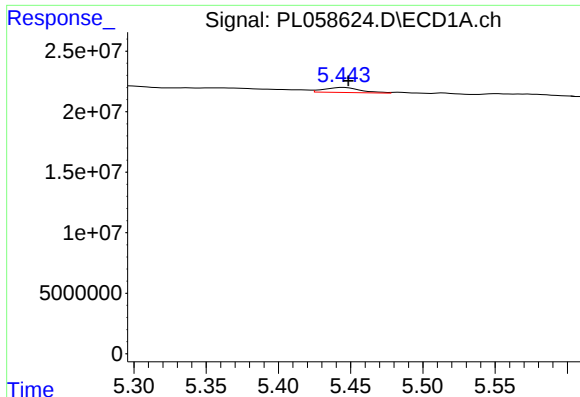

#26 Chlordane-4


R.T.: 5.445 min
Delta R.T.: -0.003 min
Response: 7209766
Conc: 6.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13A

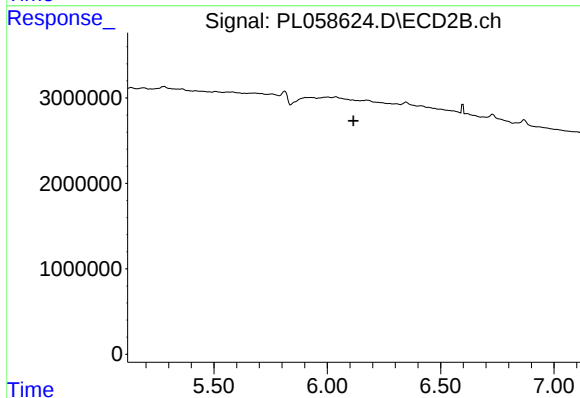


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.116 min
Response: 0
Conc: N.D.

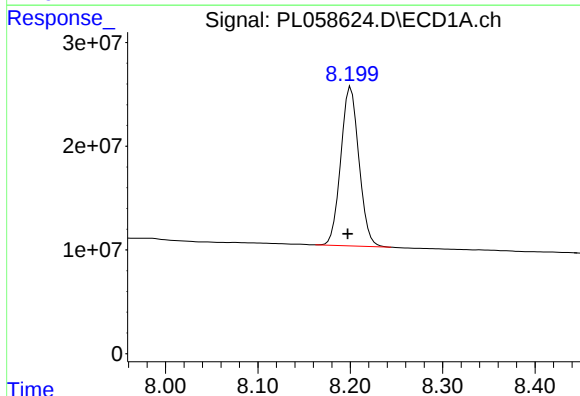

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.003 min
Response: 209277224
Conc: 19.35 ng/ml

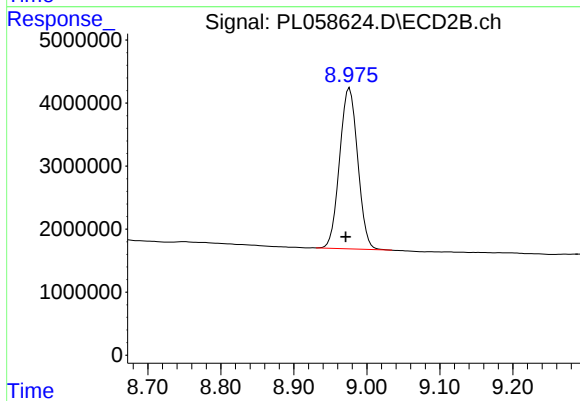

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.005 min
Response: 43939726
Conc: 19.80 ng/ml