

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050823\
 Data File : PL082580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2023 14:23
 Operator : AR\AJ
 Sample : 02652-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CLAY-LINER

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/09/2023
 Supervised By : Ankita Jodhani 05/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 08 20:59:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.325	2.642	31656928	39554804	11.851	17.074 #
2) SA Decachlor...	8.743	7.753	37814058	35321247	19.807	15.475
Target Compounds						
16) A 4,4'-DDD	6.454	5.648	25747450	20969311	12.701m	11.211m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050823\
Data File : PL082580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2023 14:23
Operator : AR\AJ
Sample : 02652-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CLAY-LINER


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/09/2023
Supervised By : Ankita Jodhani 05/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 08 20:59:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

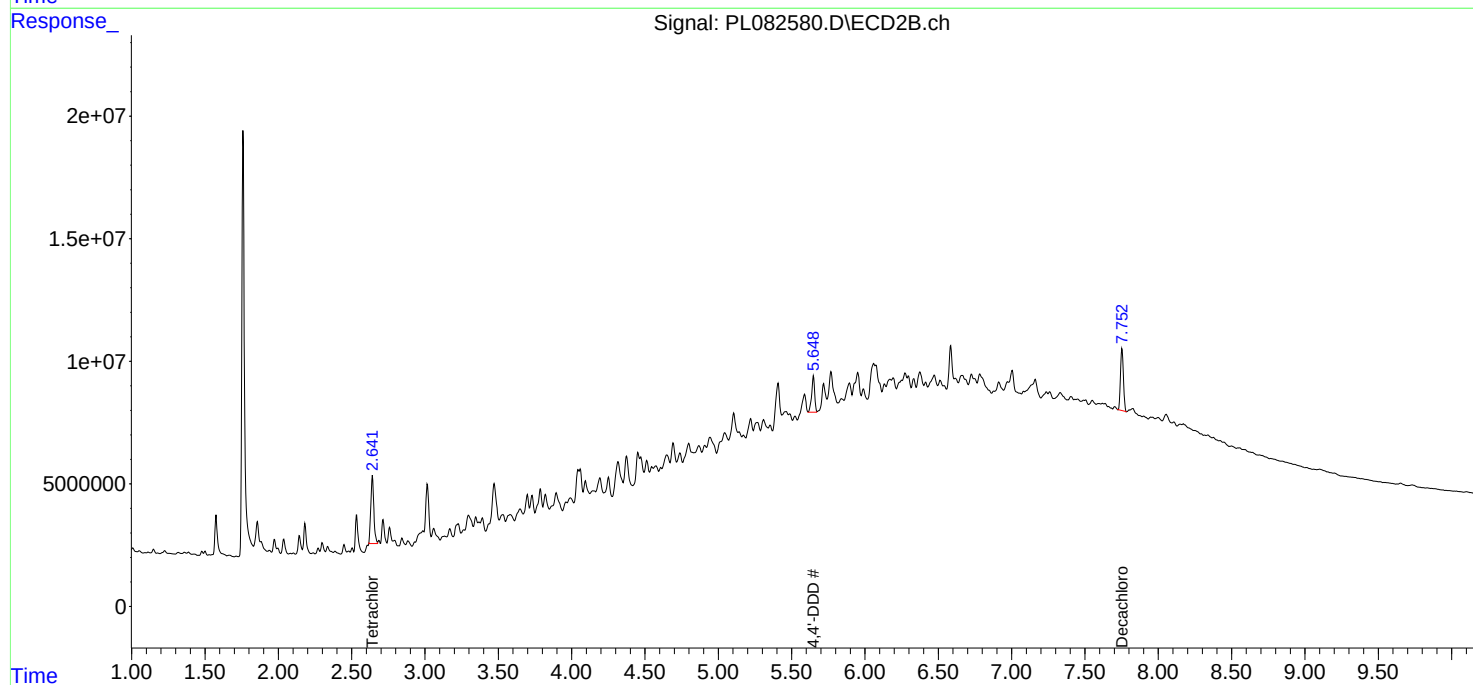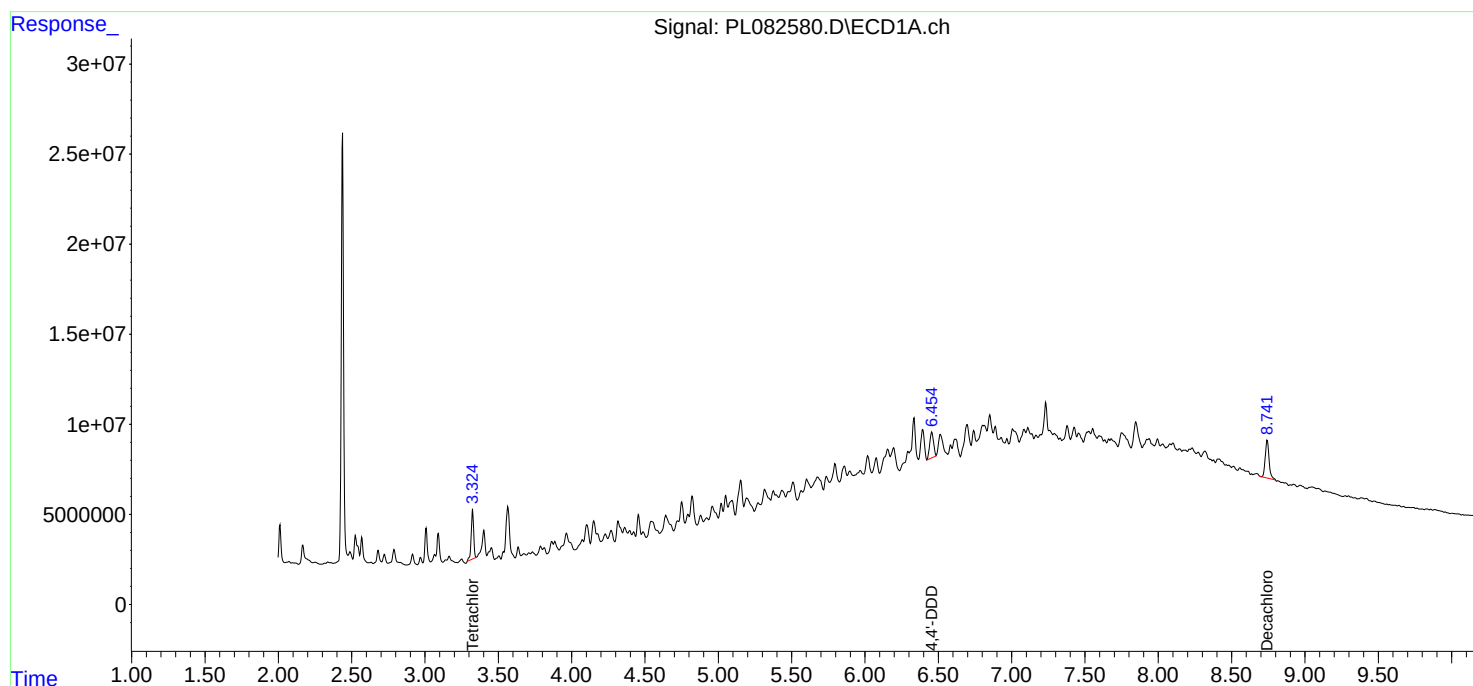

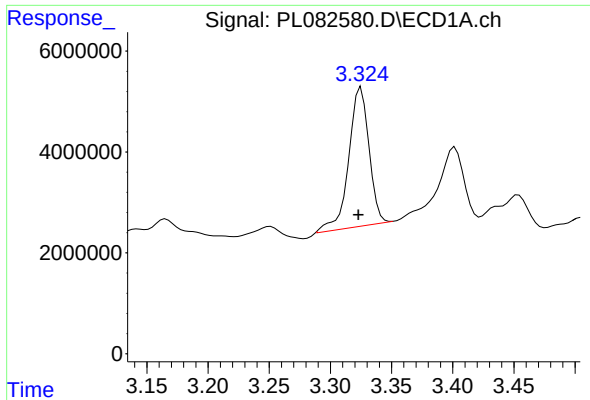


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: 0.002 min
Response: 31656928
Conc: 11.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
CLAY-LINER


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/09/2023
Supervised By :Ankita Jodhani 05/09/2023

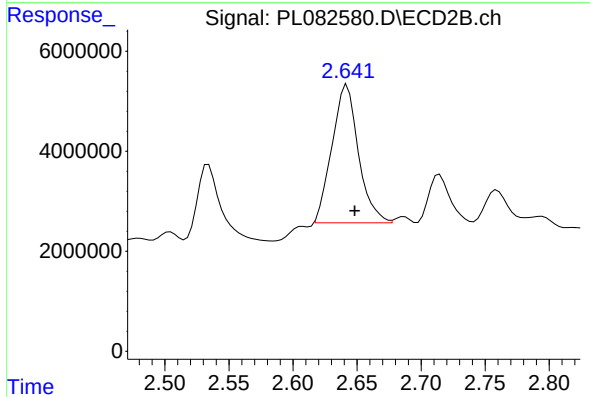


#1 Tetrachloro-m-xylene

R.T.: 2.642 min
Delta R.T.: -0.006 min
Response: 39554804
Conc: 17.07 ng/ml

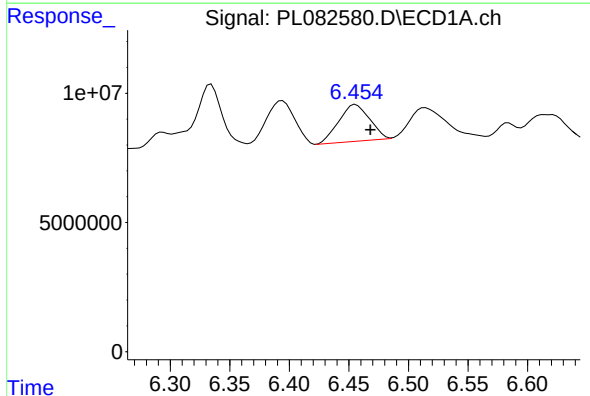


#16 4,4'-DDD

R.T.: 6.454 min
Delta R.T.: -0.014 min
Response: 25747450
Conc: 12.70 ng/ml m

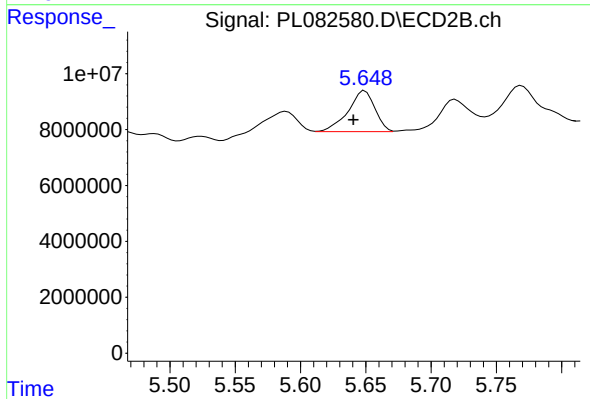

#16 4,4'-DDD

R.T.: 5.648 min
Delta R.T.: 0.008 min
Response: 20969311
Conc: 11.21 ng/ml m

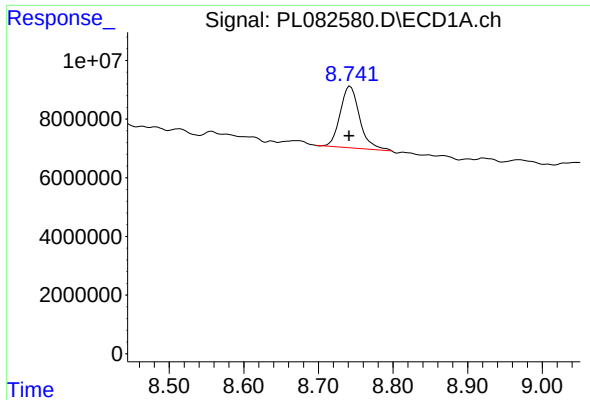

#28 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.002 min
Response: 37814058
Conc: 19.81 ng/ml

Instrument :

ECD_L

ClientSampleId :


CLAY-LINER

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 05/09/2023

Supervised By :Ankita Jodhani 05/09/2023

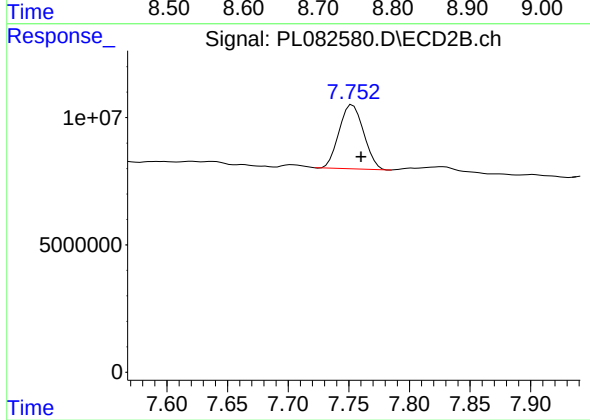

#28 Decachlorobiphenyl

R.T.: 7.753 min
Delta R.T.: -0.007 min
Response: 35321247
Conc: 15.47 ng/ml