

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050825\
 Data File : PL095585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2025 15:00
 Operator : AR\AJ
 Sample : Q1972-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SUB-WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 02:05:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.595	2.913	58952718	70352440	18.058	22.125
28)	SA Decachlor...	9.122	8.093	37946617	44787214	13.695	15.135
Target Compounds							
15)	B Endosulfa...	6.864f	0.000	15032803	0	4.709	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050825\
Data File : PL095585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2025 15:00
Operator : AR\AJ
Sample : Q1972-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SUB-WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 02:05:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

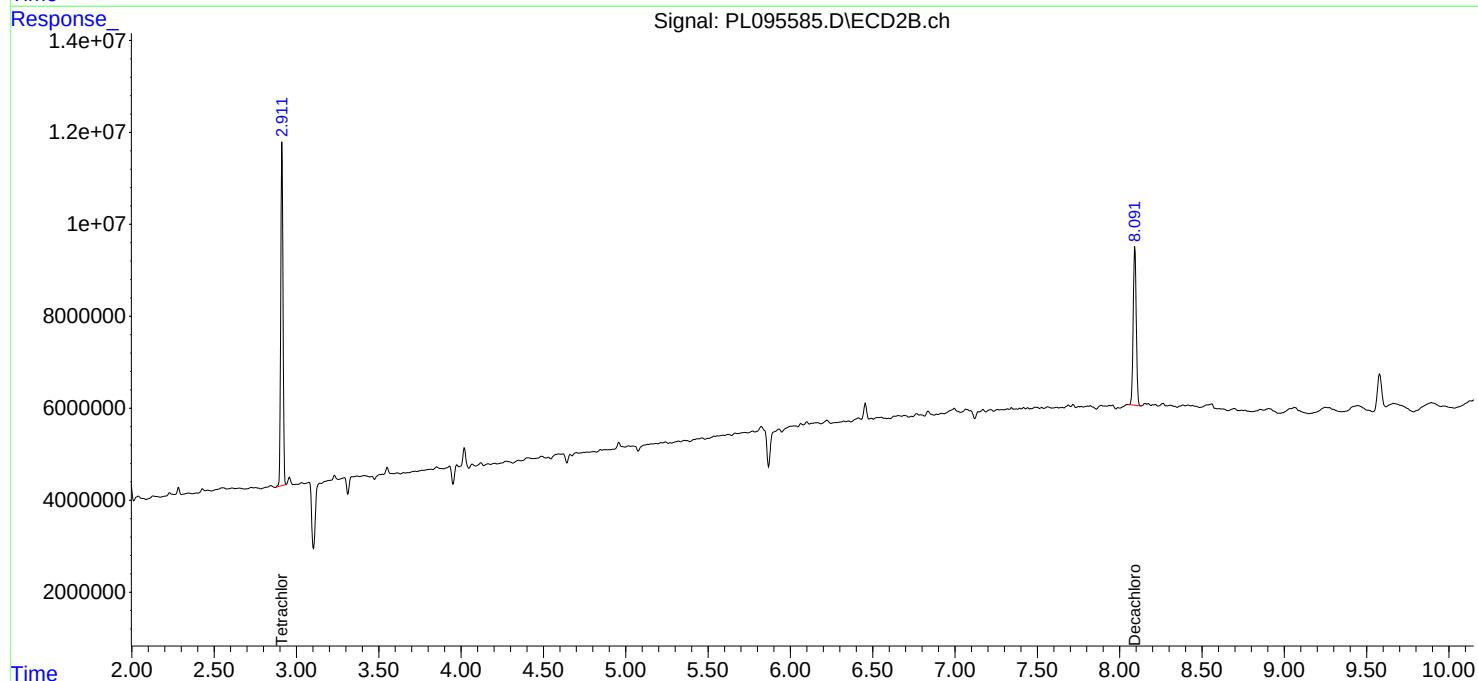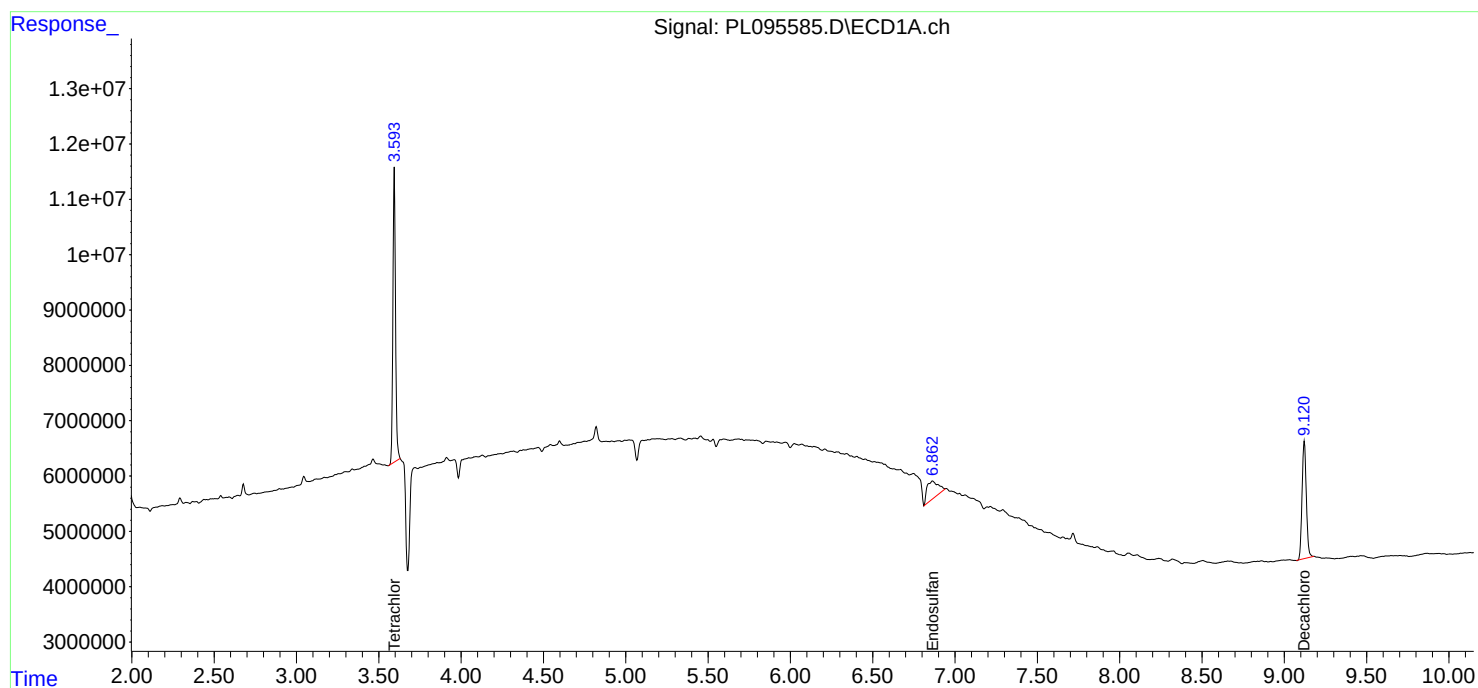


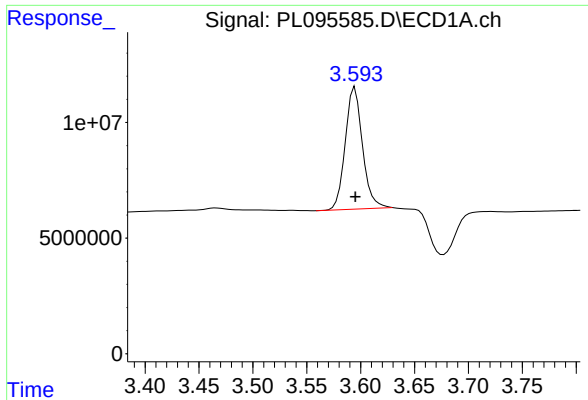

#1 Tetrachloro-m-xylene


R.T.: 3.595 min
Delta R.T.: 0.000 min
Response: 58952718
Conc: 18.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
SUB-WC

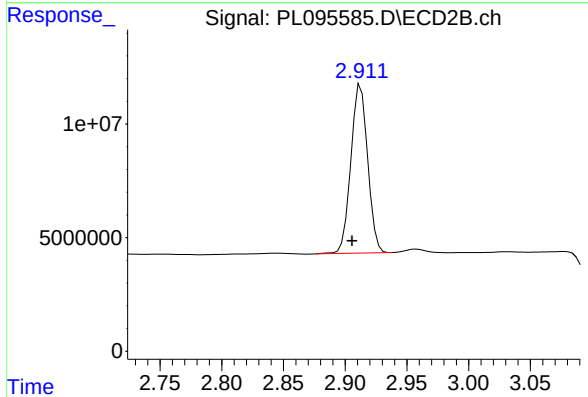


#1 Tetrachloro-m-xylene

R.T.: 2.913 min
Delta R.T.: 0.007 min
Response: 70352440
Conc: 22.13 ng/ml

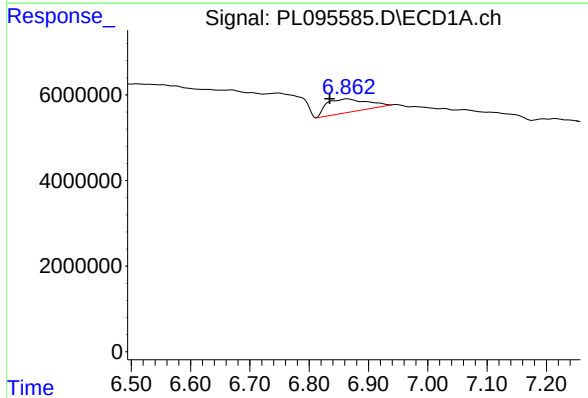


#15 Endosulfan II

R.T.: 6.864 min
Delta R.T.: 0.029 min
Response: 15032803
Conc: 4.71 ng/ml

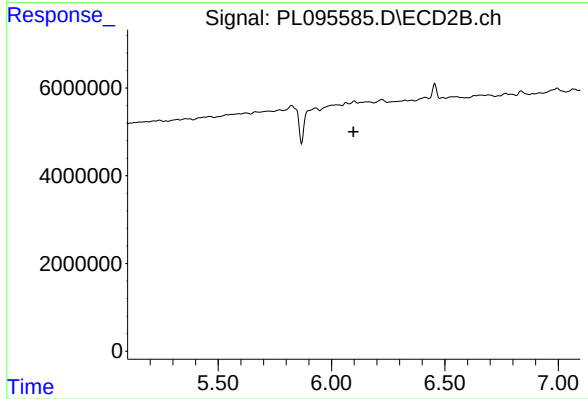

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.097 min
Response: 0
Conc: N.D.

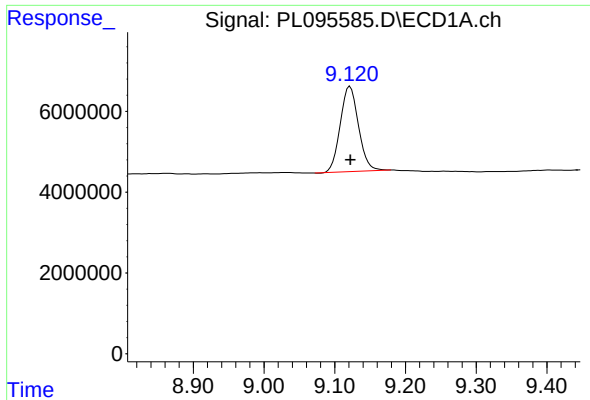

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: 0.000 min
Response: 37946617
Conc: 13.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
SUB-WC

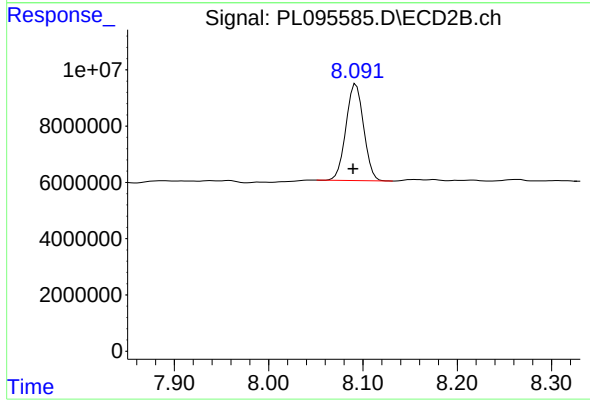

#28 Decachlorobiphenyl

R.T.: 8.093 min
Delta R.T.: 0.003 min
Response: 44787214
Conc: 15.13 ng/ml