

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050825\
 Data File : PL095588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2025 15:41
 Operator : AR\AJ
 Sample : Q1972-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-B-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 02:06:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.594	2.912	45718898	68330889	14.004	21.489 #
28)	SA Decachlor...	9.119	8.090	27348975	35209333	9.870	11.898
Target Compounds							
6)	B beta-BHC	0.000	4.019f	0	6101751	N.D.	2.939 #
9)	A Endosulfan I	6.143f	5.288f	37822877	25845950	9.960	7.061 #
10)	B gamma-Chl...	6.009f	0.000	37370663	0	9.161	N.D. #
11)	B alpha-Chl...	6.075	0.000	31155576	0	7.662	N.D. #
13)	MA Dieldrin	0.000	5.533	0	17369574	N.D.	4.271 #
15)	B Endosulfa...	6.856f	6.101	5555180	12914418	1.740	3.596 #
25)	Chlordane-3	6.009	0.000	37370663	0	47.977	N.D. #
26)	Chlordane-4	6.075	0.000	31155576	0	33.041	N.D. #
27)	Chlordane-5	0.000	6.101	0	12914418	N.D.	69.906 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050825\
Data File : PL095588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2025 15:41
Operator : AR\AJ
Sample : Q1972-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-B-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 02:06:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

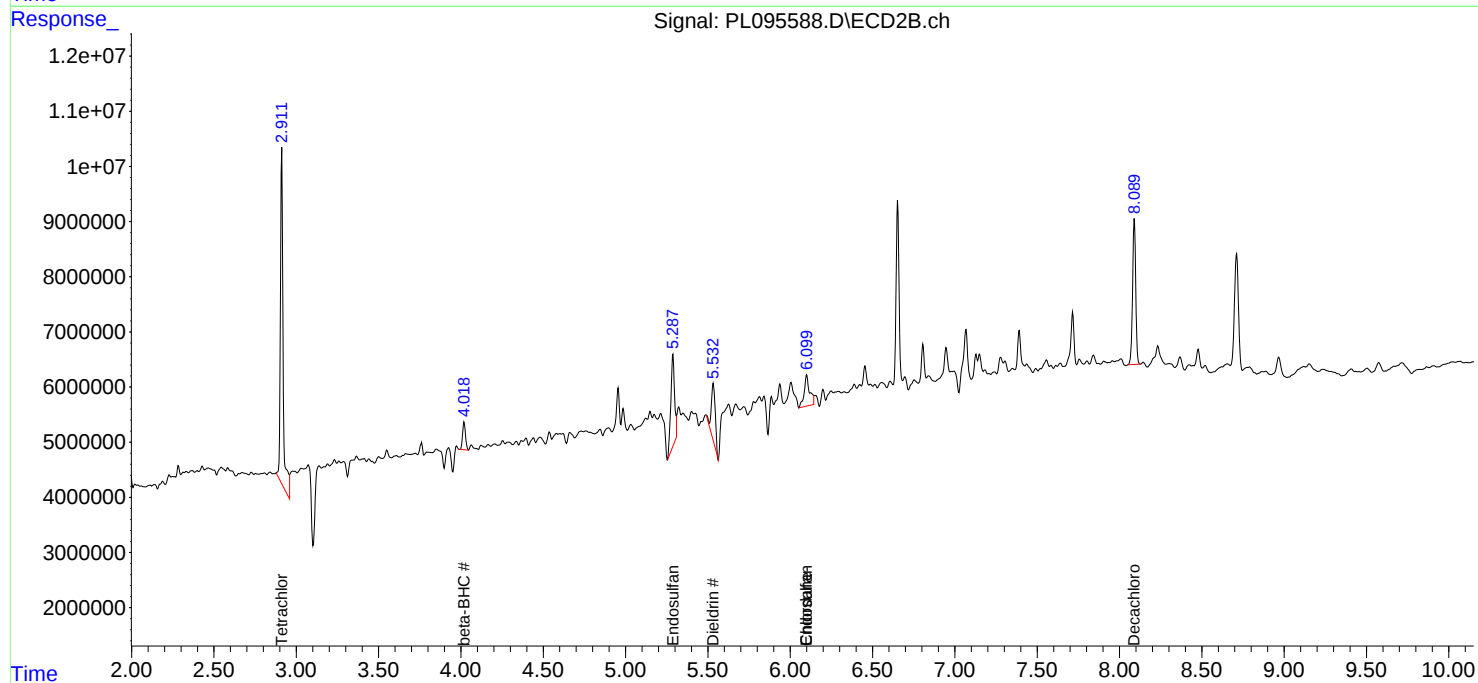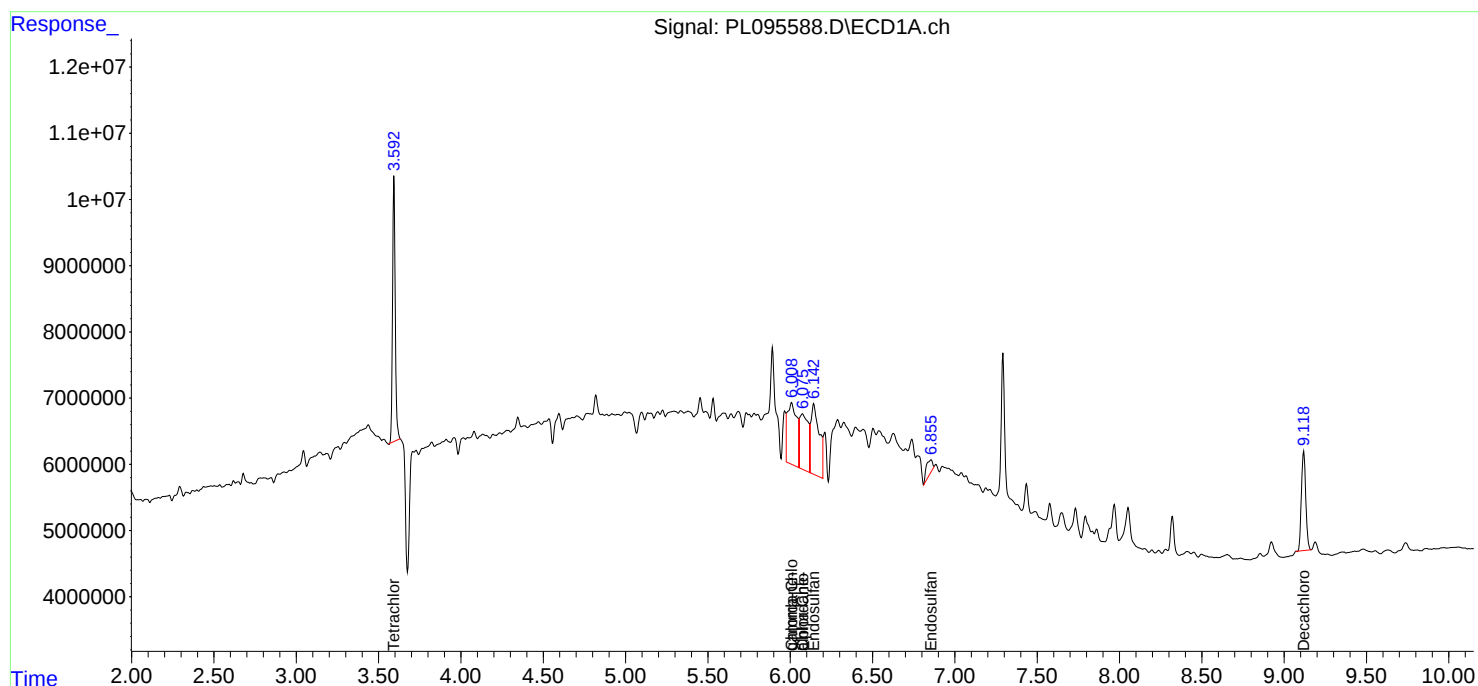


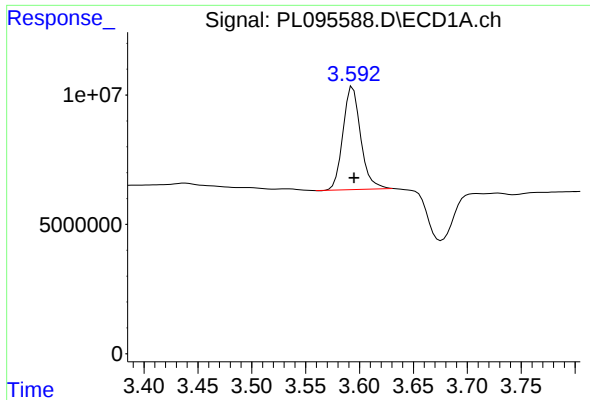

#1 Tetrachloro-m-xylene


R.T.: 3.594 min
Delta R.T.: -0.001 min
Response: 45718898
Conc: 14.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-B-7

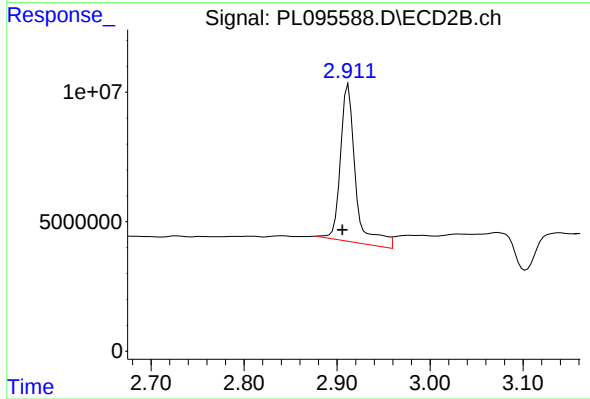


#1 Tetrachloro-m-xylene

R.T.: 2.912 min
Delta R.T.: 0.007 min
Response: 68330889
Conc: 21.49 ng/ml

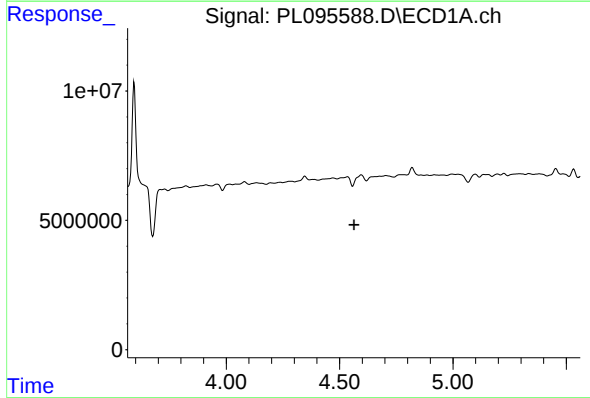


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.564 min
Response: 0
Conc: N.D.

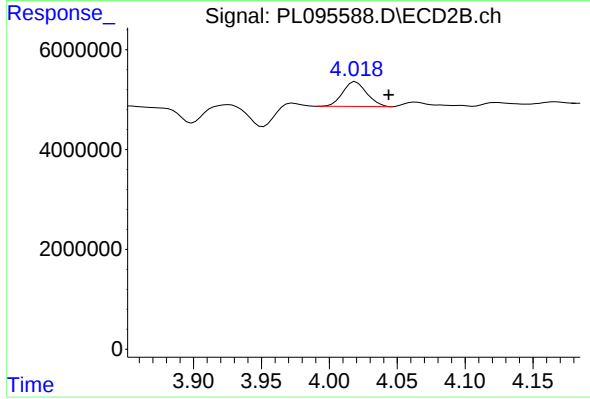

#6 beta-BHC


R.T.: 4.019 min
Delta R.T.: -0.024 min
Response: 6101751
Conc: 2.94 ng/ml

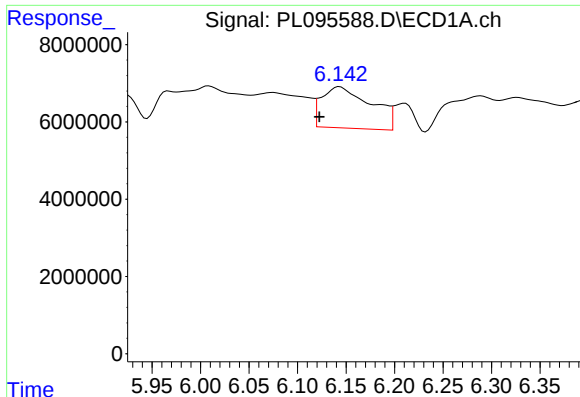

#9 Endosulfan I


R.T.: 6.143 min
Delta R.T.: 0.021 min
Response: 37822877
Conc: 9.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-B-7

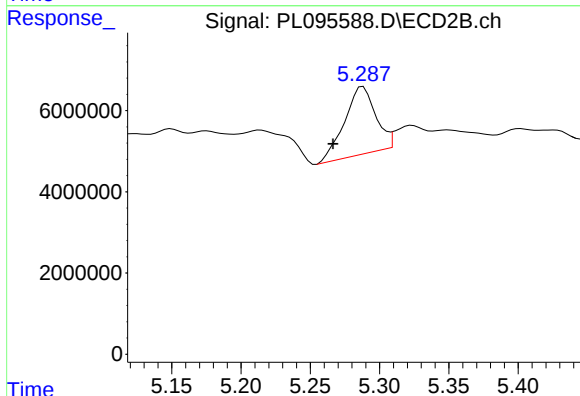


#9 Endosulfan I

R.T.: 5.288 min
Delta R.T.: 0.022 min
Response: 25845950
Conc: 7.06 ng/ml

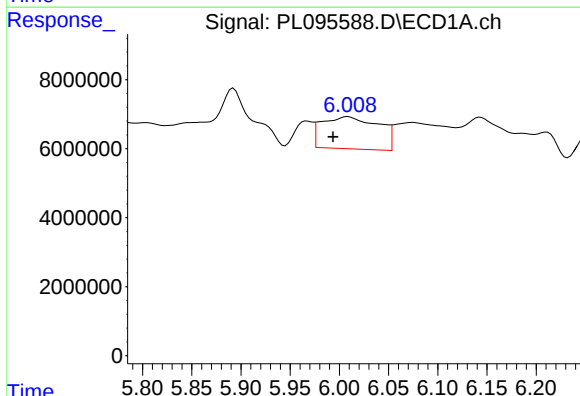


#10 gamma-Chlordane

R.T.: 6.009 min
Delta R.T.: 0.015 min
Response: 37370663
Conc: 9.16 ng/ml

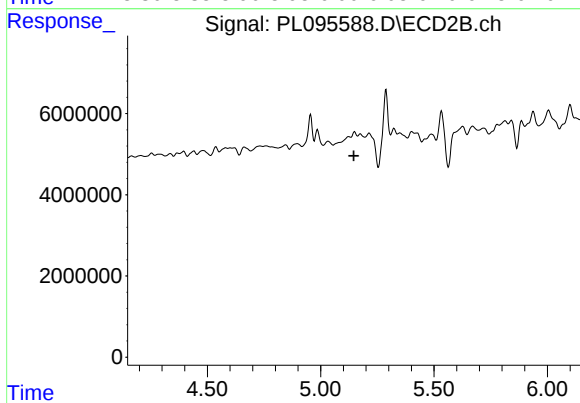

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.147 min
Response: 0
Conc: N.D.

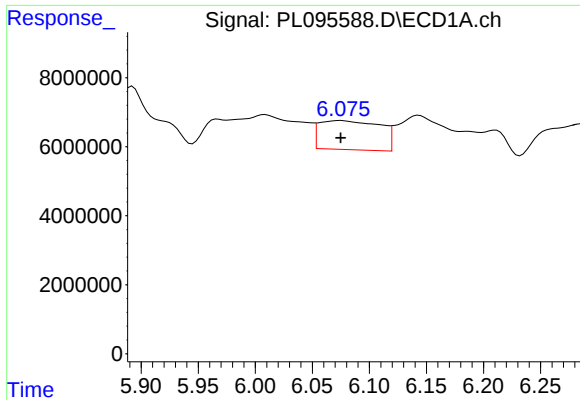

#11 alpha-Chlordane


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 31155576
Conc: 7.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-B-7

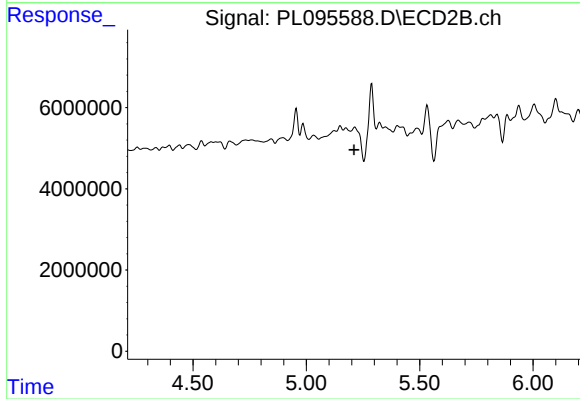


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.211 min
Response: 0
Conc: N.D.

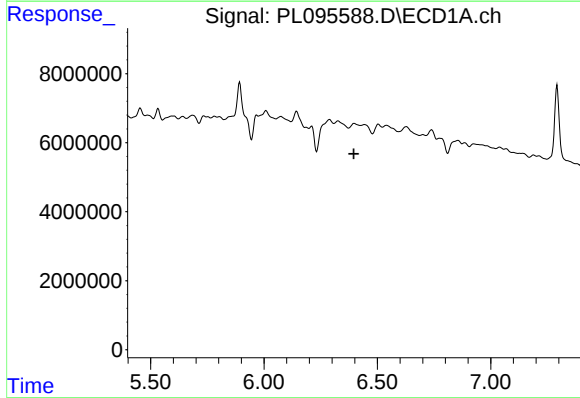


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

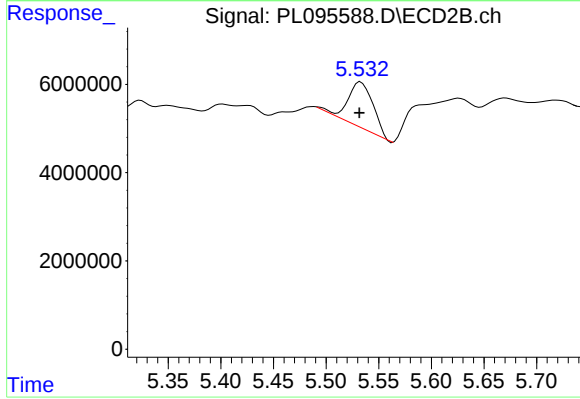

#13 Dieldrin


R.T.: 5.533 min
Delta R.T.: 0.001 min
Response: 17369574
Conc: 4.27 ng/ml

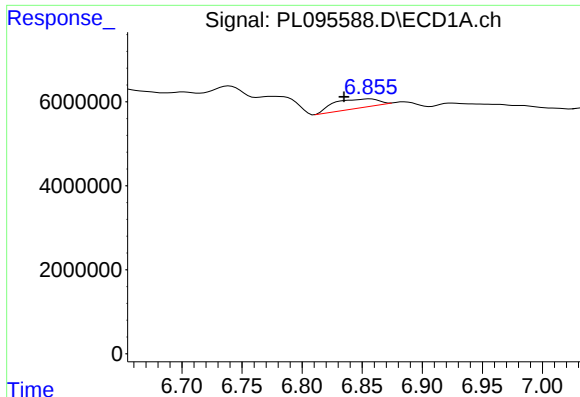

#15 Endosulfan II


R.T.: 6.856 min
Delta R.T.: 0.022 min
Response: 5555180
Conc: 1.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-B-7

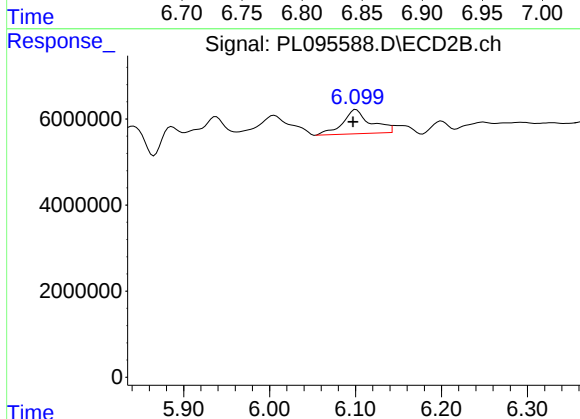


#15 Endosulfan II

R.T.: 6.101 min
Delta R.T.: 0.003 min
Response: 12914418
Conc: 3.60 ng/ml

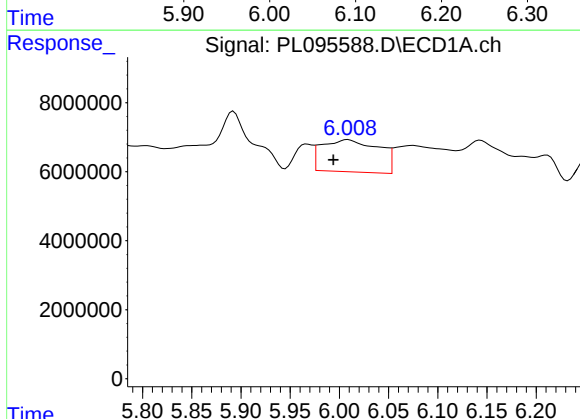


#25 Chlordane-3

R.T.: 6.009 min
Delta R.T.: 0.015 min
Response: 37370663
Conc: 47.98 ng/ml

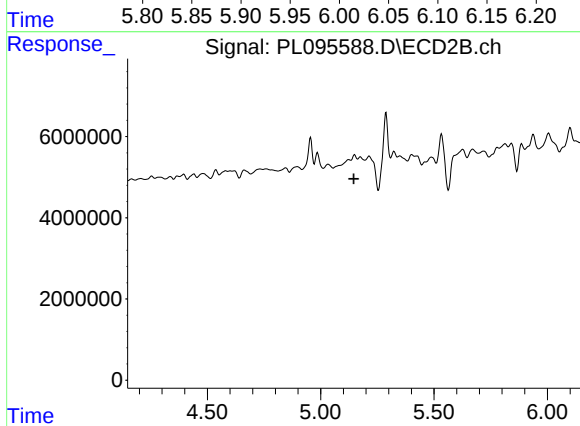

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.147 min
Response: 0
Conc: N.D.

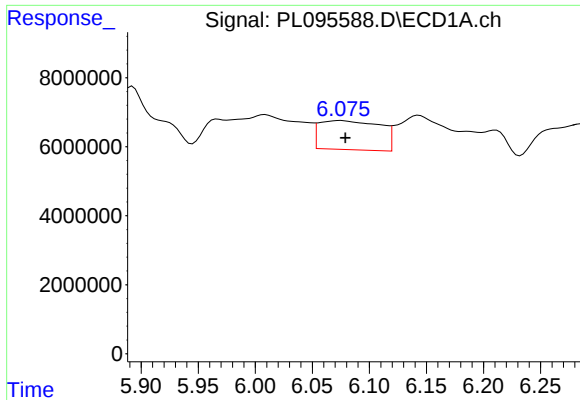

#26 Chlordane-4


R.T.: 6.075 min
Delta R.T.: -0.004 min
Response: 31155576
Conc: 33.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-B-7

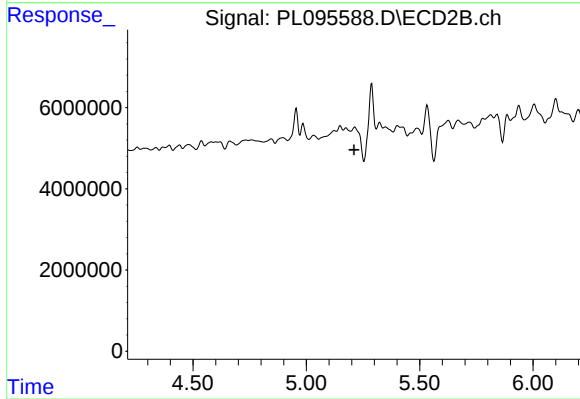


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.211 min
Response: 0
Conc: N.D.

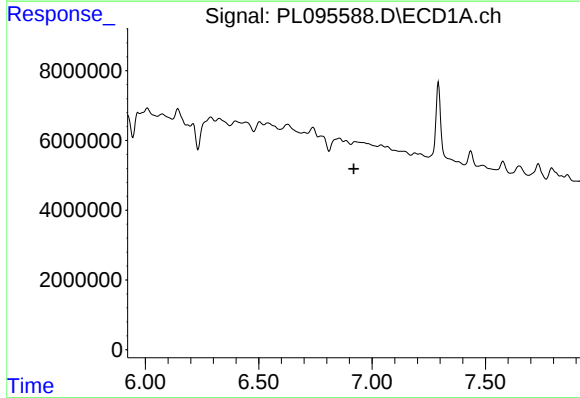


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.919 min
Response: 0
Conc: N.D.

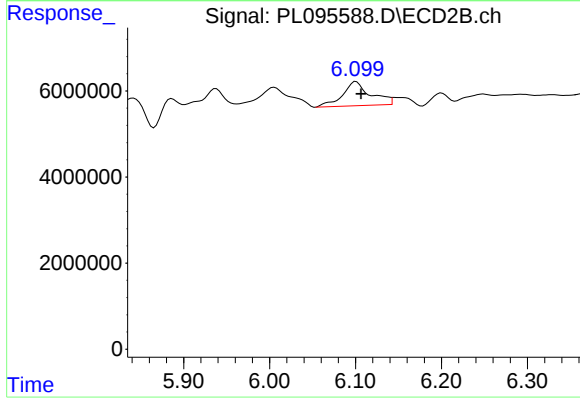

#27 Chlordane-5


R.T.: 6.101 min
Delta R.T.: -0.006 min
Response: 12914418
Conc: 69.91 ng/ml

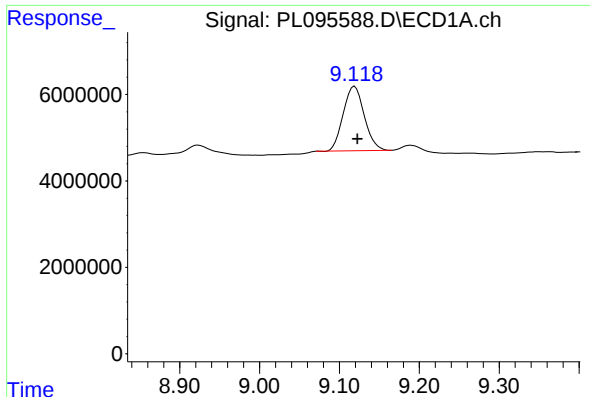

#28 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: -0.003 min
Response: 27348975
Conc: 9.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-B-7

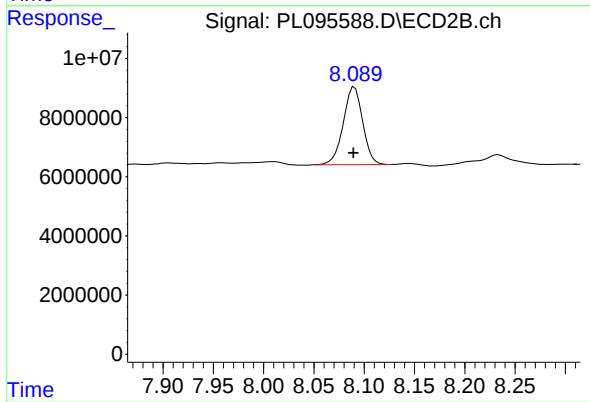

#28 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 35209333
Conc: 11.90 ng/ml