

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
 Data File : PL048305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2019 10:57
 Operator : AJ\SJ
 Sample : INDA201
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA201

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 11:50:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 09 11:49:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.939	105.6E6	26664628	10.135	10.152
27)	SA Decachlor...	7.995	8.975	225.8E6	57650207	21.338	20.910
Target Compounds							
2)	A alpha-BHC	3.756	4.328	159.7E6	34988365	9.799	9.769
3)	MA gamma-BHC...	4.032	4.611	143.6E6	33407723	9.655	9.843
4)	MA Heptachlor	4.316	5.115	158.5E6	36401567	9.936	10.054
9)	A Endosulfan I	5.322	6.160	129.5E6	30451261	9.793	10.224
13)	MA Dieldrin	5.562	6.416	285.7E6	61847405	19.489	19.566
14)	MA Endrin	5.814	6.633	250.2E6	51651661	19.707	19.511
16)	A 4,4'-DDD	5.949	6.759	215.3E6	48036671	19.591	19.602
17)	MA 4,4'-DDT	6.183	7.056	211.1E6	48404276	18.703	19.390
20)	A Methoxychlor	6.728	7.516	579.7E6	140.4E6	102.350	101.661


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
Data File : PL048305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2019 10:57
Operator : AJ\SJ
Sample : INDA201
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 11:50:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 09 11:49:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

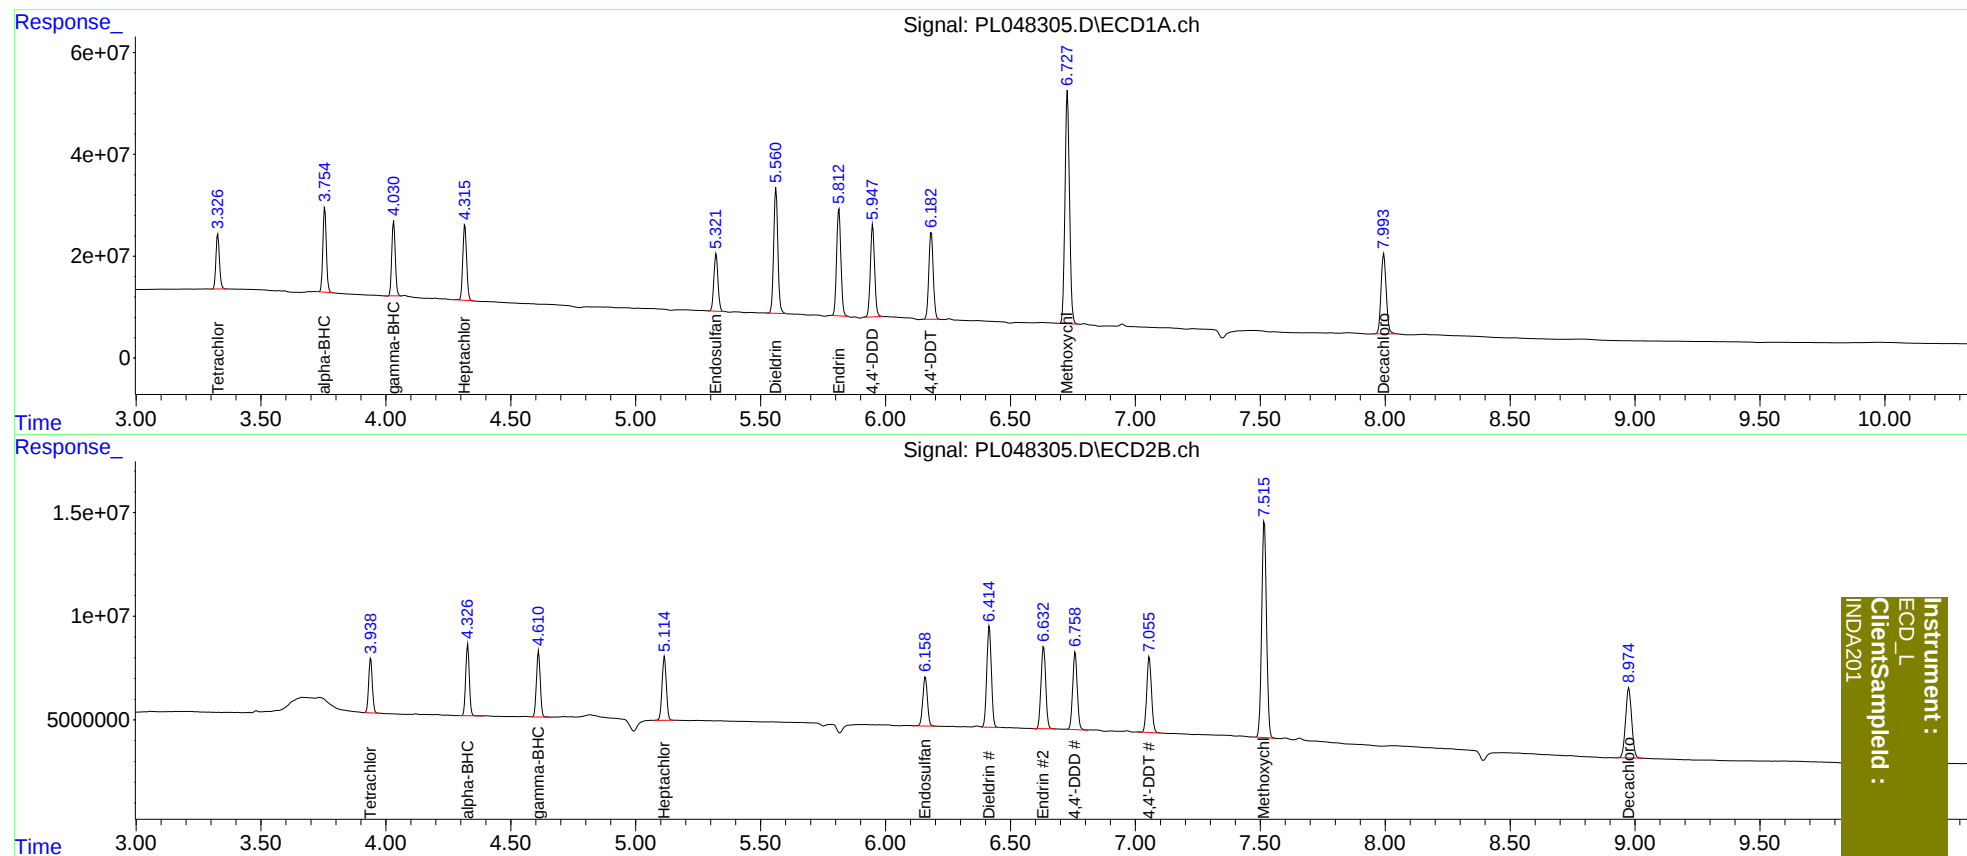


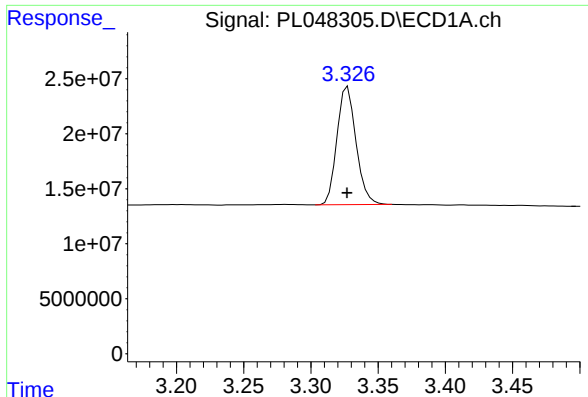

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 105577485
Conc: 10.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

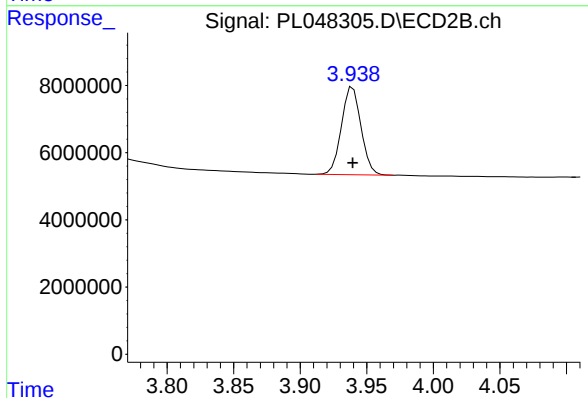


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 26664628
Conc: 10.15 ng/ml

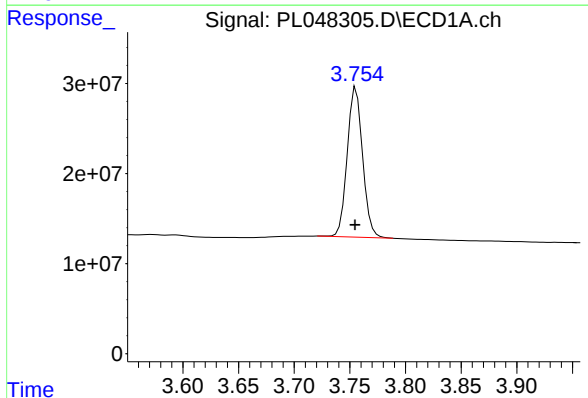


#2 alpha-BHC

R.T.: 3.756 min
Delta R.T.: 0.000 min
Response: 159740292
Conc: 9.80 ng/ml

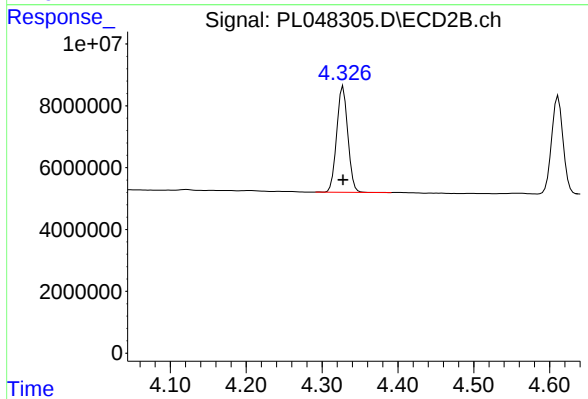

#2 alpha-BHC


R.T.: 4.328 min
Delta R.T.: 0.000 min
Response: 34988365
Conc: 9.77 ng/ml

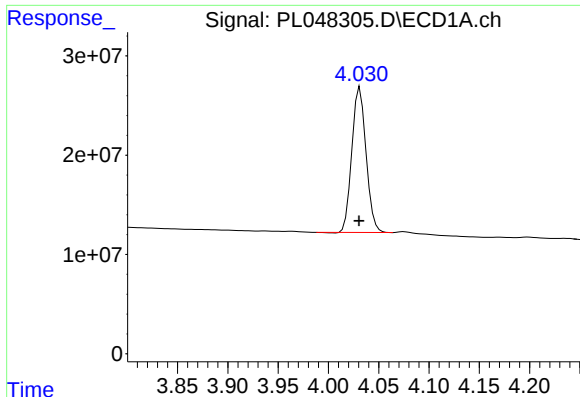

#3 gamma-BHC (Lindane)


R.T.: 4.032 min
Delta R.T.: 0.001 min
Response: 143636289
Conc: 9.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

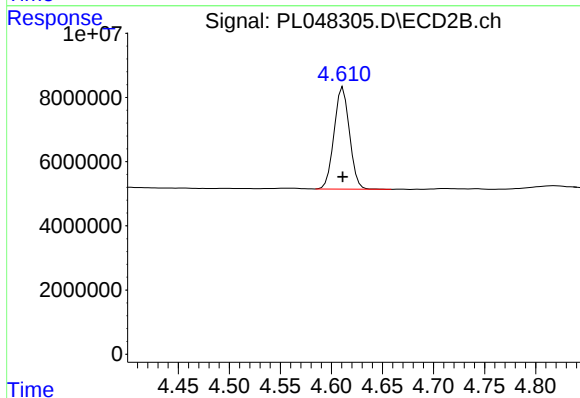


#3 gamma-BHC (Lindane)

R.T.: 4.611 min
Delta R.T.: 0.000 min
Response: 33407723
Conc: 9.84 ng/ml

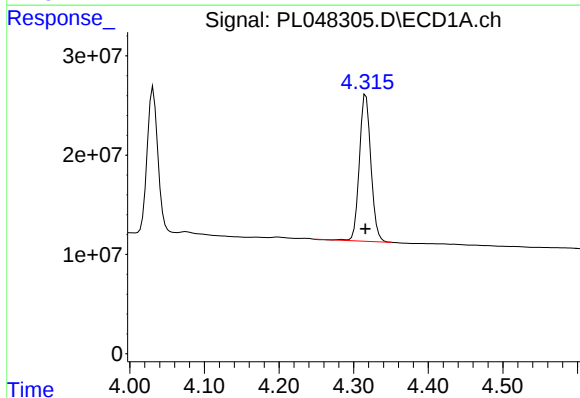


#4 Heptachlor

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 158534493
Conc: 9.94 ng/ml

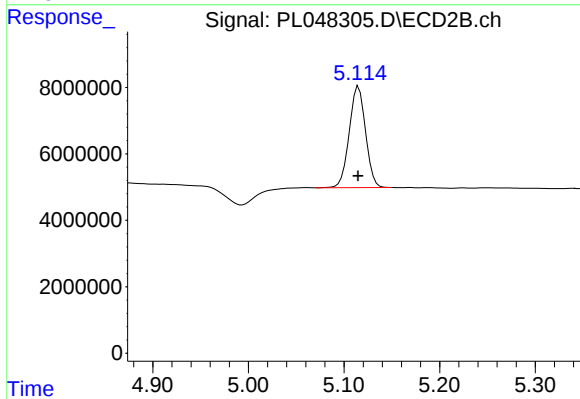

#4 Heptachlor


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 36401567
Conc: 10.05 ng/ml

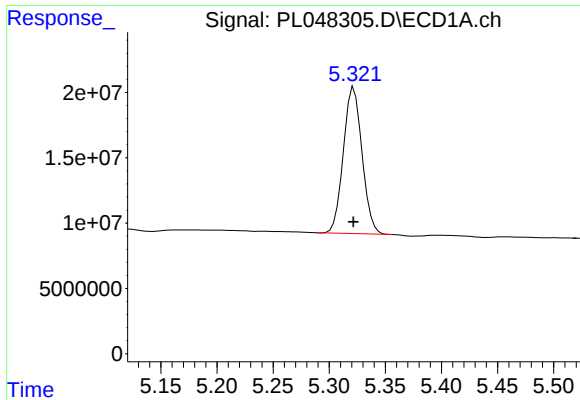

#9 Endosulfan I


R.T.: 5.322 min
Delta R.T.: 0.000 min
Response: 129466677
Conc: 9.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

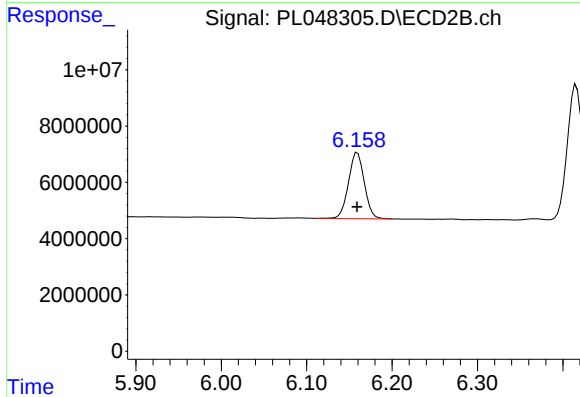


#9 Endosulfan I

R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 30451261
Conc: 10.22 ng/ml

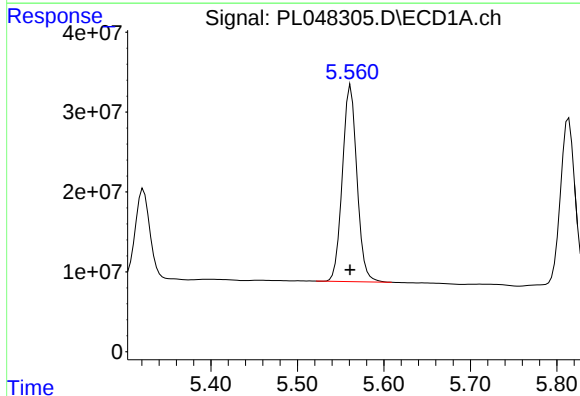


#13 Dieldrin

R.T.: 5.562 min
Delta R.T.: 0.000 min
Response: 285657151
Conc: 19.49 ng/ml

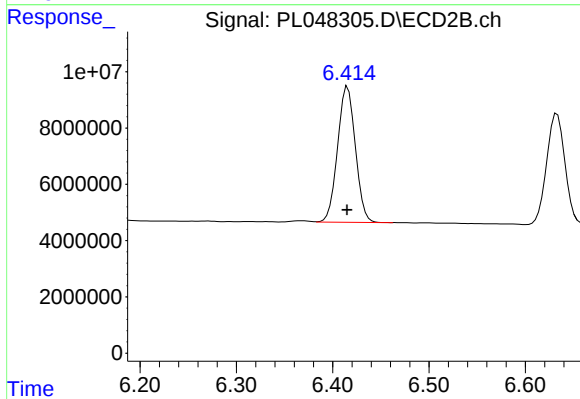

#13 Dieldrin


R.T.: 6.416 min
Delta R.T.: 0.000 min
Response: 61847405
Conc: 19.57 ng/ml

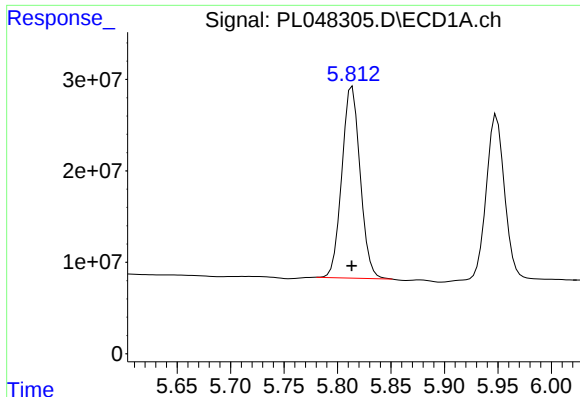

#14 Endrin


R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 250194191
Conc: 19.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

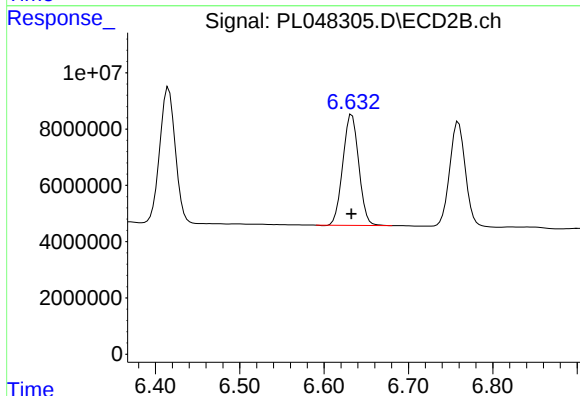


#14 Endrin

R.T.: 6.633 min
Delta R.T.: 0.000 min
Response: 51651661
Conc: 19.51 ng/ml

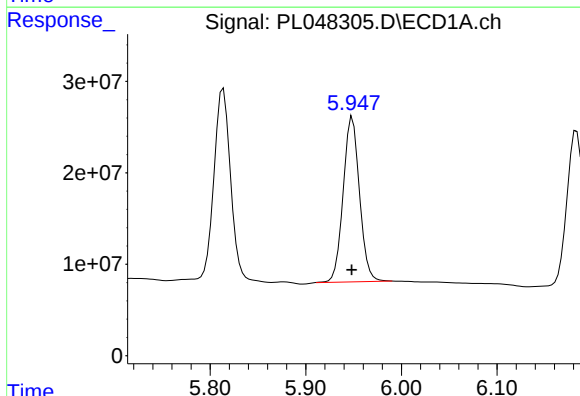


#16 4,4'-DDD

R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 215256975
Conc: 19.59 ng/ml

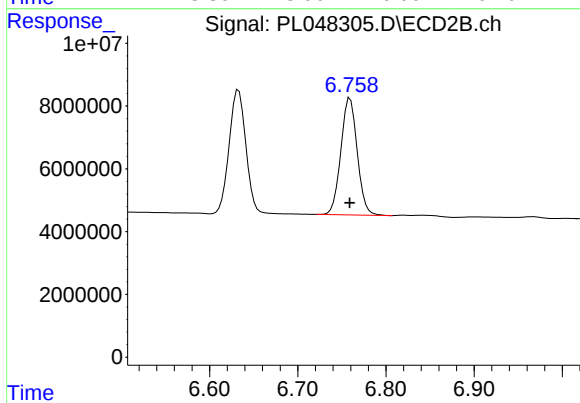

#16 4,4'-DDD


R.T.: 6.759 min
Delta R.T.: 0.000 min
Response: 48036671
Conc: 19.60 ng/ml

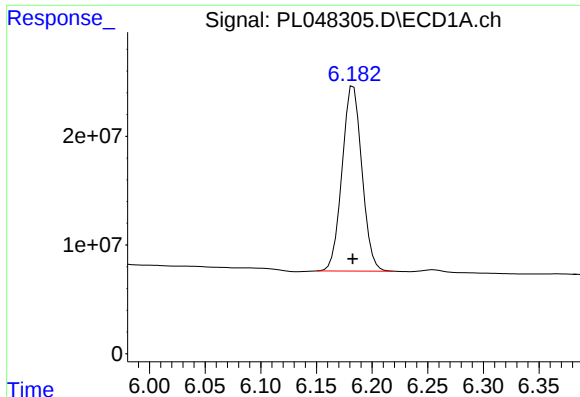

#17 4,4'-DDT


R.T.: 6.183 min
Delta R.T.: 0.000 min
Response: 211096236
Conc: 18.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

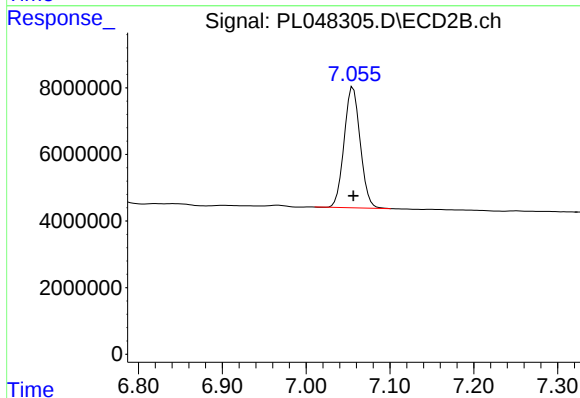


#17 4,4'-DDT

R.T.: 7.056 min
Delta R.T.: 0.000 min
Response: 48404276
Conc: 19.39 ng/ml

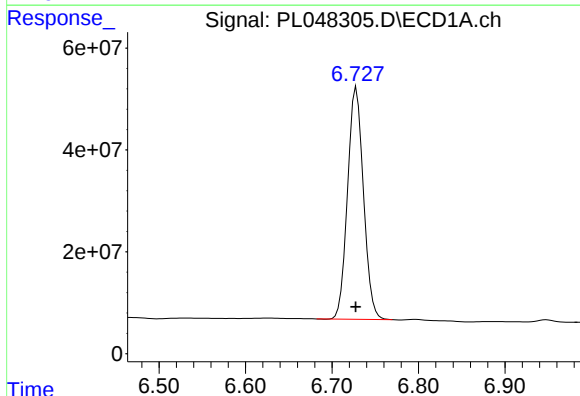


#20 Methoxychlor

R.T.: 6.728 min
Delta R.T.: 0.000 min
Response: 579652250
Conc: 102.35 ng/ml

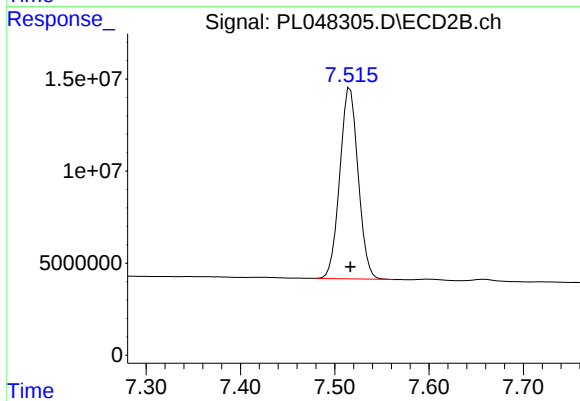

#20 Methoxychlor

R.T.: 7.516 min
Delta R.T.: 0.000 min
Response: 140354554
Conc: 101.66 ng/ml

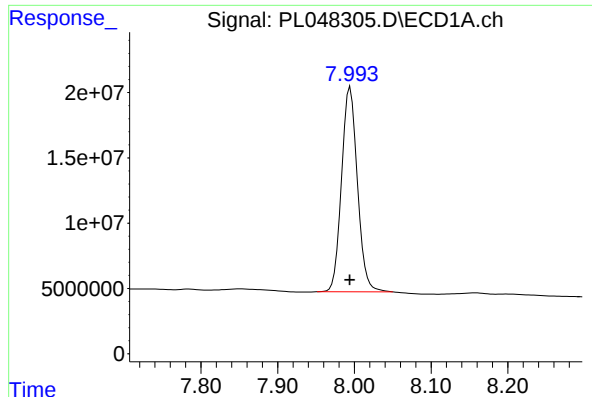

#27 Decachlorobiphenyl


R.T.: 7.995 min

Delta R.T.: 0.000 min

Response: 225823758

Conc: 21.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA201

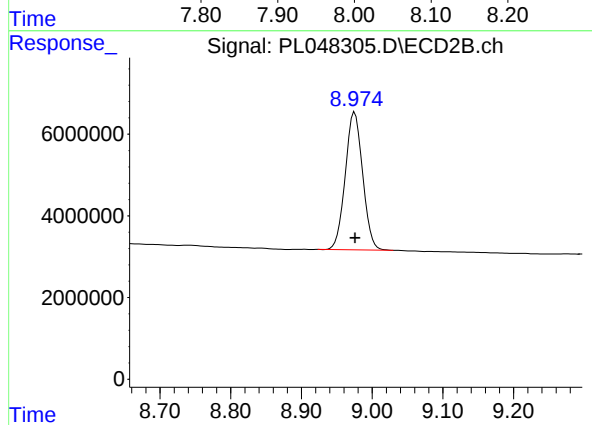

#27 Decachlorobiphenyl

R.T.: 8.975 min

Delta R.T.: 0.000 min

Response: 57650207

Conc: 20.91 ng/ml