

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
 Data File : PL048309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2019 11:57
 Operator : AJ\SJ
 Sample : INDA401
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 12:17:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 09 11:52:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.939	420.2E6	107.2E6	40.356	40.654
27)	SA Decachlor...	7.995	8.975	829.6E6	213.4E6	75.383	75.811
Target Compounds							
2)	A alpha-BHC	3.755	4.327	676.0E6	152.5E6	43.168	43.588
3)	MA gamma-BHC...	4.031	4.611	619.4E6	142.2E6	43.067	42.718
4)	MA Heptachlor	4.316	5.114	648.5E6	147.4E6	41.960	40.638
9)	A Endosulfan I	5.321	6.158	531.5E6	119.4E6	40.327	37.008
13)	MA Dieldrin	5.560	6.415	1186.3E6	260.1E6	84.146	84.236
14)	MA Endrin	5.813	6.632	1020.4E6	216.2E6	81.973	83.794
16)	A 4,4'-DDD	5.947	6.758	893.4E6	200.1E6	84.642	83.216
17)	MA 4,4'-DDT	6.182	7.056	942.1E6	205.3E6	88.197	83.333
20)	A Methoxychlor	6.727	7.515	2191.1E6	542.6E6	386.632	390.734


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
Data File : PL048309.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2019 11:57
Operator : AJ\SJ
Sample : INDA401
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 12:17:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 09 11:52:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

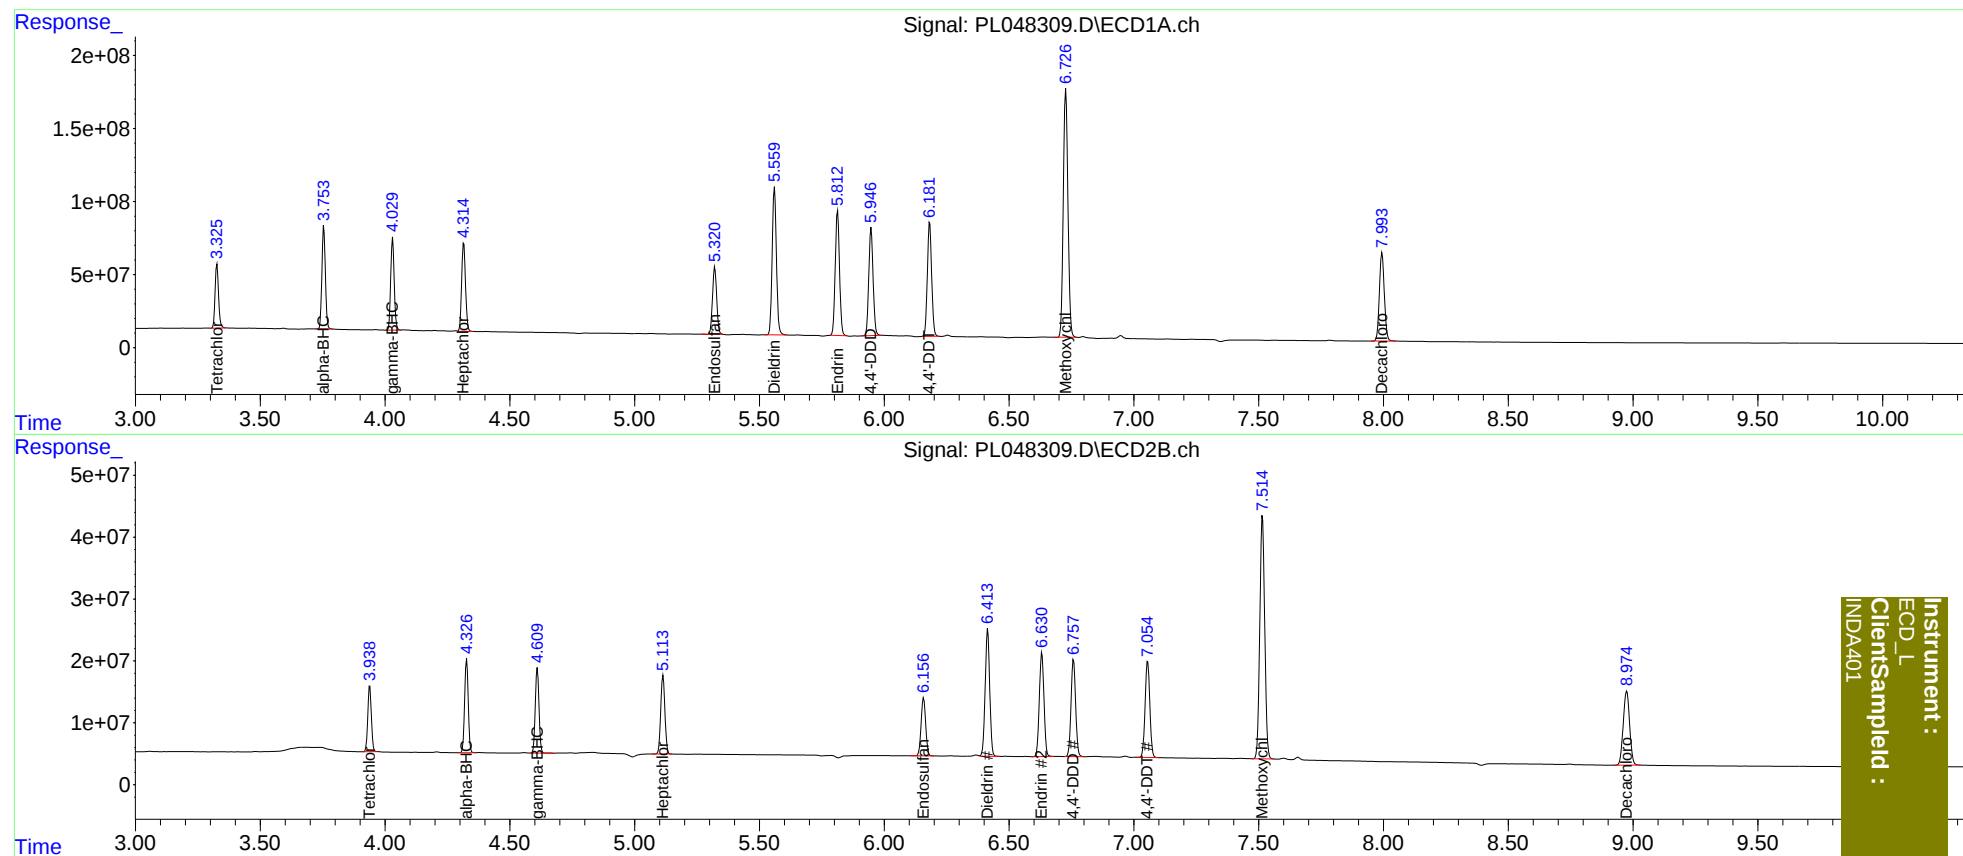


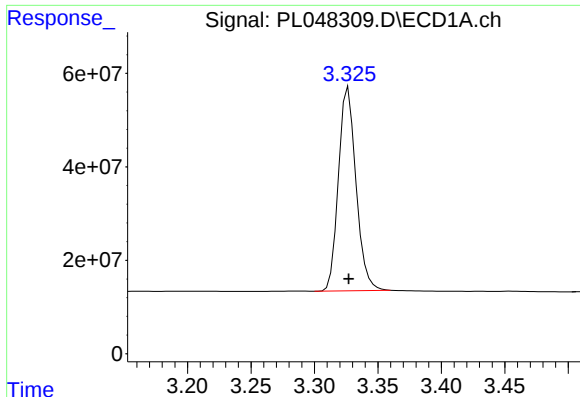

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 420155199
Conc: 40.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

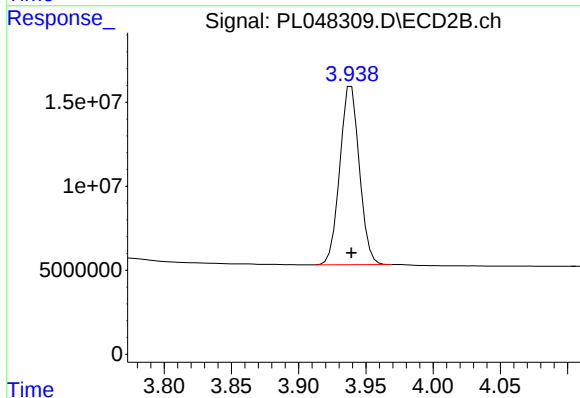


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 107161626
Conc: 40.65 ng/ml

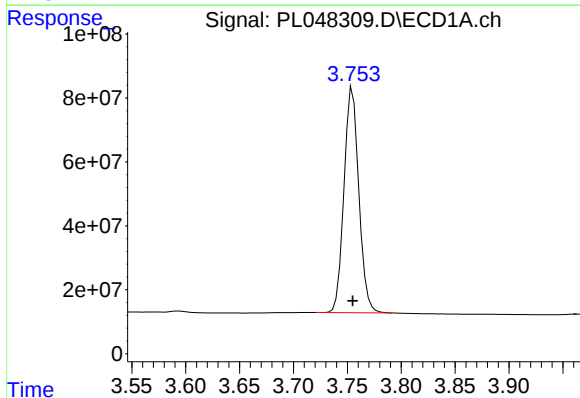


#2 alpha-BHC

R.T.: 3.755 min
Delta R.T.: 0.000 min
Response: 675958830
Conc: 43.17 ng/ml

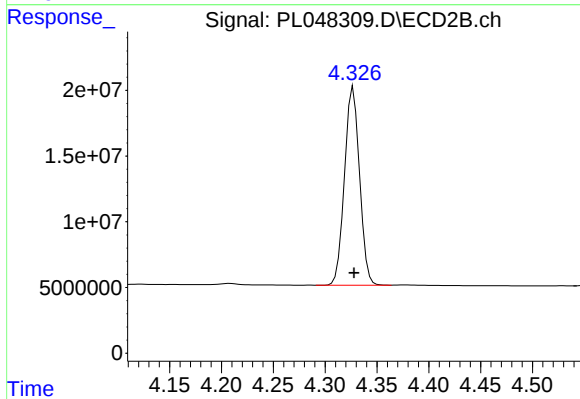

#2 alpha-BHC


R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 152499385
Conc: 43.59 ng/ml

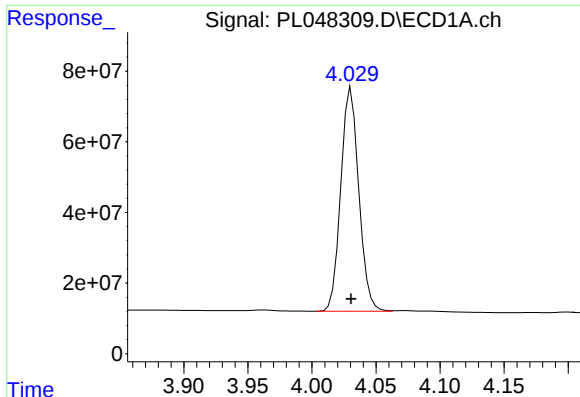

#3 gamma-BHC (Lindane)


R.T.: 4.031 min
Delta R.T.: 0.000 min
Response: 619412987
Conc: 43.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

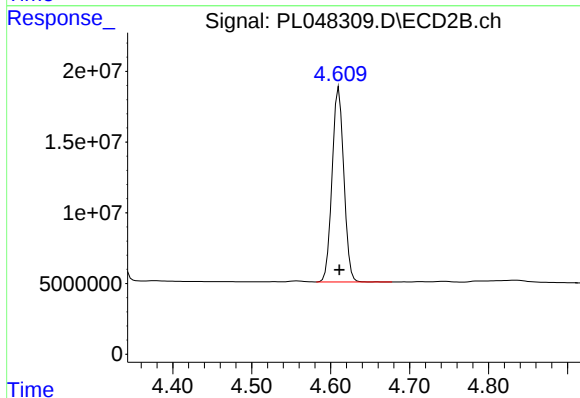


#3 gamma-BHC (Lindane)

R.T.: 4.611 min
Delta R.T.: 0.000 min
Response: 142248218
Conc: 42.72 ng/ml

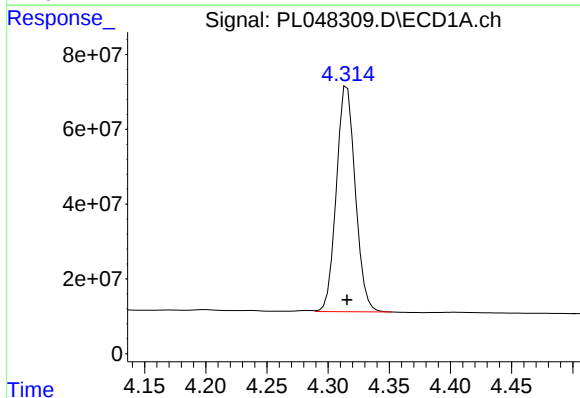


#4 Heptachlor

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 648510430
Conc: 41.96 ng/ml

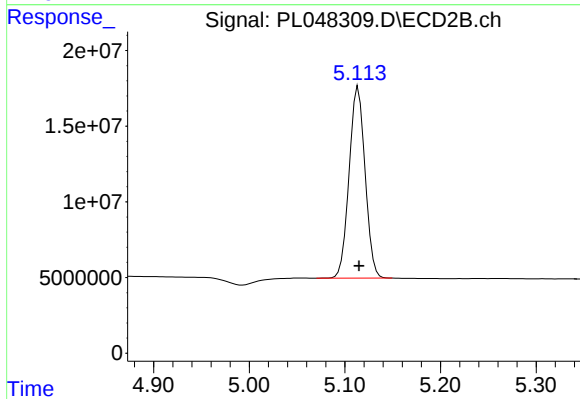

#4 Heptachlor


R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 147395913
Conc: 40.64 ng/ml

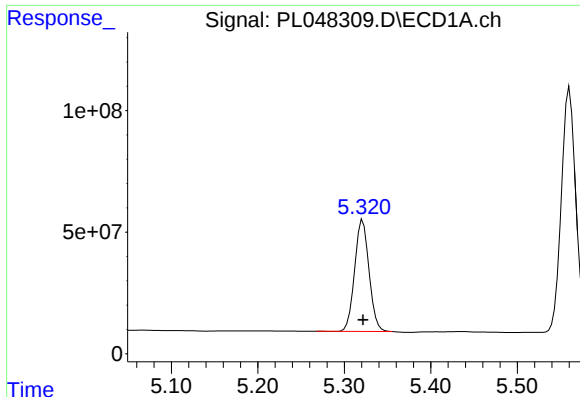

#9 Endosulfan I


R.T.: 5.321 min
Delta R.T.: 0.000 min
Response: 531453905
Conc: 40.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

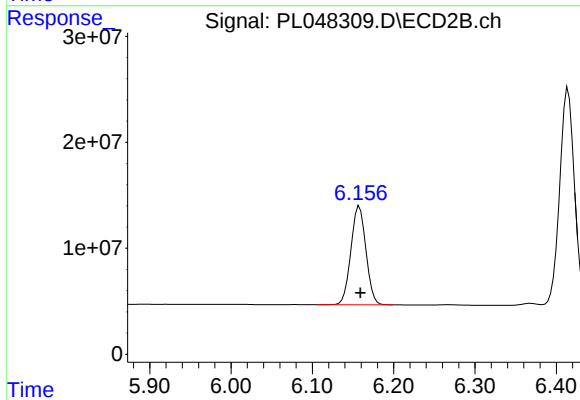


#9 Endosulfan I

R.T.: 6.158 min
Delta R.T.: 0.000 min
Response: 119356985
Conc: 37.01 ng/ml

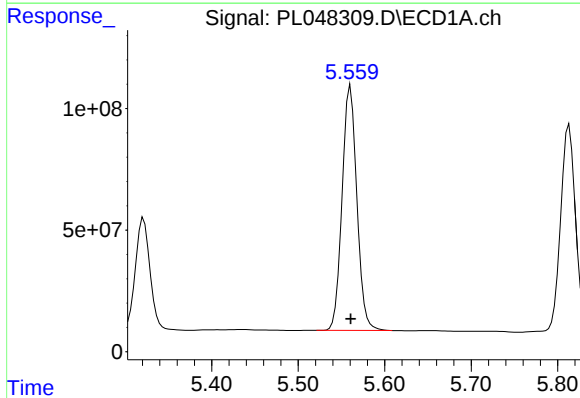


#13 Dieldrin

R.T.: 5.560 min
Delta R.T.: 0.000 min
Response: 1186295187
Conc: 84.15 ng/ml

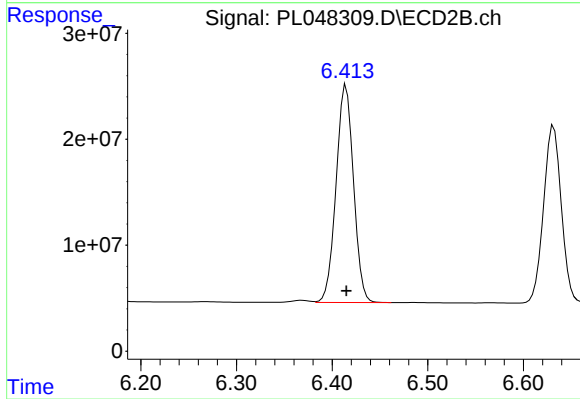

#13 Dieldrin


R.T.: 6.415 min
Delta R.T.: 0.000 min
Response: 260084299
Conc: 84.24 ng/ml

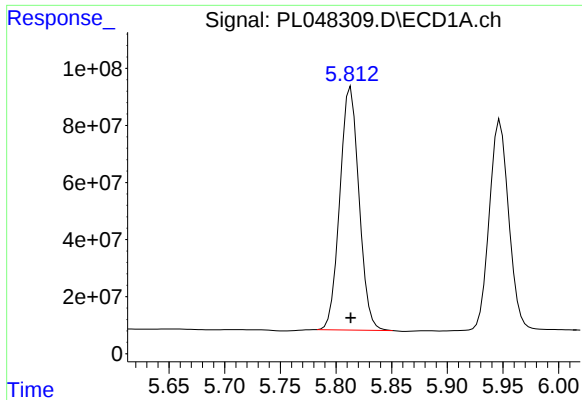

#14 Endrin


R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 1020358592
Conc: 81.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

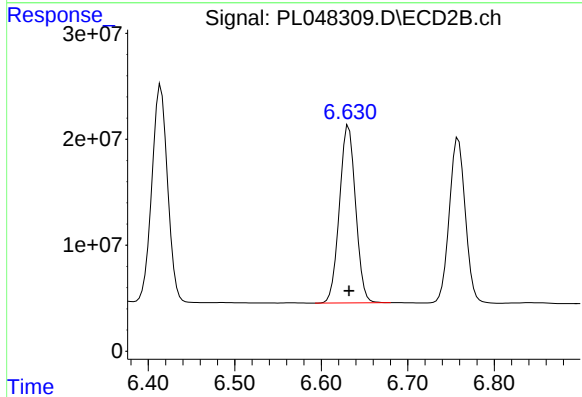


#14 Endrin

R.T.: 6.632 min
Delta R.T.: 0.000 min
Response: 216231132
Conc: 83.79 ng/ml

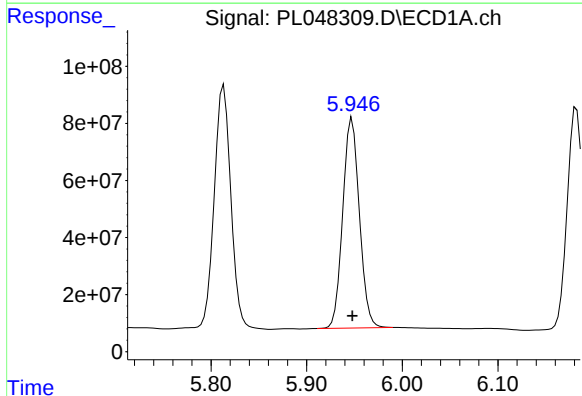


#16 4,4'-DDD

R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 893355183
Conc: 84.64 ng/ml

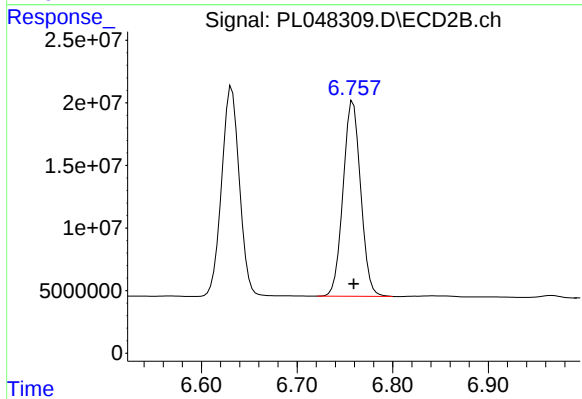

#16 4,4'-DDD


R.T.: 6.758 min
Delta R.T.: 0.000 min
Response: 200116454
Conc: 83.22 ng/ml

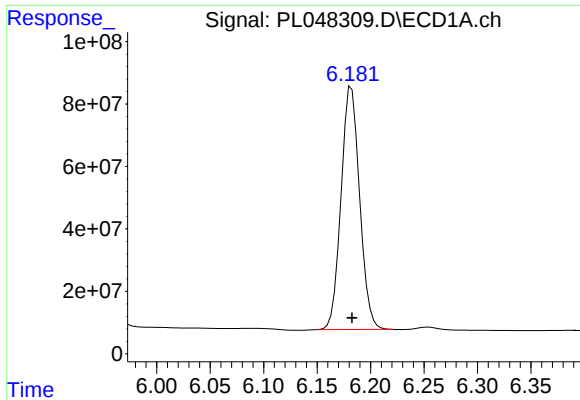

#17 4,4'-DDT


R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 942062008
Conc: 88.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

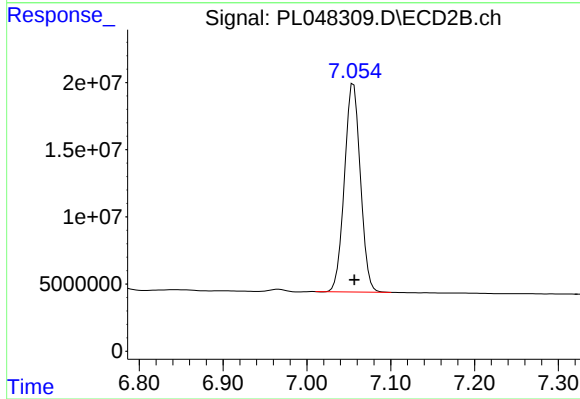


#17 4,4'-DDT

R.T.: 7.056 min
Delta R.T.: 0.000 min
Response: 205293468
Conc: 83.33 ng/ml

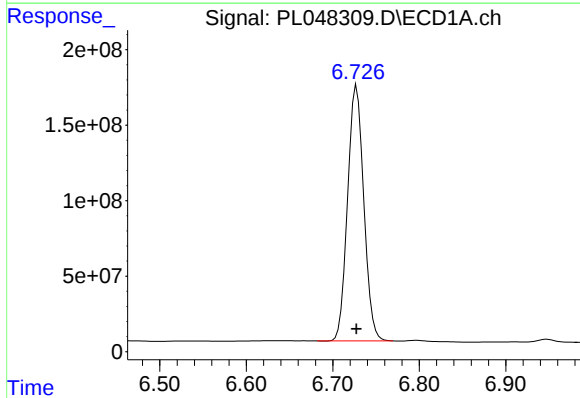


#20 Methoxychlor

R.T.: 6.727 min
Delta R.T.: 0.000 min
Response: 2191099140
Conc: 386.63 ng/ml

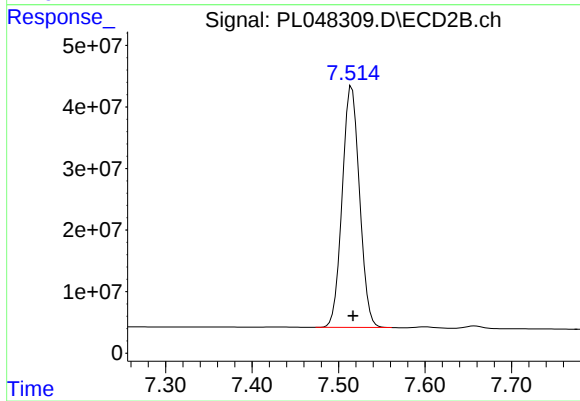

#20 Methoxychlor


R.T.: 7.515 min
Delta R.T.: -0.001 min
Response: 542641160
Conc: 390.73 ng/ml

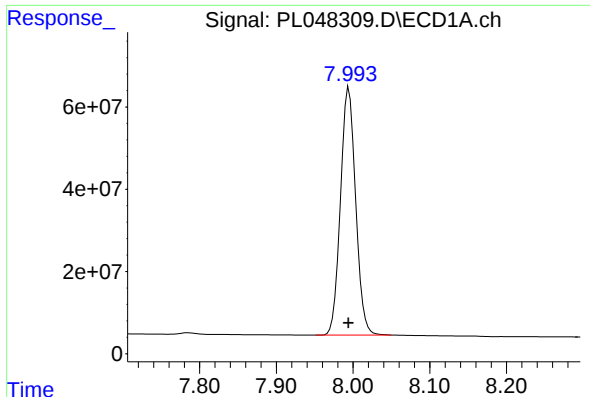

#27 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 829613227
Conc: 75.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA401

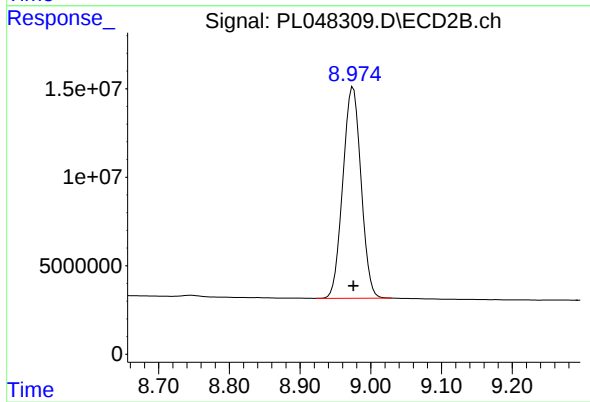

#27 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 213414097
Conc: 75.81 ng/ml