

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
 Data File : PL048311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2019 12:27
 Operator : AJ\SJ
 Sample : INDA501
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 12:52:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 09 12:18:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.939	808.2E6	207.6E6	77.452	78.420
27)	SA Decachlor...	7.994	8.975	1583.2E6	402.9E6	145.961	145.009
Target Compounds							
2)	A alpha-BHC	3.755	4.328	1329.0E6	306.5E6	83.225	85.680
3)	MA gamma-BHC...	4.031	4.611	1221.5E6	284.7E6	83.331	84.072
4)	MA Heptachlor	4.316	5.115	1261.6E6	290.8E6	80.638	79.866
9)	A Endosulfan I	5.322	6.159	1042.6E6	233.9E6	78.954	73.911
13)	MA Dieldrin	5.561	6.416	2299.6E6	518.3E6	161.028	165.663
14)	MA Endrin	5.813	6.633	1969.4E6	432.9E6	157.245	165.810
16)	A 4,4'-DDD	5.948	6.759	1766.1E6	402.3E6	164.938	165.610
17)	MA 4,4'-DDT	6.182	7.057	1901.7E6	418.6E6	173.591	168.150
20)	A Methoxychlor	6.728	7.516	4073.1E6	1043.3E6	724.785	755.646


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
Data File : PL048311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2019 12:27
Operator : AJ\SJ
Sample : INDA501
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 12:52:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 09 12:18:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

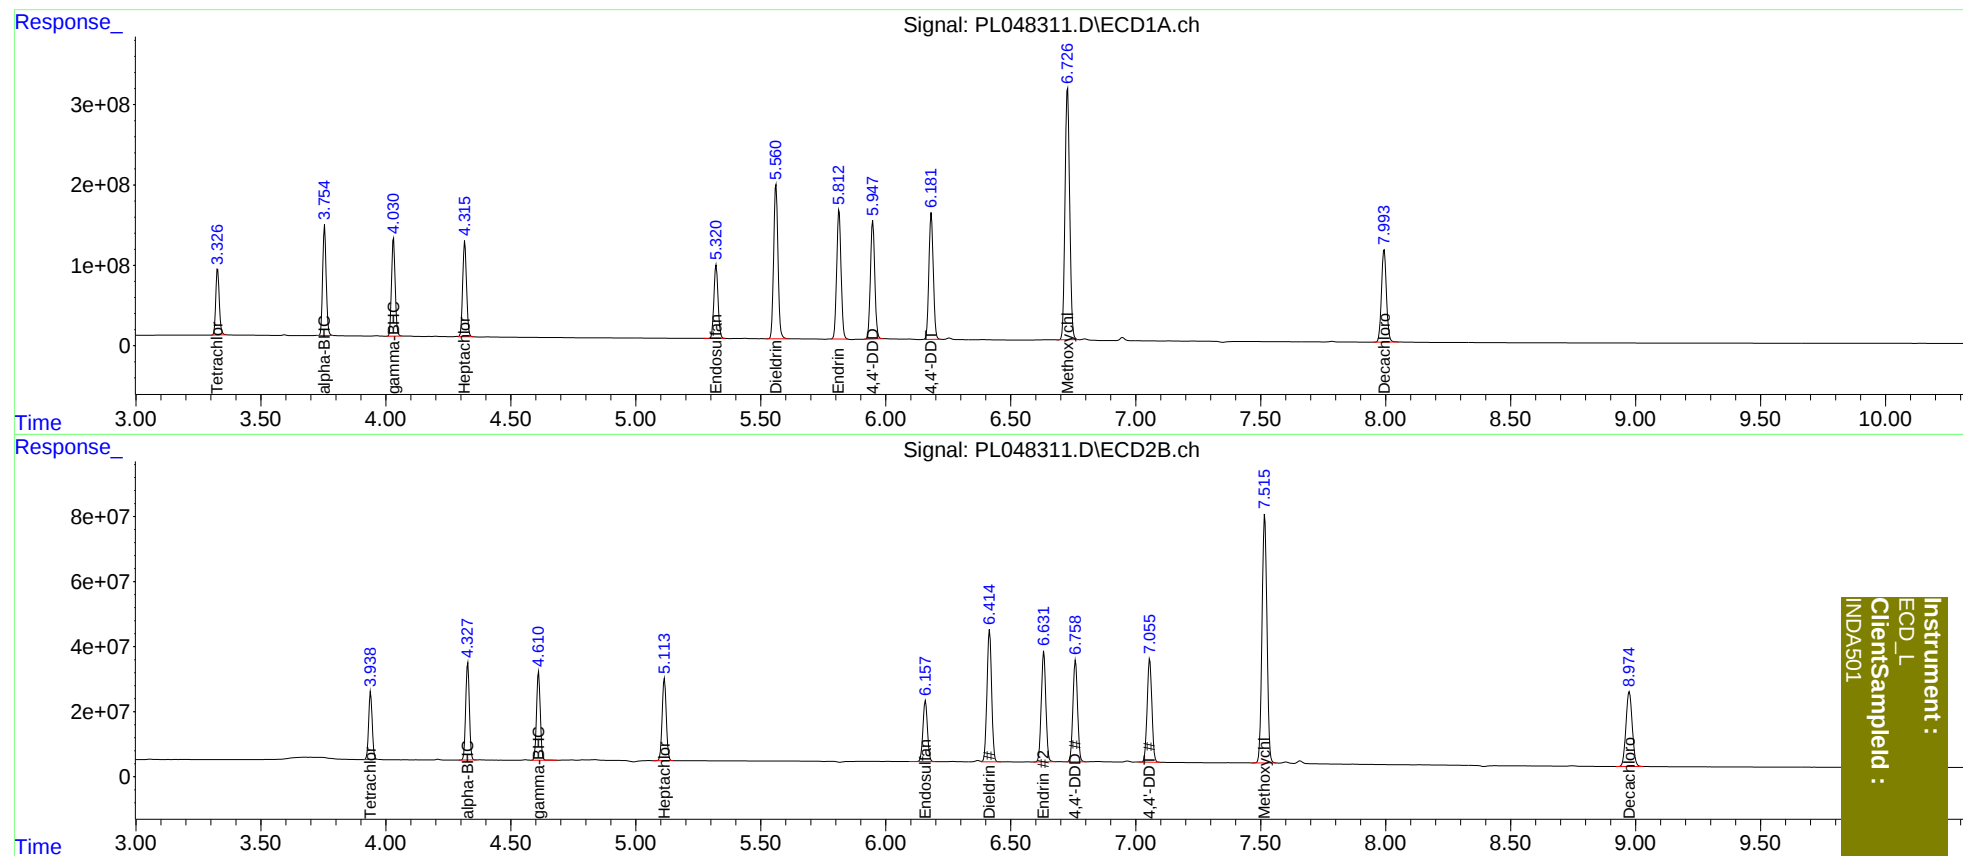


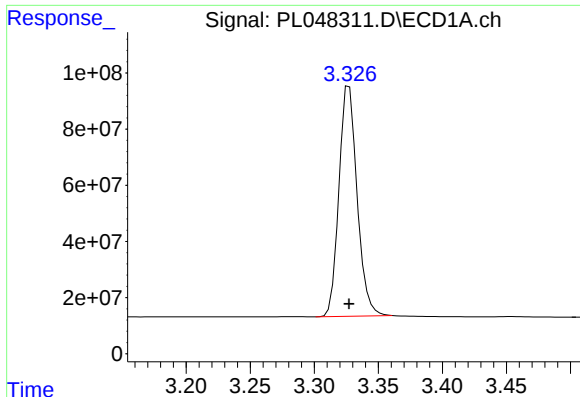

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 808169675
Conc: 77.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

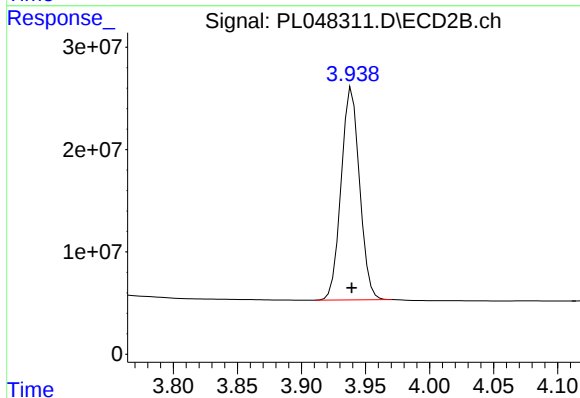


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 207556507
Conc: 78.42 ng/ml

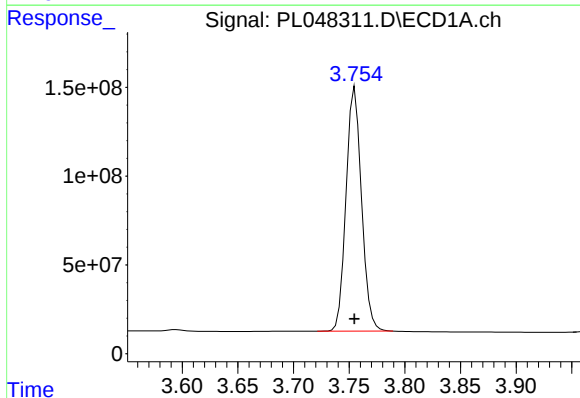


#2 alpha-BHC

R.T.: 3.755 min
Delta R.T.: 0.000 min
Response: 1329014419
Conc: 83.23 ng/ml

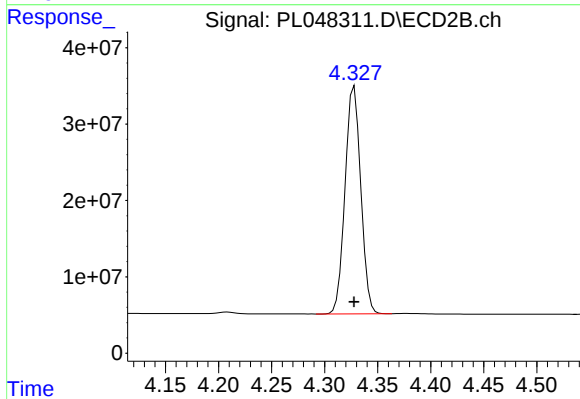

#2 alpha-BHC


R.T.: 4.328 min
Delta R.T.: 0.000 min
Response: 306490789
Conc: 85.68 ng/ml

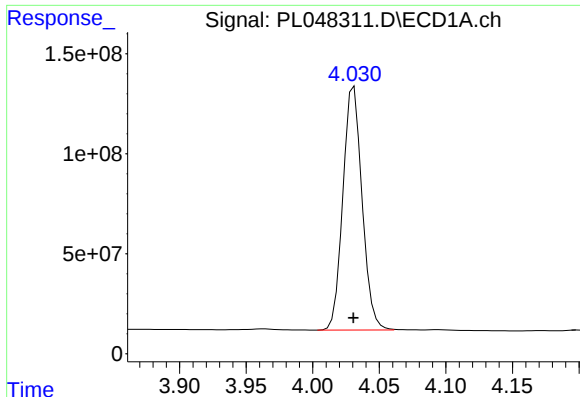

#3 gamma-BHC (Lindane)


R.T.: 4.031 min
Delta R.T.: 0.000 min
Response: 1221488962
Conc: 83.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

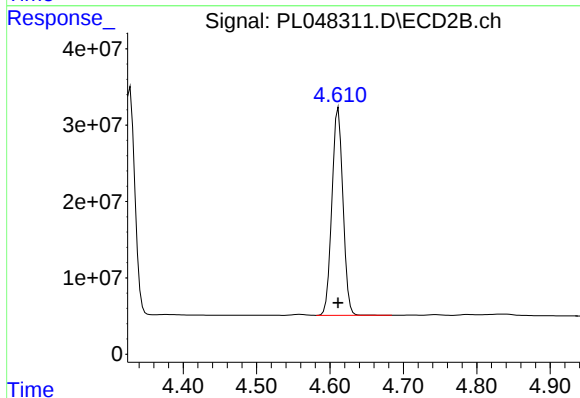


#3 gamma-BHC (Lindane)

R.T.: 4.611 min
Delta R.T.: 0.000 min
Response: 284711735
Conc: 84.07 ng/ml

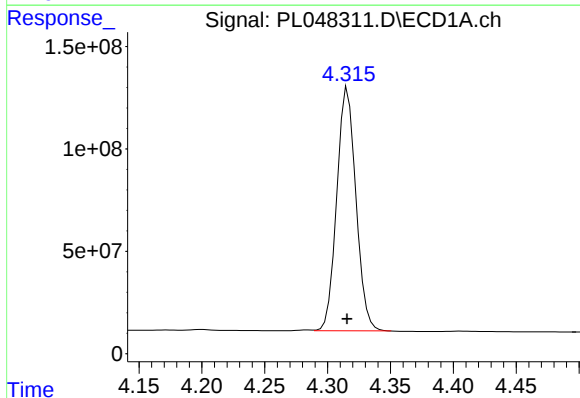


#4 Heptachlor

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 1261564165
Conc: 80.64 ng/ml

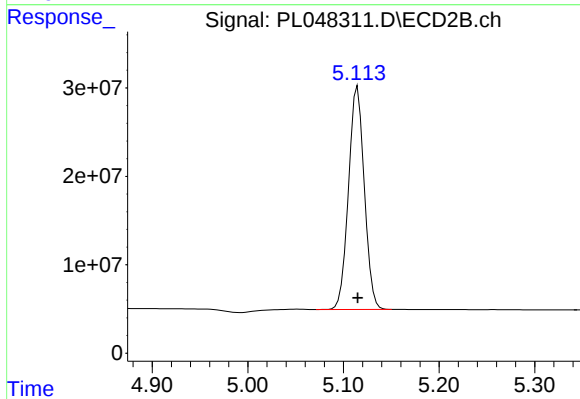

#4 Heptachlor


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 290835611
Conc: 79.87 ng/ml

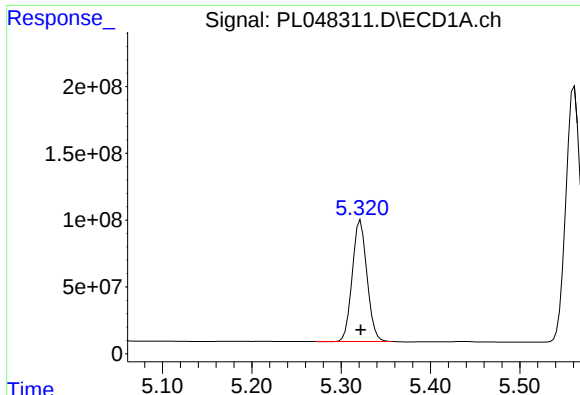

#9 Endosulfan I


R.T.: 5.322 min
Delta R.T.: 0.000 min
Response: 1042631871
Conc: 78.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

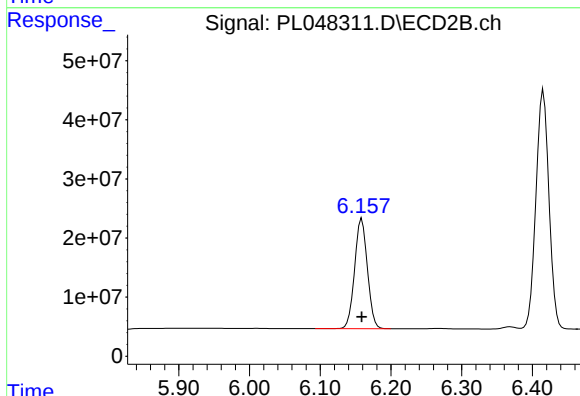


#9 Endosulfan I

R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 233918241
Conc: 73.91 ng/ml

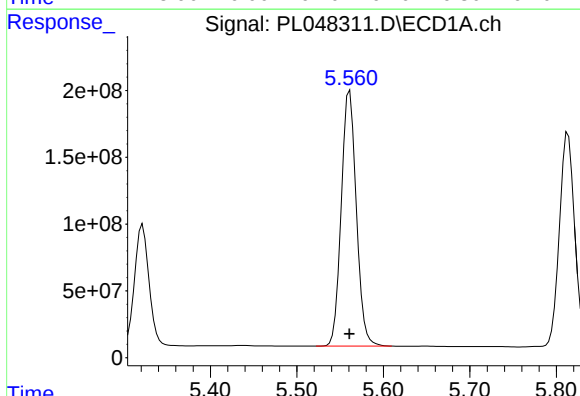


#13 Dieldrin

R.T.: 5.561 min
Delta R.T.: 0.000 min
Response: 2299594738
Conc: 161.03 ng/ml

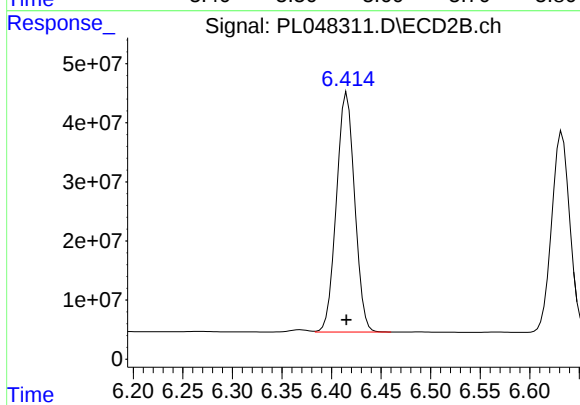

#13 Dieldrin


R.T.: 6.416 min
Delta R.T.: 0.000 min
Response: 518264776
Conc: 165.66 ng/ml

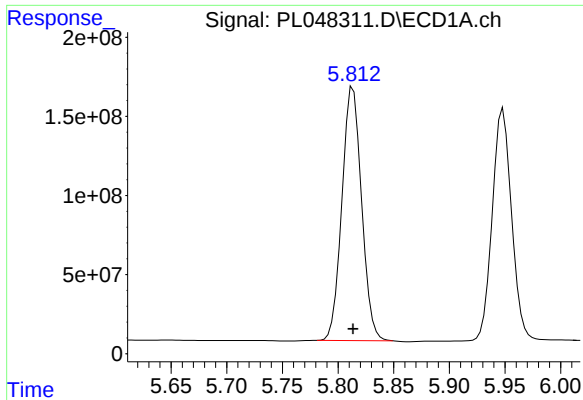

#14 Endrin


R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 1969366634
Conc: 157.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

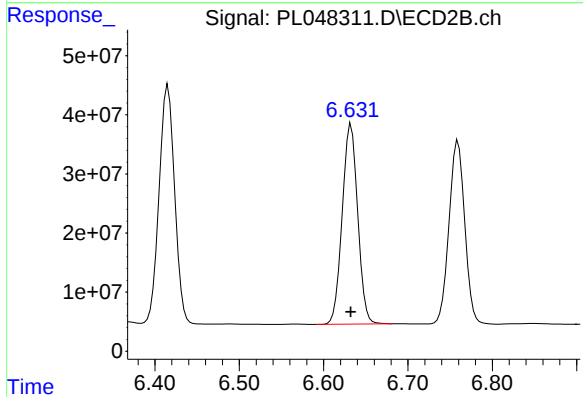


#14 Endrin

R.T.: 6.633 min
Delta R.T.: 0.000 min
Response: 432946781
Conc: 165.81 ng/ml

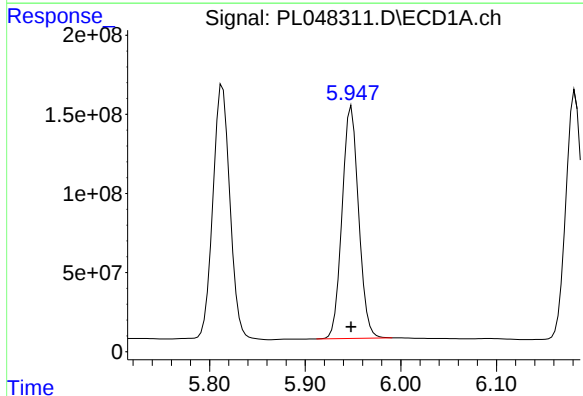


#16 4,4'-DDD

R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 1766094161
Conc: 164.94 ng/ml

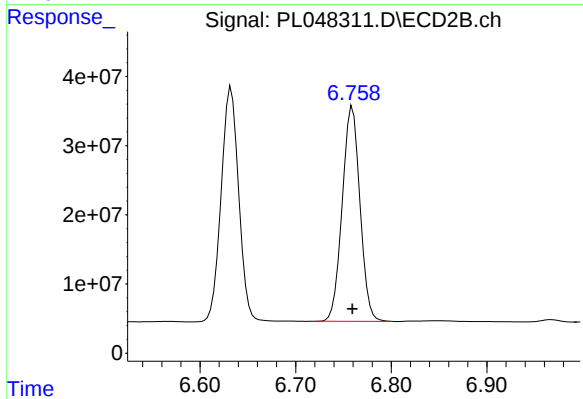

#16 4,4'-DDD


R.T.: 6.759 min
Delta R.T.: 0.000 min
Response: 402258300
Conc: 165.61 ng/ml

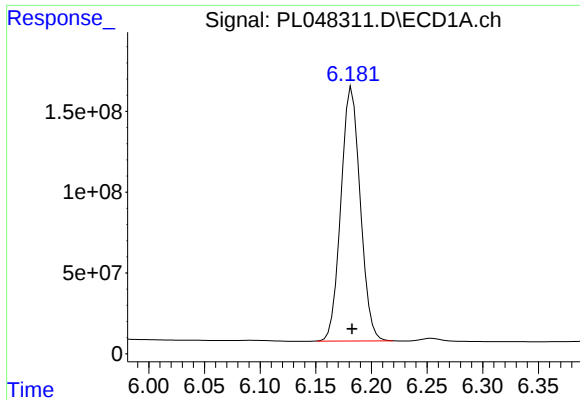

#17 4,4'-DDT


R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 1901686091
Conc: 173.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

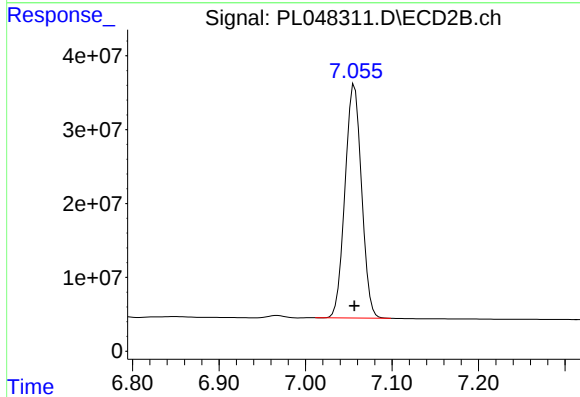


#17 4,4'-DDT

R.T.: 7.057 min
Delta R.T.: 0.000 min
Response: 418556263
Conc: 168.15 ng/ml

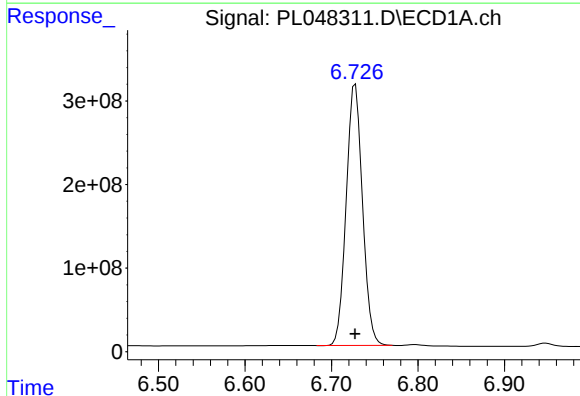


#20 Methoxychlor

R.T.: 6.728 min
Delta R.T.: 0.000 min
Response: 4073143869
Conc: 724.78 ng/ml

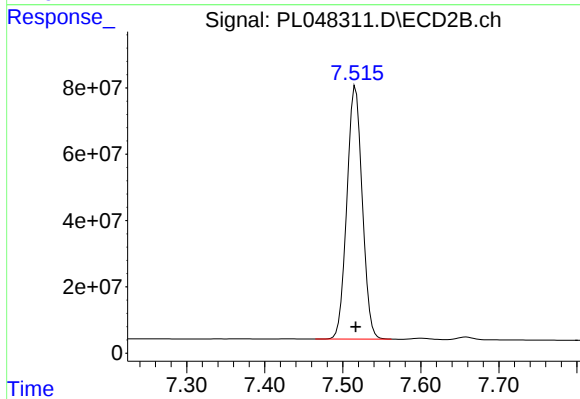

#20 Methoxychlor

R.T.: 7.516 min
Delta R.T.: 0.000 min
Response: 1043343820
Conc: 755.65 ng/ml

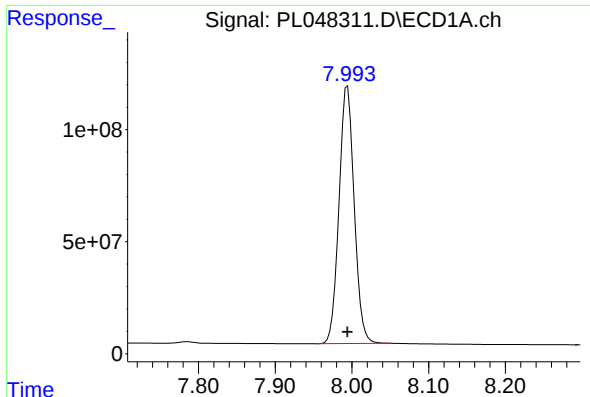

#27 Decachlorobiphenyl


R.T.: 7.994 min

Delta R.T.: 0.000 min

Response: 1583172774

Conc: 145.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA501

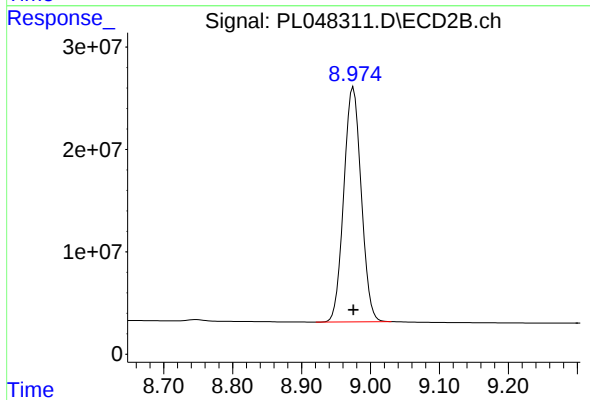

#27 Decachlorobiphenyl

R.T.: 8.975 min

Delta R.T.: 0.000 min

Response: 402869147

Conc: 145.01 ng/ml