

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
 Data File : PL048326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2019 16:29
 Operator : AJ\SJ
 Sample : K2607-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A5140

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 01:43:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 10 01:24:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.939	243.0E6	62516063	23.441	23.714
27)	SA Decachlor...	7.994	8.975	459.6E6	119.1E6	43.134	43.674
Target Compounds							
3)	MA gamma-BHC...	4.073f	0.000	16276646	0	1.101	N.D. #
9)	A Endosulfan I	0.000	6.113f	0	14651458	N.D.	4.835
11)	B cis-Chlor...	0.000	6.113	0	14651458	N.D.	4.589
15)	B Endosulfa...	0.000	6.856	0	18746790	N.D.	6.657


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
Data File : PL048326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2019 16:29
Operator : AJ\SJ
Sample : K2607-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
A5140

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 01:43:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 10 01:24:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

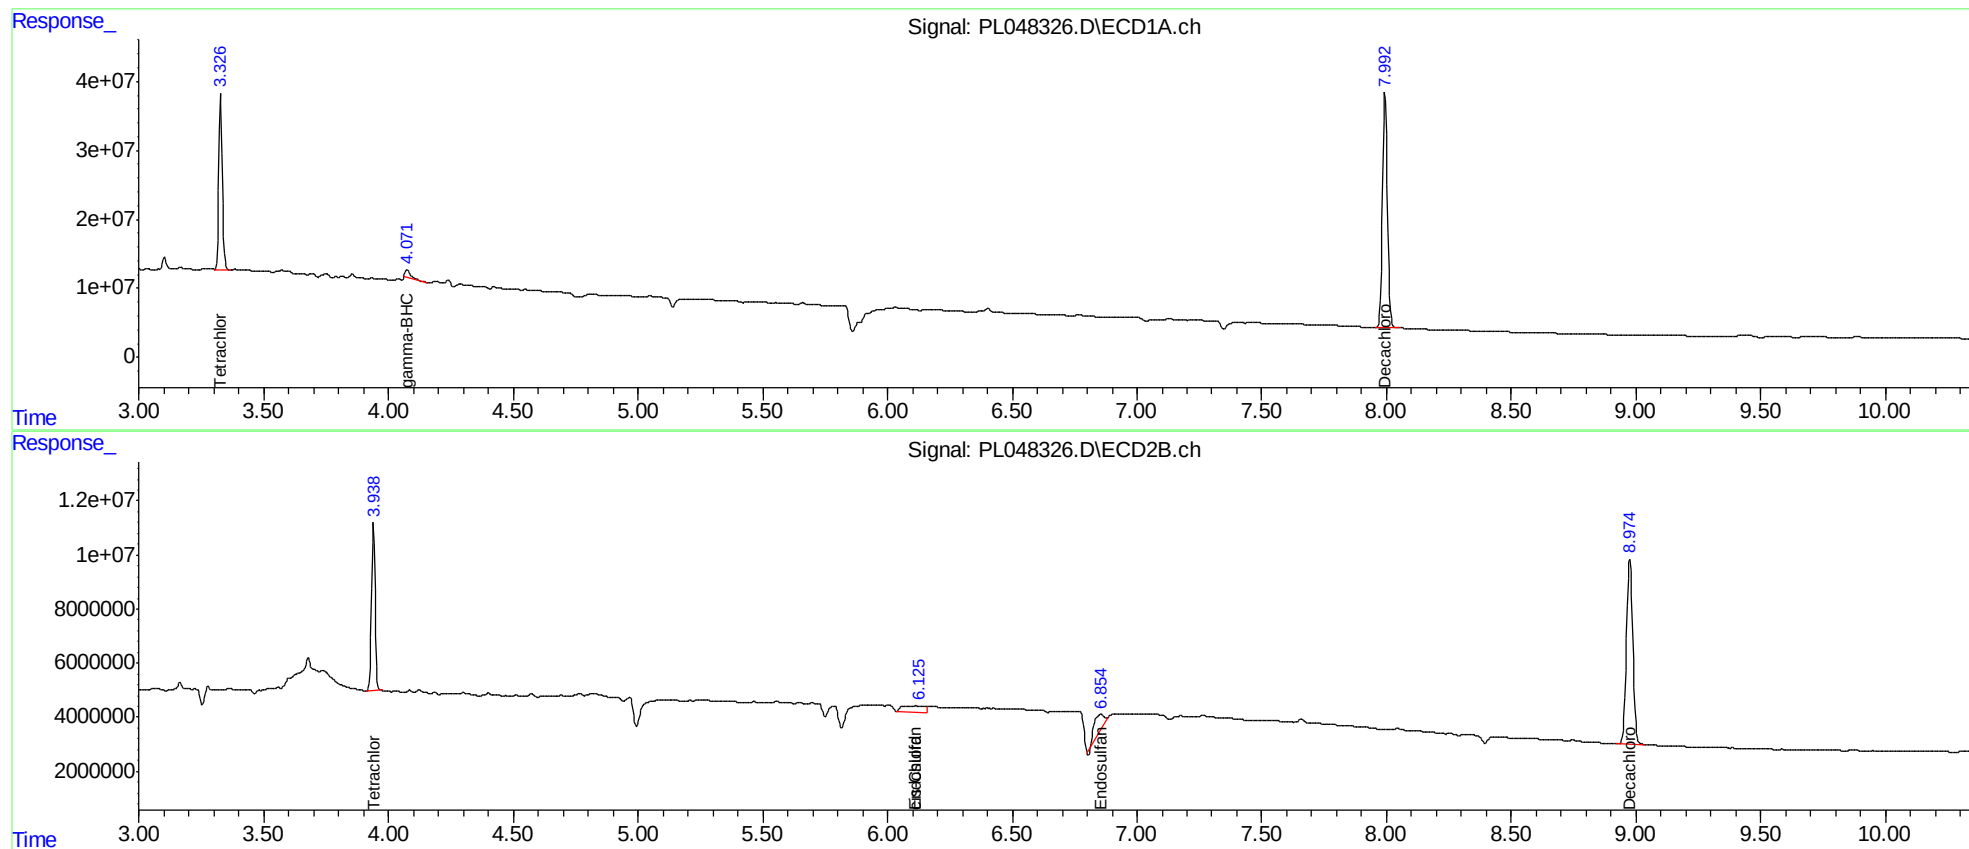


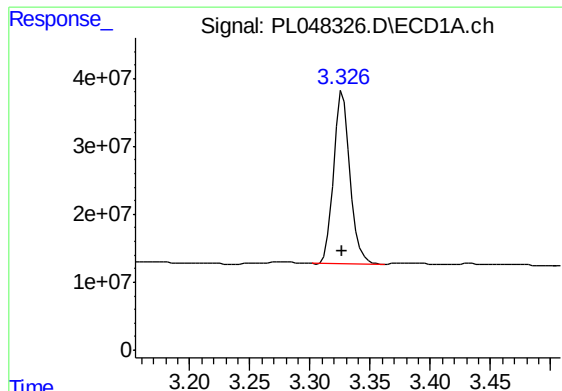

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 243031448
Conc: 23.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
A5140

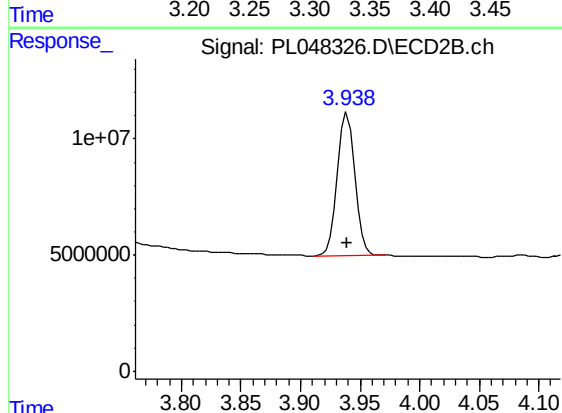


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 62516063
Conc: 23.71 ng/ml

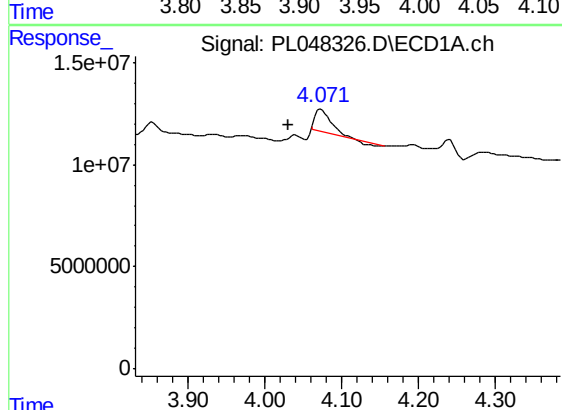


#3 gamma-BHC (Lindane)

R.T.: 4.073 min
Delta R.T.: 0.042 min
Response: 16276646
Conc: 1.10 ng/ml

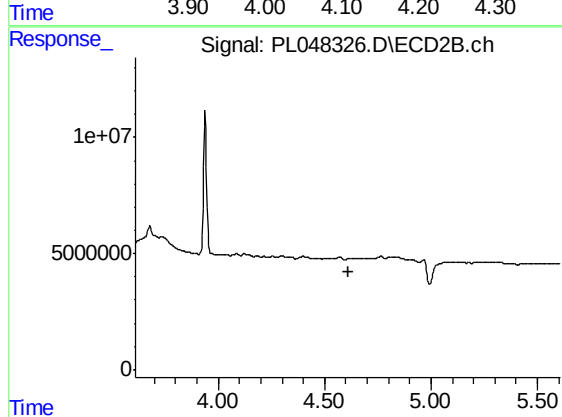

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.611 min
Response: 0
Conc: N.D.

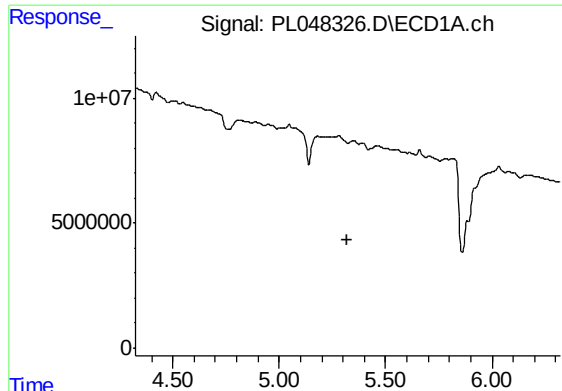

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.322 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
A5140

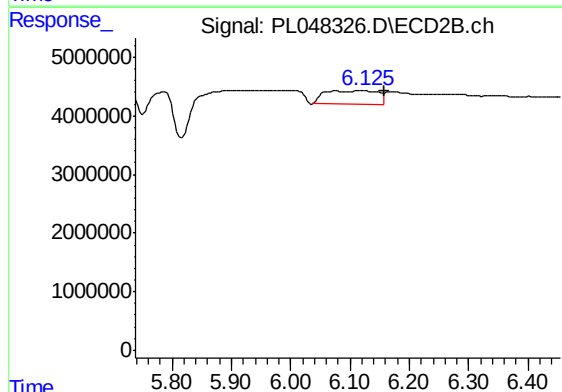


#9 Endosulfan I

R.T.: 6.113 min
Delta R.T.: -0.045 min
Response: 14651458
Conc: 4.83 ng/ml

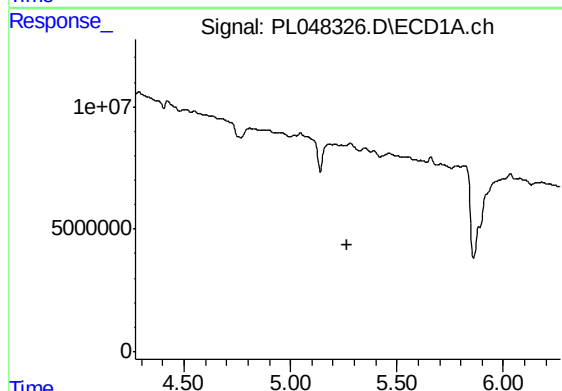


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.270 min
Response: 0
Conc: N.D.

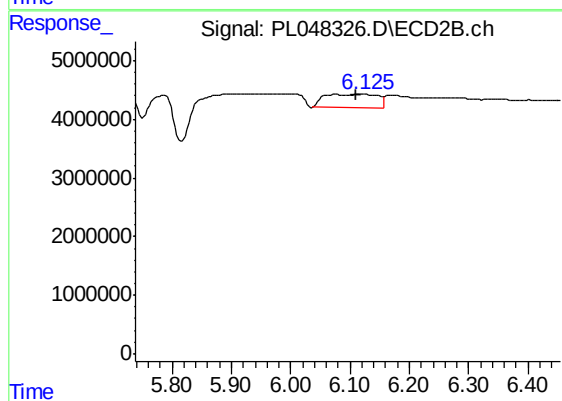

#11 cis-Chlordane


R.T.: 6.113 min
Delta R.T.: 0.004 min
Response: 14651458
Conc: 4.59 ng/ml

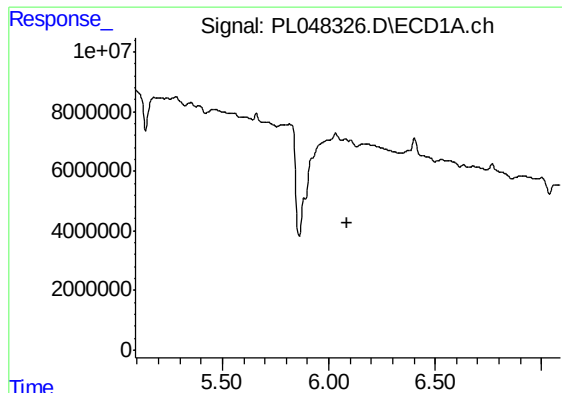

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
A5140

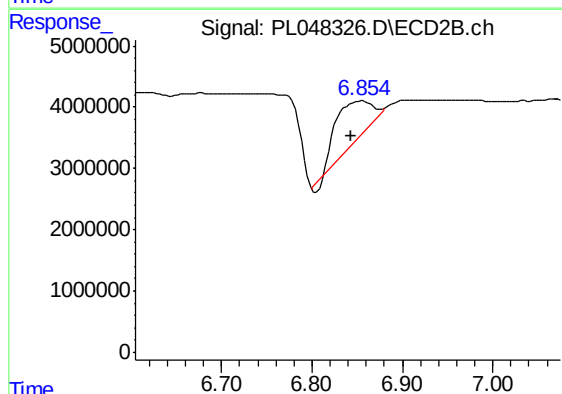


#15 Endosulfan II

R.T.: 6.856 min
Delta R.T.: 0.013 min
Response: 18746790
Conc: 6.66 ng/ml

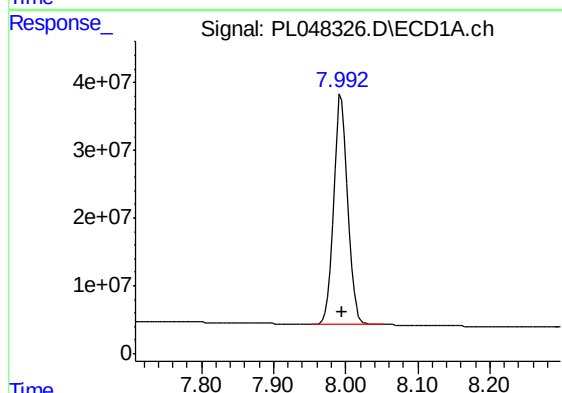

#27 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: -0.001 min
Response: 459645982
Conc: 43.13 ng/ml

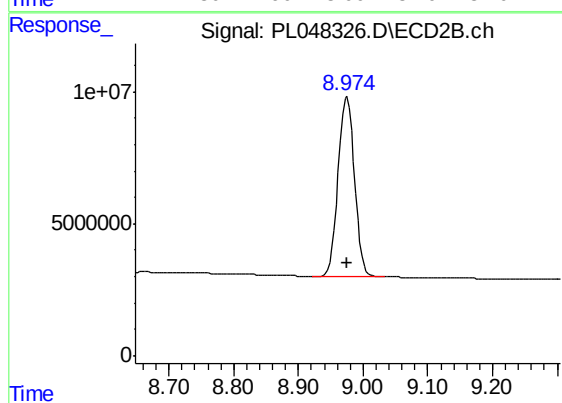

#27 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 119062764
Conc: 43.67 ng/ml