

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
 Data File : PL048342.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2019 20:30
 Operator : AJ\SJ
 Sample : K2694-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BFHG0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 01:48:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 10 01:24:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.328	3.940	204.5E6	54065700	19.722	20.508
27) SA	Decachlor...	7.995	8.975	287.3E6	75813760	26.963	27.810
Target Compounds							
8) B	Heptachlo...	0.000	5.830	0	89120636	N.D.	30.185
9) A	Endosulfan I	5.293	0.000	357.3E6	0	27.126	N.D. #
11) B	cis-Chlor...	5.293	0.000	357.3E6	0	25.556	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
Data File : PL048342.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2019 20:30
Operator : AJ\SJ
Sample : K2694-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BFHG0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 01:48:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 10 01:24:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

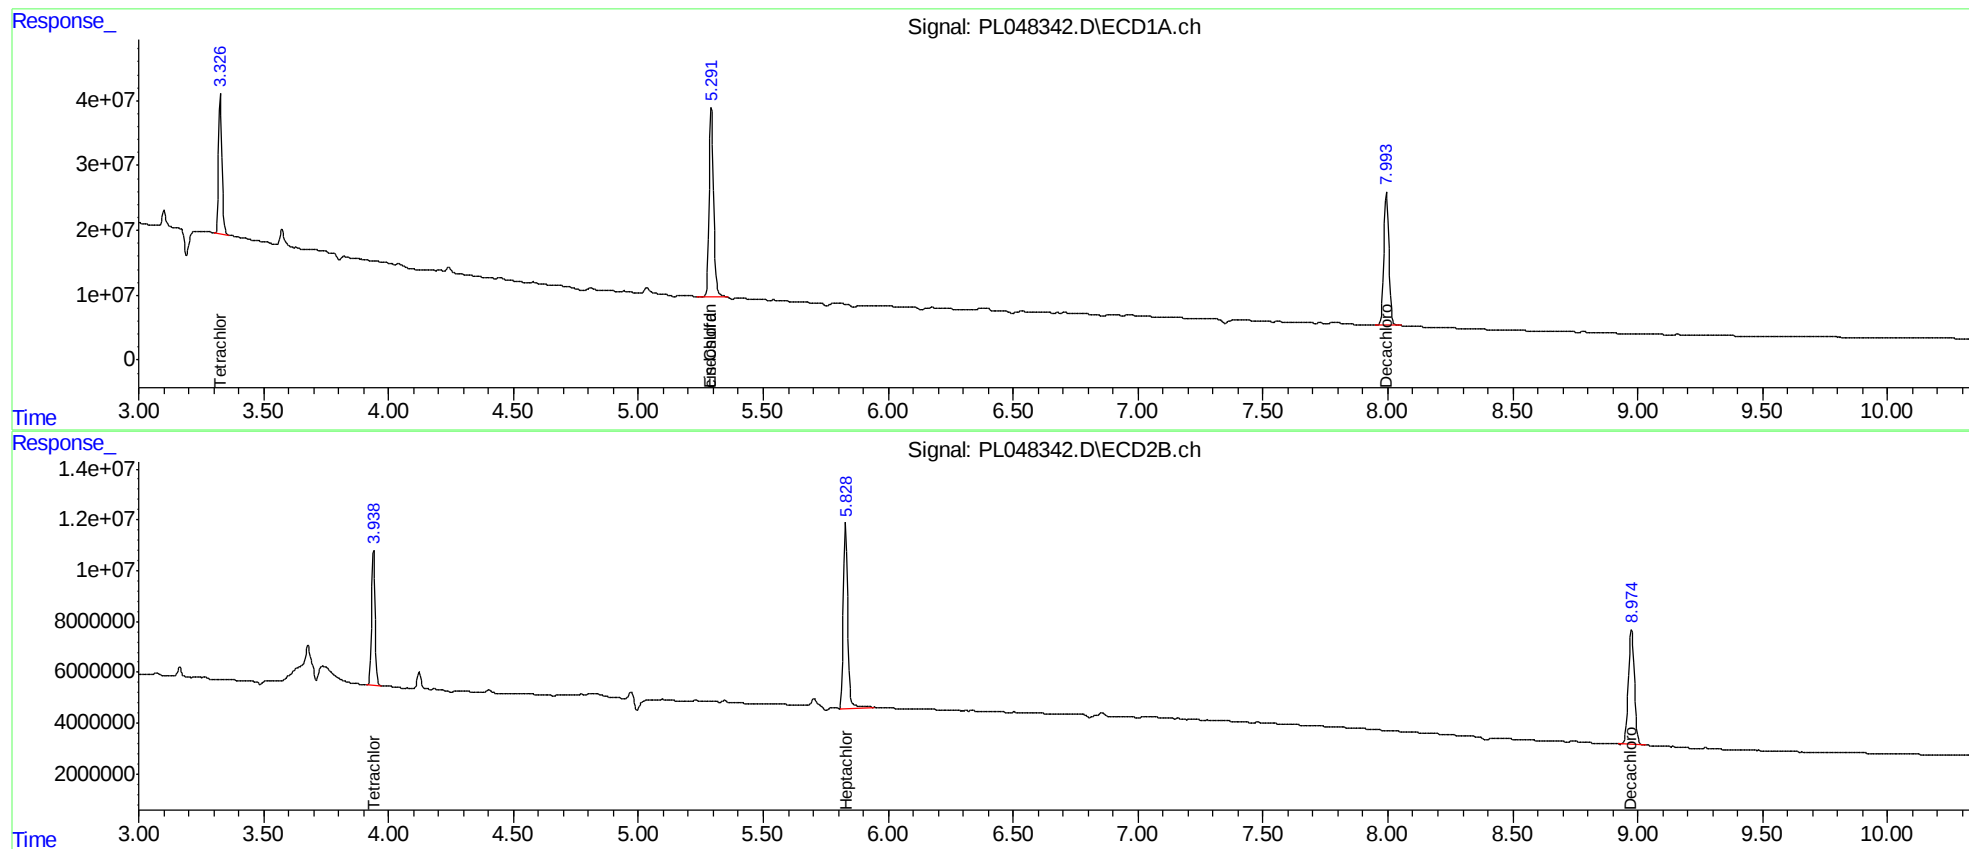


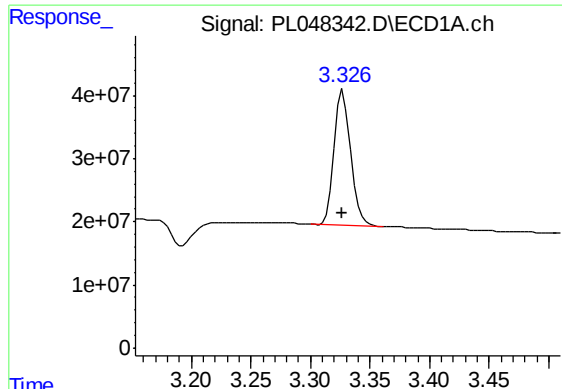

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 204472520
Conc: 19.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHG0

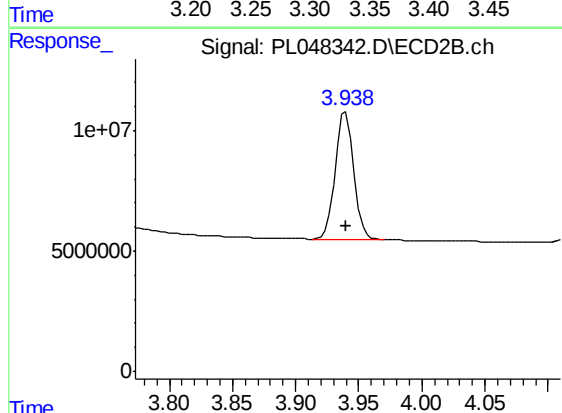


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 54065700
Conc: 20.51 ng/ml

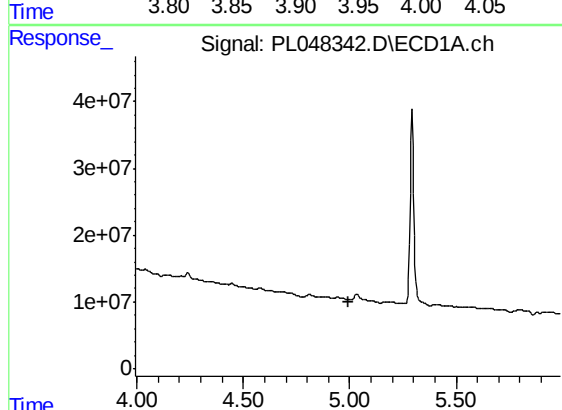


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.992 min
Response: 0
Conc: N.D.

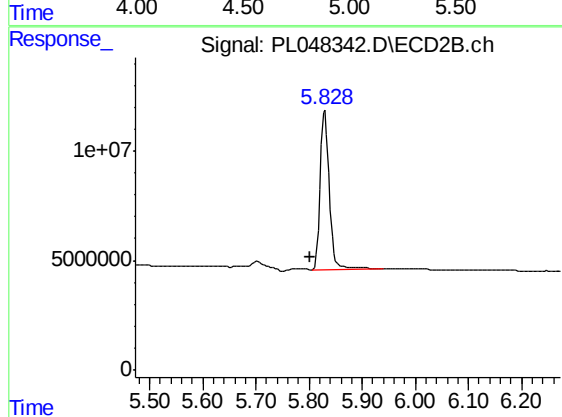

#8 Heptachlor epoxide


R.T.: 5.830 min
Delta R.T.: 0.027 min
Response: 89120636
Conc: 30.18 ng/ml

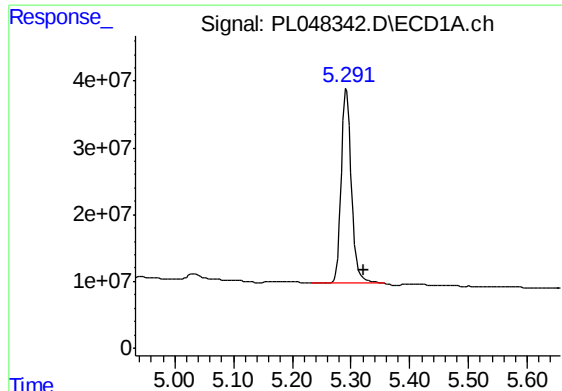

#9 Endosulfan I


R.T.: 5.293 min
Delta R.T.: -0.029 min
Response: 357282852
Conc: 27.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHG0

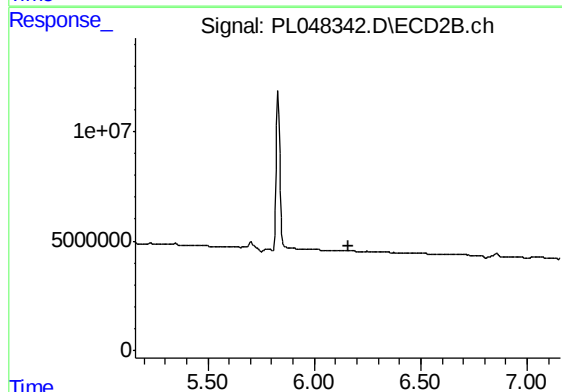


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

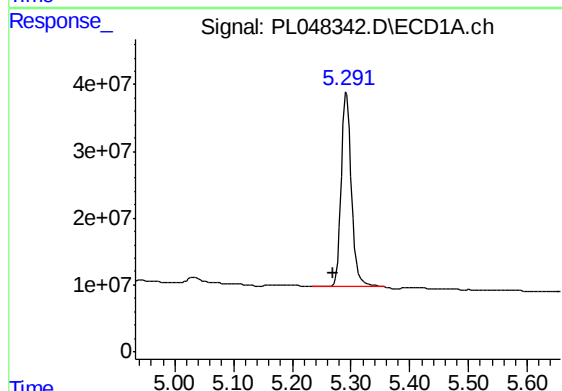


#11 cis-Chlordane

R.T.: 5.293 min
Delta R.T.: 0.023 min
Response: 357282852
Conc: 25.56 ng/ml

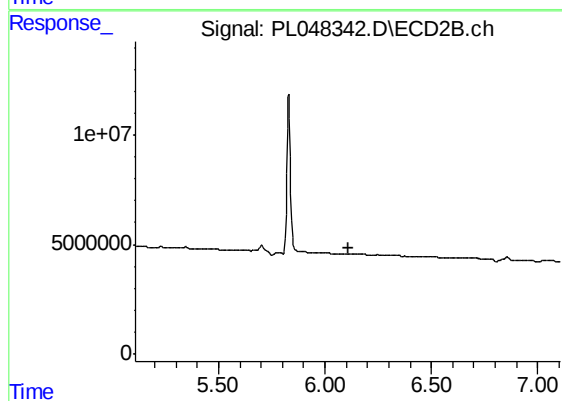

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

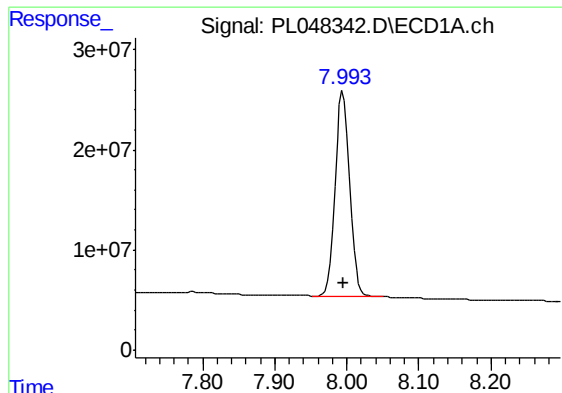

#27 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 287325061
Conc: 26.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHG0

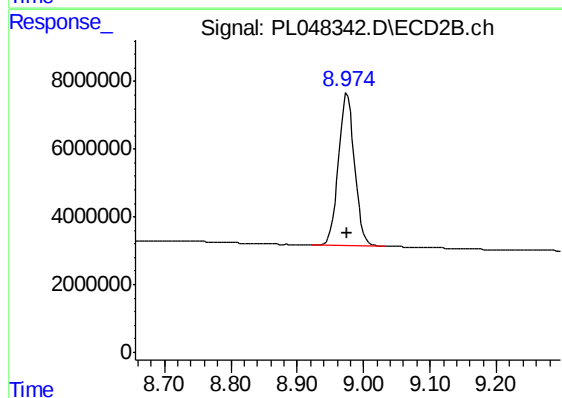

#27 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 75813760
Conc: 27.81 ng/ml