

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
 Data File : PL048350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2019 22:30
 Operator : AJ\SJ
 Sample : K2694-12
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BFHH7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 01:50:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 10 01:24:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	199.3E6	53247590	19.219	20.198
27)	SA Decachlor...	7.995	8.976	387.2E6	101.3E6	36.337	37.141
Target Compounds							
4)	MA Heptachlor	4.329	0.000	19159874	0	1.223	N.D. #
5)	MB Aldrin	4.535	5.444f	18853644	4736869	1.265	1.436
6)	B beta-BHC	4.329f	0.000	19159874	0	2.777	N.D. #
7)	B delta-BHC	4.483	5.026f	-7399113	1399740	N.D.	0.484
8)	B Heptachlo...	5.047f	5.795	15410197	3145556	1.114	1.065
9)	A Endosulfan I	5.293	0.000	199.1E6	0	15.116	N.D. #
11)	B cis-Chlor...	5.293	0.000	199.1E6	0	14.241	N.D. #
19)	B Endosulfa...	6.536f	7.190	24060431	6336818	2.100	2.391


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
Data File : PL048350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2019 22:30
Operator : AJ\SJ
Sample : K2694-12
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BFHH7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 01:50:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 10 01:24:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

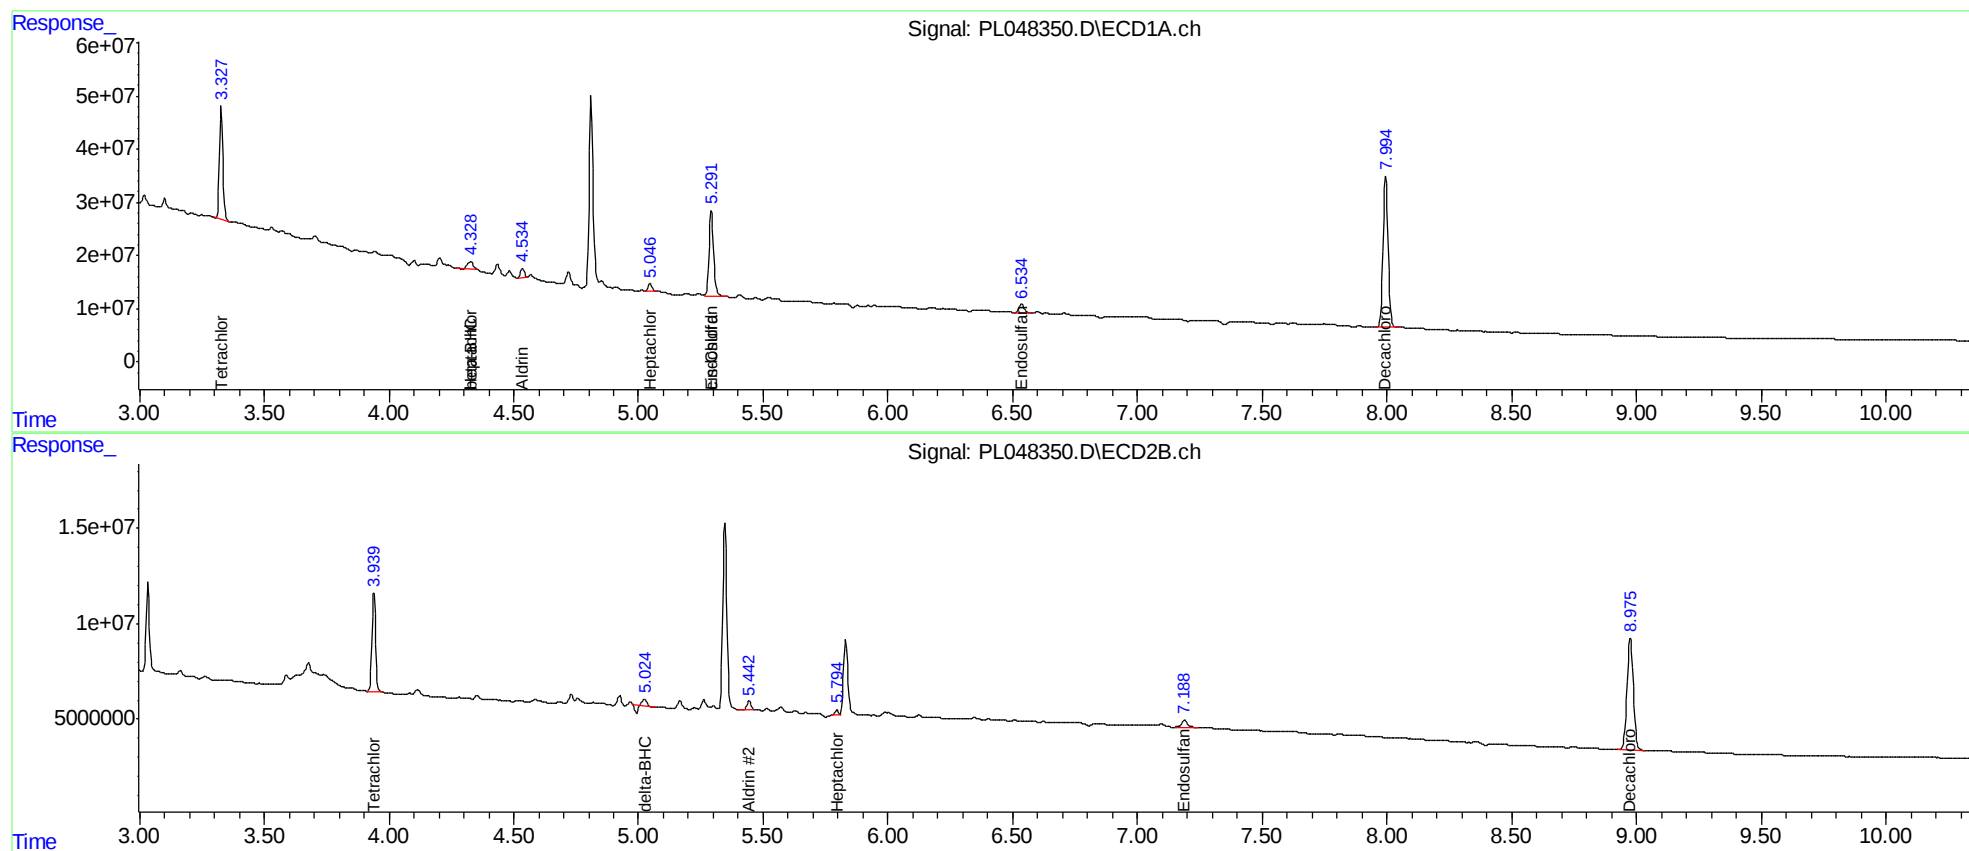


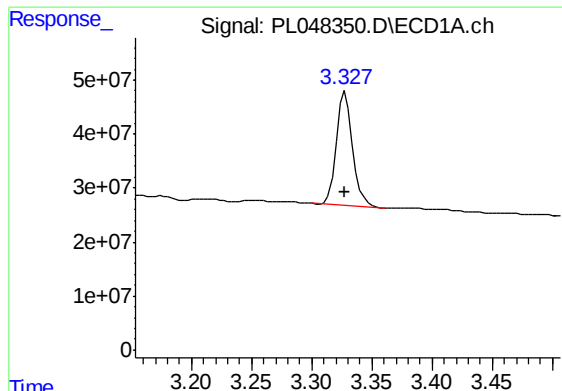

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 199265115
Conc: 19.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHH7

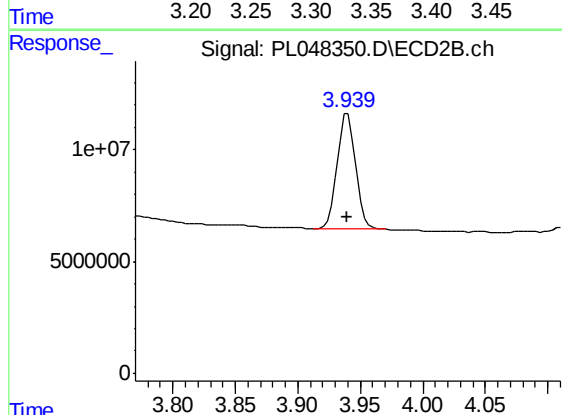


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 53247590
Conc: 20.20 ng/ml

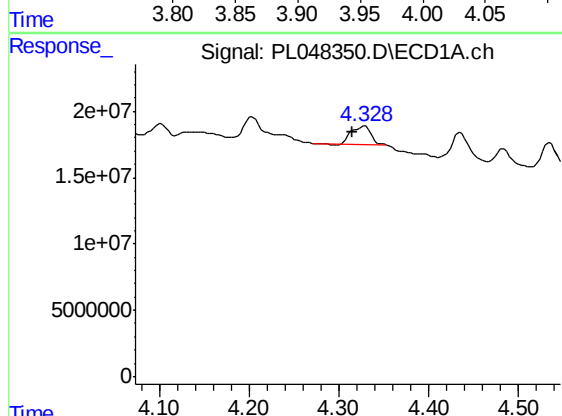


#4 Heptachlor

R.T.: 4.329 min
Delta R.T.: 0.013 min
Response: 19159874
Conc: 1.22 ng/ml

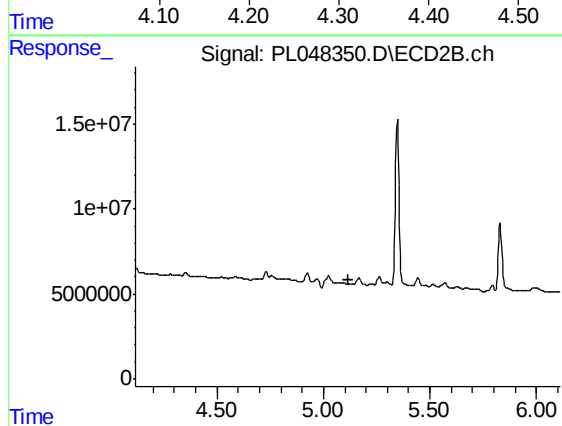

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

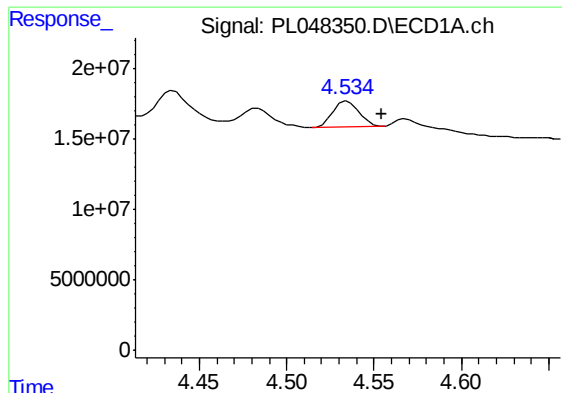

#5 Aldrin


R.T.: 4.535 min
Delta R.T.: -0.020 min
Response: 18853644
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHH7

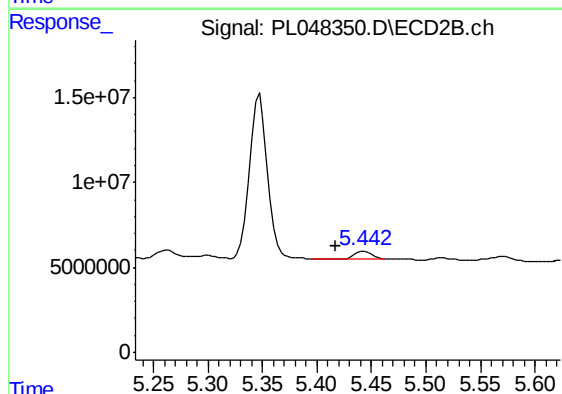


#5 Aldrin

R.T.: 5.444 min
Delta R.T.: 0.027 min
Response: 4736869
Conc: 1.44 ng/ml

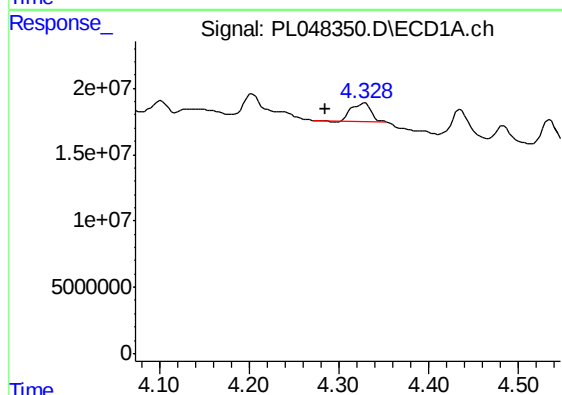


#6 beta-BHC

R.T.: 4.329 min
Delta R.T.: 0.044 min
Response: 19159874
Conc: 2.78 ng/ml

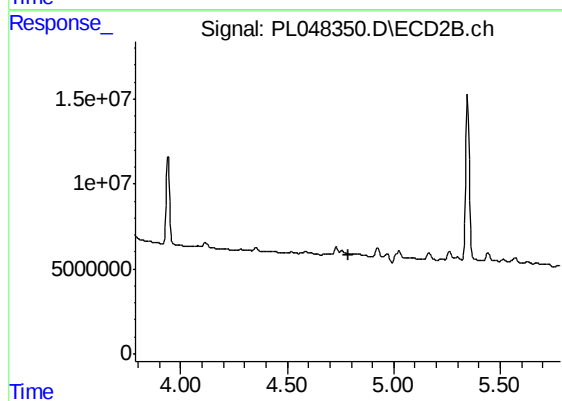

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

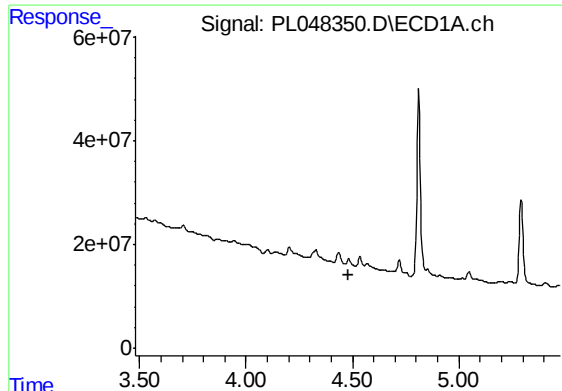

#7 delta-BHC


R.T.: 4.483 min
Delta R.T.: 0.005 min
Response: -7399113
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BFHH7

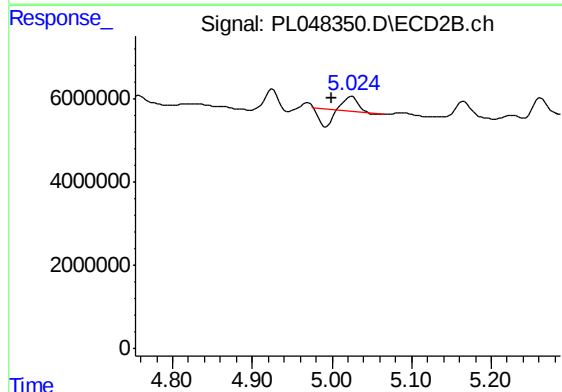


#7 delta-BHC

R.T.: 5.026 min
Delta R.T.: 0.026 min
Response: 1399740
Conc: 0.48 ng/ml

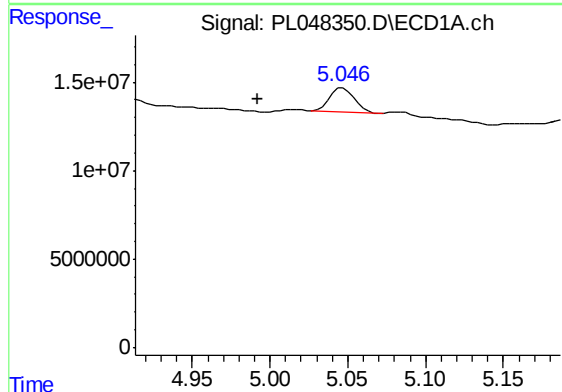


#8 Heptachlor epoxide

R.T.: 5.047 min
Delta R.T.: 0.055 min
Response: 15410197
Conc: 1.11 ng/ml

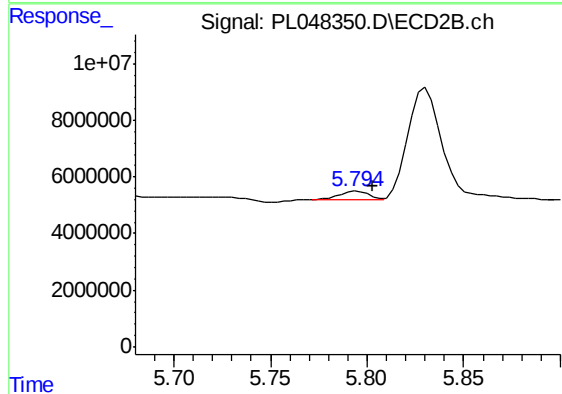

#8 Heptachlor epoxide


R.T.: 5.795 min
Delta R.T.: -0.008 min
Response: 3145556
Conc: 1.07 ng/ml

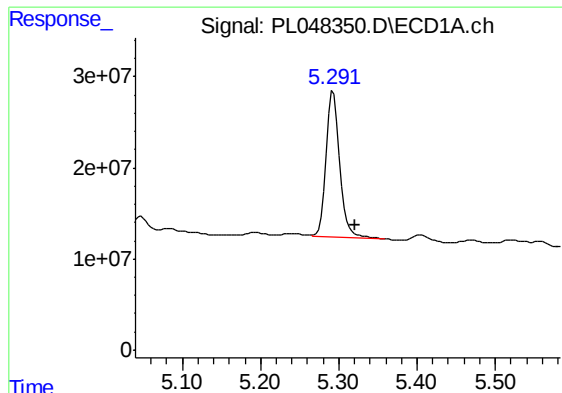

#9 Endosulfan I


R.T.: 5.293 min
Delta R.T.: -0.029 min
Response: 199091632
Conc: 15.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHH7

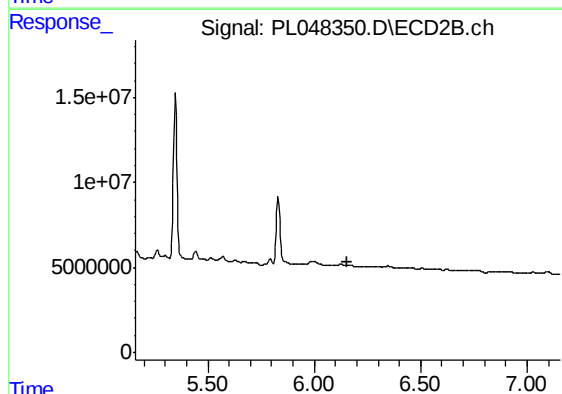


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

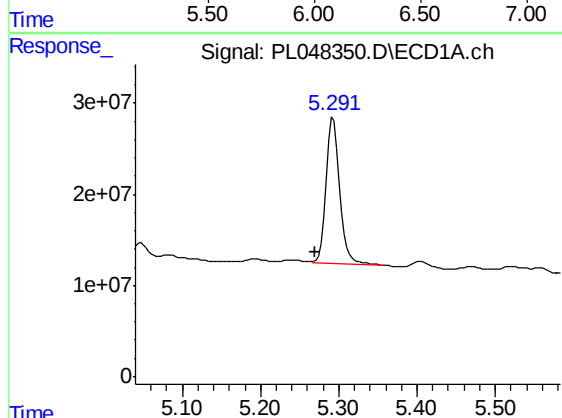


#11 cis-Chlordane

R.T.: 5.293 min
Delta R.T.: 0.023 min
Response: 199091632
Conc: 14.24 ng/ml

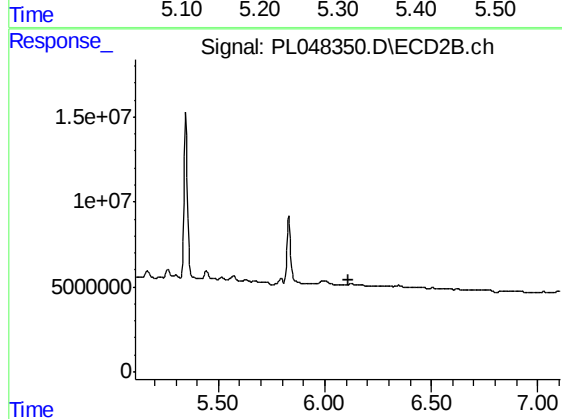

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

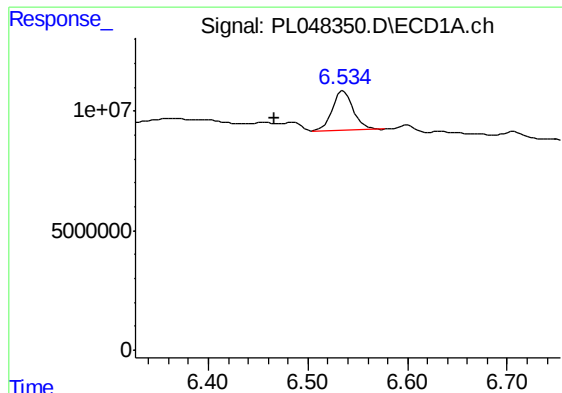

#19 Endosulfan Sulfate


R.T.: 6.536 min
Delta R.T.: 0.070 min
Response: 24060431
Conc: 2.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHH7

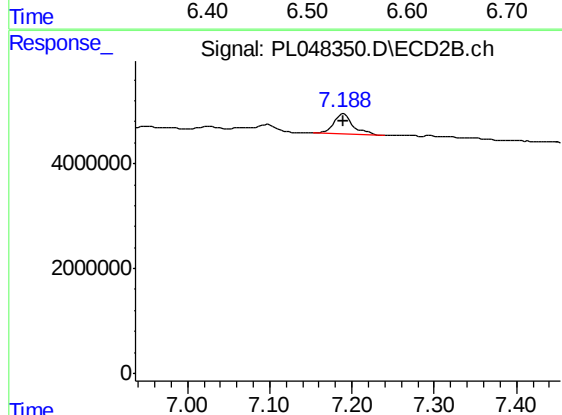


#19 Endosulfan Sulfate

R.T.: 7.190 min
Delta R.T.: 0.000 min
Response: 6336818
Conc: 2.39 ng/ml

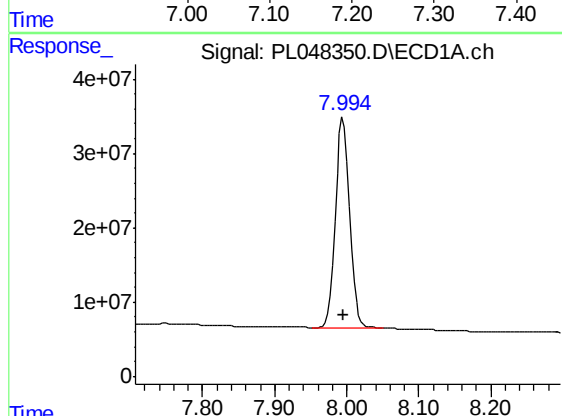

#27 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 387214001
Conc: 36.34 ng/ml

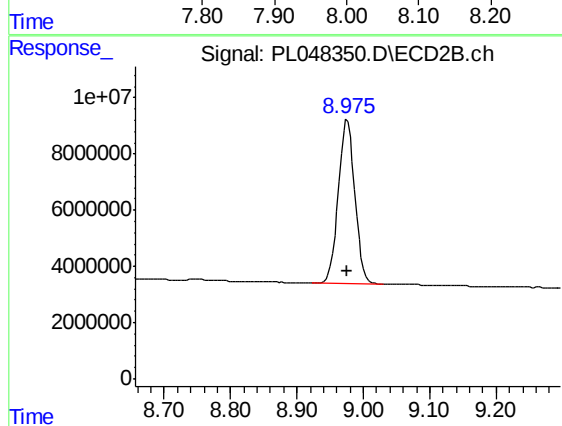

#27 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.001 min
Response: 101251416
Conc: 37.14 ng/ml