

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
 Data File : PL048351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2019 22:45
 Operator : AJ\SJ
 Sample : K2694-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BFHG3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 01:50:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 10 01:24:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	196.6E6	51760998	18.965	19.634
27)	SA Decachlor...	7.995	8.975	213.2E6	56368973	20.012	20.677
Target Compounds							
3)	MA gamma-BHC...	0.000	4.587	0	4107126	N.D.	1.201
4)	MA Heptachlor	4.329	0.000	44010617	0	2.809	N.D. #
5)	MB Aldrin	4.568	5.444f	13617366	7879456	0.914	2.389 #
6)	B beta-BHC	4.329f	0.000	44010617	0	6.378	N.D. #
7)	B delta-BHC	4.483	5.025f	19748626	15144796	1.254	5.236 #
8)	B Heptachlo...	5.047f	5.796	19667493	3941798	1.422	1.335
9)	A Endosulfan I	5.292	0.000	47013979	0	3.570	N.D. #
11)	B cis-Chlor...	5.292	0.000	47013979	0	3.363	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
Data File : PL048351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2019 22:45
Operator : AJ\SJ
Sample : K2694-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BFHG3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 01:50:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 10 01:24:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

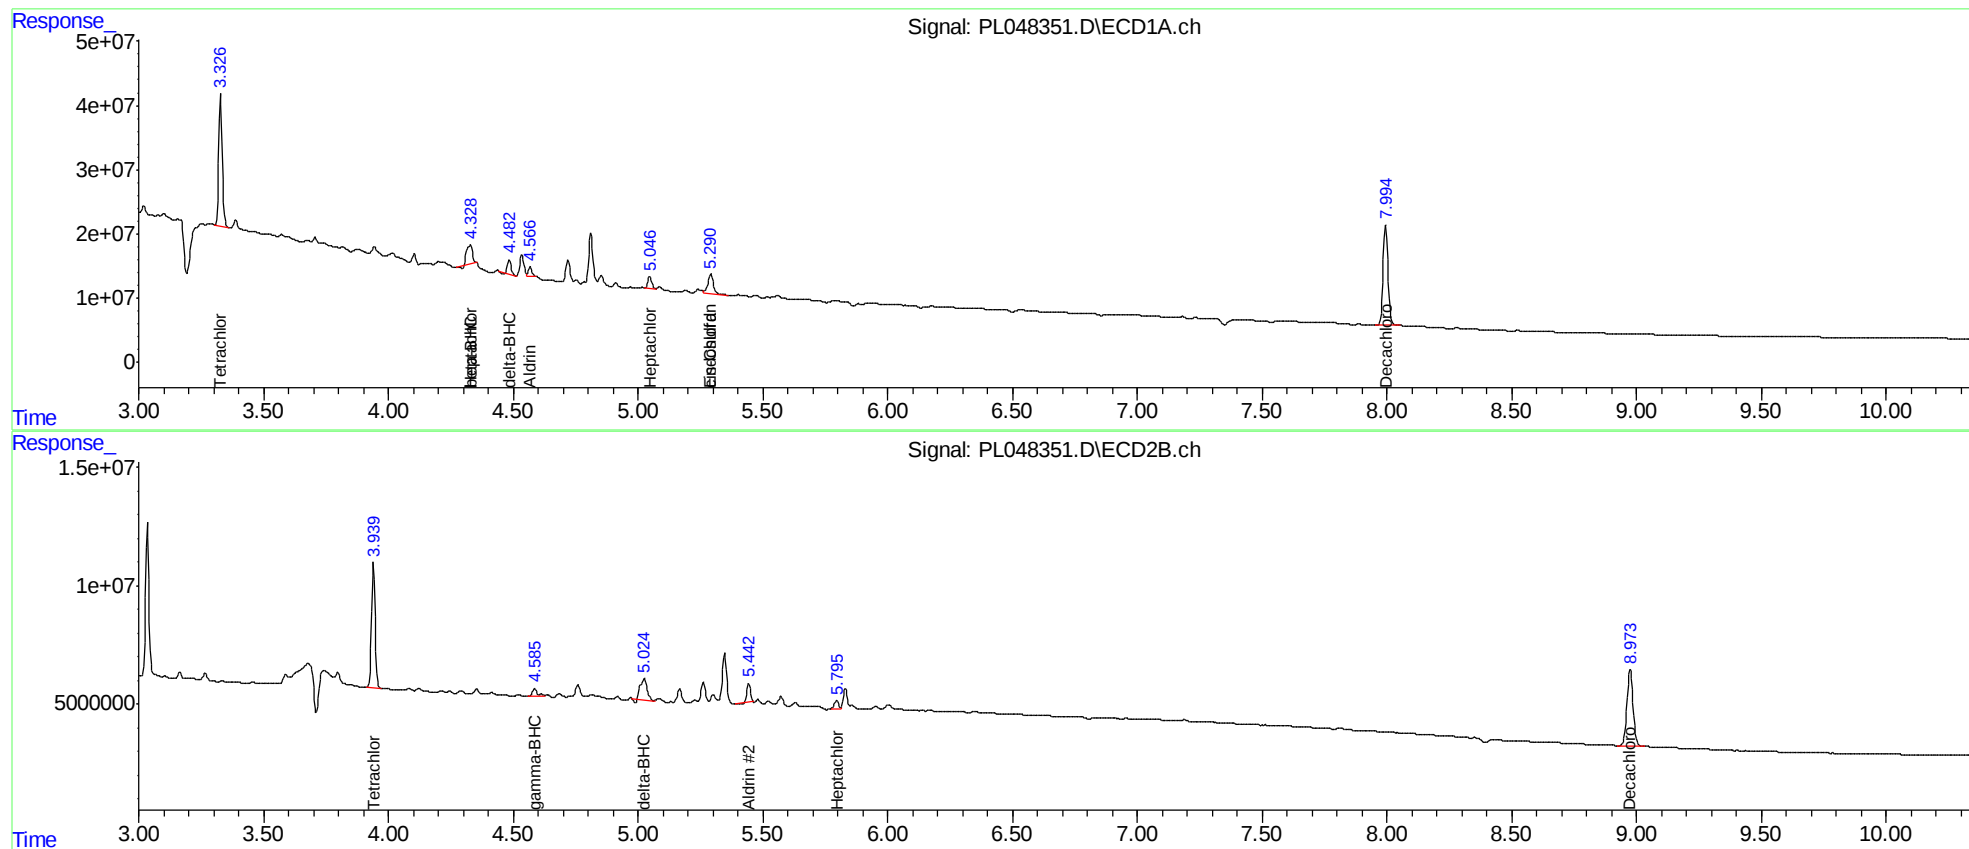


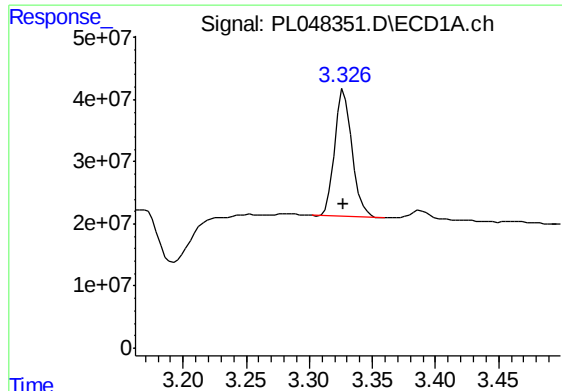

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 196631333
Conc: 18.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHG3

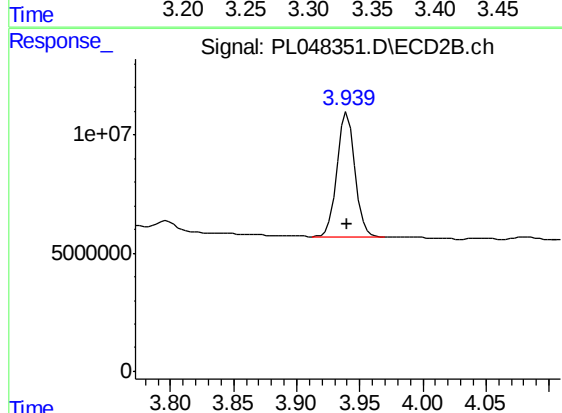


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 51760998
Conc: 19.63 ng/ml

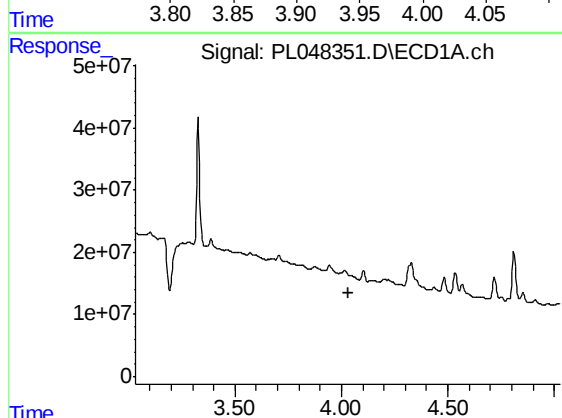


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.031 min
Response: 0
Conc: N.D.

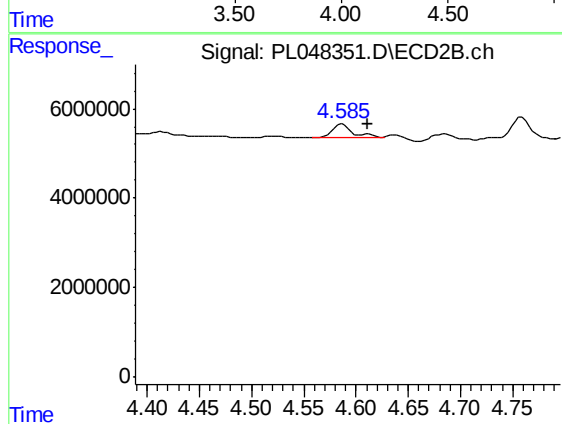

#3 gamma-BHC (Lindane)


R.T.: 4.587 min
Delta R.T.: -0.025 min
Response: 4107126
Conc: 1.20 ng/ml

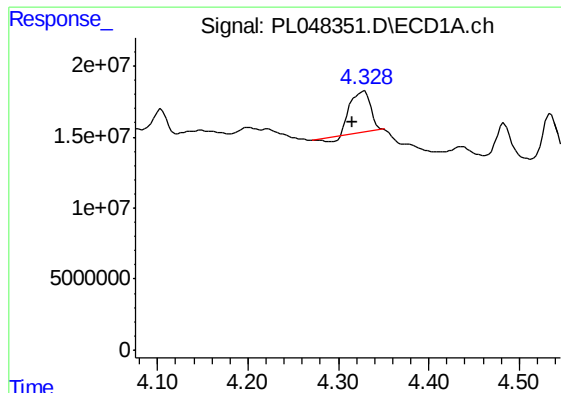

#4 Heptachlor


R.T.: 4.329 min
Delta R.T.: 0.013 min
Response: 44010617
Conc: 2.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHG3

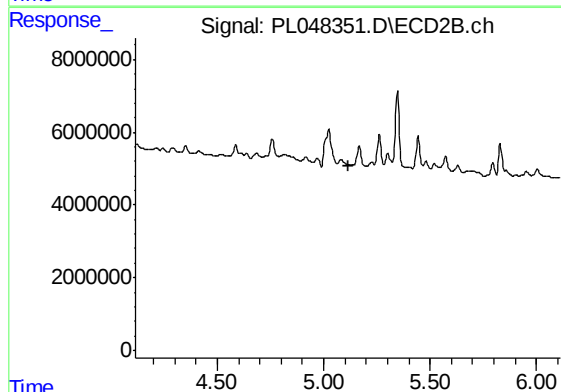


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

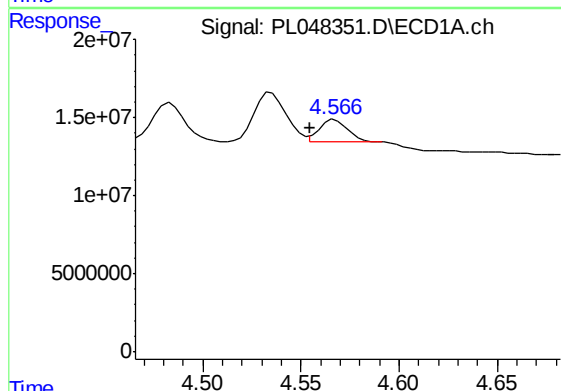


#5 Aldrin

R.T.: 4.568 min
Delta R.T.: 0.013 min
Response: 13617366
Conc: 0.91 ng/ml

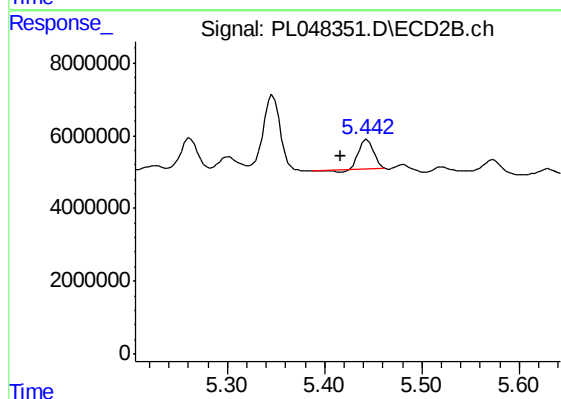

#5 Aldrin


R.T.: 5.444 min
Delta R.T.: 0.027 min
Response: 7879456
Conc: 2.39 ng/ml

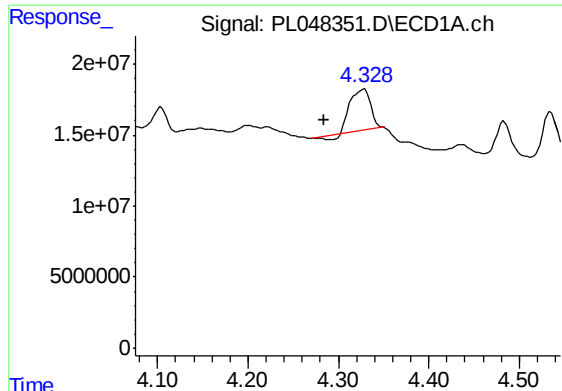

#6 beta-BHC


R.T.: 4.329 min
Delta R.T.: 0.044 min
Response: 44010617
Conc: 6.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHG3

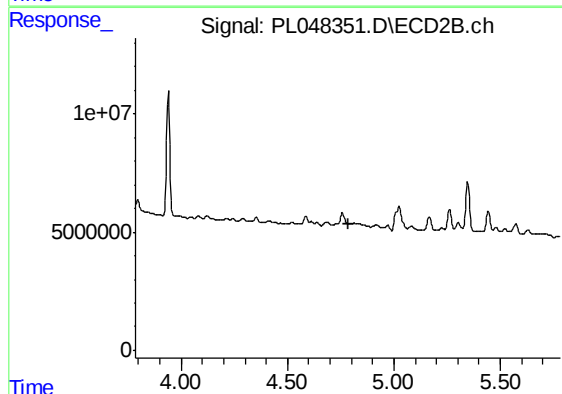


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

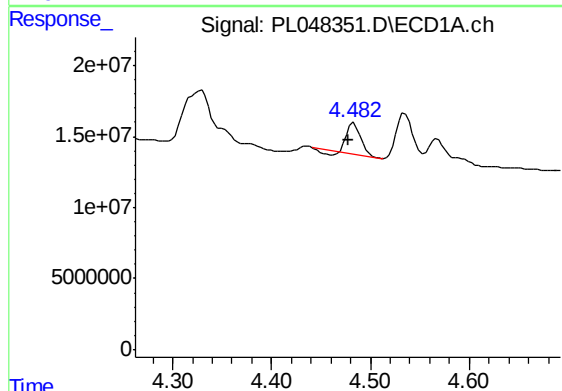


#7 delta-BHC

R.T.: 4.483 min
Delta R.T.: 0.005 min
Response: 19748626
Conc: 1.25 ng/ml

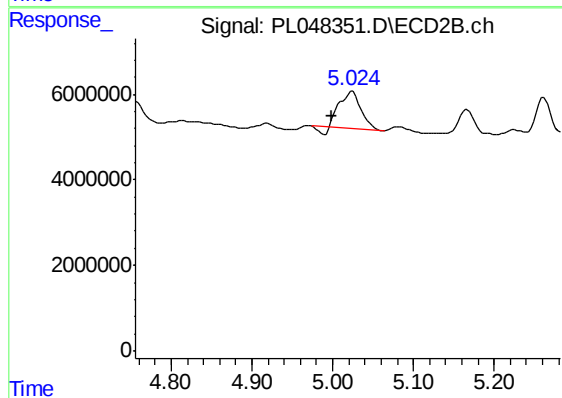

#7 delta-BHC


R.T.: 5.025 min
Delta R.T.: 0.025 min
Response: 15144796
Conc: 5.24 ng/ml

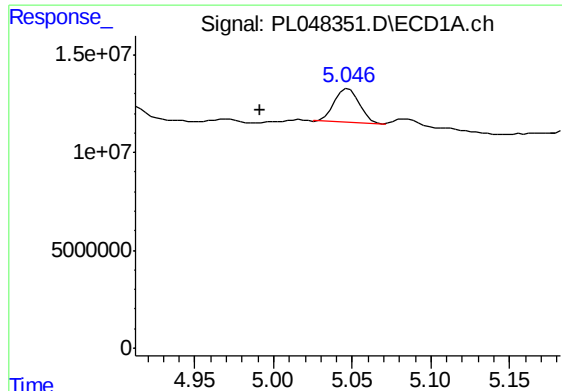

#8 Heptachlor epoxide


R.T.: 5.047 min
Delta R.T.: 0.056 min
Response: 19667493
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHG3

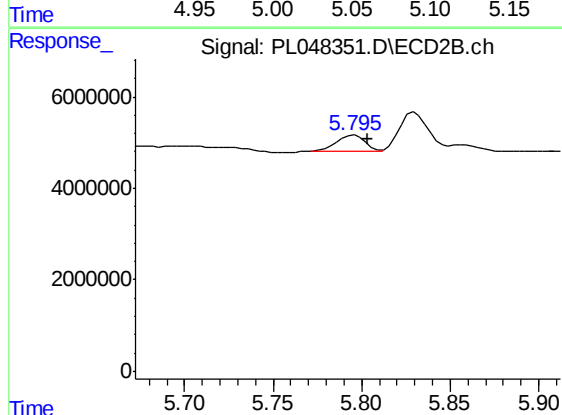


#8 Heptachlor epoxide

R.T.: 5.796 min
Delta R.T.: -0.007 min
Response: 3941798
Conc: 1.34 ng/ml

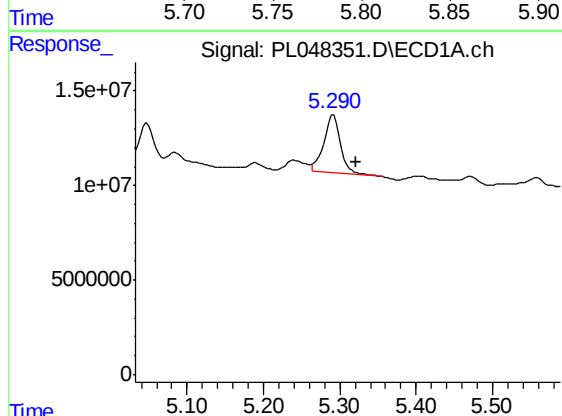


#9 Endosulfan I

R.T.: 5.292 min
Delta R.T.: -0.030 min
Response: 47013979
Conc: 3.57 ng/ml

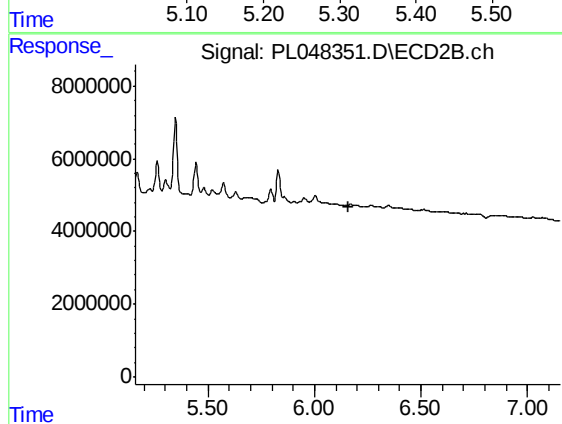

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

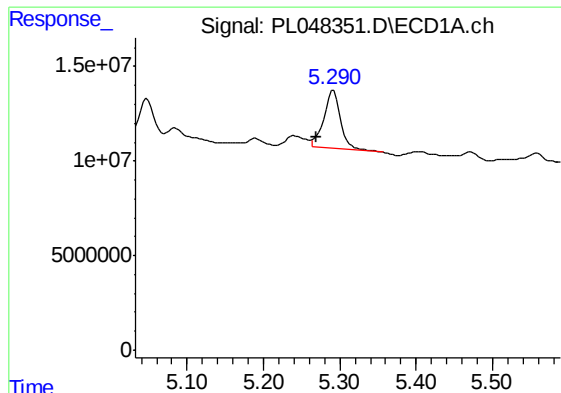

#11 cis-Chlordane


R.T.: 5.292 min
Delta R.T.: 0.022 min
Response: 47013979
Conc: 3.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
BFHG3

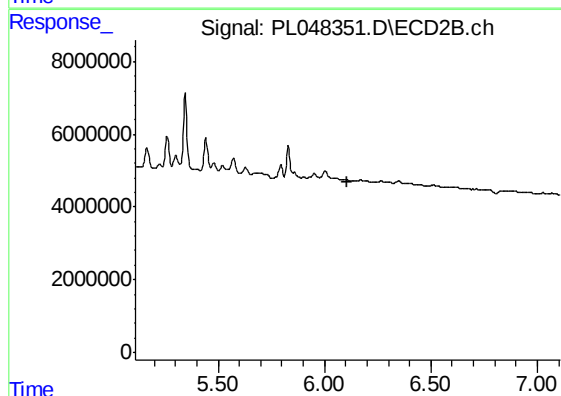


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

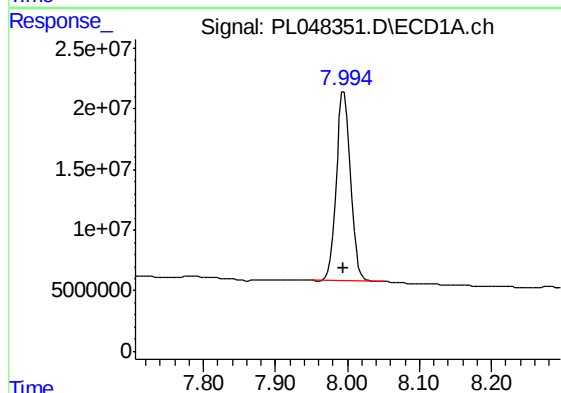

#27 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 213247629
Conc: 20.01 ng/ml

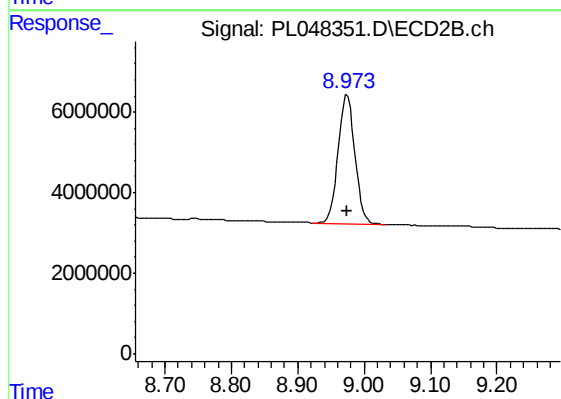

#27 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 56368973
Conc: 20.68 ng/ml