

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
 Data File : PL048354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2019 23:30
 Operator : AJ\SJ
 Sample : PB119537BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PBLK37

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 01:51:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 10 01:24:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.939	191.7E6	49755591	18.489	18.874
27)	SA Decachlor...	7.995	8.975	371.8E6	95307900	34.889	34.960
Target Compounds							
15)	B Endosulfa...	0.000	6.859	0	4227659	N.D.	1.501


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050919\
Data File : PL048354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2019 23:30
Operator : AJ\SJ
Sample : PB119537BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PBLK37

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 01:51:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 10 01:24:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

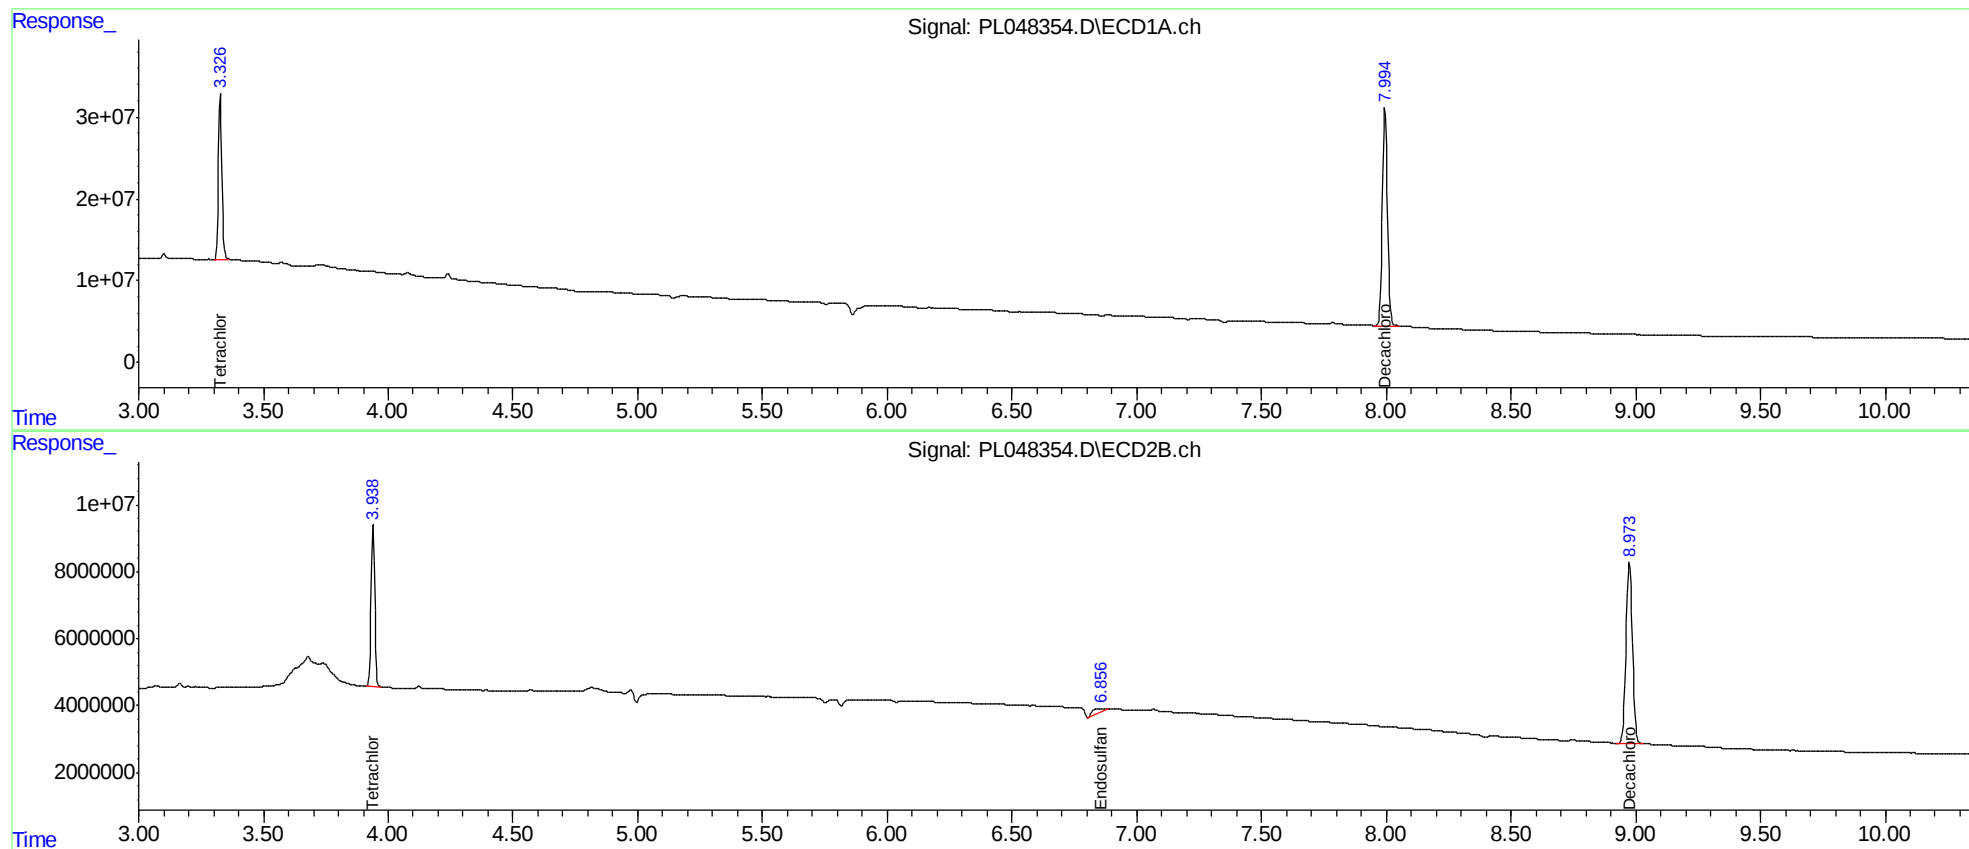


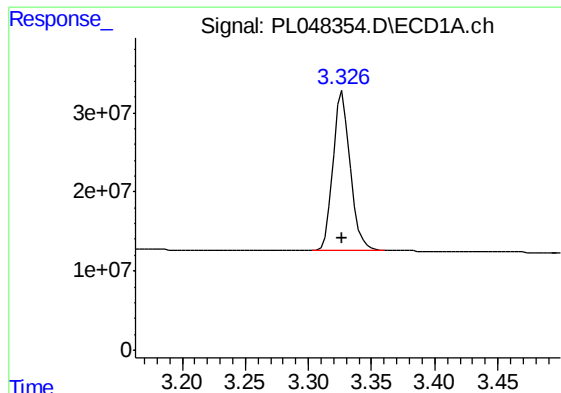

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 191698497
Conc: 18.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PBLK37

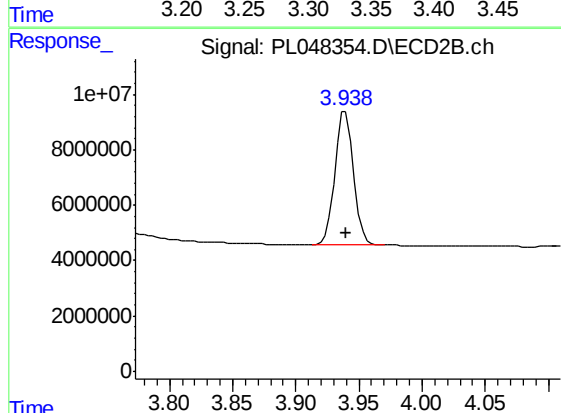


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 49755591
Conc: 18.87 ng/ml

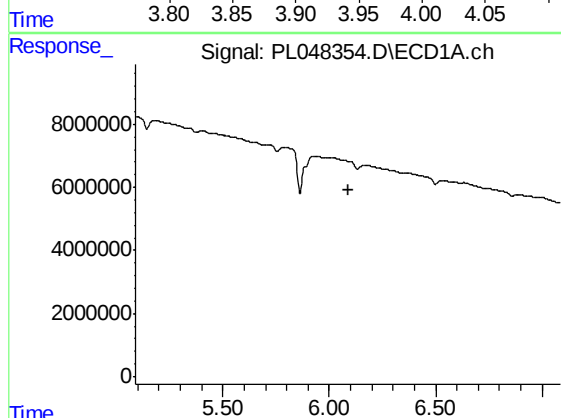


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

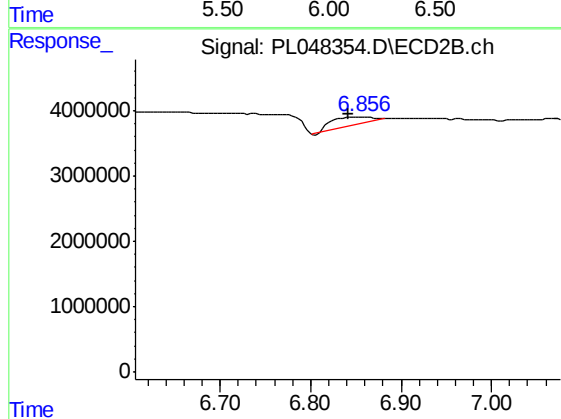

#15 Endosulfan II


R.T.: 6.859 min
Delta R.T.: 0.016 min
Response: 4227659
Conc: 1.50 ng/ml

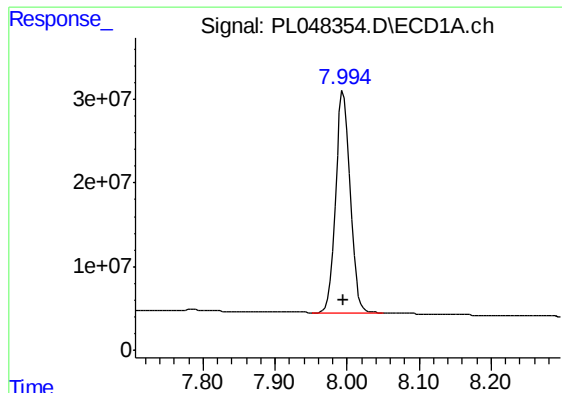

#27 Decachlorobiphenyl

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 371783651
Conc: 34.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PBLK37

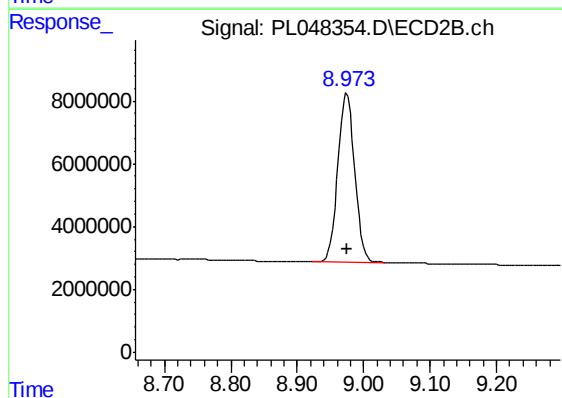

#27 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 95307900
Conc: 34.96 ng/ml