

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050925\
 Data File : PL095619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2025 19:40
 Operator : AR\AJ
 Sample : Q1983-37
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 23:18:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.593	2.907	65254818	81465880	19.988	25.620 #
28)	SA Decachlor...	9.117	8.085	53680818	70046160	19.374	23.670
Target Compounds							
10)	B gamma-Chl...	5.989	5.144	5858695	5949583	1.436	1.468
11)	B alpha-Chl...	6.075	5.209	14544300	7407939	3.577	1.861 #
25)	Chlordane-3	5.989	5.144	5858695	5949583	7.521	11.516 #
26)	Chlordane-4	6.075	5.209	14544300	7407939	15.425	17.045


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050925\
Data File : PL095619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2025 19:40
Operator : AR\AJ
Sample : Q1983-37
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 23:18:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

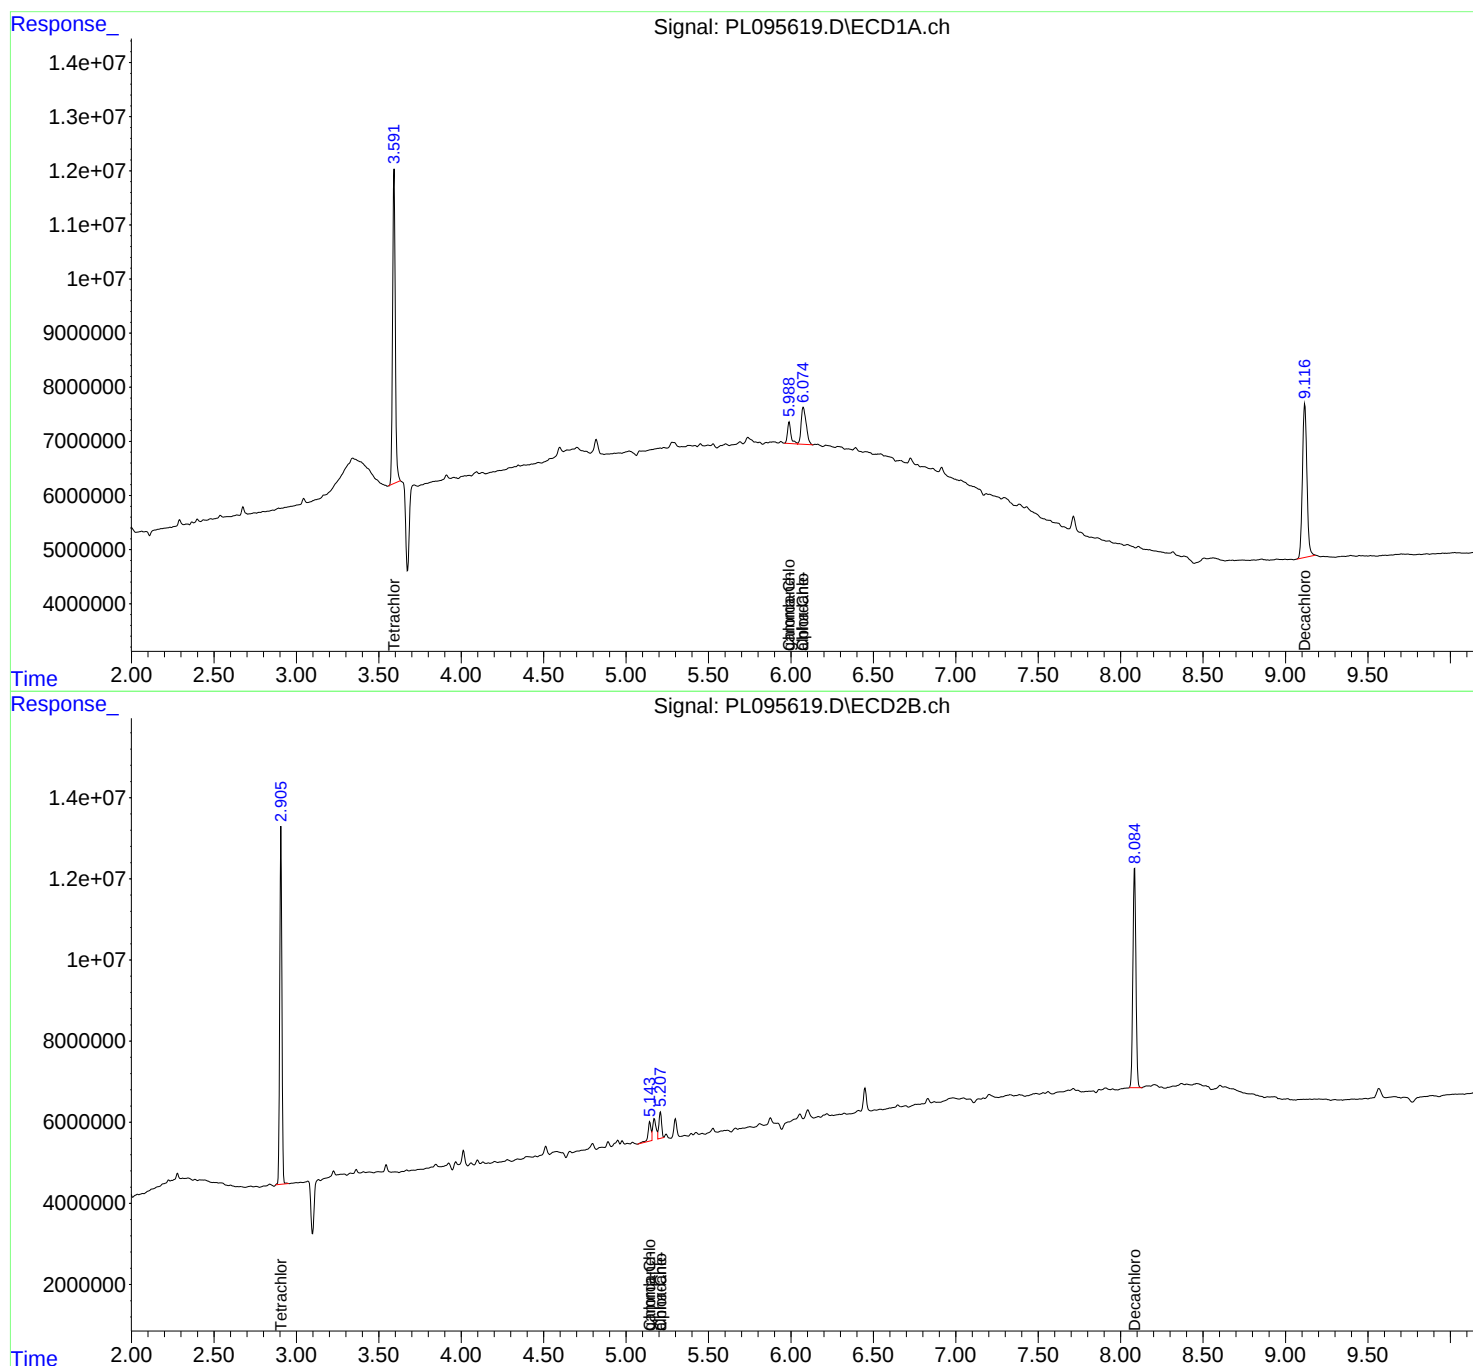


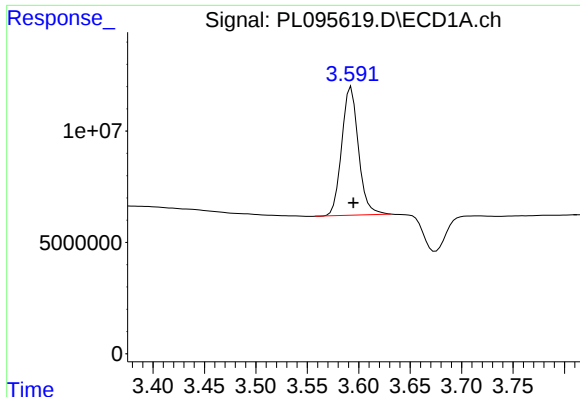

#1 Tetrachloro-m-xylene


R.T.: 3.593 min
Delta R.T.: -0.002 min
Response: 65254818
Conc: 19.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

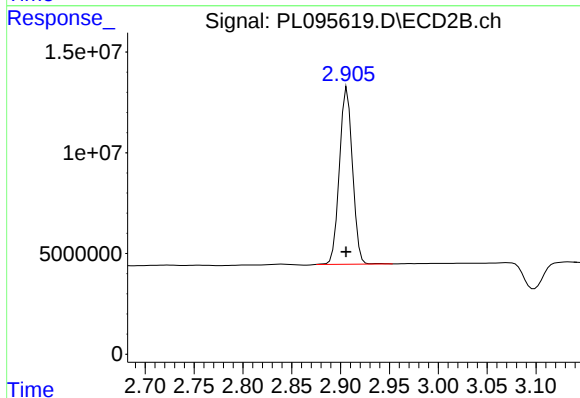


#1 Tetrachloro-m-xylene

R.T.: 2.907 min
Delta R.T.: 0.001 min
Response: 81465880
Conc: 25.62 ng/ml

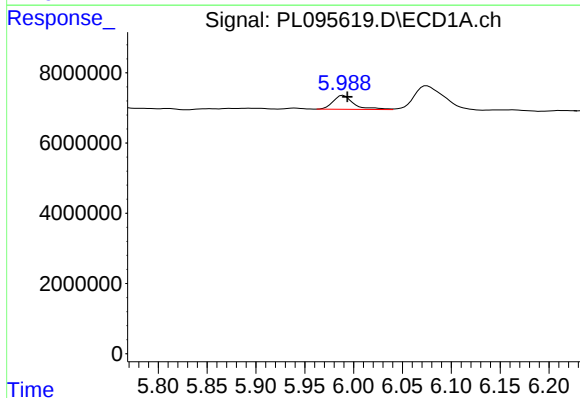


#10 gamma-Chlordane

R.T.: 5.989 min
Delta R.T.: -0.004 min
Response: 5858695
Conc: 1.44 ng/ml

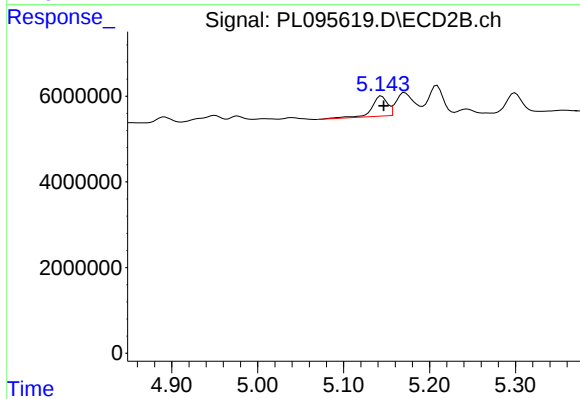

#10 gamma-Chlordane


R.T.: 5.144 min
Delta R.T.: -0.002 min
Response: 5949583
Conc: 1.47 ng/ml

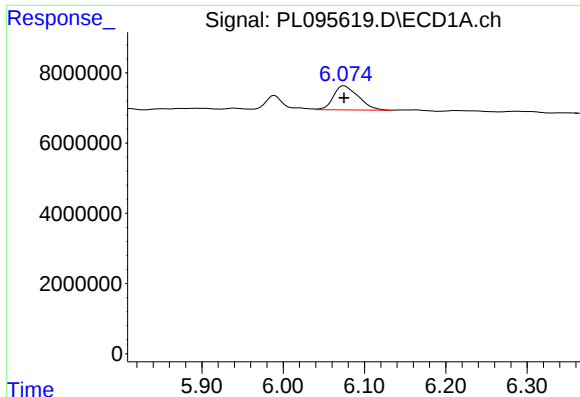

#11 alpha-Chlordane


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 14544300
Conc: 3.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

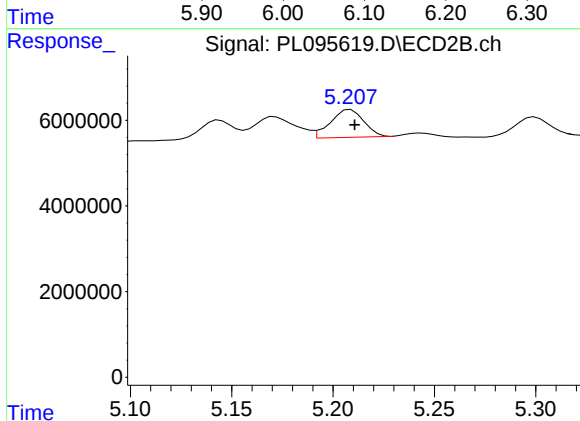


#11 alpha-Chlordane

R.T.: 5.209 min
Delta R.T.: -0.002 min
Response: 7407939
Conc: 1.86 ng/ml

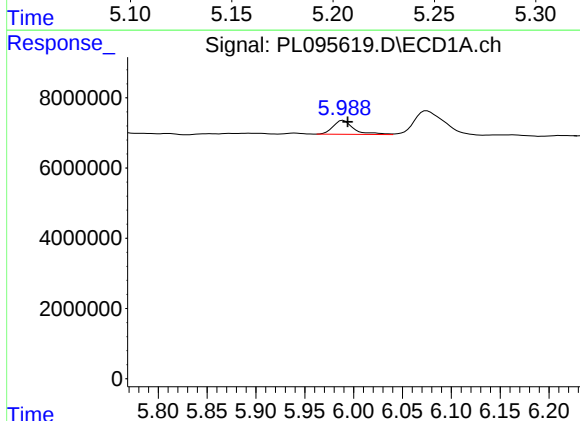


#25 Chlordane-3

R.T.: 5.989 min
Delta R.T.: -0.004 min
Response: 5858695
Conc: 7.52 ng/ml

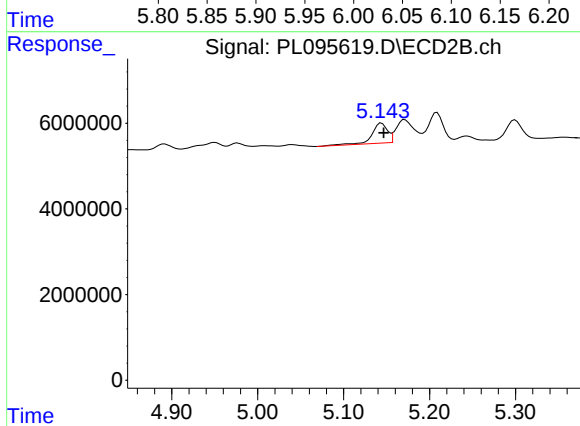

#25 Chlordane-3


R.T.: 5.144 min
Delta R.T.: -0.002 min
Response: 5949583
Conc: 11.52 ng/ml

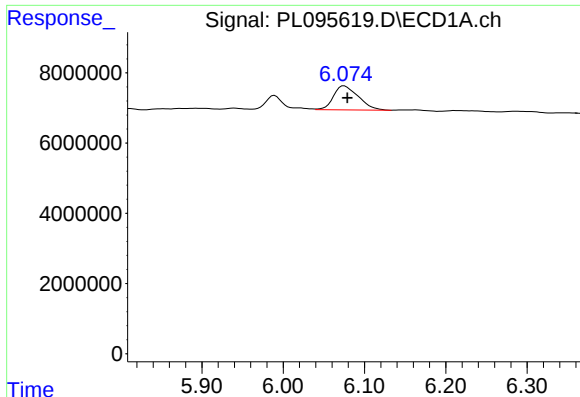

#26 Chlordane-4


R.T.: 6.075 min
Delta R.T.: -0.004 min
Response: 14544300
Conc: 15.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

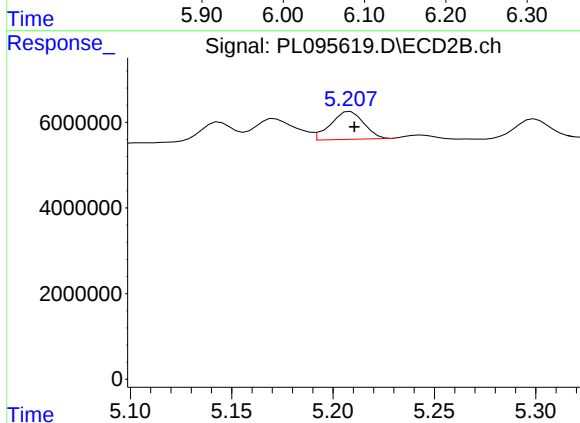


#26 Chlordane-4

R.T.: 5.209 min
Delta R.T.: -0.002 min
Response: 7407939
Conc: 17.04 ng/ml

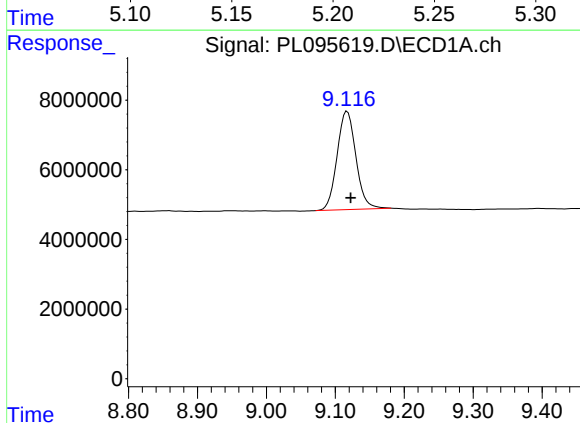

#28 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: -0.005 min
Response: 53680818
Conc: 19.37 ng/ml

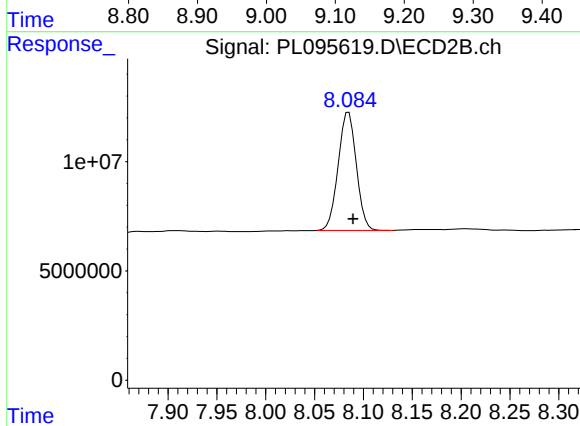

#28 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: -0.005 min
Response: 70046160
Conc: 23.67 ng/ml