

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050925\
 Data File : PL095620.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2025 19:53
 Operator : AR\AJ
 Sample : Q1983-43
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 23:18:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.593	2.907	61107893	76416190	18.718	24.032 #
28)	SA Decachlor...	9.118	8.085	48076676	62712822	17.351	21.192
Target Compounds							
6)	B beta-BHC	0.000	4.015f	0	13920135	N.D.	6.706 #
7)	B delta-BHC	4.820	0.000	2814227	0	0.605	N.D. #
10)	B gamma-Chl...	0.000	5.171f	0	9477433	N.D.	2.339 #
11)	B alpha-Chl...	6.084	0.000	15216521	0	3.742	N.D. #
15)	B Endosulfa...	0.000	6.095	0	8862594	N.D.	2.468 #
25)	Chlordane-3	0.000	5.171f	0	9477433	N.D.	18.345 #
26)	Chlordane-4	6.084	0.000	15216521	0	16.138	N.D. #
27)	Chlordane-5	0.000	6.095	0	8862594	N.D.	47.974 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050925\
Data File : PL095620.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2025 19:53
Operator : AR\AJ
Sample : Q1983-43
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 23:18:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

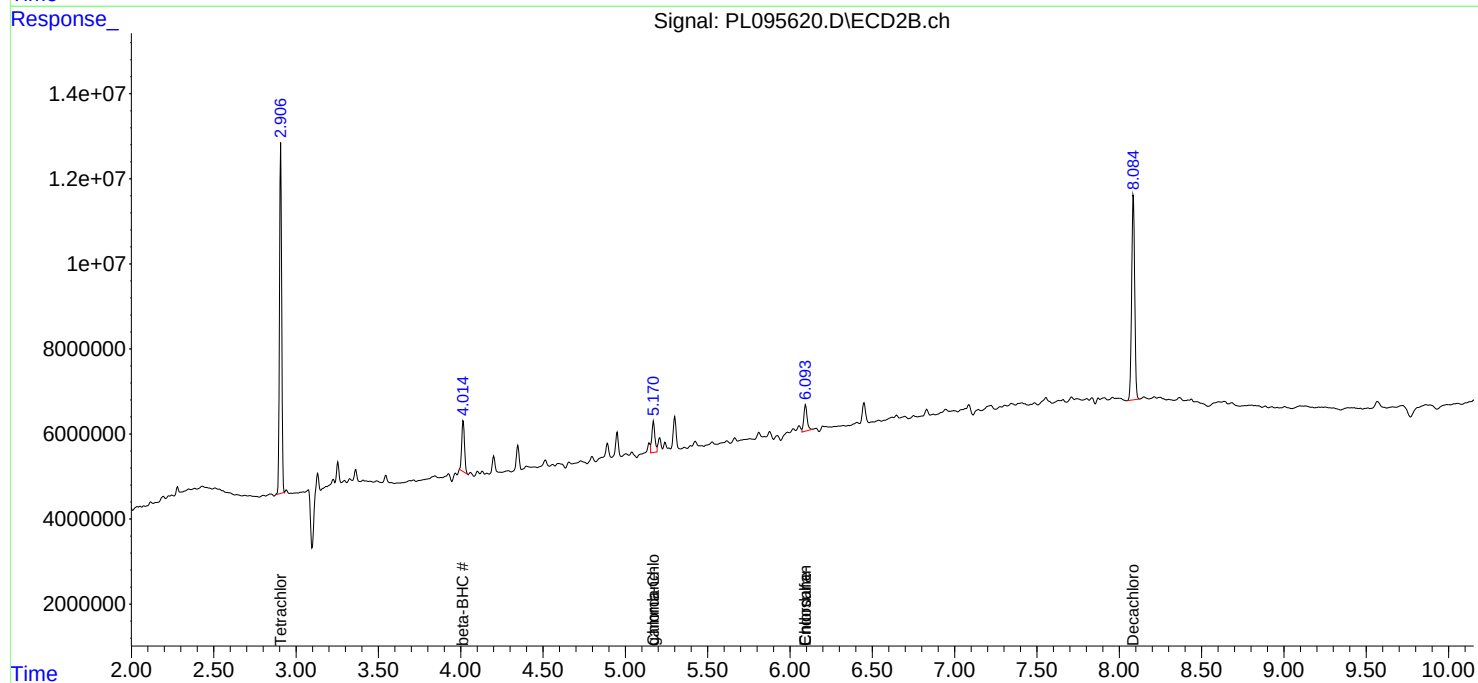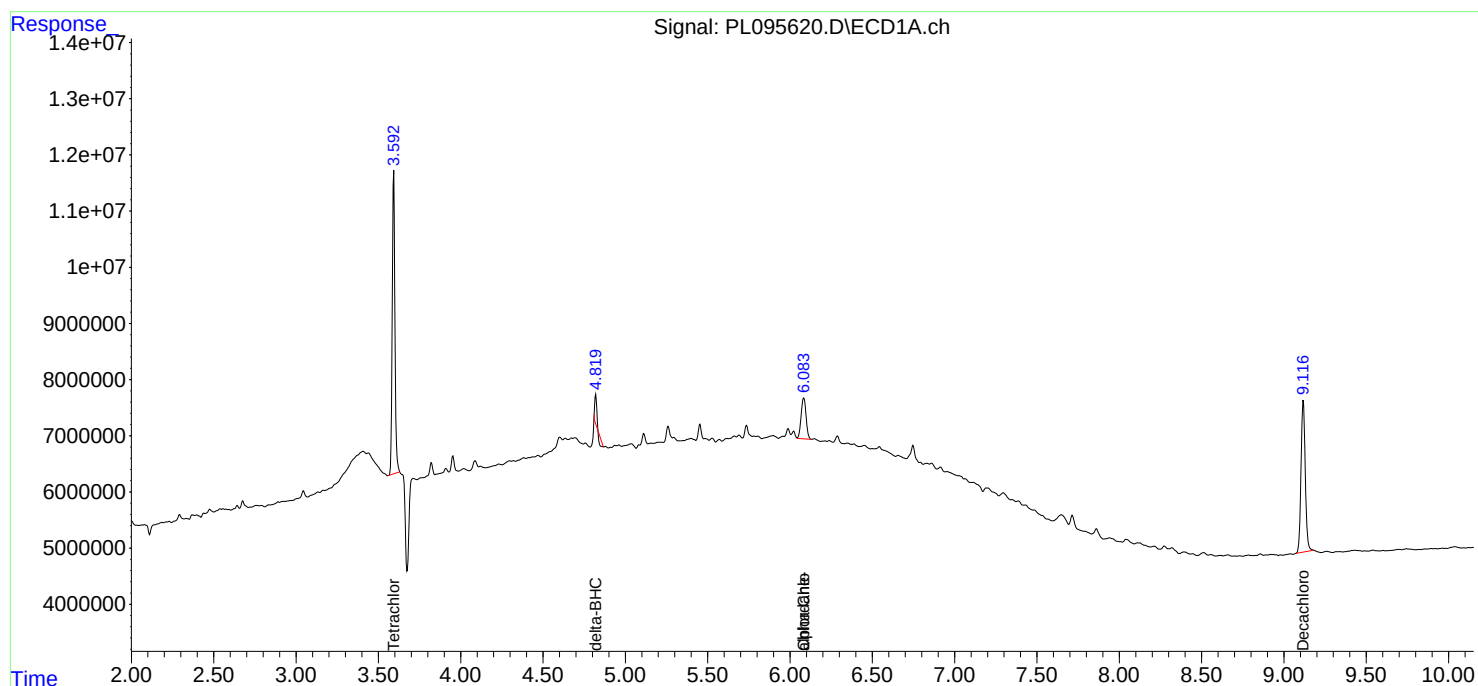


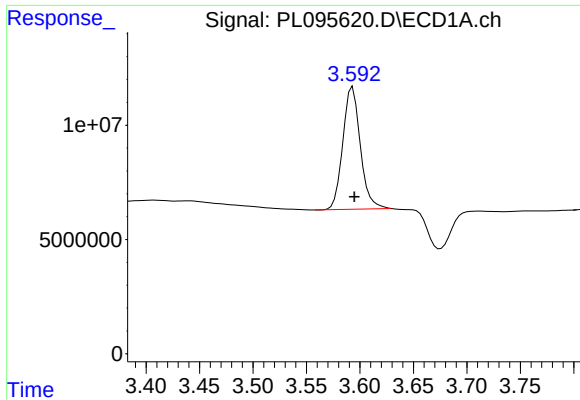

#1 Tetrachloro-m-xylene


R.T.: 3.593 min
Delta R.T.: -0.002 min
Response: 61107893
Conc: 18.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

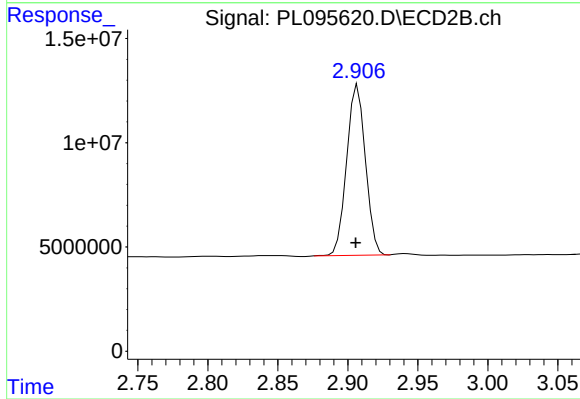


#1 Tetrachloro-m-xylene

R.T.: 2.907 min
Delta R.T.: 0.001 min
Response: 76416190
Conc: 24.03 ng/ml

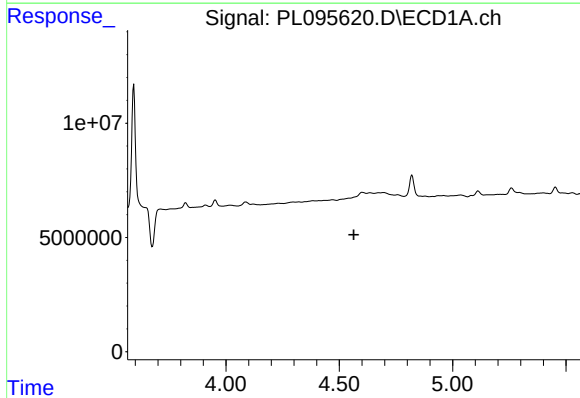


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.564 min
Response: 0
Conc: N.D.

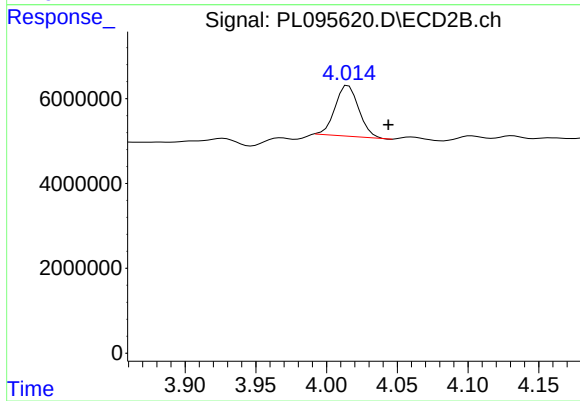

#6 beta-BHC


R.T.: 4.015 min
Delta R.T.: -0.028 min
Response: 13920135
Conc: 6.71 ng/ml

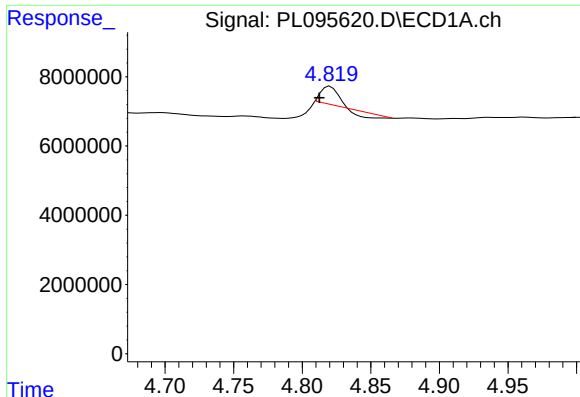

#7 delta-BHC


R.T.: 4.820 min
Delta R.T.: 0.008 min
Response: 2814227
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

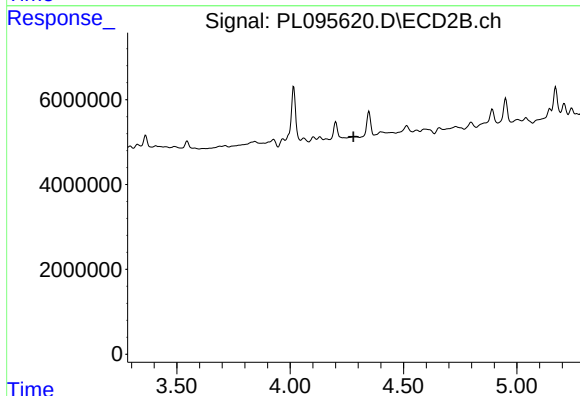


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.280 min
Response: 0
Conc: N.D.

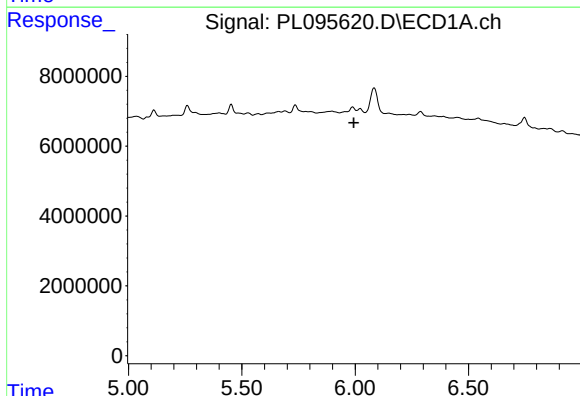


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.994 min
Response: 0
Conc: N.D.

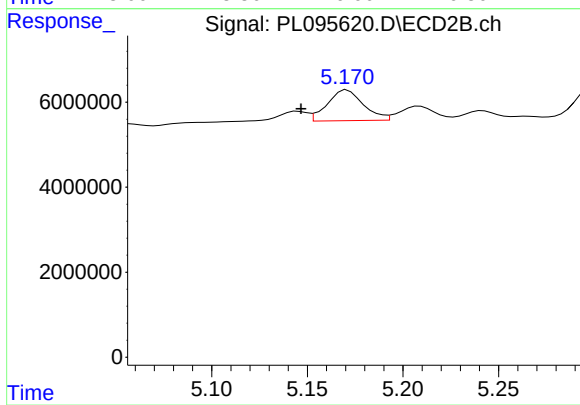

#10 gamma-Chlordane


R.T.: 5.171 min
Delta R.T.: 0.024 min
Response: 9477433
Conc: 2.34 ng/ml

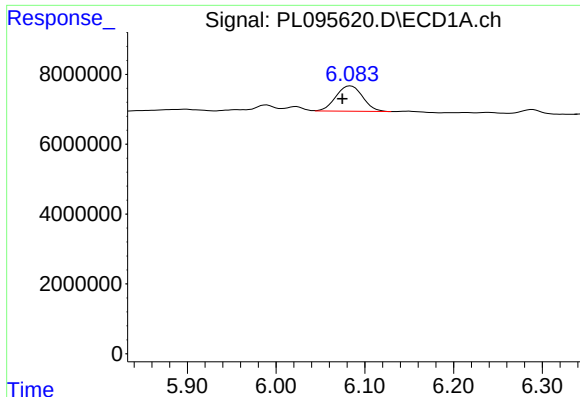

#11 alpha-Chlordane


R.T.: 6.084 min
Delta R.T.: 0.009 min
Response: 15216521
Conc: 3.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

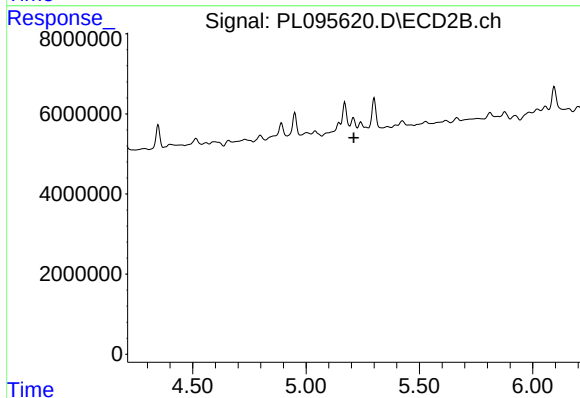


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.211 min
Response: 0
Conc: N.D.

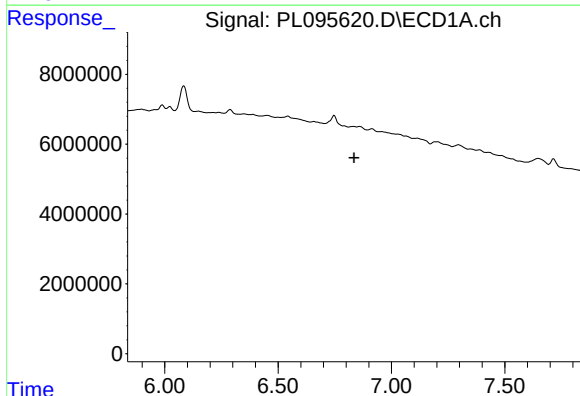


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.835 min
Response: 0
Conc: N.D.

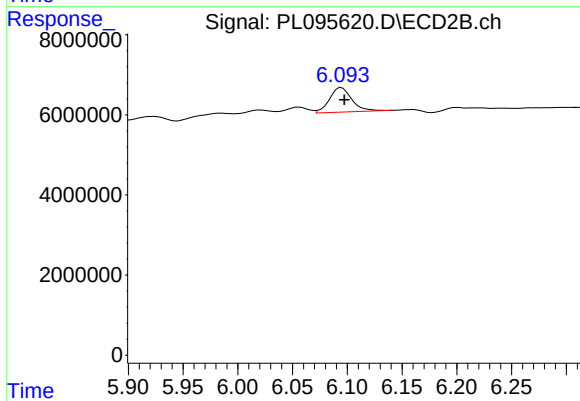

#15 Endosulfan II


R.T.: 6.095 min
Delta R.T.: -0.003 min
Response: 8862594
Conc: 2.47 ng/ml

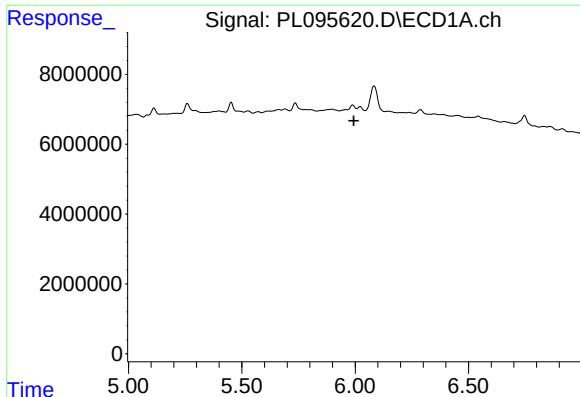

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.994 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

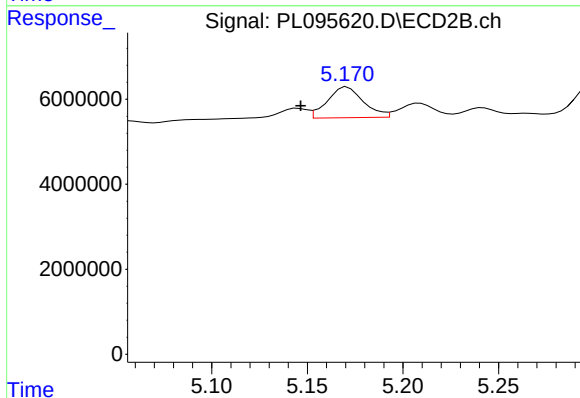


#25 Chlordane-3

R.T.: 5.171 min
Delta R.T.: 0.024 min
Response: 9477433
Conc: 18.35 ng/ml

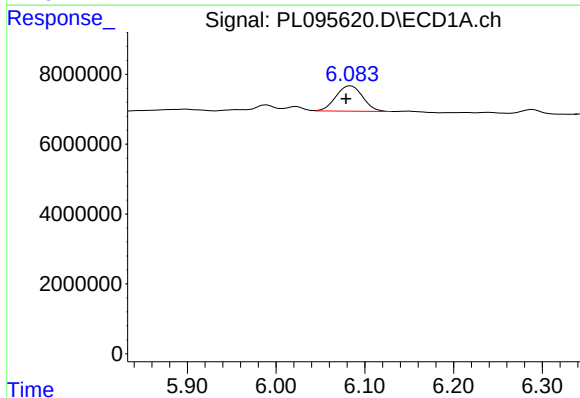


#26 Chlordane-4

R.T.: 6.084 min
Delta R.T.: 0.005 min
Response: 15216521
Conc: 16.14 ng/ml

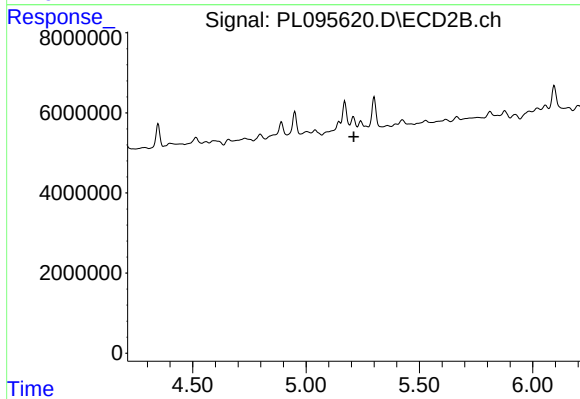

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.211 min
Response: 0
Conc: N.D.

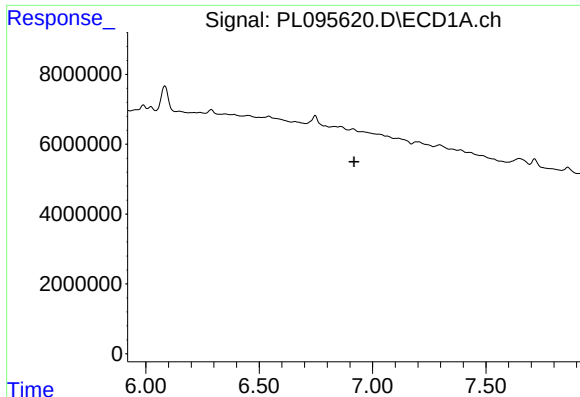

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

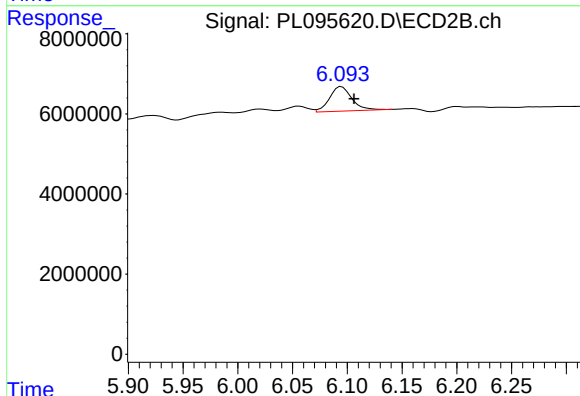


#27 Chlordane-5

R.T.: 6.095 min
Delta R.T.: -0.012 min
Response: 8862594
Conc: 47.97 ng/ml

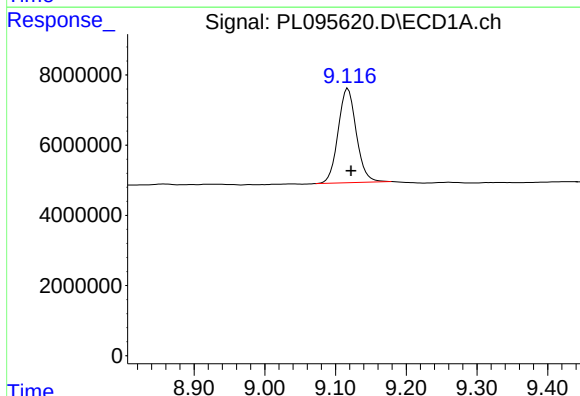

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.005 min
Response: 48076676
Conc: 17.35 ng/ml

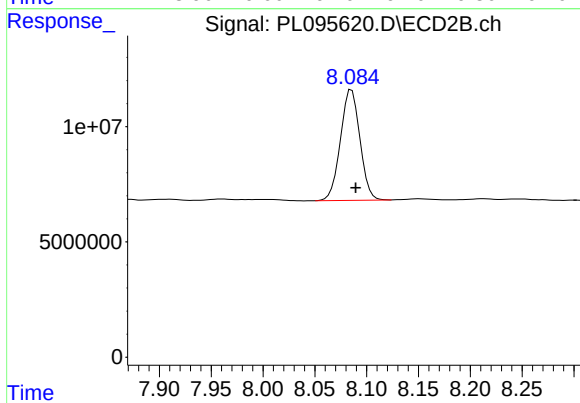

#28 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: -0.004 min
Response: 62712822
Conc: 21.19 ng/ml