

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050925\
 Data File : PL095625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2025 21:02
 Operator : AR\AJ
 Sample : Q1986-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 23:18:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.593	2.907	63091327	77101582	19.325	24.248 #
28)	SA Decachlor...	9.116	8.085	48906798	57112964	17.651	19.300
Target Compounds							
15)	B Endosulfa...	0.000	6.093	0	3410429	N.D.	0.950 #
27)	Chlordane-5	0.000	6.093	0	3410429	N.D.	18.461 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050925\
Data File : PL095625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2025 21:02
Operator : AR\AJ
Sample : Q1986-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 23:18:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

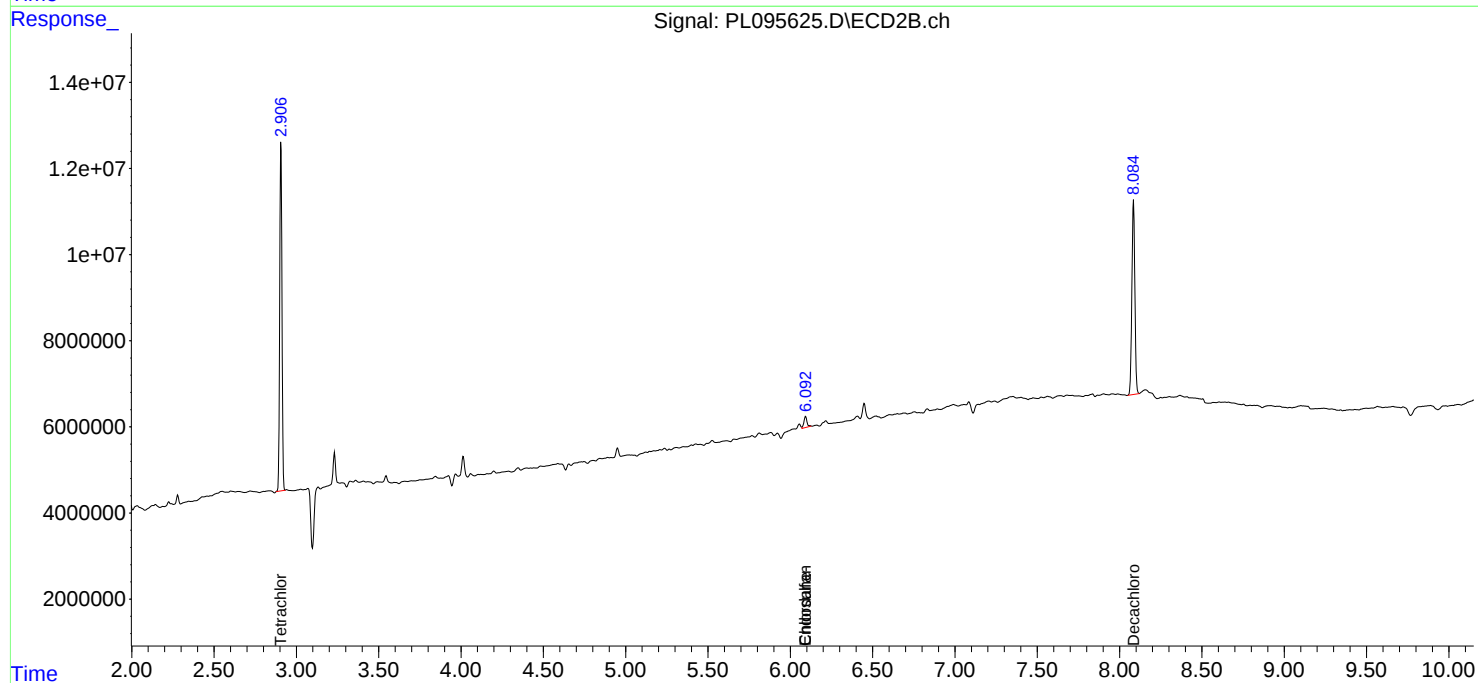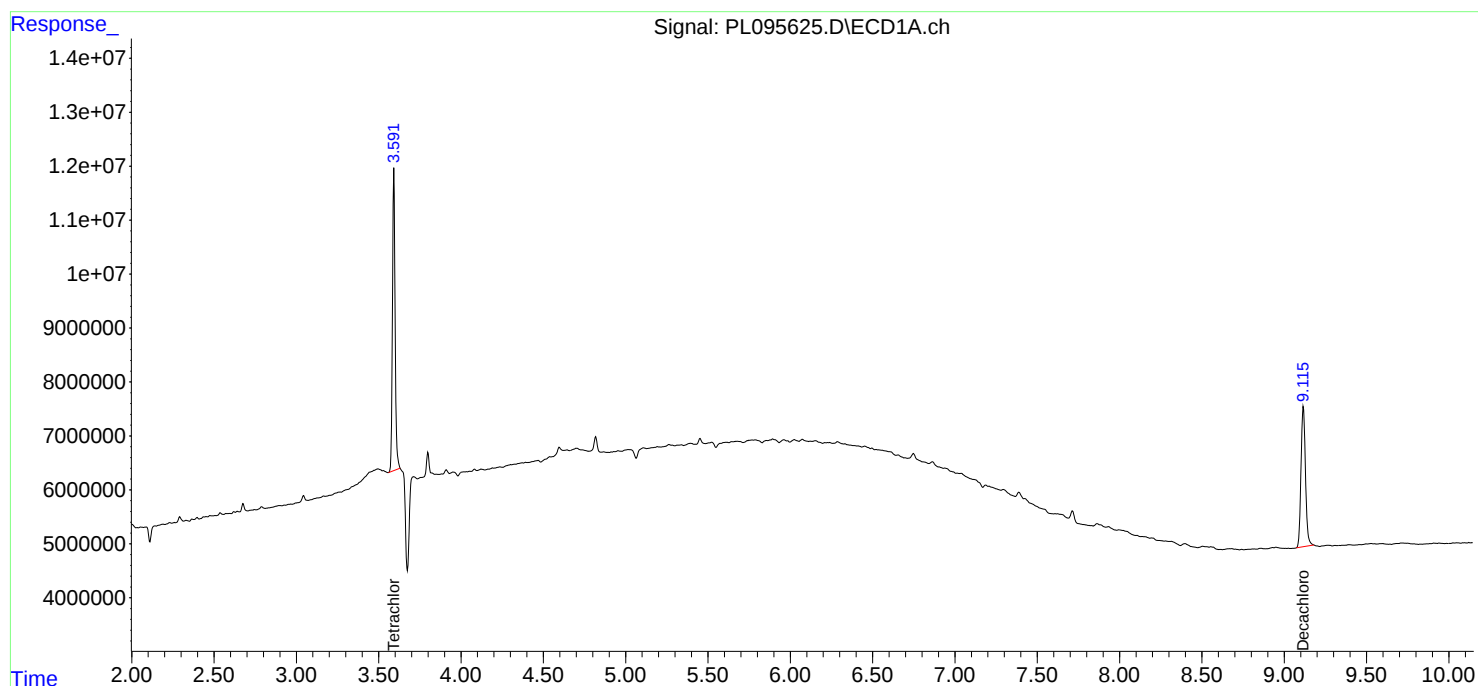


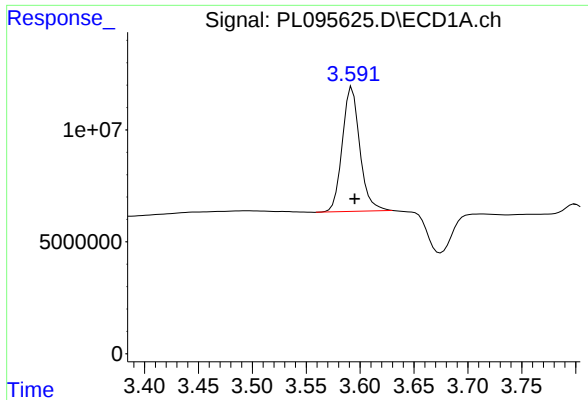

#1 Tetrachloro-m-xylene


R.T.: 3.593 min
Delta R.T.: -0.002 min
Response: 63091327
Conc: 19.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

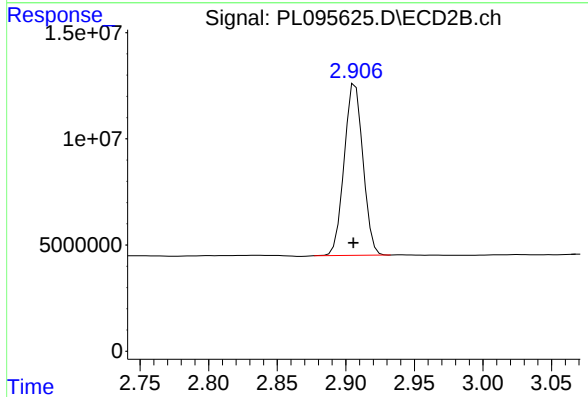


#1 Tetrachloro-m-xylene

R.T.: 2.907 min
Delta R.T.: 0.001 min
Response: 77101582
Conc: 24.25 ng/ml

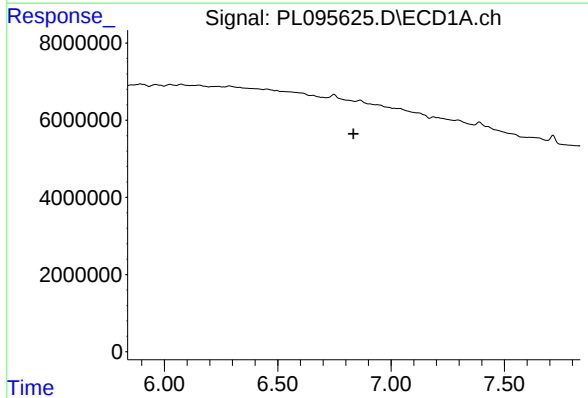


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.835 min
Response: 0
Conc: N.D.

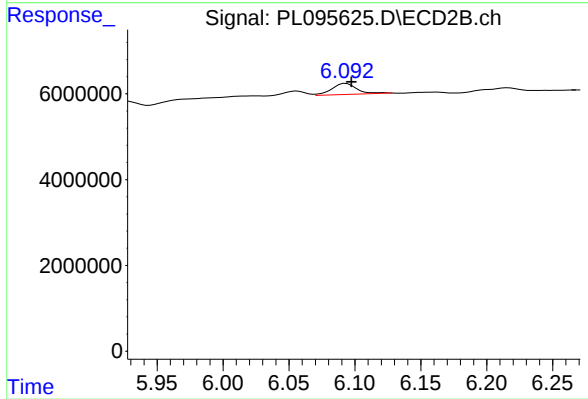

#15 Endosulfan II


R.T.: 6.093 min
Delta R.T.: -0.004 min
Response: 3410429
Conc: 0.95 ng/ml

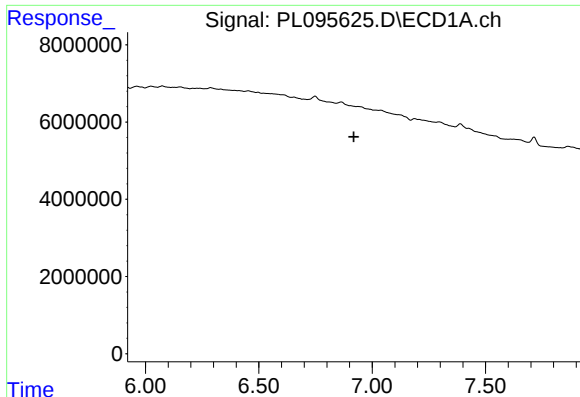

#27 Chlorine-5


R.T.: 0.000 min
Exp R.T.: 6.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

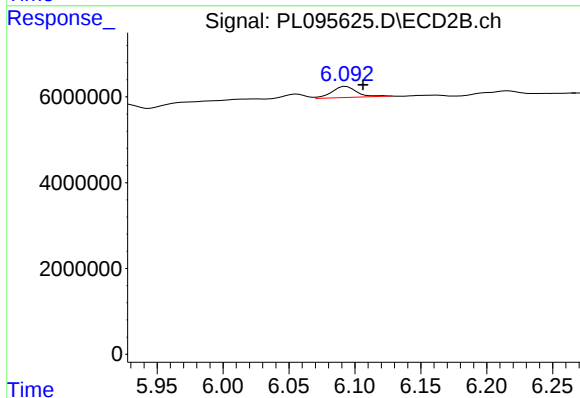


#27 Chlorine-5

R.T.: 6.093 min
Delta R.T.: -0.013 min
Response: 3410429
Conc: 18.46 ng/ml

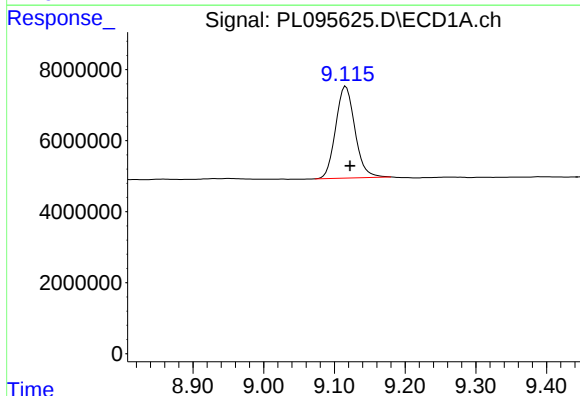

#28 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: -0.006 min
Response: 48906798
Conc: 17.65 ng/ml

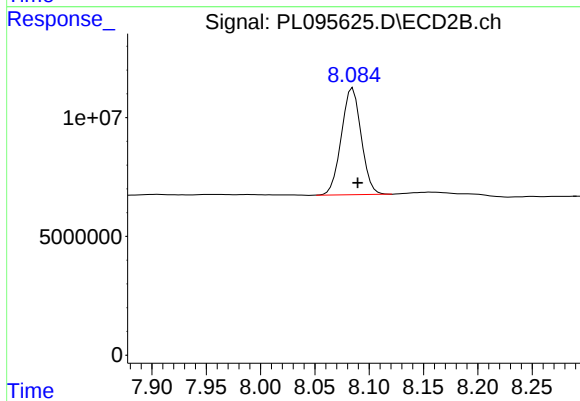

#28 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: -0.005 min
Response: 57112964
Conc: 19.30 ng/ml