

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050925\
 Data File : PL095626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 May 2025 21:16
 Operator : AR\AJ
 Sample : Q1986-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 23:19:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.593	2.907	62410838	75223361	19.117	23.657
28)	SA Decachlor...	9.118	8.084	51167574	58950961	18.467	19.921
Target Compounds							
15)	B Endosulfa...	0.000	6.085	0	5189386	N.D.	1.445 #
27)	Chlordane-5	0.000	6.085f	0	5189386	N.D.	28.090 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL050925\
Data File : PL095626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 May 2025 21:16
Operator : AR\AJ
Sample : Q1986-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 23:19:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

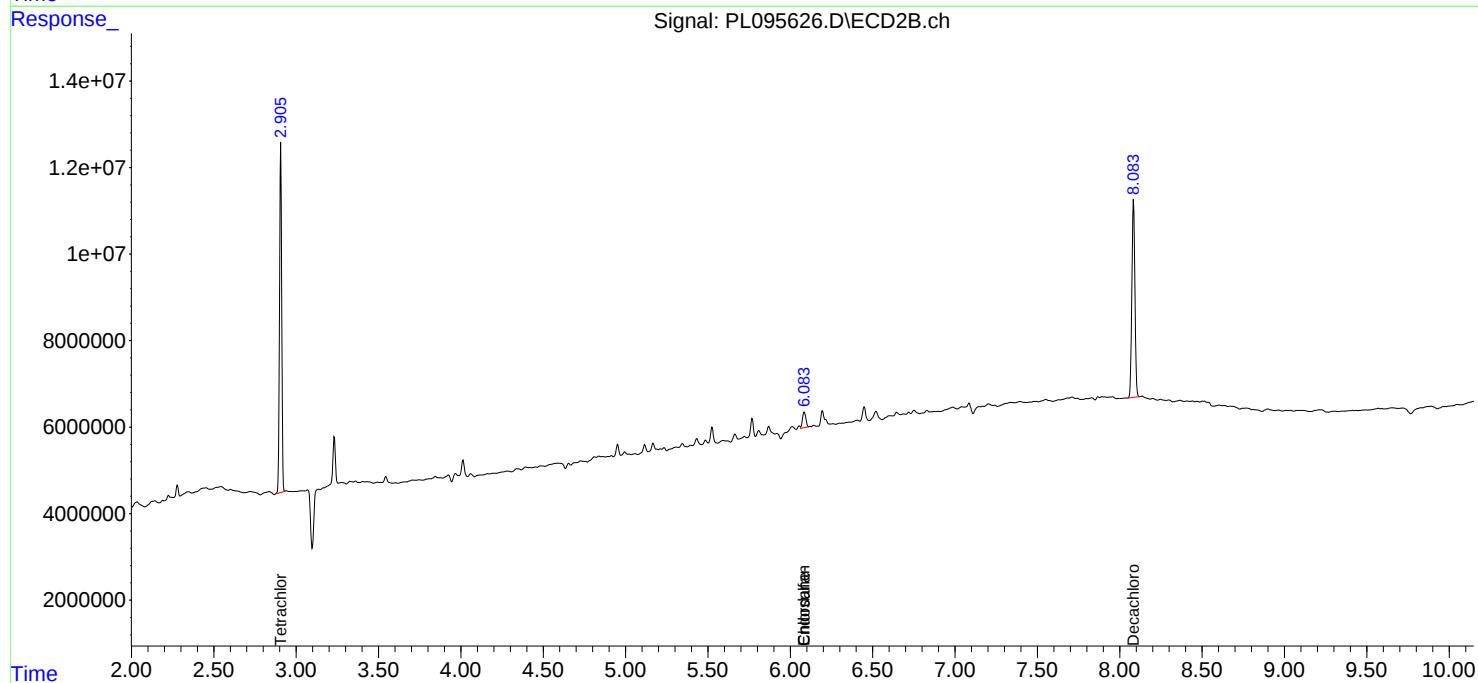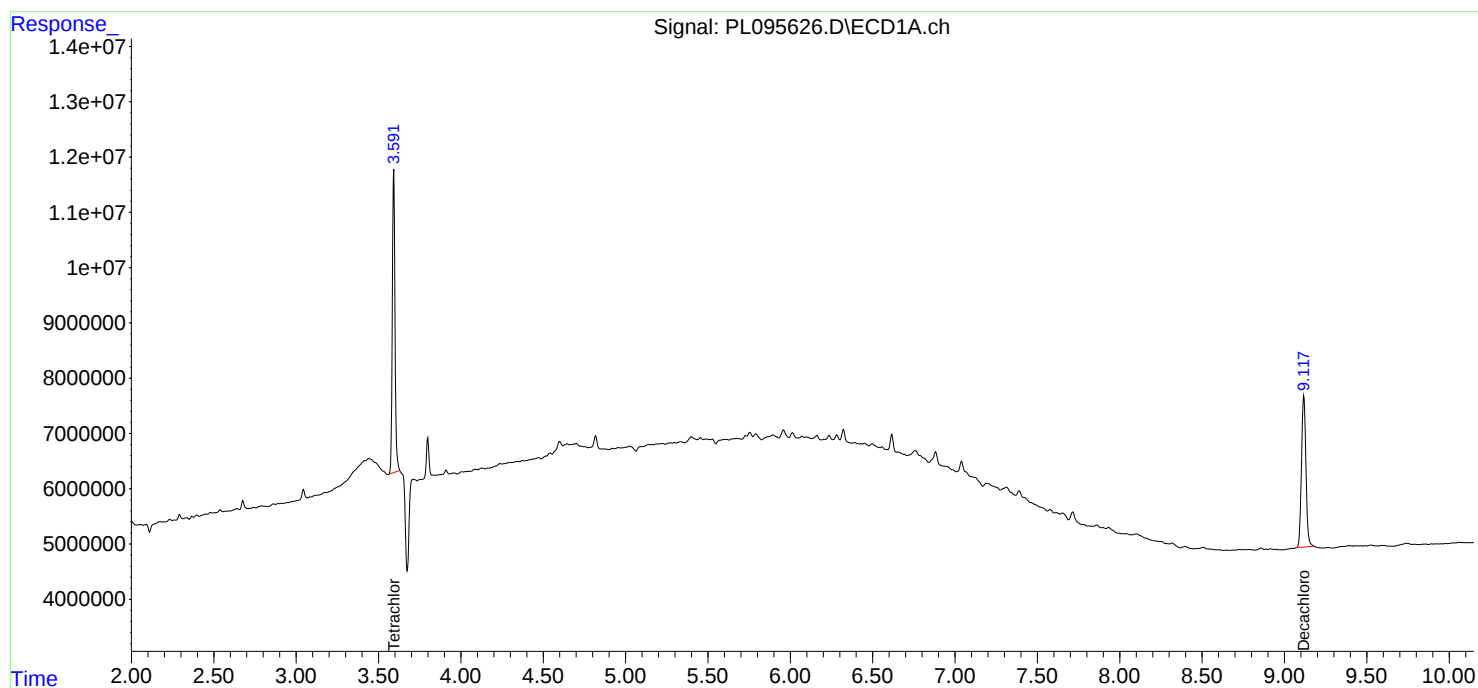


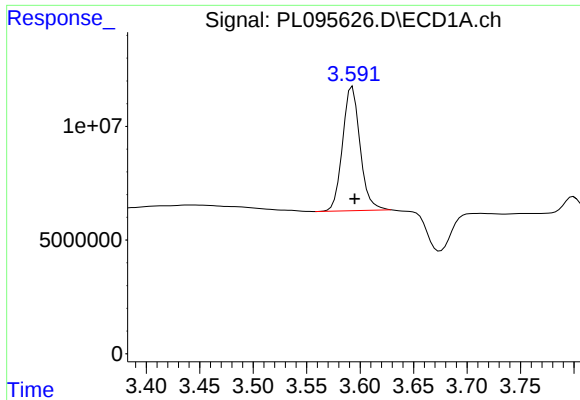

#1 Tetrachloro-m-xylene


R.T.: 3.593 min
Delta R.T.: -0.002 min
Response: 62410838
Conc: 19.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

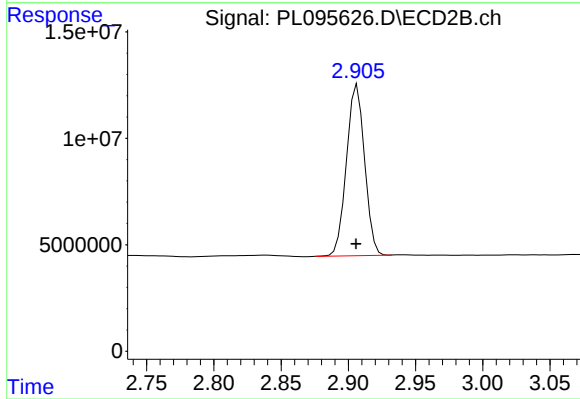


#1 Tetrachloro-m-xylene

R.T.: 2.907 min
Delta R.T.: 0.000 min
Response: 75223361
Conc: 23.66 ng/ml

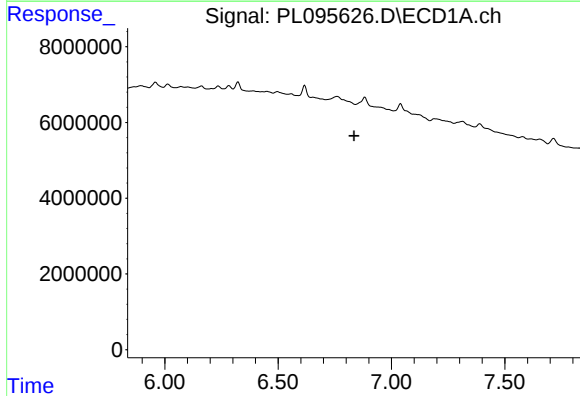


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.835 min
Response: 0
Conc: N.D.

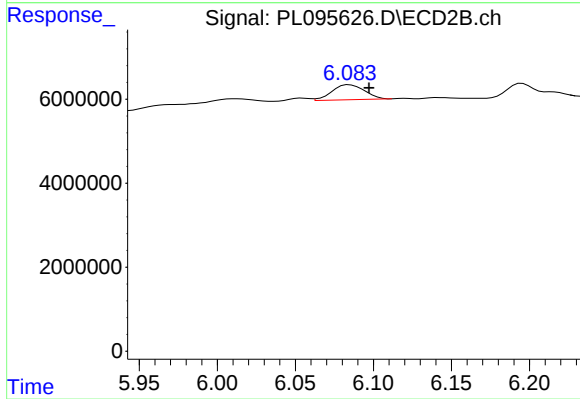

#15 Endosulfan II


R.T.: 6.085 min
Delta R.T.: -0.013 min
Response: 5189386
Conc: 1.45 ng/ml

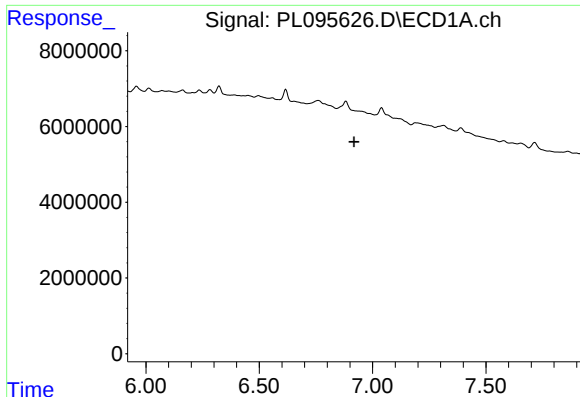

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

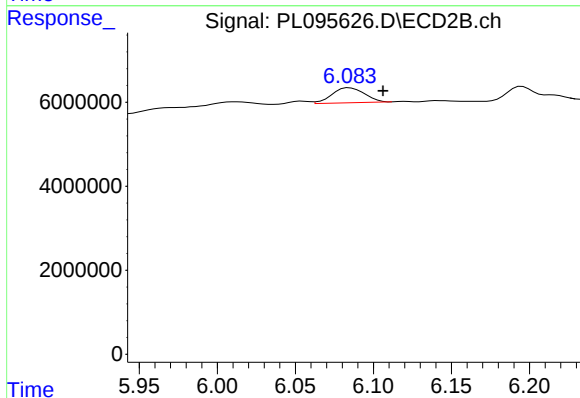


#27 Chlordane-5

R.T.: 6.085 min
Delta R.T.: -0.022 min
Response: 5189386
Conc: 28.09 ng/ml

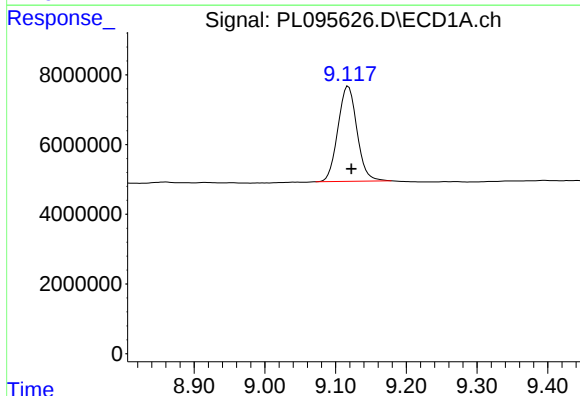

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.004 min
Response: 51167574
Conc: 18.47 ng/ml

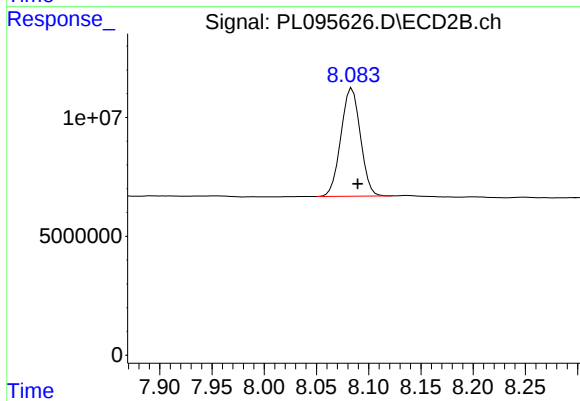

#28 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.005 min
Response: 58950961
Conc: 19.92 ng/ml