

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051019\
 Data File : PL048394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2019 11:15
 Operator : AJ\SJ
 Sample : K2746-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-5.8.19

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 22:58:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.940	73633903	19300654	7.601	7.749
28)	SA Decachlor...	7.996	8.976	135.5E6	36353961	13.480	13.696
Target Compounds							
10)	B gamma-Chl...	5.192f	0.000	5620718	0	0.421	N.D. #
13)	MA Dieldrin	5.561	0.000	10890068	0	0.836	N.D. #
14)	MA Endrin	5.785f	0.000	7925787	0	0.651	N.D. #
16)	A 4,4'-DDD	0.000	6.764	0	5397981	N.D.	2.405 #
17)	MA 4,4'-DDT	6.178	7.029f	13768019	2500942	1.370	1.066
18)	B Endrin al...	6.270	0.000	4748654	0	0.489	N.D. #
19)	B Endosulfa...	6.460	0.000	11830640	0	1.102	N.D. #
20)	A Methoxychlor	6.707f	0.000	22810492	0	4.189	N.D. #
21)	B Endrin ke...	6.977f	0.000	3476174	0	0.298	N.D. #
25)	Chlordane-3	5.192f	0.000	5620718	0	3.570	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051019\
Data File : PL048394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2019 11:15
Operator : AJ\SJ
Sample : K2746-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
COMP-5.8.19

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 22:58:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

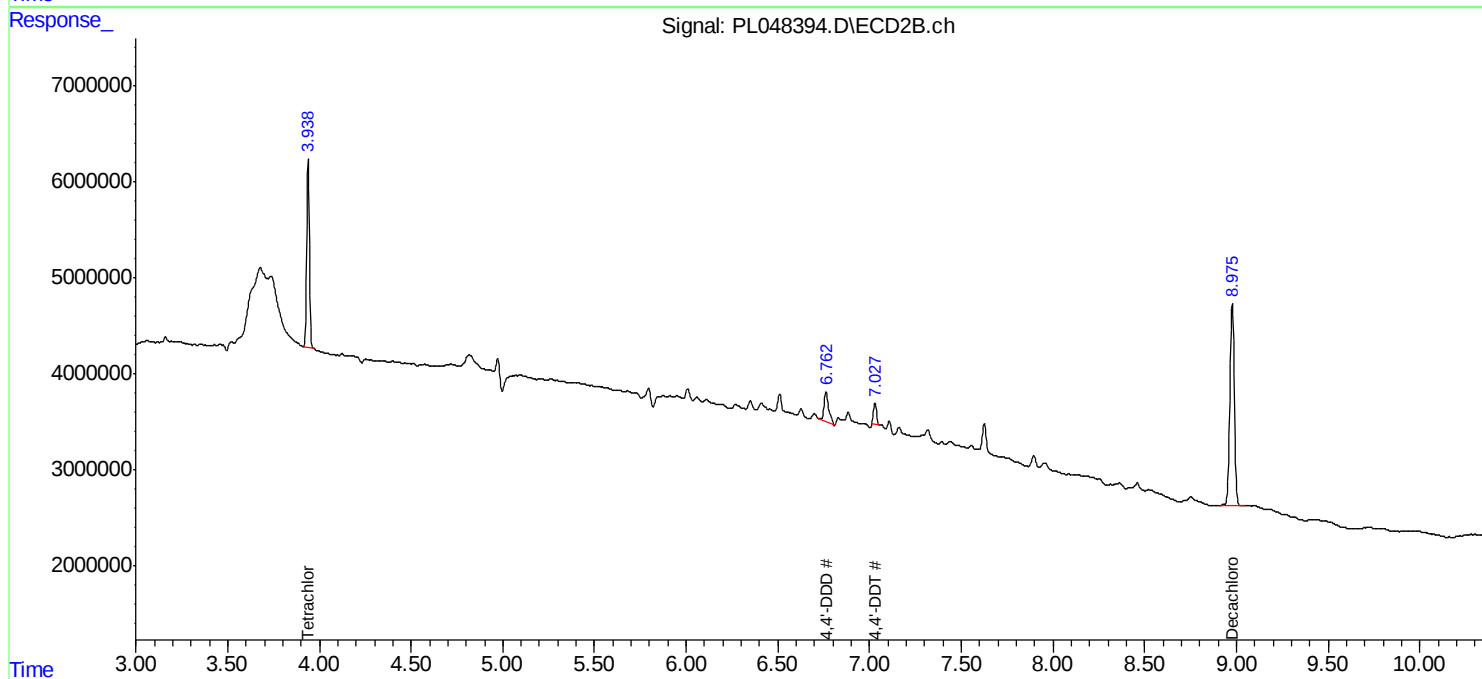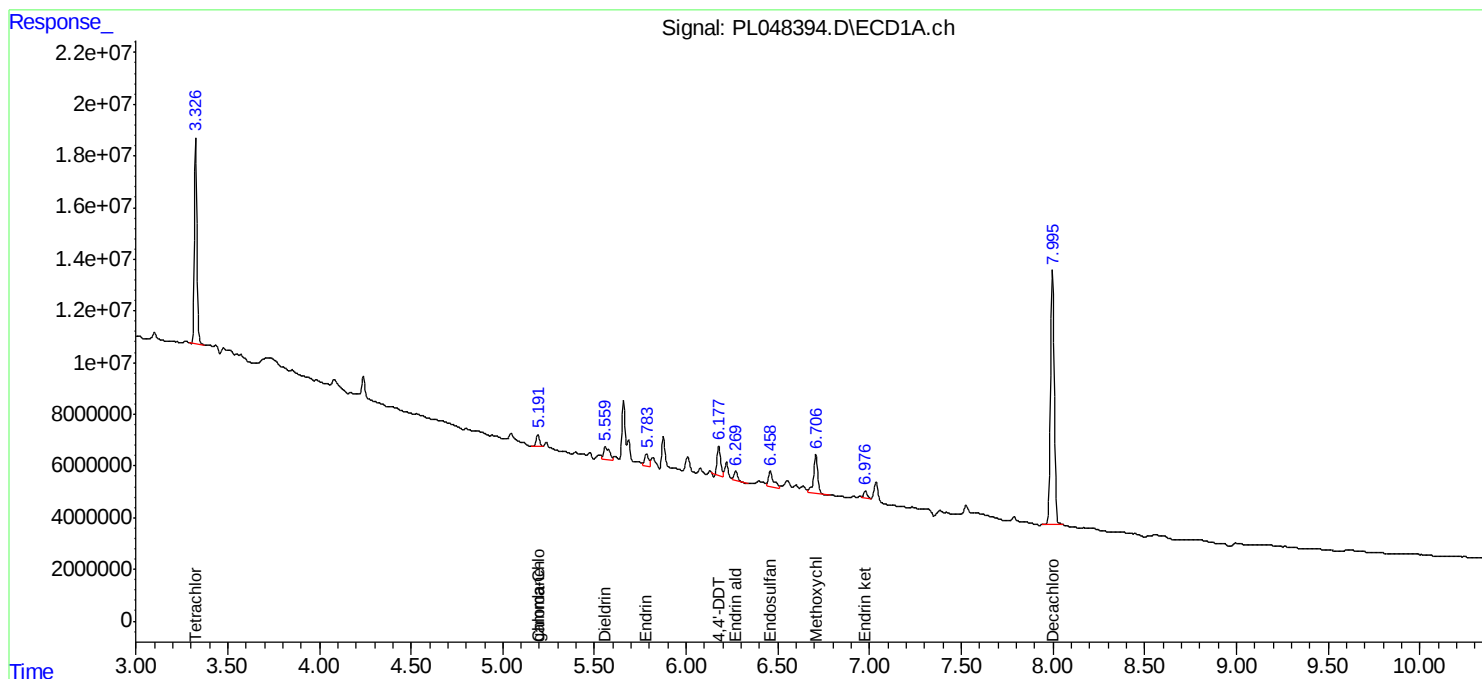


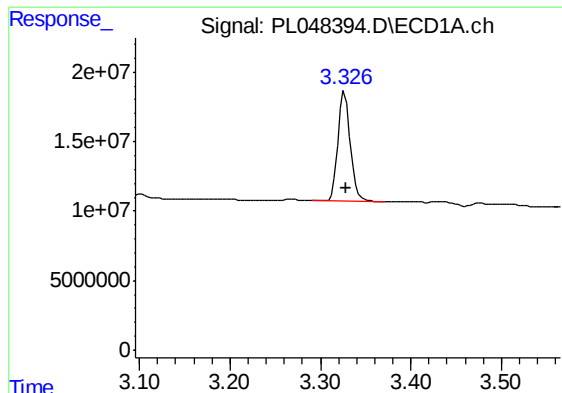

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: 0.000 min
Response: 73633903
Conc: 7.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-5.8.19

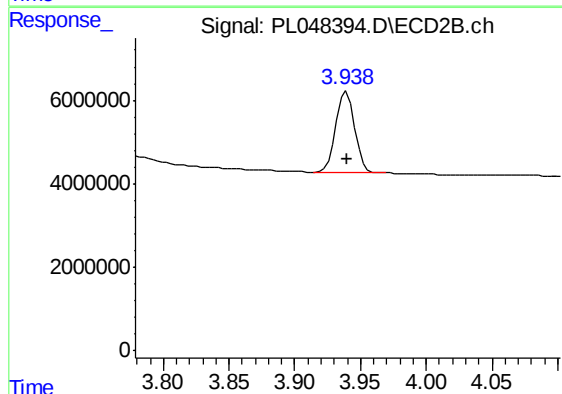


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 19300654
Conc: 7.75 ng/ml

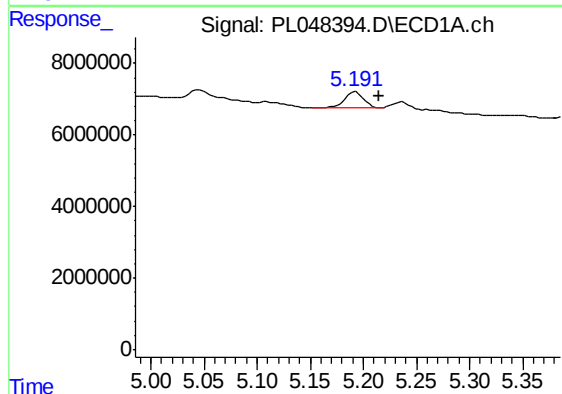


#10 gamma-Chlordane

R.T.: 5.192 min
Delta R.T.: -0.023 min
Response: 5620718
Conc: 0.42 ng/ml

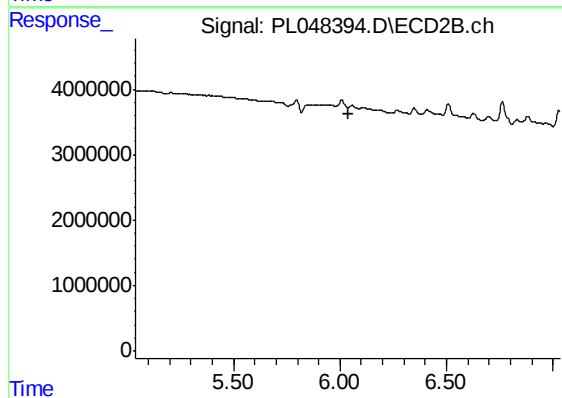

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

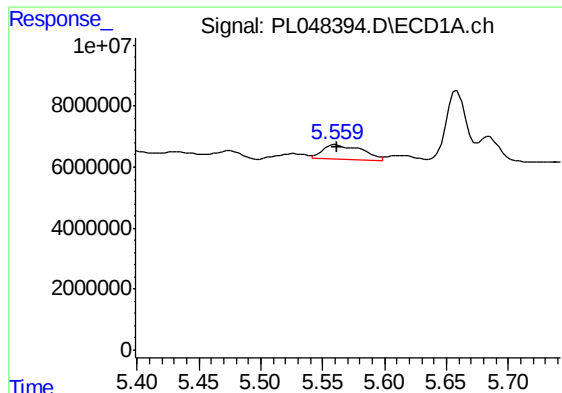

#13 Dieldrin


R.T.: 5.561 min
Delta R.T.: -0.001 min
Response: 10890068
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-5.8.19

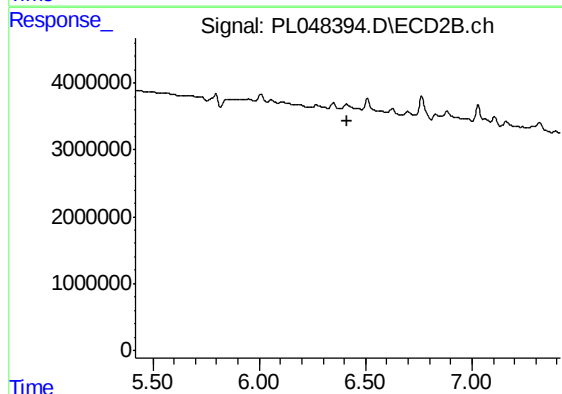


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

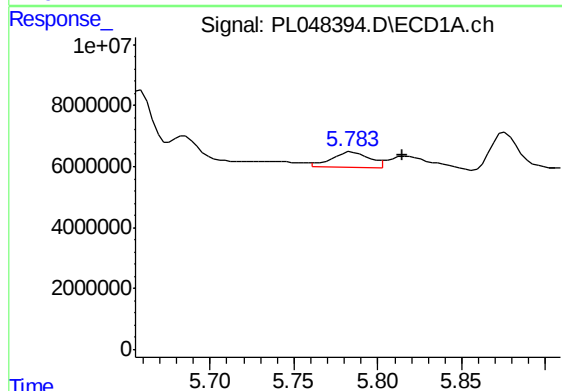


#14 Endrin

R.T.: 5.785 min
Delta R.T.: -0.030 min
Response: 7925787
Conc: 0.65 ng/ml

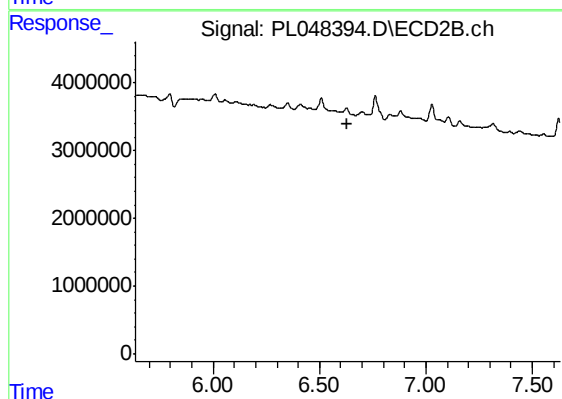

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

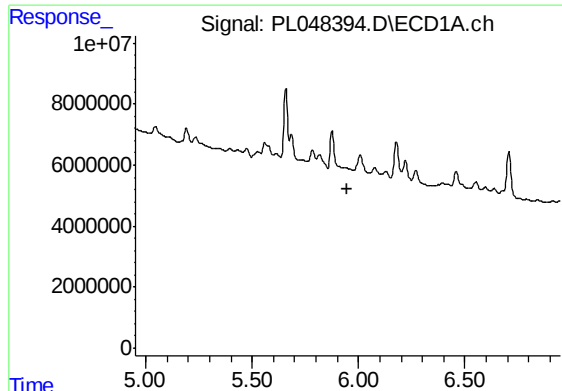

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-5.8.19

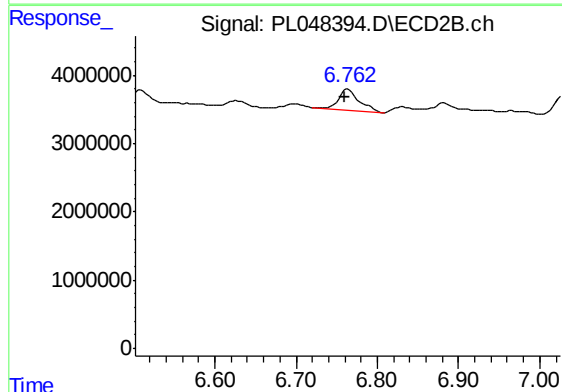


#16 4,4'-DDD

R.T.: 6.764 min
Delta R.T.: 0.004 min
Response: 5397981
Conc: 2.41 ng/ml

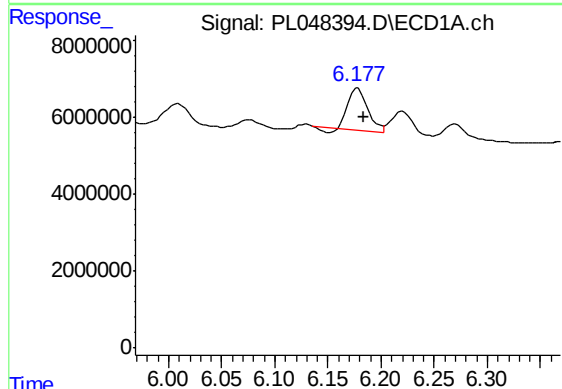


#17 4,4'-DDT

R.T.: 6.178 min
Delta R.T.: -0.006 min
Response: 13768019
Conc: 1.37 ng/ml

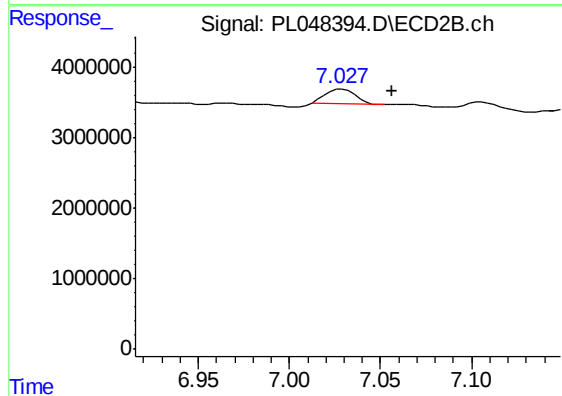

#17 4,4'-DDT


R.T.: 7.029 min
Delta R.T.: -0.028 min
Response: 2500942
Conc: 1.07 ng/ml

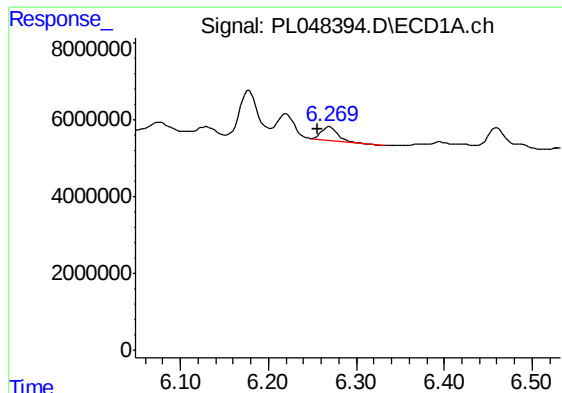

#18 Endrin aldehyde


R.T.: 6.270 min
Delta R.T.: 0.014 min
Response: 4748654
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-5.8.19

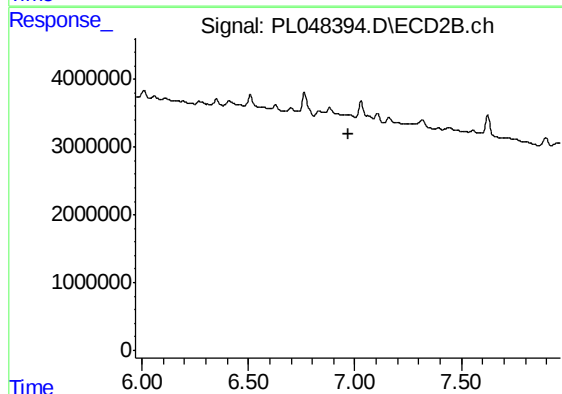


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.967 min
Response: 0
Conc: N.D.

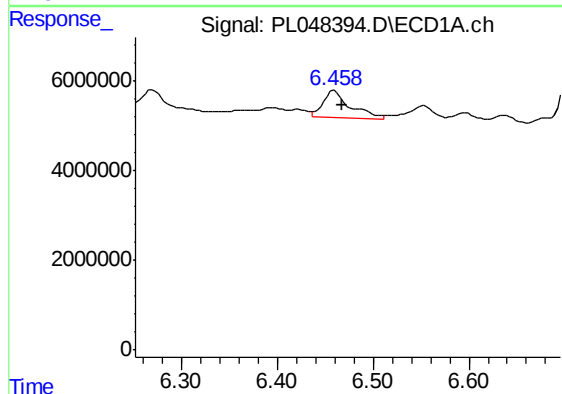


#19 Endosulfan Sulfate

R.T.: 6.460 min
Delta R.T.: -0.008 min
Response: 11830640
Conc: 1.10 ng/ml

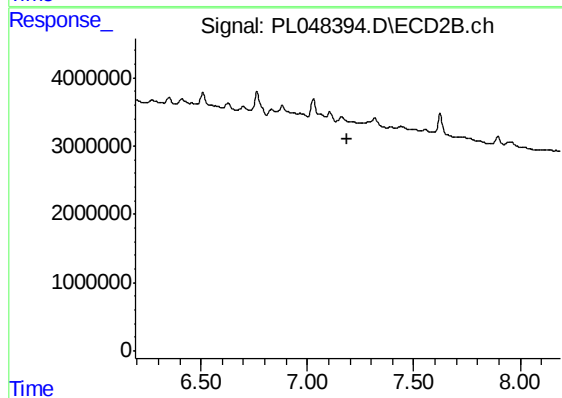

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.190 min
Response: 0
Conc: N.D.

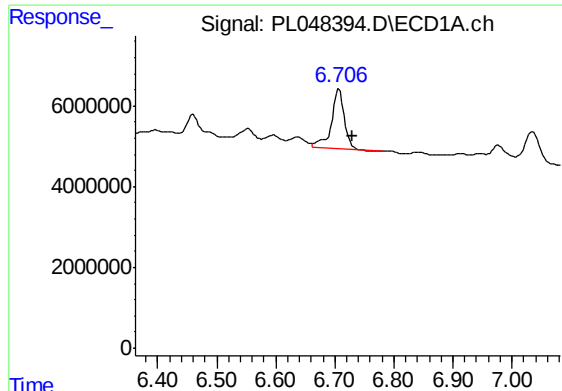

#20 Methoxychlor


R.T.: 6.707 min
Delta R.T.: -0.022 min
Response: 22810492
Conc: 4.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-5.8.19

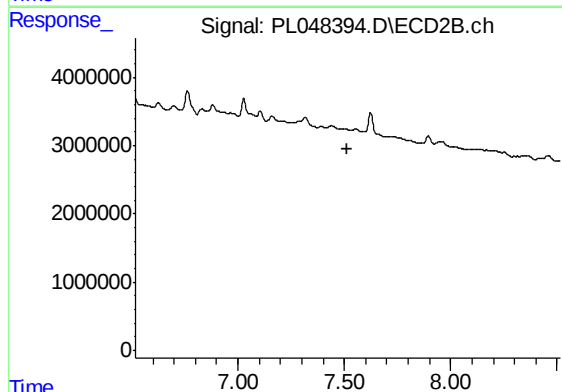


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.516 min
Response: 0
Conc: N.D.

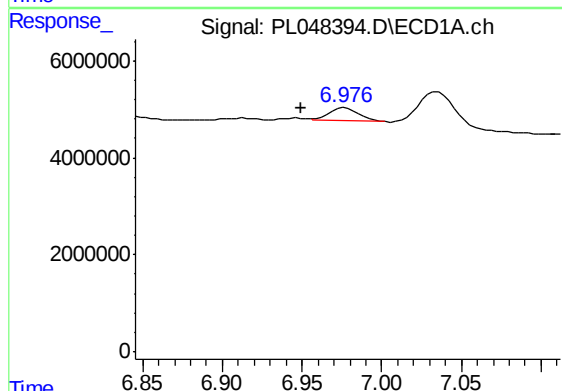


#21 Endrin ketone

R.T.: 6.977 min
Delta R.T.: 0.027 min
Response: 3476174
Conc: 0.30 ng/ml

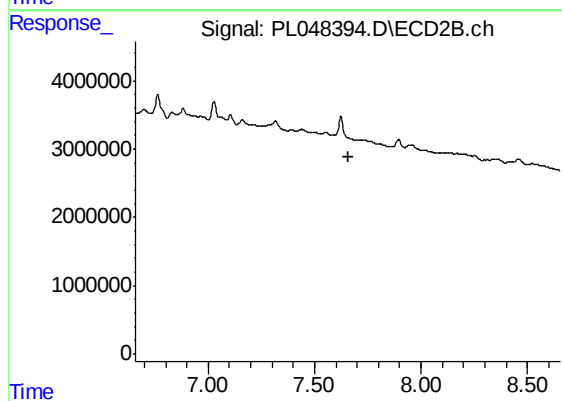

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.658 min
Response: 0
Conc: N.D.

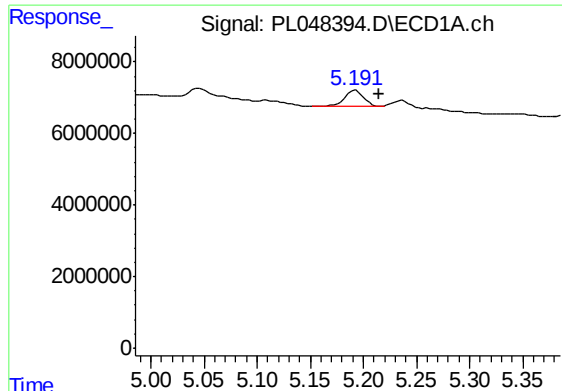

#25 Chlordane-3


R.T.: 5.192 min
Delta R.T.: -0.023 min
Response: 5620718
Conc: 3.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-5.8.19

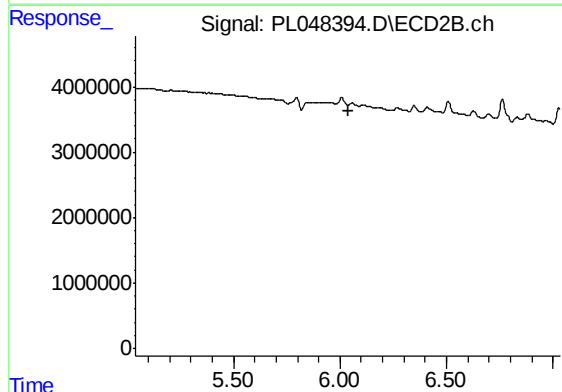


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

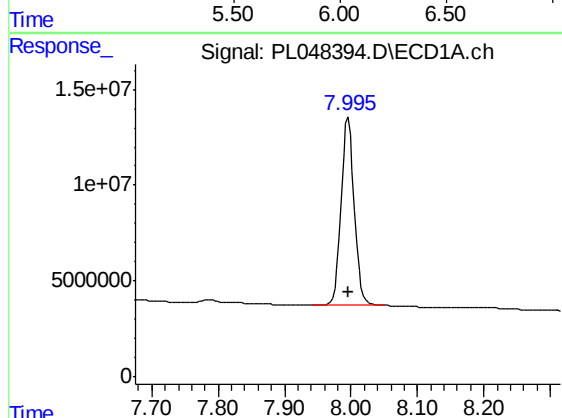

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 135531632
Conc: 13.48 ng/ml

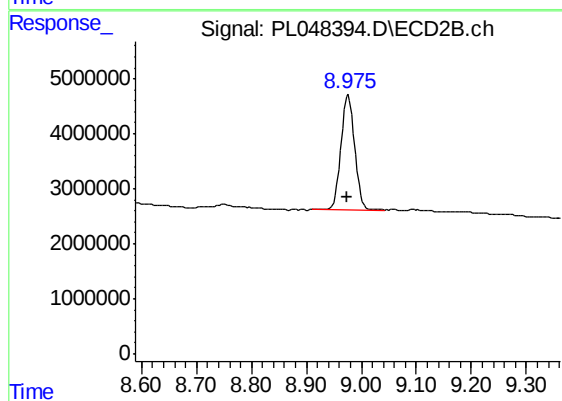

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: 0.001 min
Response: 36353961
Conc: 13.70 ng/ml