

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051019\
 Data File : PL048421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2019 18:53
 Operator : AJ\SJ
 Sample : K2801-07
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RT-3456

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 23:05:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.327	3.940	90250115	23265178	9.317	9.340
28)	SA Decachlor...	7.996	8.977	75684747	20421940	7.528	7.694
Target Compounds							
10)	B gamma-Chl...	5.234f	0.000	12322115	0	0.923	N.D. #
11)	B alpha-Chl...	5.270	0.000	5520844	0	0.422	N.D. #
12)	B 4,4'-DDE	5.438	0.000	12067121	0	0.951	N.D. #
17)	MA 4,4'-DDT	6.181	0.000	4387330	0	0.437	N.D. #
23)	Chlordane-1	4.169	0.000	2804850	0	6.248	N.D. #
25)	Chlordane-3	5.234f	0.000	12322115	0	7.826	N.D. #
26)	Chlordane-4	5.270	0.000	5520844	0	3.803	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051019\
Data File : PL048421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2019 18:53
Operator : AJ\SJ
Sample : K2801-07
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RT-3456

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 23:05:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

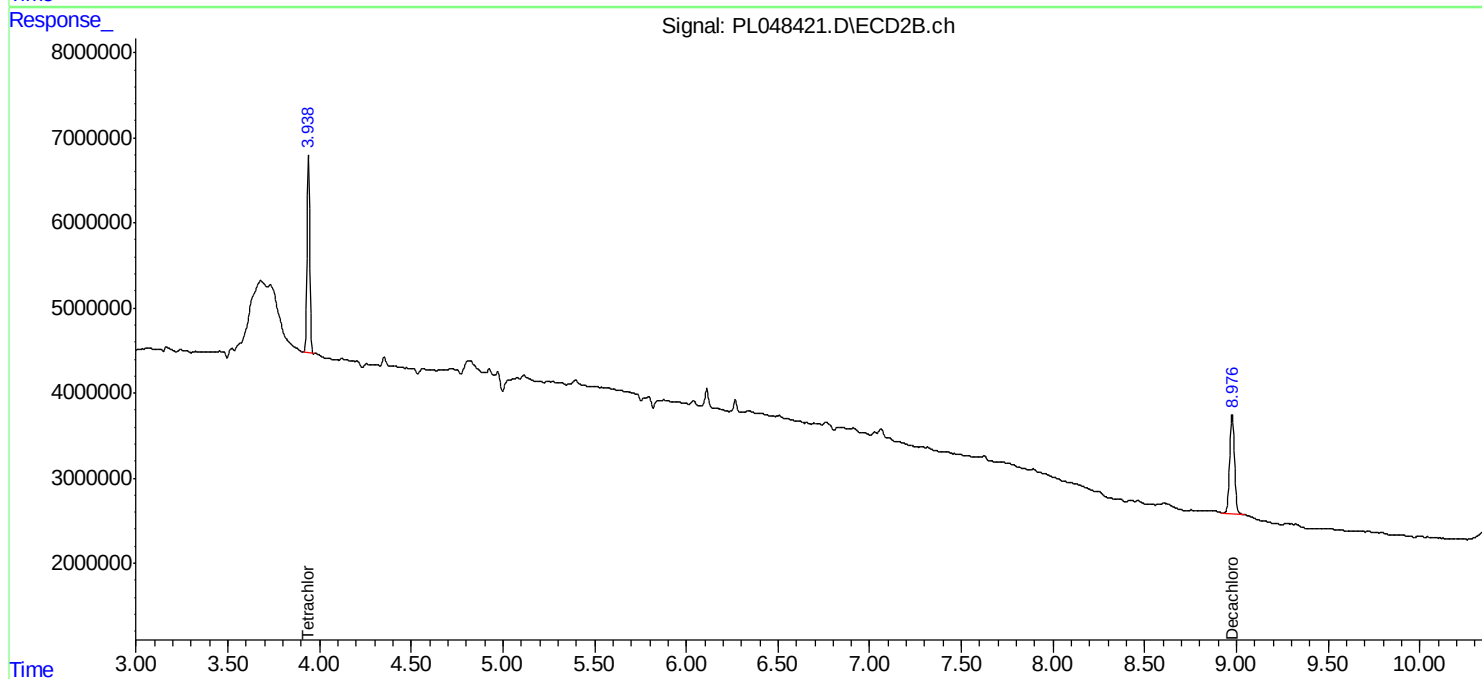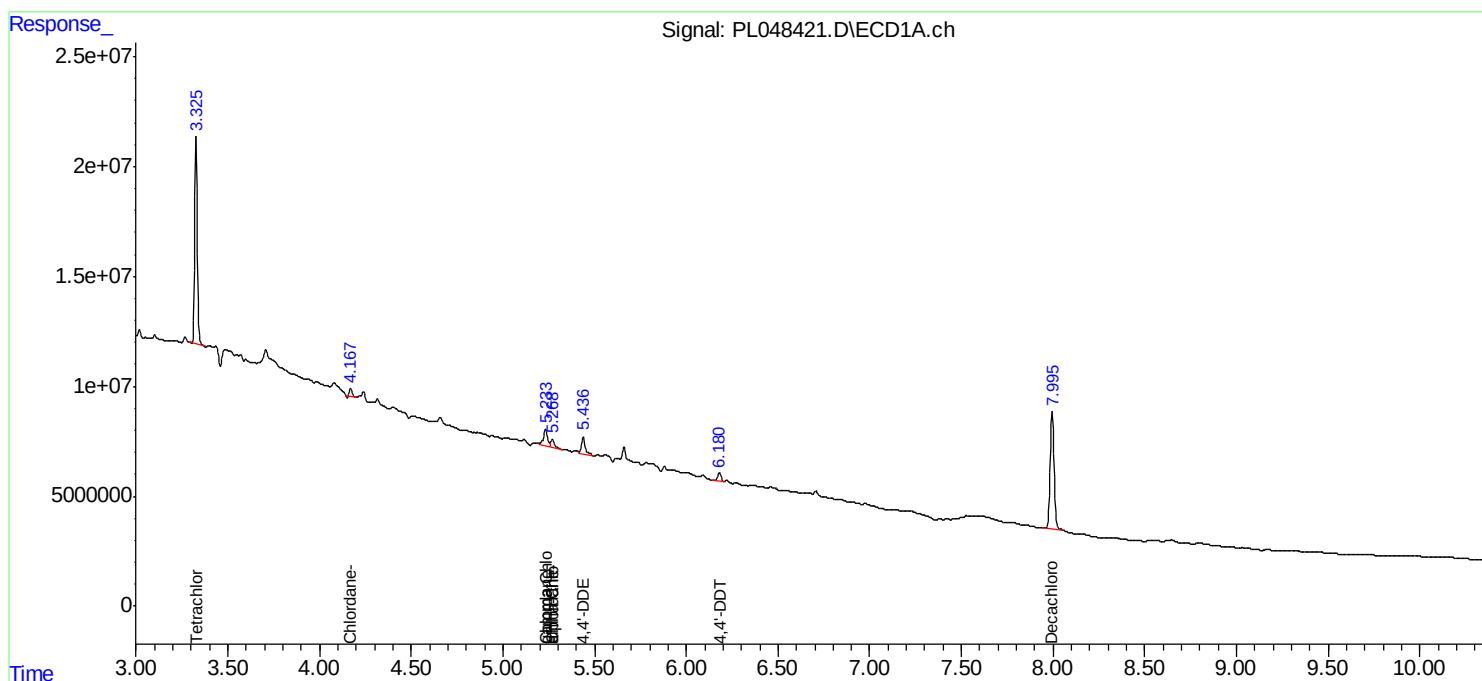


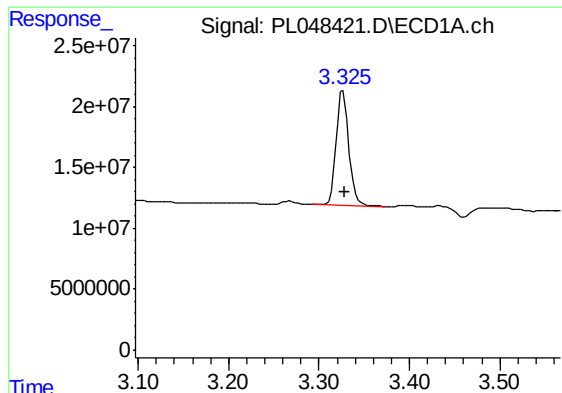

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: -0.001 min
Response: 90250115
Conc: 9.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3456

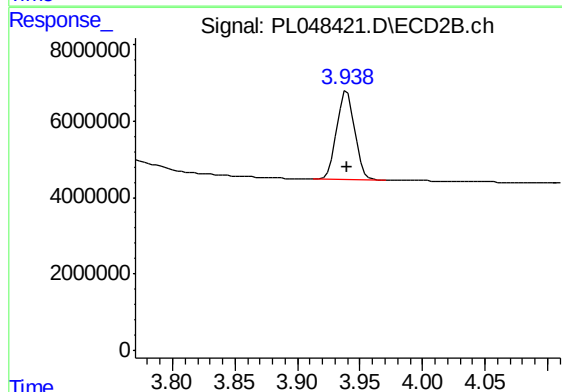


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 23265178
Conc: 9.34 ng/ml

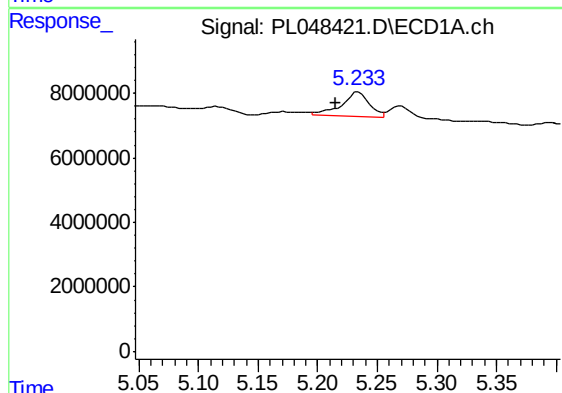


#10 gamma-Chlordane

R.T.: 5.234 min
Delta R.T.: 0.019 min
Response: 12322115
Conc: 0.92 ng/ml

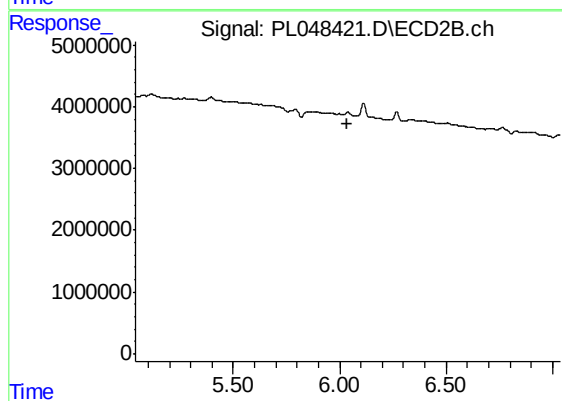

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

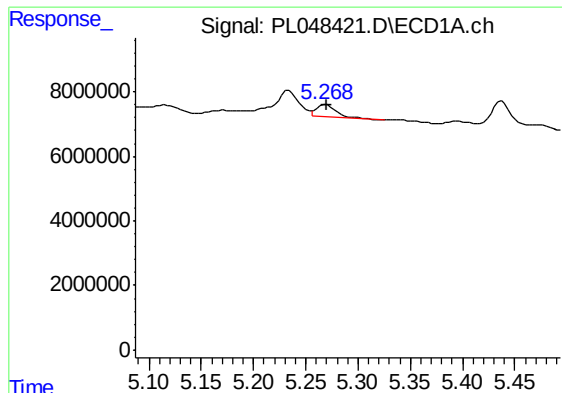

#11 alpha-Chlordane


R.T.: 5.270 min
Delta R.T.: -0.001 min
Response: 5520844
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3456

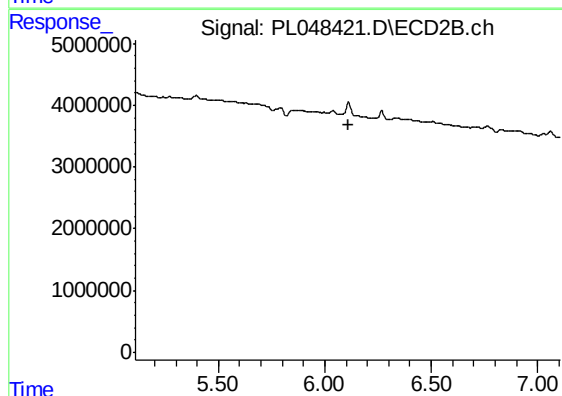


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

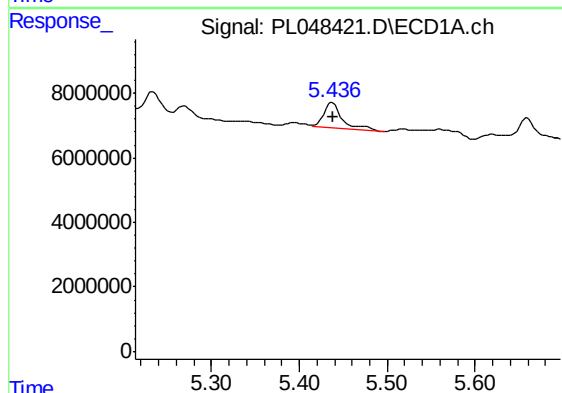


#12 4,4'-DDE

R.T.: 5.438 min
Delta R.T.: -0.001 min
Response: 12067121
Conc: 0.95 ng/ml

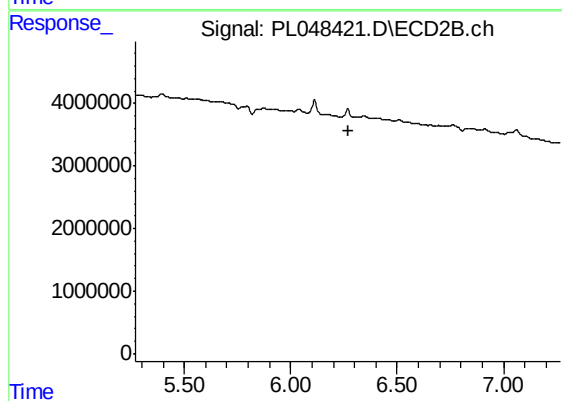

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

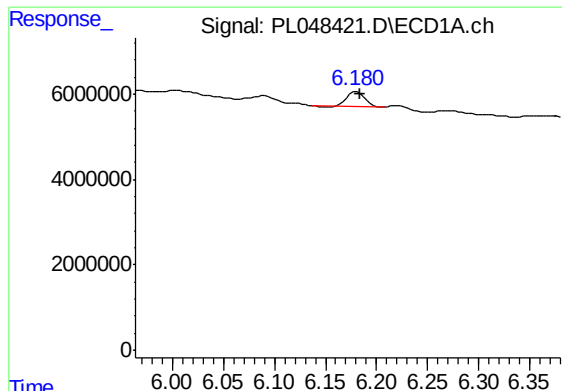

#17 4,4'-DDT


R.T.: 6.181 min
Delta R.T.: -0.003 min
Response: 4387330
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3456

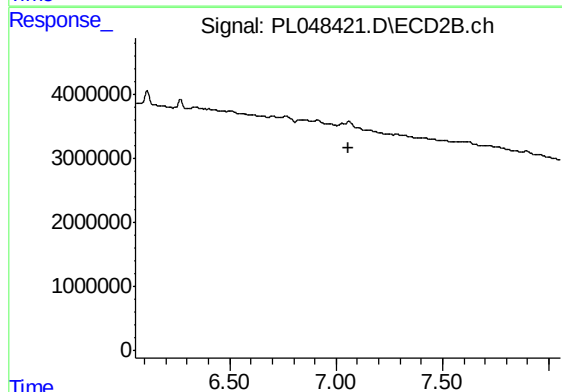


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

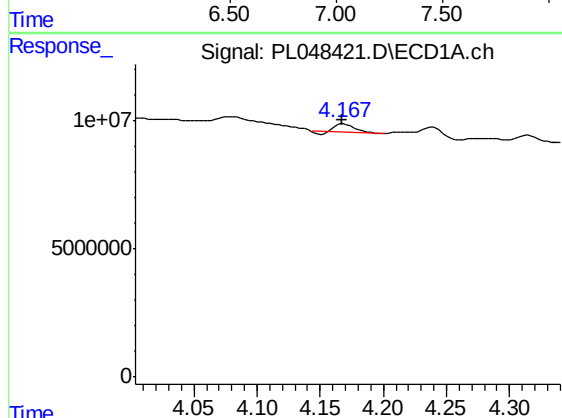


#23 Chlordane-1

R.T.: 4.169 min
Delta R.T.: 0.001 min
Response: 2804850
Conc: 6.25 ng/ml

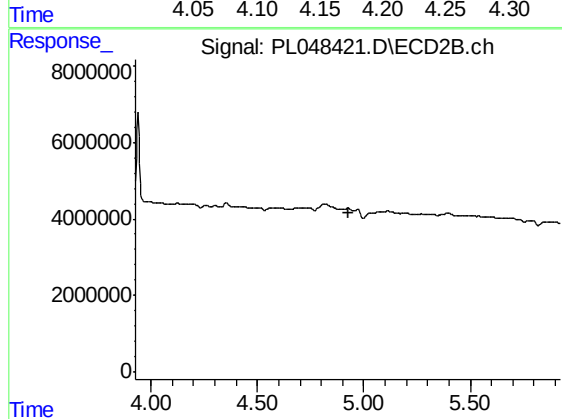

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.925 min
Response: 0
Conc: N.D.

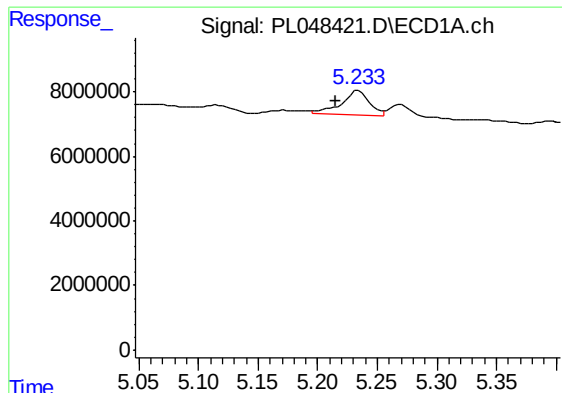

#25 Chlordane-3


R.T.: 5.234 min
Delta R.T.: 0.019 min
Response: 12322115
Conc: 7.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3456

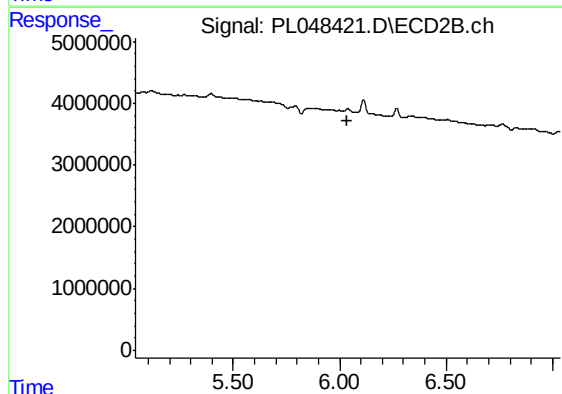


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

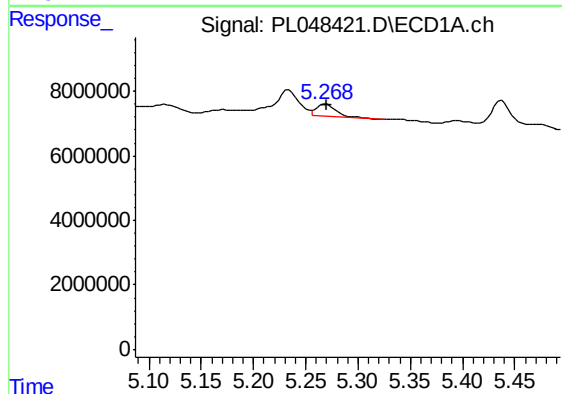


#26 Chlordane-4

R.T.: 5.270 min
Delta R.T.: 0.000 min
Response: 5520844
Conc: 3.80 ng/ml

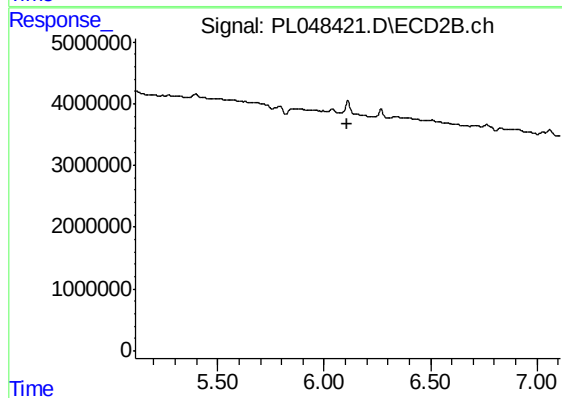

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

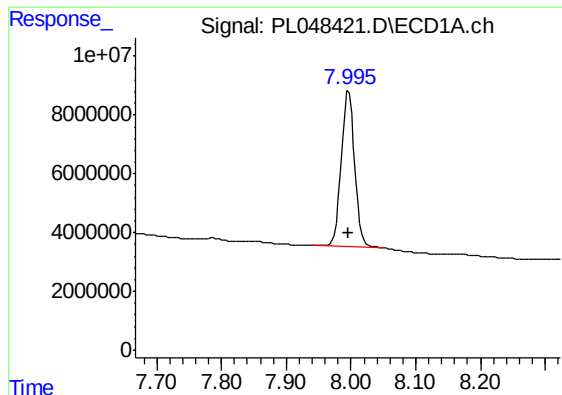

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 75684747
Conc: 7.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3456

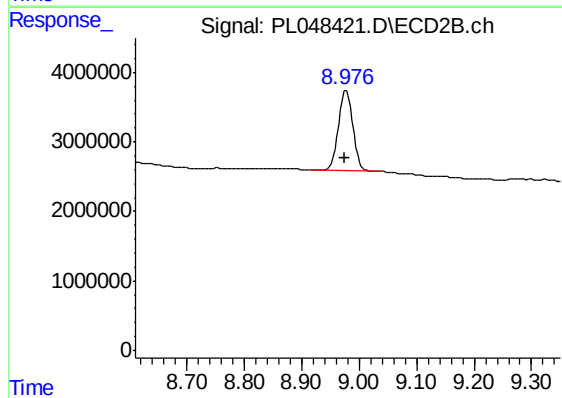

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.002 min
Response: 20421940
Conc: 7.69 ng/ml