

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051019\
 Data File : PL048441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2019 00:11
 Operator : AJ\SJ
 Sample : K2792-01
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DRUM-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 01:49:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.328	3.940	216.2E6	54229840	22.321	21.771
28)	SA Decachlor...	7.996	8.977	211.2E6	58045678	21.003	21.869
Target Compounds							
2)	A alpha-BHC	3.726f	4.301f	-1487478	29843593	N.D.	8.498
4)	MA Heptachlor	0.000	5.100f	0	6068349	N.D.	1.753 #
7)	B delta-BHC	4.467	4.975f	6141225	14337725	0.435	5.070 #
11)	B alpha-Chl...	5.279	0.000	216.4E6	0	16.555	N.D. #
12)	B 4,4'-DDE	5.457f	0.000	23518589	0	1.854	N.D. #
13)	MA Dieldrin	5.587f	0.000	11354136	0	0.872	N.D. #
16)	A 4,4'-DDD	5.960	0.000	6240226	0	0.641	N.D. #
26)	Chlordane-4	5.279	0.000	216.4E6	0	149.075	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051019\
Data File : PL048441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2019 00:11
Operator : AJ\SJ
Sample : K2792-01
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DRUM-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 01:49:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

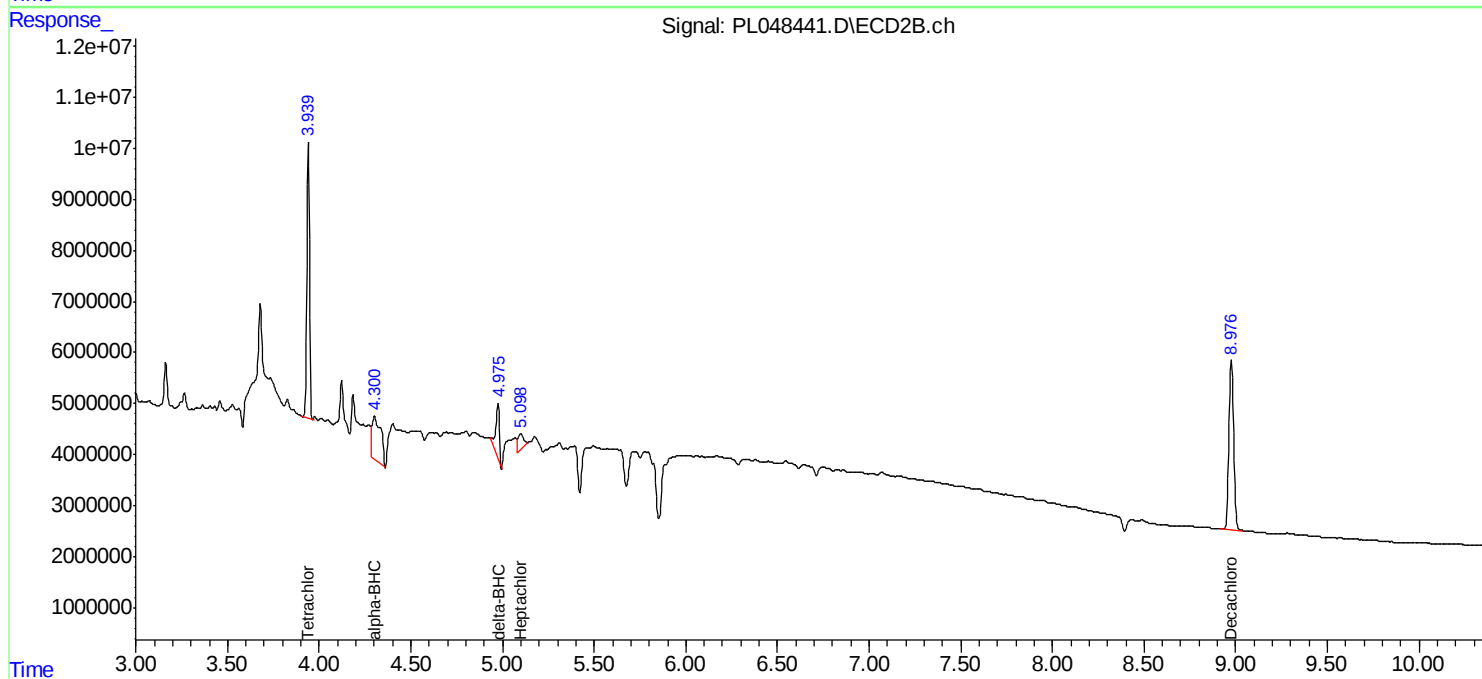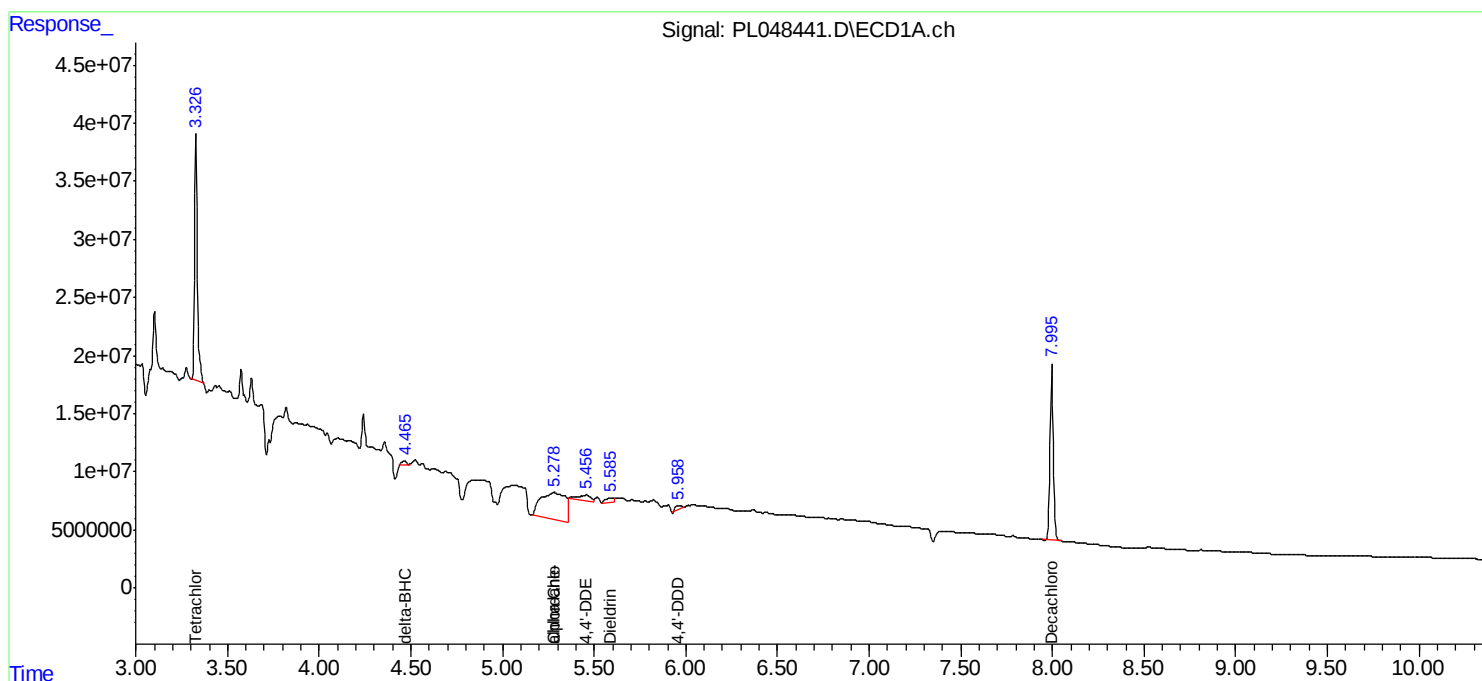


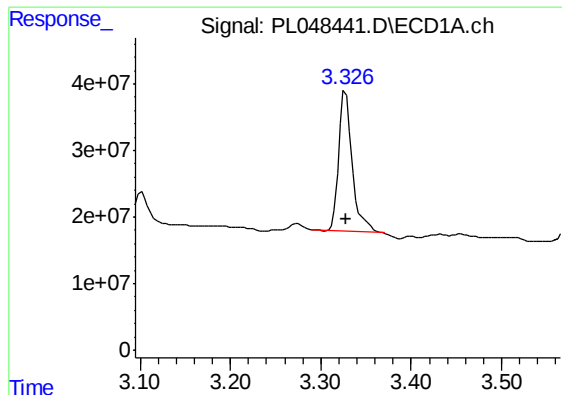

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 216219597
Conc: 22.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-COMP

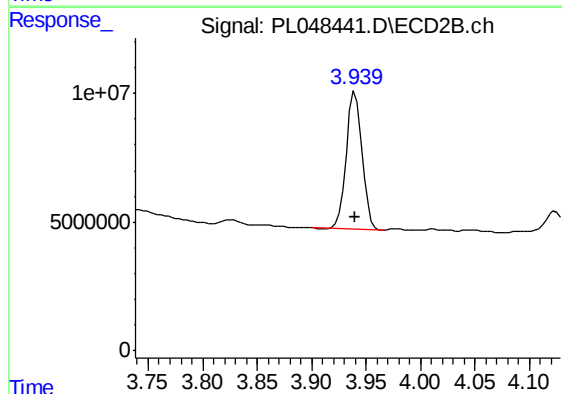


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 54229840
Conc: 21.77 ng/ml

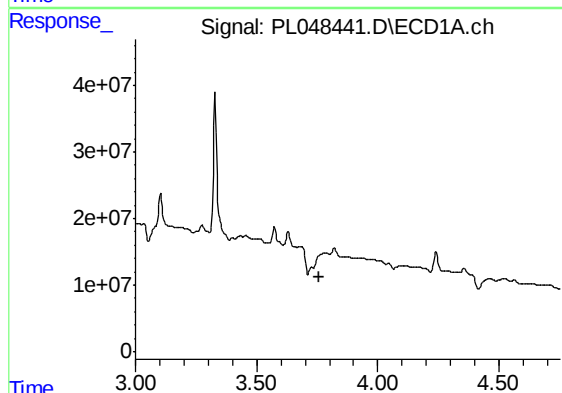


#2 alpha-BHC

R.T.: 3.726 min
Delta R.T.: -0.030 min
Response: -1487478
Conc: N.D.

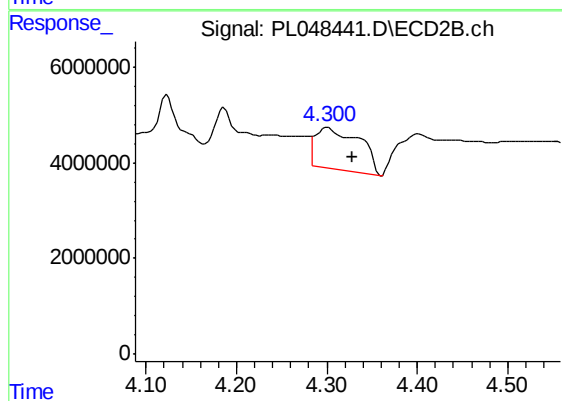

#2 alpha-BHC


R.T.: 4.301 min
Delta R.T.: -0.027 min
Response: 29843593
Conc: 8.50 ng/ml

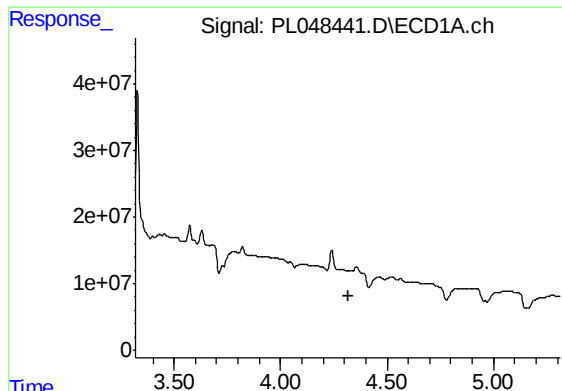

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
DRUM-COMP

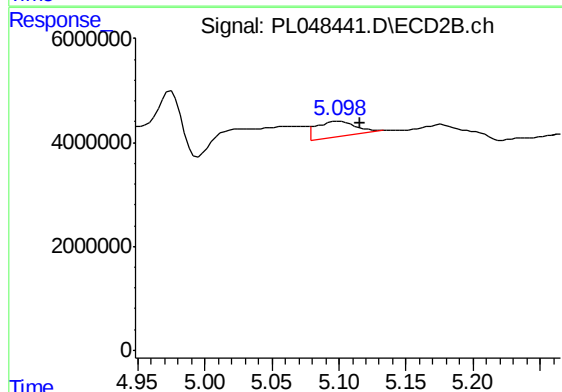


#4 Heptachlor

R.T.: 5.100 min
Delta R.T.: -0.015 min
Response: 6068349
Conc: 1.75 ng/ml

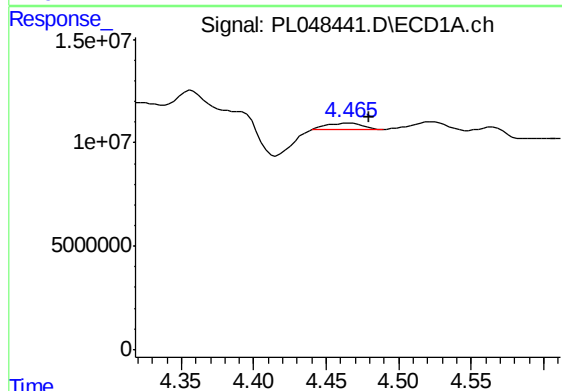


#7 delta-BHC

R.T.: 4.467 min
Delta R.T.: -0.013 min
Response: 6141225
Conc: 0.43 ng/ml

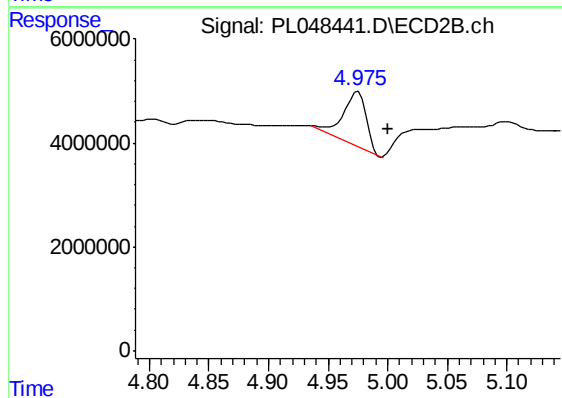

#7 delta-BHC


R.T.: 4.975 min
Delta R.T.: -0.025 min
Response: 14337725
Conc: 5.07 ng/ml

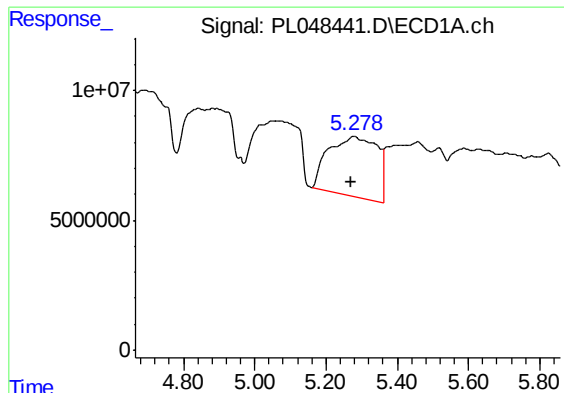

#11 alpha-Chlordane


R.T.: 5.279 min
Delta R.T.: 0.008 min
Response: 216430269
Conc: 16.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-COMP

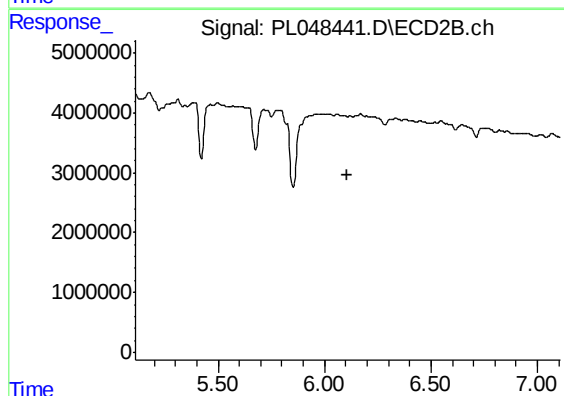


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

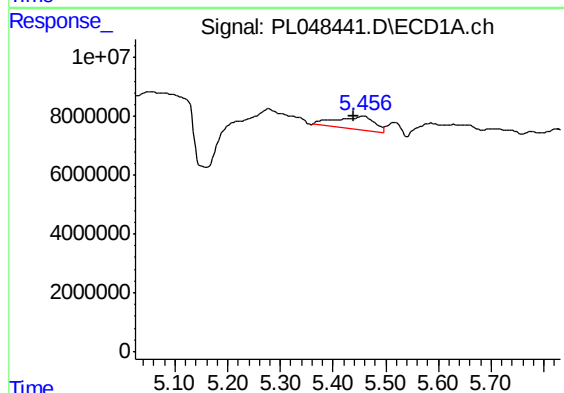


#12 4,4'-DDE

R.T.: 5.457 min
Delta R.T.: 0.019 min
Response: 23518589
Conc: 1.85 ng/ml

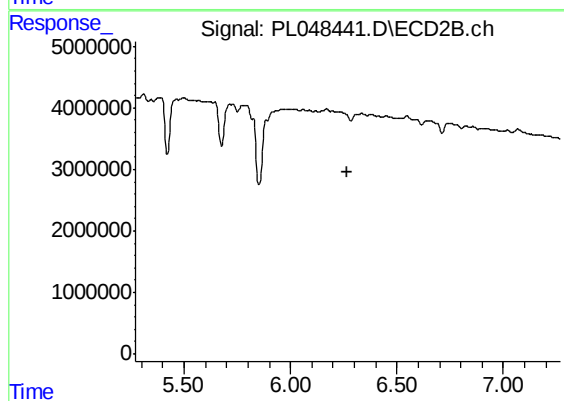

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.269 min
Response: 0
Conc: N.D.

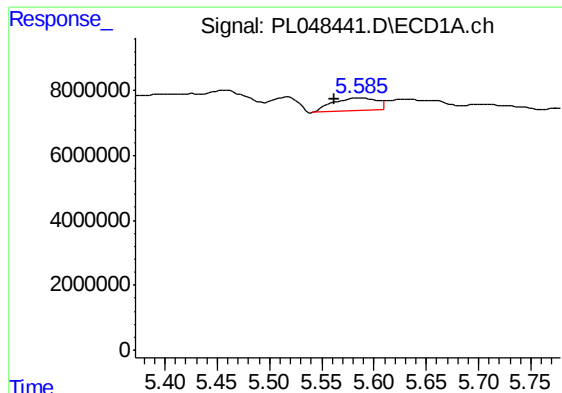

#13 Dieldrin


R.T.: 5.587 min
Delta R.T.: 0.025 min
Response: 11354136
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-COMP

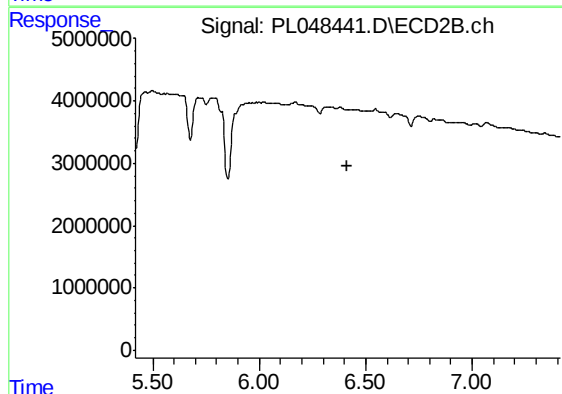


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

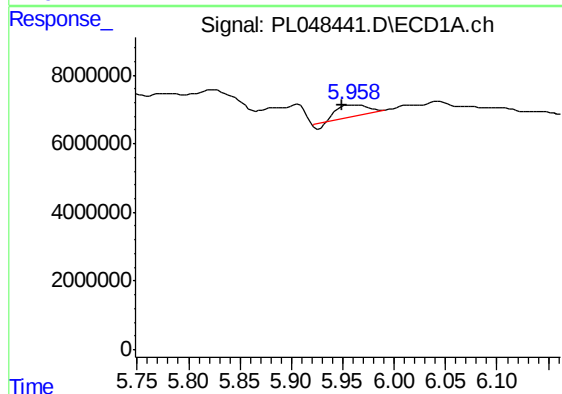


#16 4,4'-DDD

R.T.: 5.960 min
Delta R.T.: 0.010 min
Response: 6240226
Conc: 0.64 ng/ml

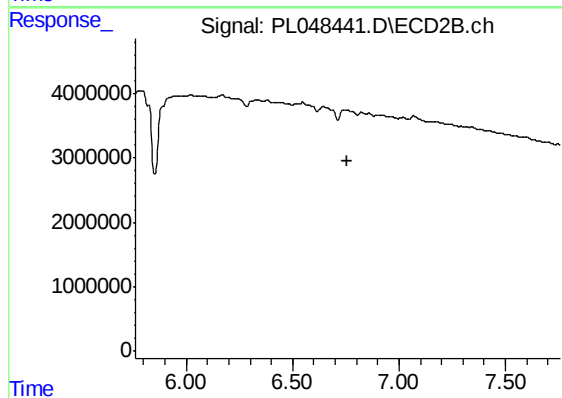

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.759 min
Response: 0
Conc: N.D.

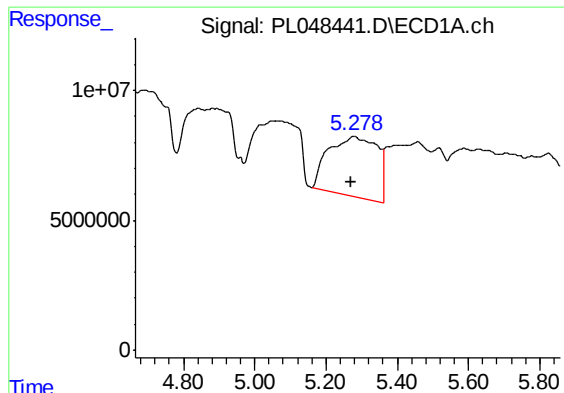

#26 Chlordane-4


R.T.: 5.279 min
Delta R.T.: 0.008 min
Response: 216430269
Conc: 149.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-COMP

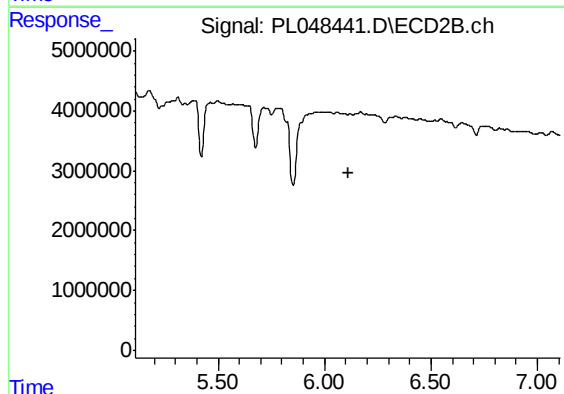


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.111 min
Response: 0
Conc: N.D.

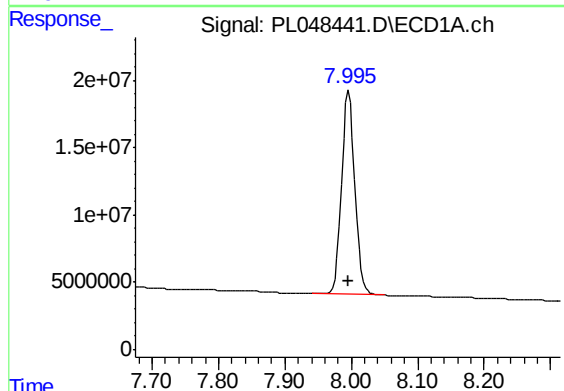

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 211167564
Conc: 21.00 ng/ml

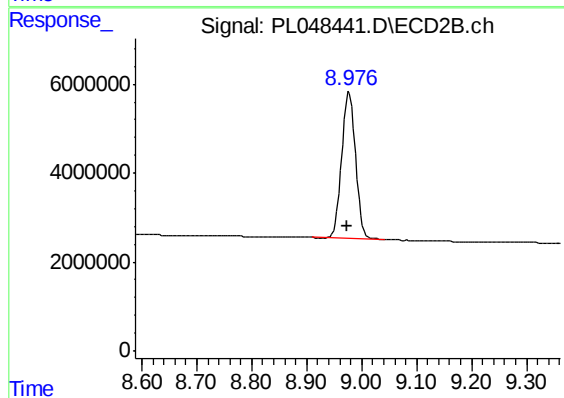

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.002 min
Response: 58045678
Conc: 21.87 ng/ml