

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051019\
 Data File : PL048402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2019 13:46
 Operator : AJ\SJ
 Sample : K2642-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-050919

Manual Integrations
 APPROVED

Ankita
 5/13/2019 12:48:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 23:00:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.333	3.939	49058758	11025947	5.064m	4.427
28) SA Decachlor...	7.996	8.977	67474813	20254597	6.711	7.631
Target Compounds						
12) B 4,4'-DDE	5.437	6.267	75022731	12989610	5.914m	4.705m
17) MA 4,4'-DDT	6.182	7.058	13634903	6257452	1.357m	2.667 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051019\
Data File : PL048402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2019 13:46
Operator : AJ\SJ
Sample : K2642-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-03-050919


Manual Integrations
APPROVED

Ankita
5/13/2019 12:48:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 23:00:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

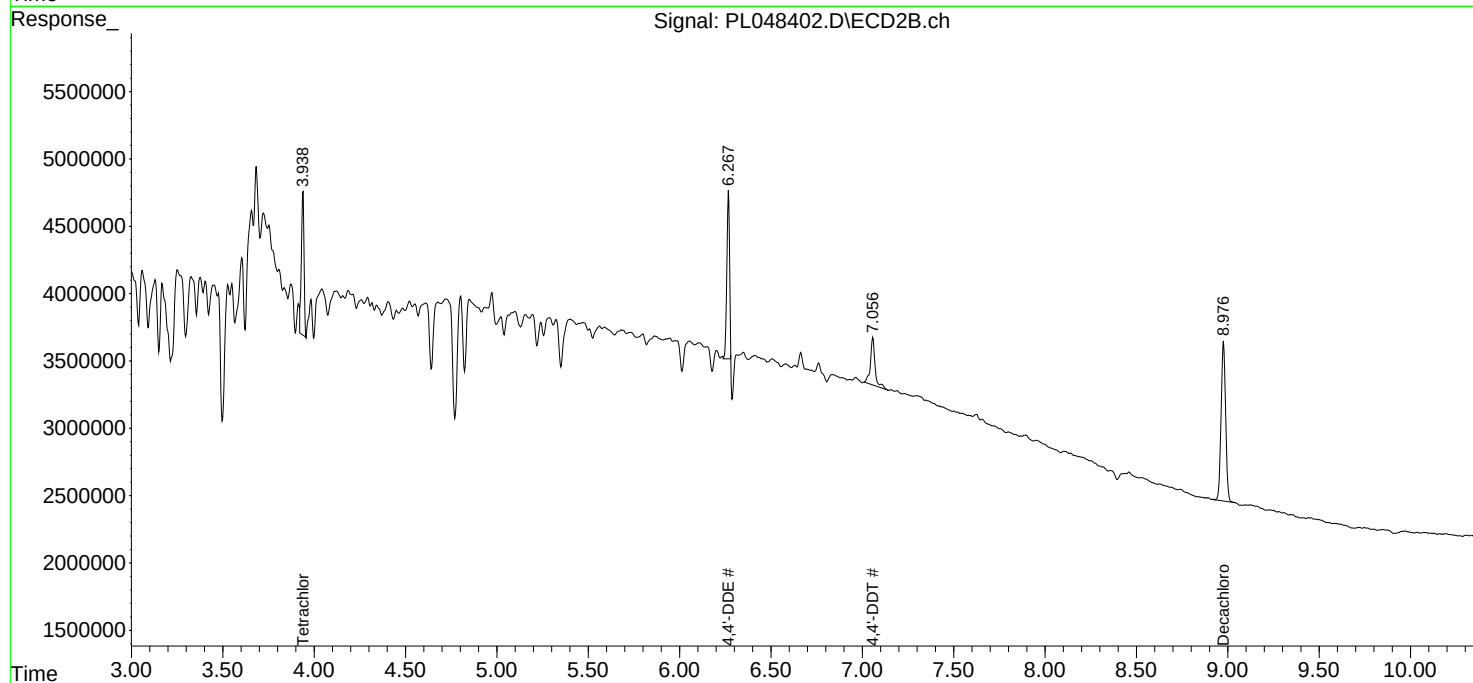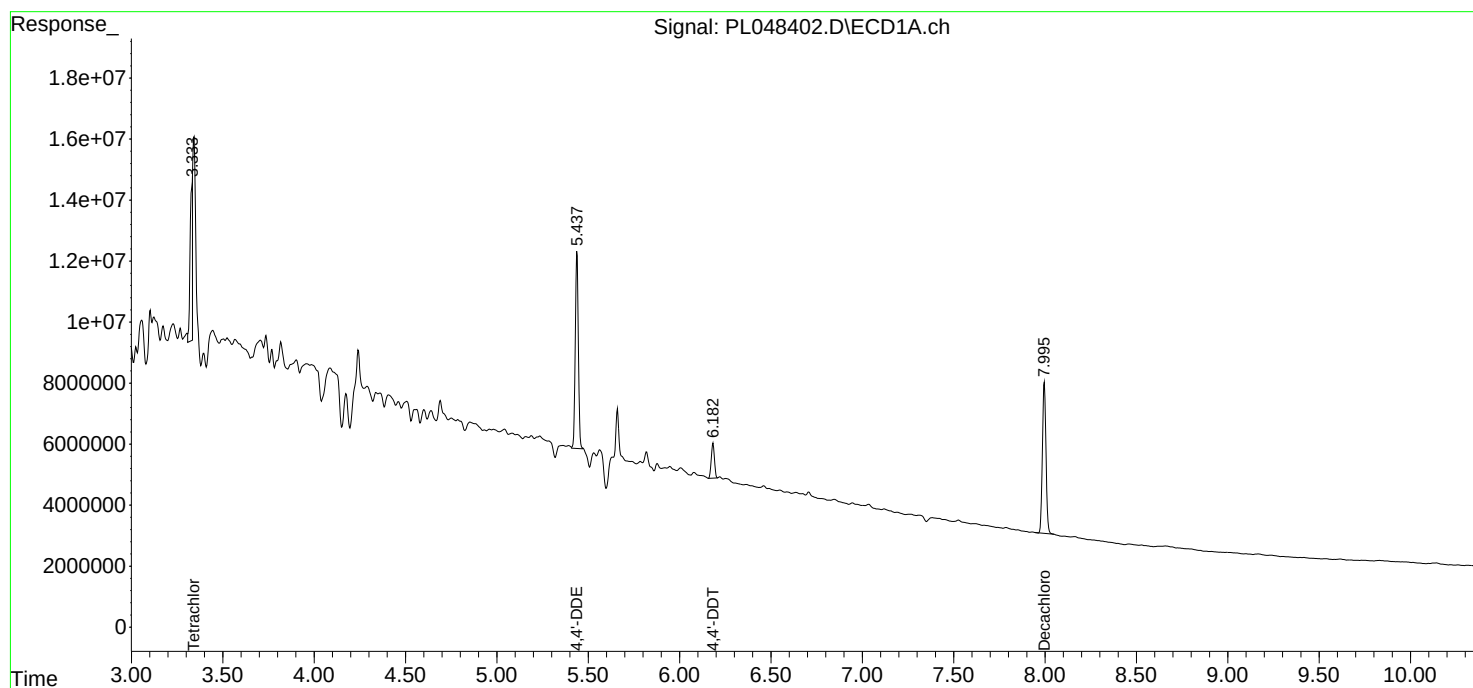

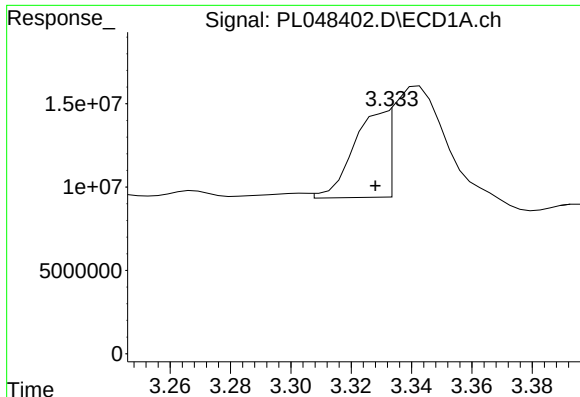


#1 Tetrachloro-m-xylene

R.T.: 3.333 min
Delta R.T.: 0.005 min
Response: 49058758
Conc: 5.06 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-03-050919


Manual Integrations
APPROVED

Ankita
5/13/2019 12:48:00 PM

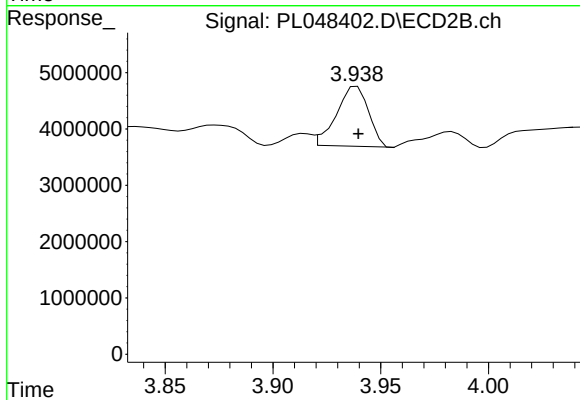


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 11025947
Conc: 4.43 ng/ml

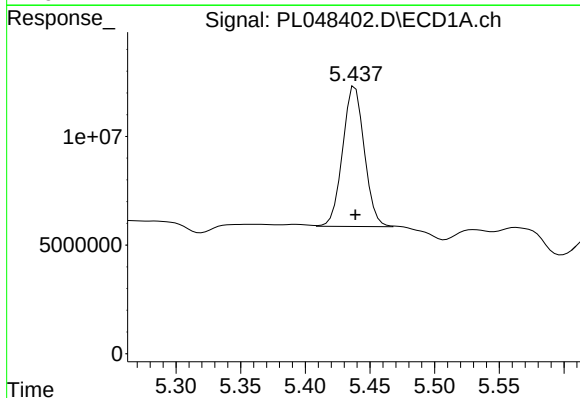


#12 4,4'-DDE

R.T.: 5.437 min
Delta R.T.: -0.002 min
Response: 75022731
Conc: 5.91 ng/ml m

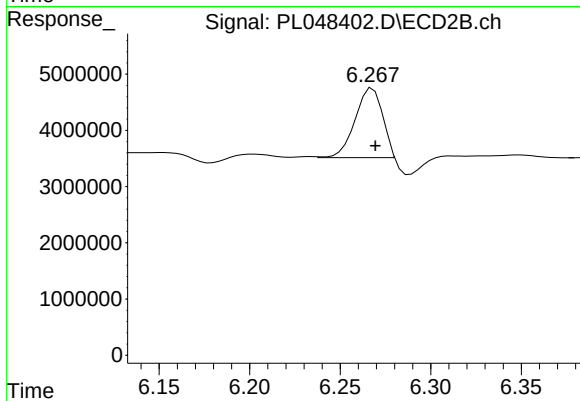

#12 4,4'-DDE

R.T.: 6.267 min
Delta R.T.: -0.003 min
Response: 12989610
Conc: 4.70 ng/ml m

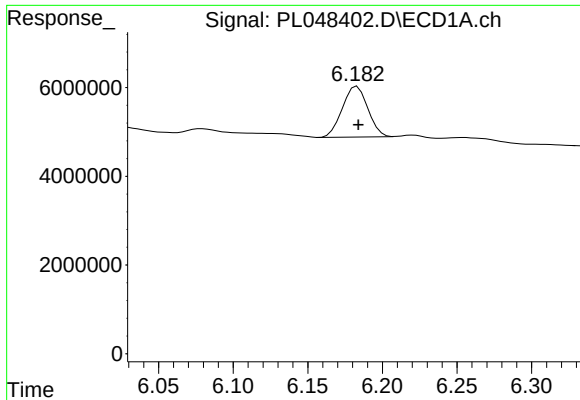


#17 4,4'-DDT

R.T.: 6.182 min
Delta R.T.: -0.002 min
Response: 13634903
Conc: 1.36 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-03-050919


Manual Integrations
APPROVED

Ankita
5/13/2019 12:48:00 PM

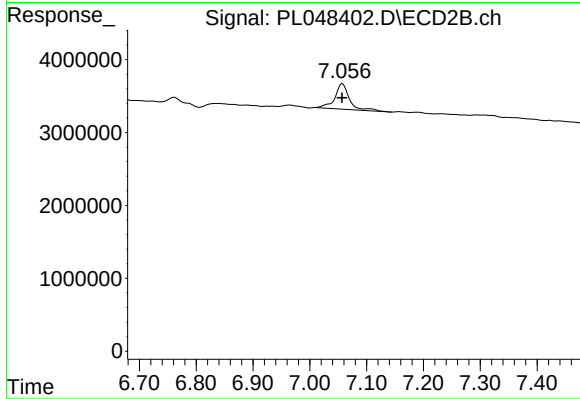


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.001 min
Response: 6257452
Conc: 2.67 ng/ml

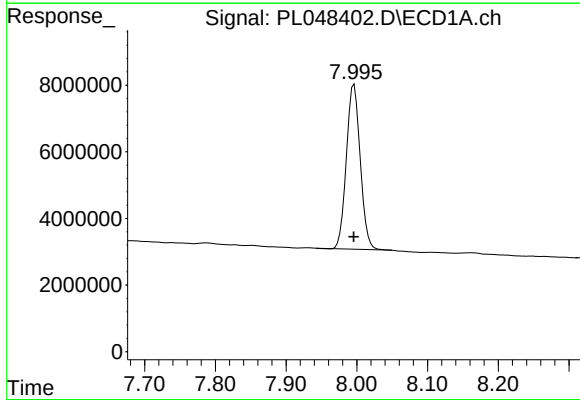

#28 Decachlorobiphenyl

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 67474813
Conc: 6.71 ng/ml

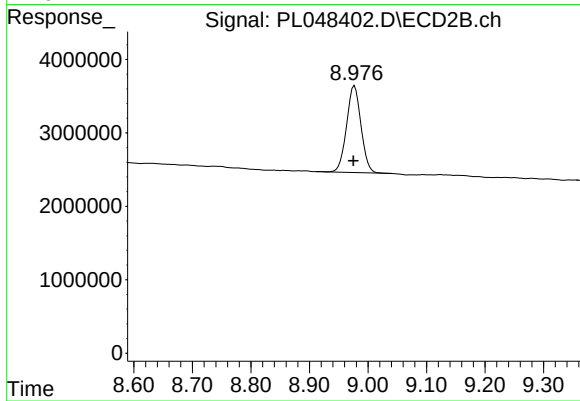

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: 0.002 min
Response: 20254597
Conc: 7.63 ng/ml