

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051119\
 Data File : PL048447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2019 02:05
 Operator : AJ\SJ
 Sample : PB119440BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PBLK40

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 03:17:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri May 10 01:24:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.332	3.941	224.6E6	56584210	21.660	21.464
27) SA Decachlor...	8.001	8.980	395.0E6	104.6E6	37.065	38.360
Target Compounds						
15) B Endosulfa...	0.000	6.861	0	1106664	N.D.	0.393


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051119\
Data File : PL048447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2019 02:05
Operator : AJ\SJ
Sample : PB119440BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PBLK40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 03:17:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050919CLP.M
Quant Title : GC Extractables
QLast Update : Fri May 10 01:24:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

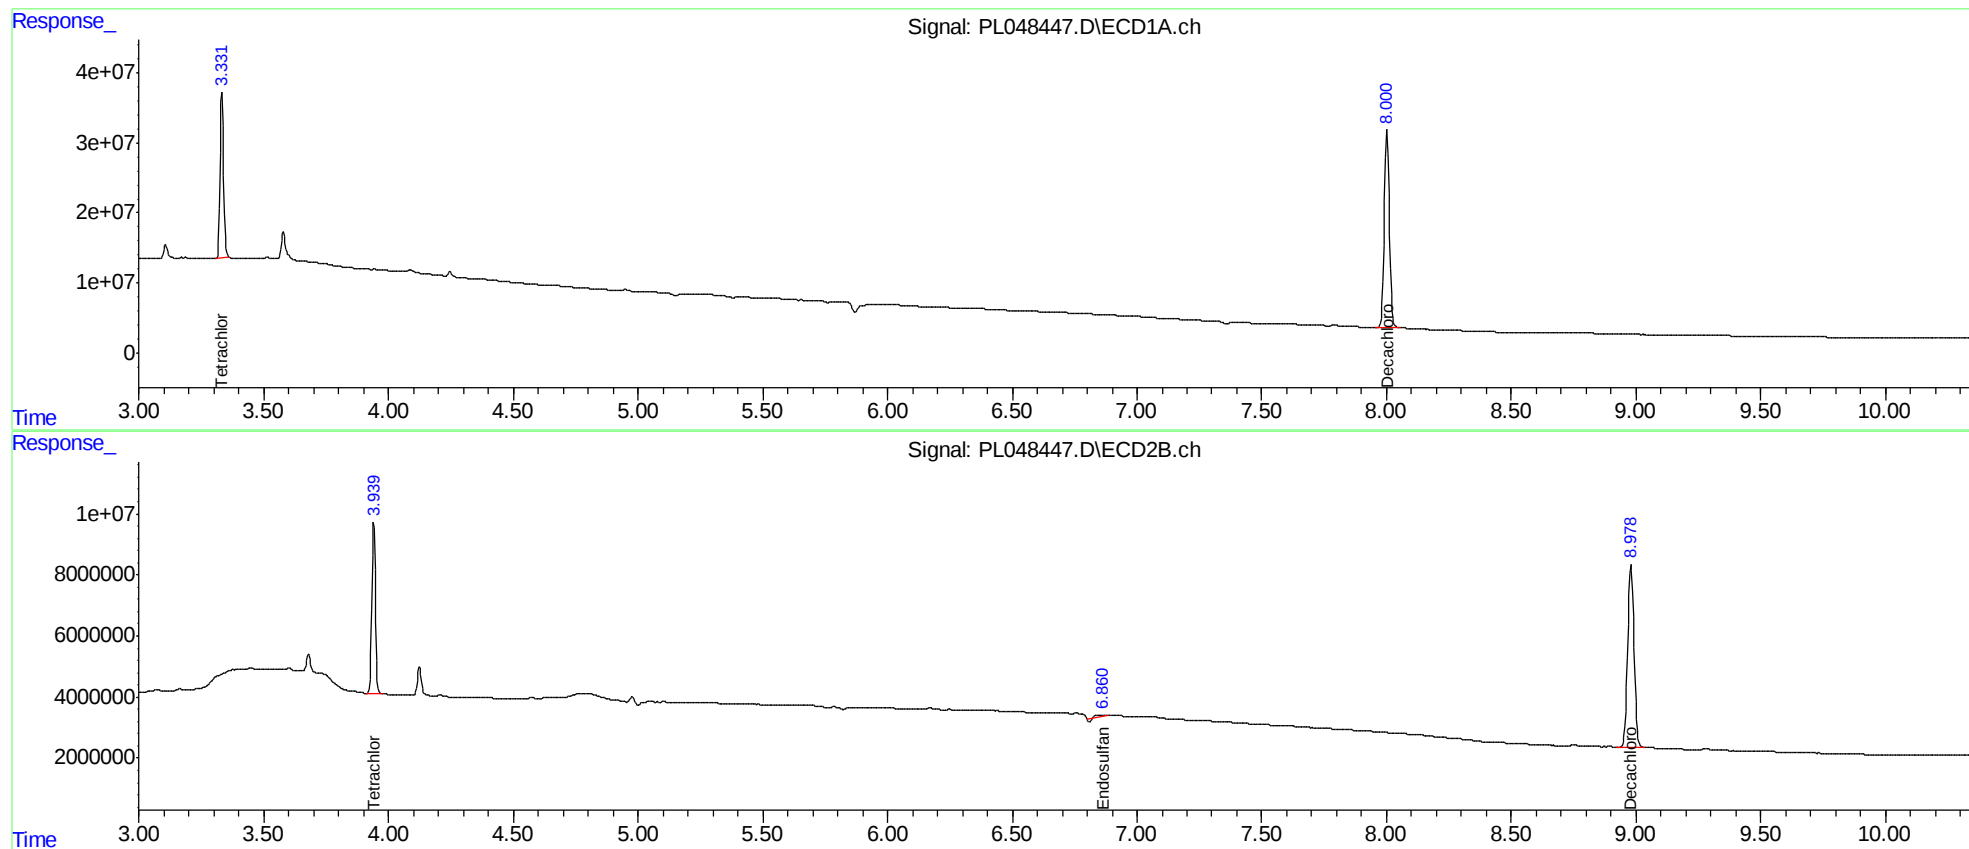


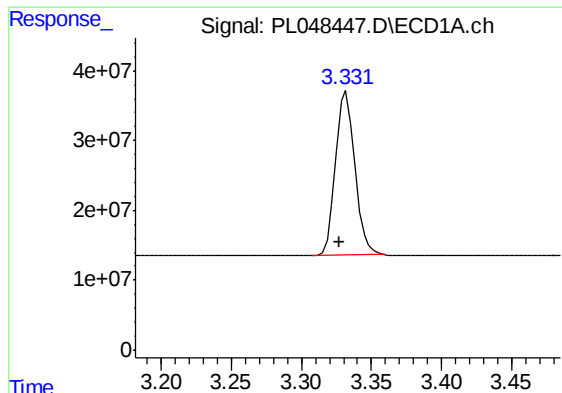

#1 Tetrachloro-m-xylene


R.T.: 3.332 min
Delta R.T.: 0.005 min
Response: 224574171
Conc: 21.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PBLK40

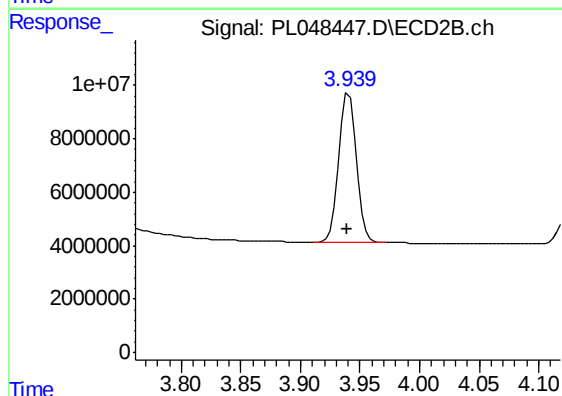


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.001 min
Response: 56584210
Conc: 21.46 ng/ml

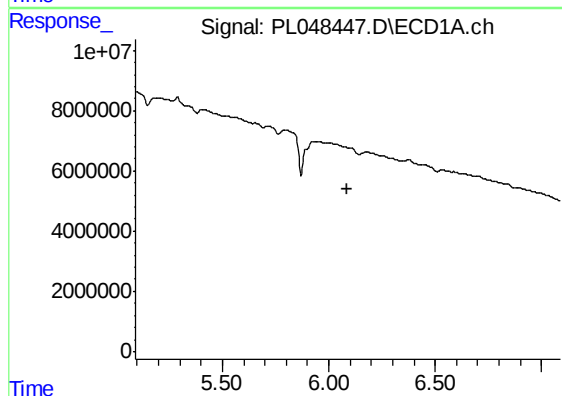


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

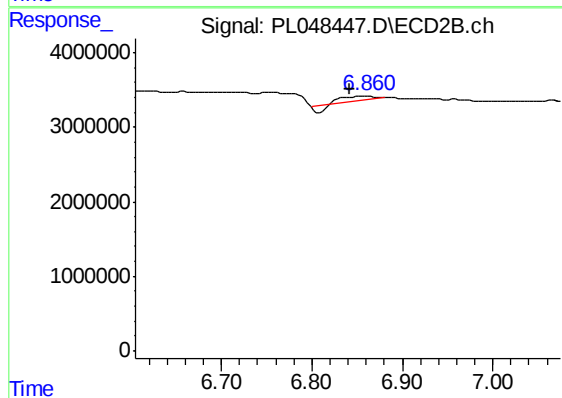

#15 Endosulfan II


R.T.: 6.861 min
Delta R.T.: 0.018 min
Response: 1106664
Conc: 0.39 ng/ml

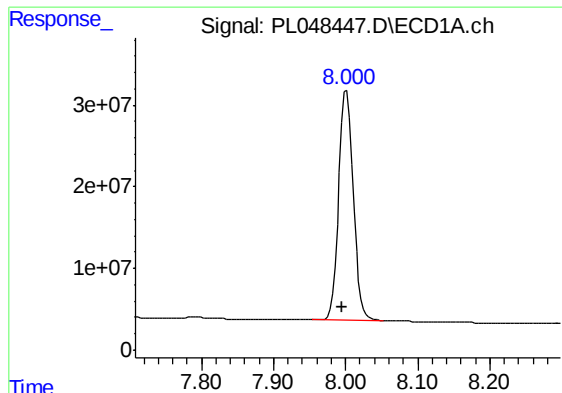

#27 Decachlorobiphenyl

R.T.: 8.001 min
Delta R.T.: 0.006 min
Response: 394971791
Conc: 37.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PBLK40

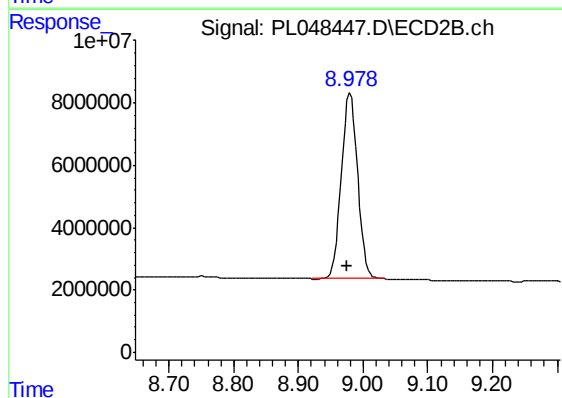

#27 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: 0.005 min
Response: 104575067
Conc: 38.36 ng/ml