

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
 Data File : PL074599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2022 09:18
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 16:11:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 15:38:28 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	10.425f	0	206781	N.D.	0.201 #
Target Compounds							
4)	MA Heptachlor	0.000	6.177	0	141290	N.D.	0.093 #
6)	B beta-BHC	0.000	6.131f	0	264627	N.D.	0.333 #
8)	B Heptachlo...	8.131	0.000	13117061	0	23.063	N.D. #
9)	A Endosulfan I	8.513f	7.467f	5142289	1177943	8.920	0.941 #
13)	MA Dieldrin	0.000	7.783	0	1635236	N.D.	1.284 #
14)	MA Endrin	0.000	8.088f	0	6062621	N.D.	5.739 #
15)	B Endosulfa...	0.000	8.379	0	489853	N.D.	0.434 #
19)	B Endosulfa...	0.000	8.807f	0	142748	N.D.	0.131 #
24)	Chlordane-2	0.000	6.654	0	1945292	N.D.	35.034 #
27)	Chlordane-5	0.000	8.161f	0	22850	N.D.	0.618 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
Data File : PL074599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2022 09:18
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 16:11:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 15:38:28 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

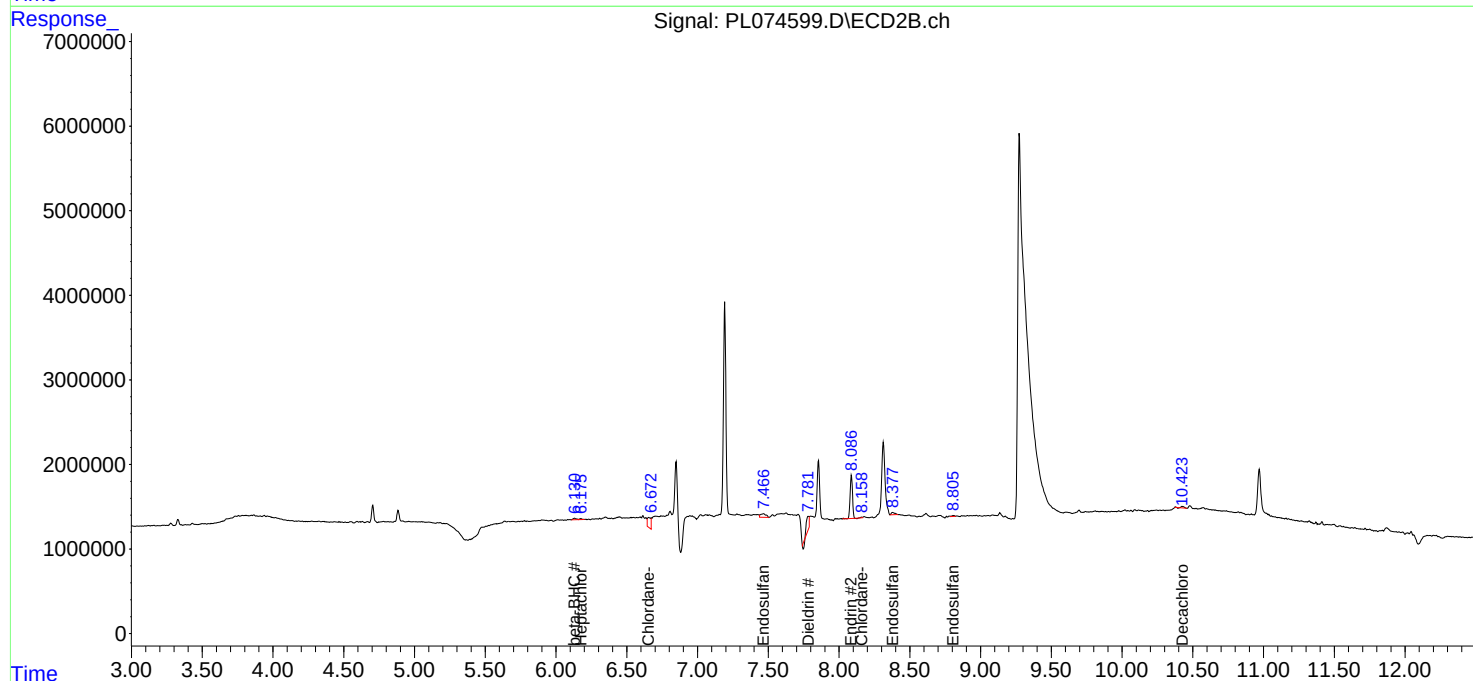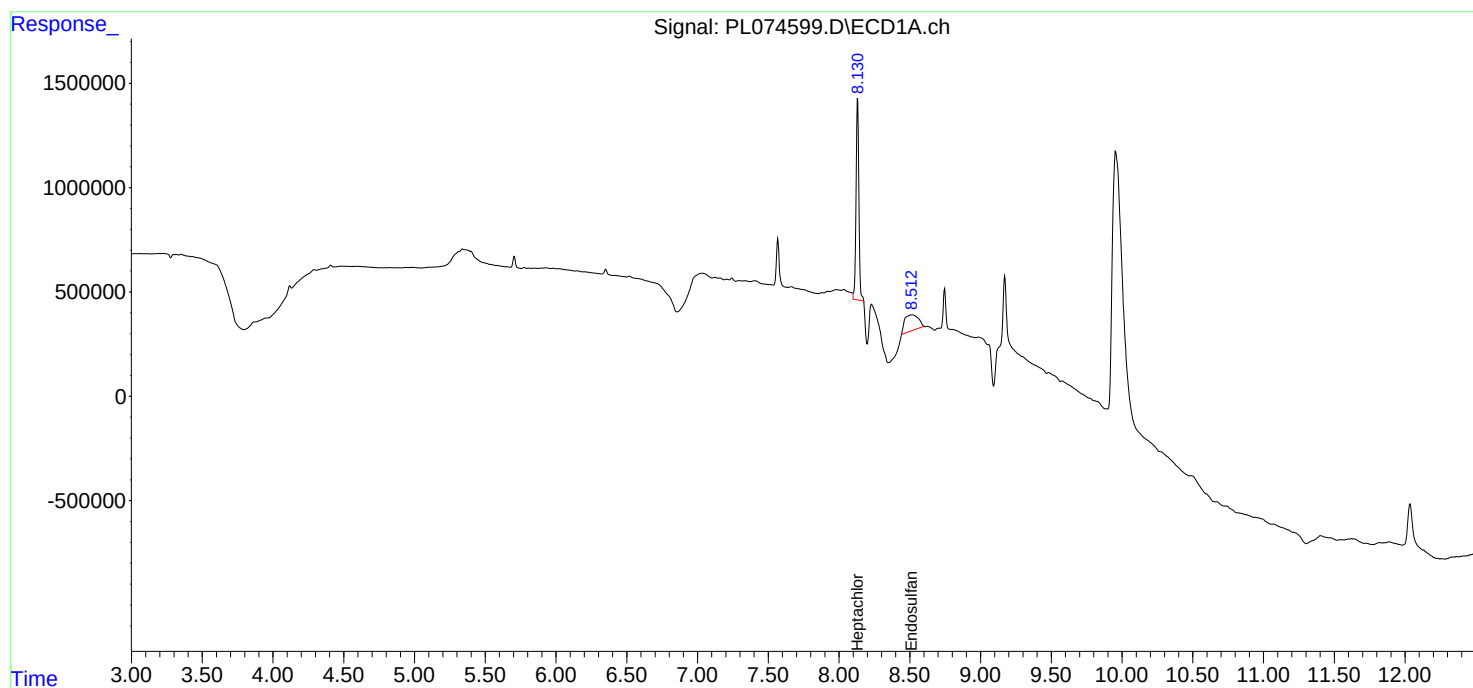


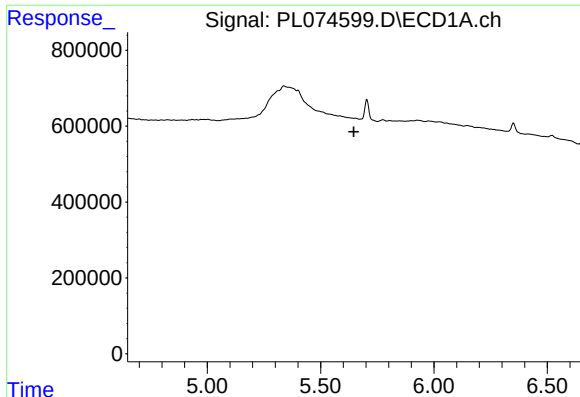

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 5.647 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

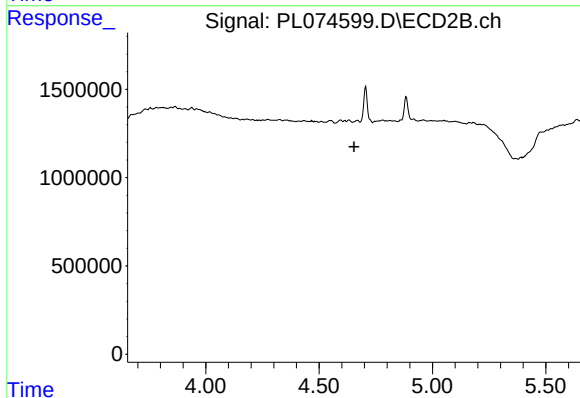


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.654 min
Response: 0
Conc: N.D.

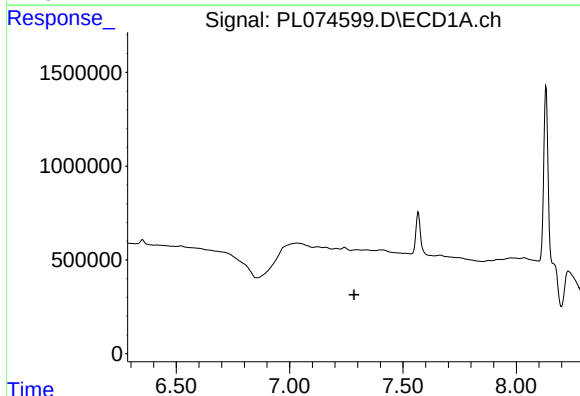


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.284 min
Response: 0
Conc: N.D.

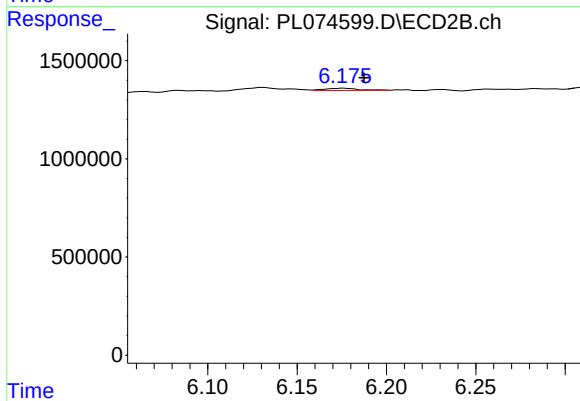

#4 Heptachlor


R.T.: 6.177 min
Delta R.T.: -0.011 min
Response: 141290
Conc: 0.09 ng/ml

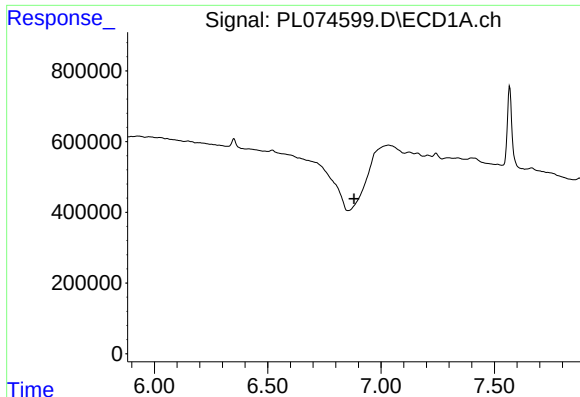

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.881 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

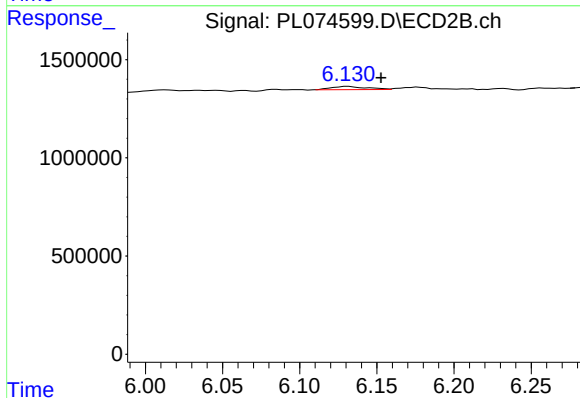


#6 beta-BHC

R.T.: 6.131 min
Delta R.T.: -0.021 min
Response: 264627
Conc: 0.33 ng/ml

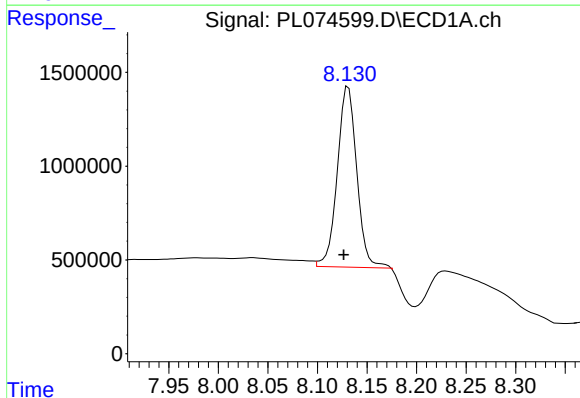


#8 Heptachlor epoxide

R.T.: 8.131 min
Delta R.T.: 0.005 min
Response: 13117061
Conc: 23.06 ng/ml

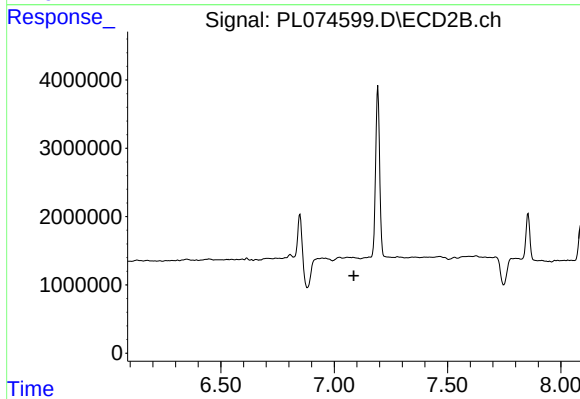

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.086 min
Response: 0
Conc: N.D.

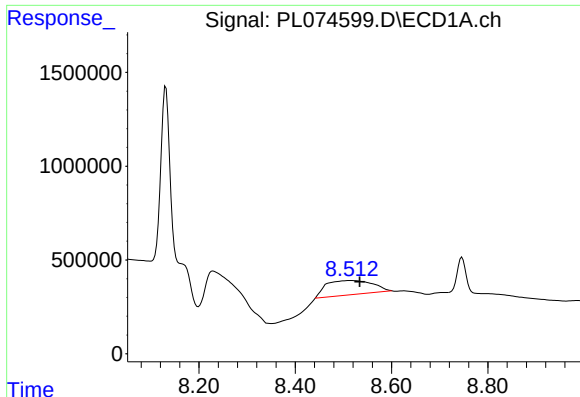

#9 Endosulfan I


R.T.: 8.513 min
Delta R.T.: -0.020 min
Response: 5142289
Conc: 8.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

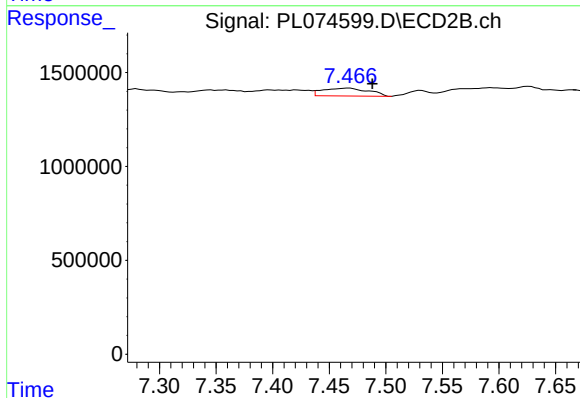


#9 Endosulfan I

R.T.: 7.467 min
Delta R.T.: -0.021 min
Response: 1177943
Conc: 0.94 ng/ml

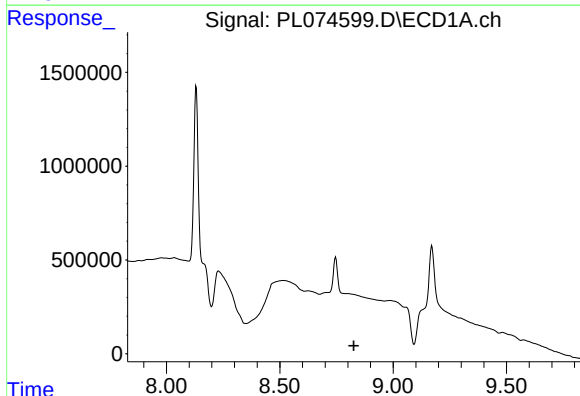


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.826 min
Response: 0
Conc: N.D.

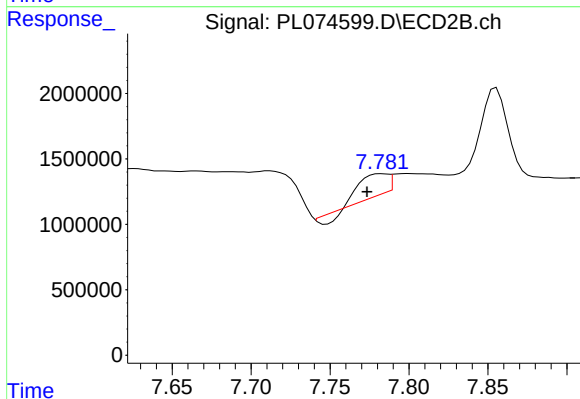

#13 Dieldrin


R.T.: 7.783 min
Delta R.T.: 0.009 min
Response: 1635236
Conc: 1.28 ng/ml

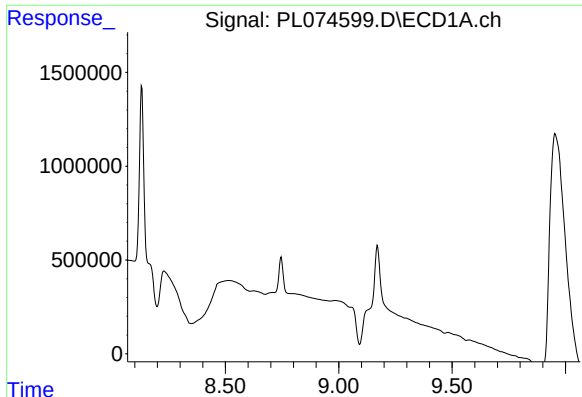

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.067 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

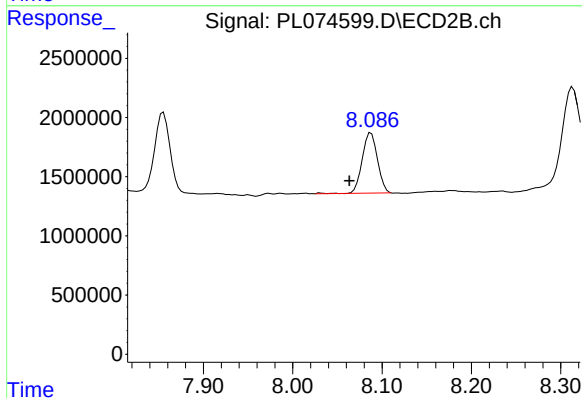


#14 Endrin

R.T.: 8.088 min
Delta R.T.: 0.024 min
Response: 6062621
Conc: 5.74 ng/ml

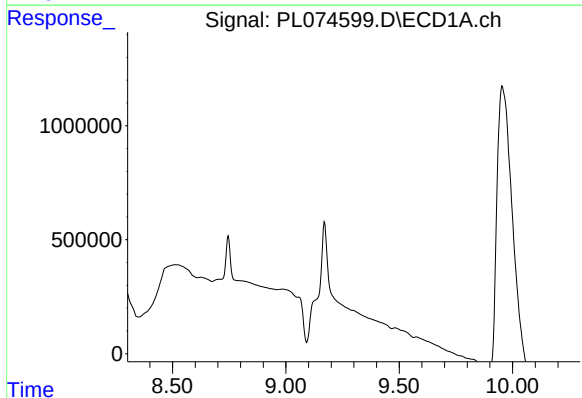


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 9.301 min
Response: 0
Conc: N.D.

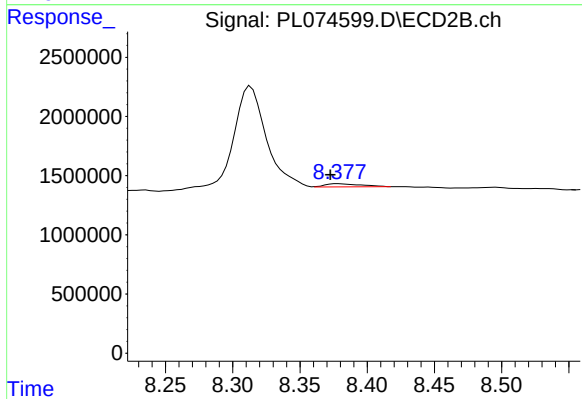

#15 Endosulfan II


R.T.: 8.379 min
Delta R.T.: 0.006 min
Response: 489853
Conc: 0.43 ng/ml

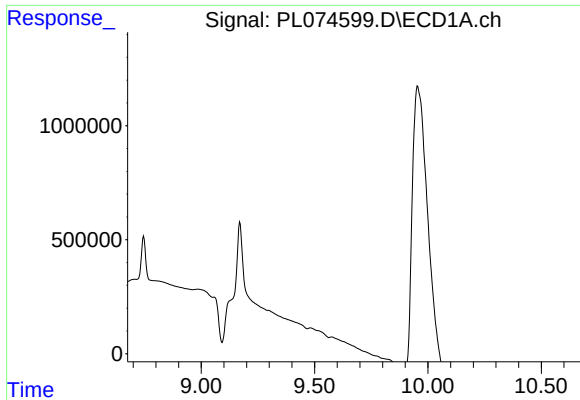

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

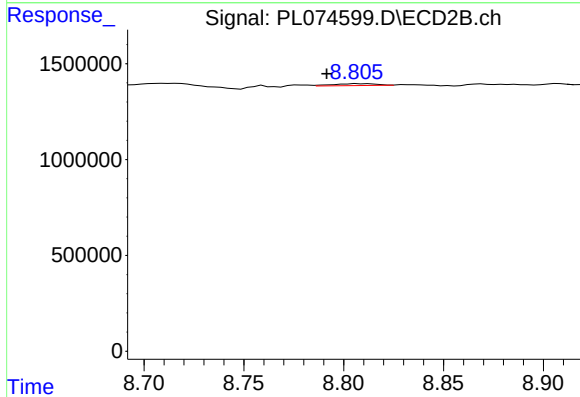


#19 Endosulfan Sulfate

R.T.: 8.807 min
Delta R.T.: 0.016 min
Response: 142748
Conc: 0.13 ng/ml

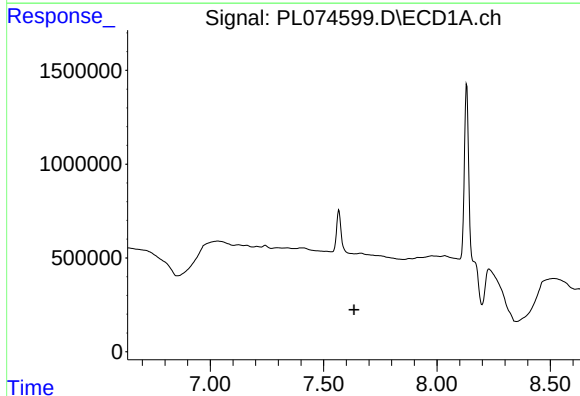


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 7.634 min
Response: 0
Conc: N.D.

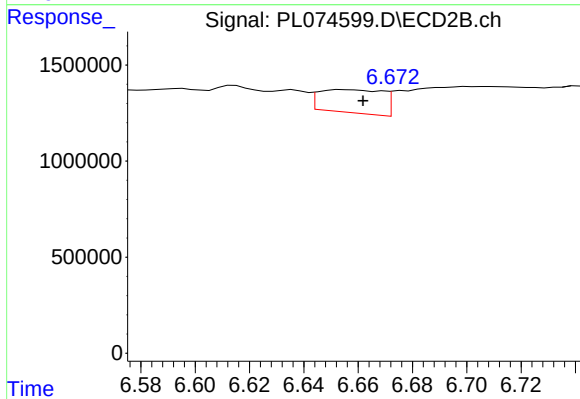

#24 Chlordane-2


R.T.: 6.654 min
Delta R.T.: -0.008 min
Response: 1945292
Conc: 35.03 ng/ml

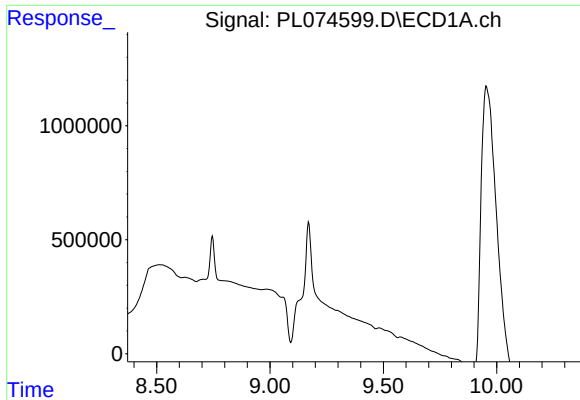

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

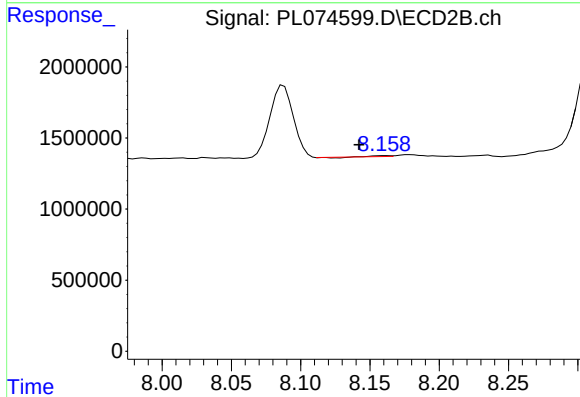


#27 Chlordane-5

R.T.: 8.161 min
Delta R.T.: 0.019 min
Response: 22850
Conc: 0.62 ng/ml

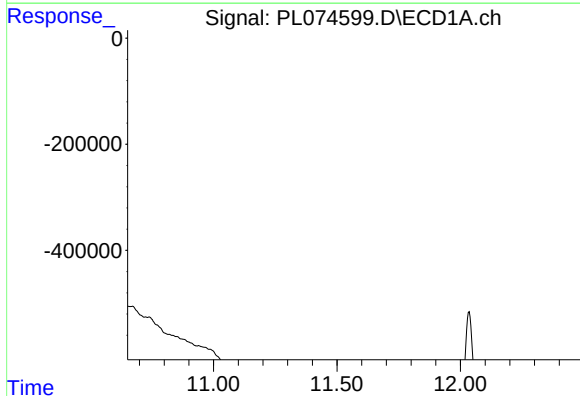

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 11.650 min
Response: 0
Conc: N.D.

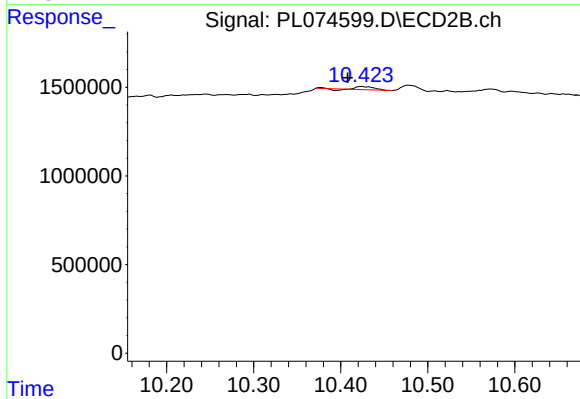

#28 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: 0.017 min
Response: 206781
Conc: 0.20 ng/ml