

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
 Data File : PL074637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2022 22:51
 Operator : AR\AJ
 Sample : N2749-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 01:40:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.652	5875972	14348398	11.573	10.454
28)	SA Decachlor...	11.647	10.405	7909623	17073378	17.711	16.634
Target Compounds							
6)	B beta-BHC	0.000	6.128f	0	501230	N.D.	0.631 #
8)	B Heptachlo...	8.122	0.000	217348	0	0.382	N.D. #
9)	A Endosulfan I	8.526	0.000	5377240	0	9.327	N.D. #
12)	B 4,4'-DDE	8.661	7.642	331615	502919	0.716	0.427 #
13)	MA Dieldrin	8.818	7.779	339414	730069	0.646	0.573
14)	MA Endrin	9.060	8.079f	307215	515529	0.744	0.488 #
16)	A 4,4'-DDD	9.204	0.000	1715971	0	3.795	N.D. #
17)	MA 4,4'-DDT	0.000	8.480	0	3307578	N.D.	3.306 #
19)	B Endosulfa...	0.000	8.792	0	1083160	N.D.	0.995 #
23)	Chlordane-1	0.000	5.956f	0	169165	N.D.	3.733 #
27)	Chlordane-5	0.000	8.142	0	2191978	N.D.	59.285 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
Data File : PL074637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2022 22:51
Operator : AR\AJ
Sample : N2749-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 01:40:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

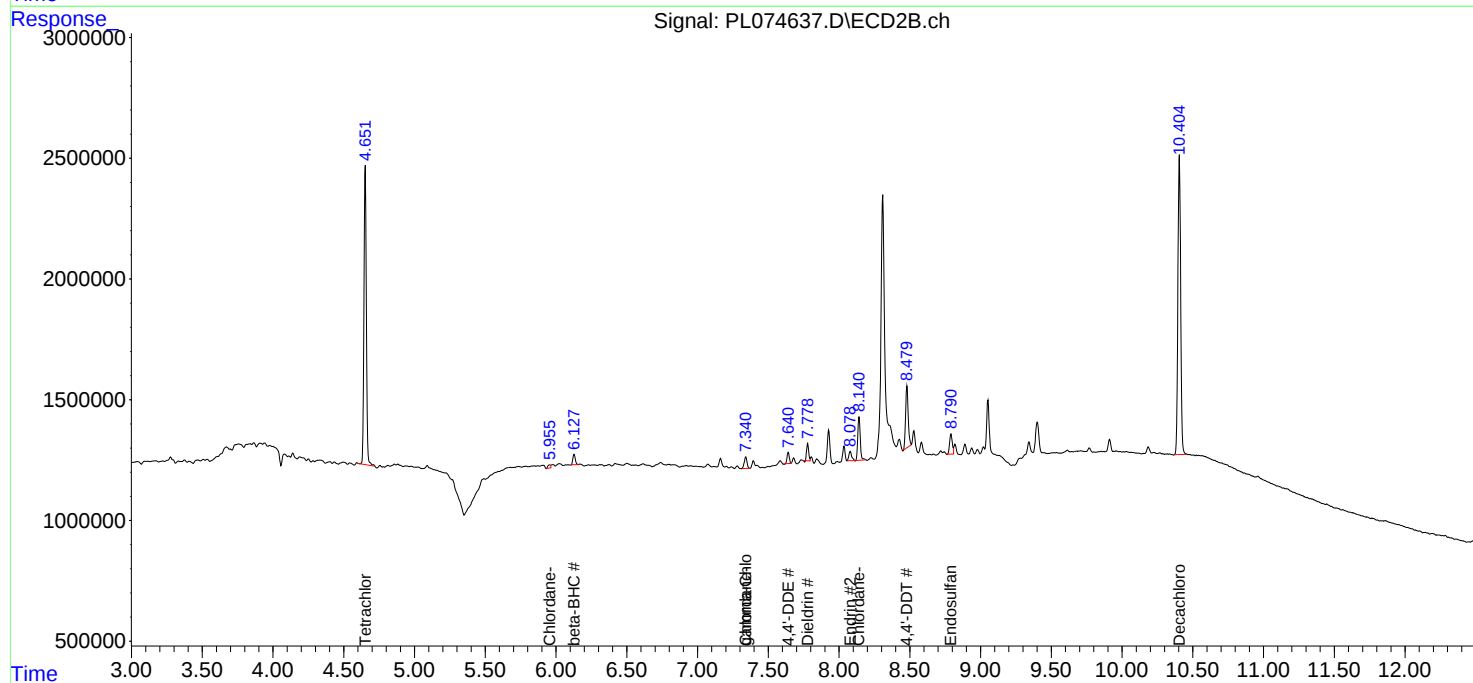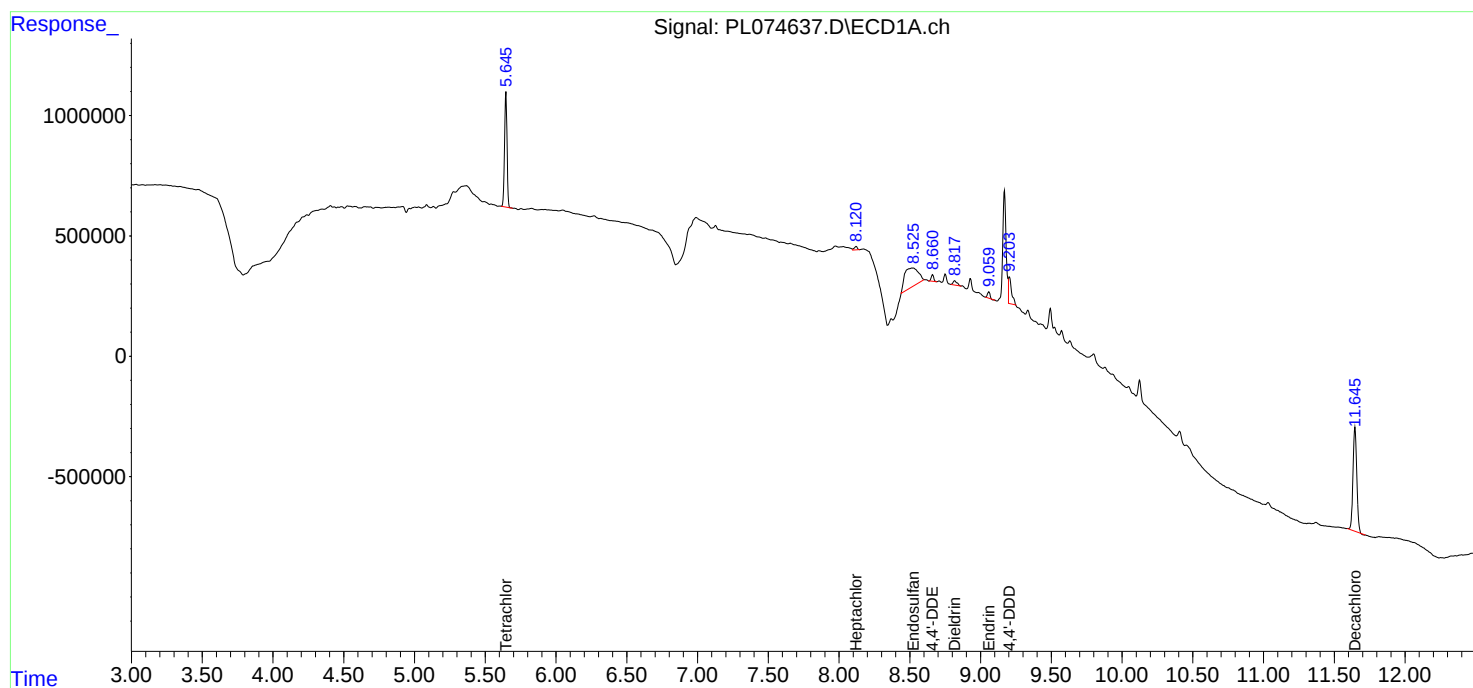


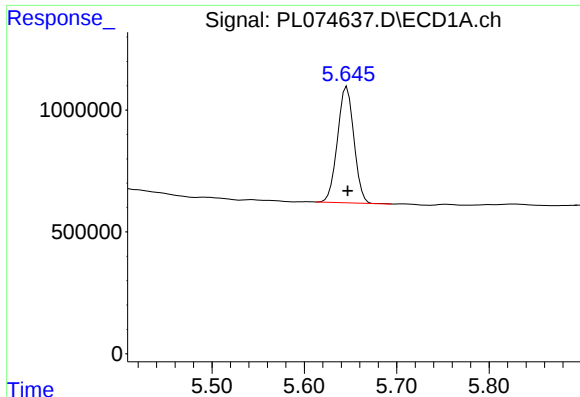

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 5875972
Conc: 11.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

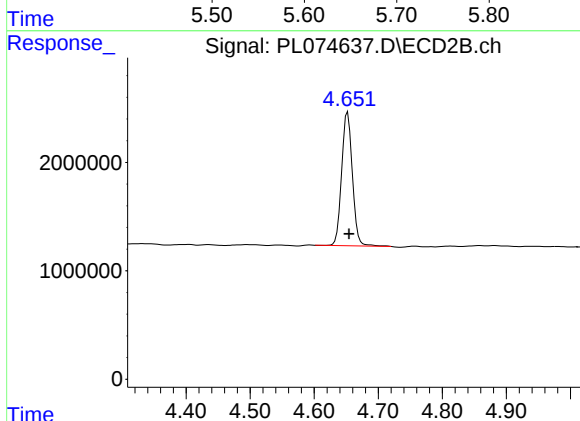


#1 Tetrachloro-m-xylene

R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 14348398
Conc: 10.45 ng/ml

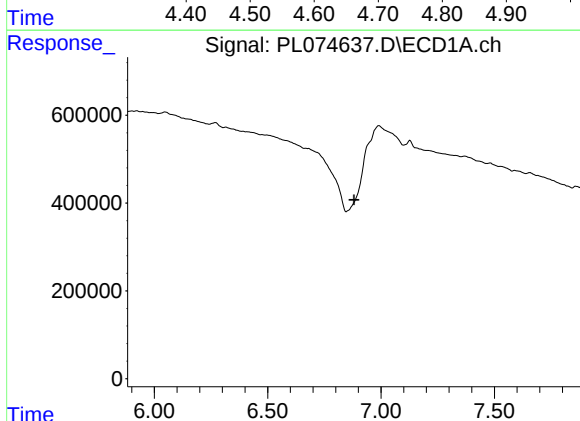


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.881 min
Response: 0
Conc: N.D.

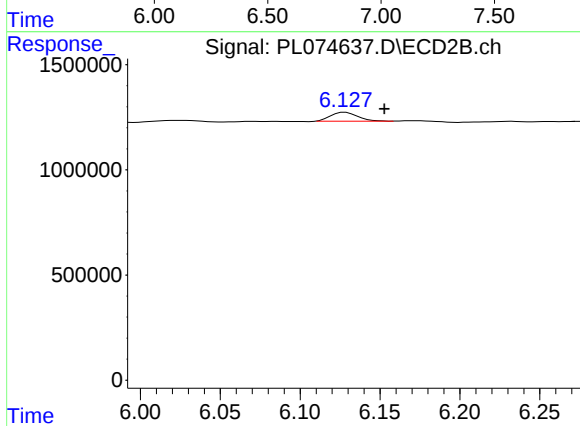

#6 beta-BHC


R.T.: 6.128 min
Delta R.T.: -0.024 min
Response: 501230
Conc: 0.63 ng/ml

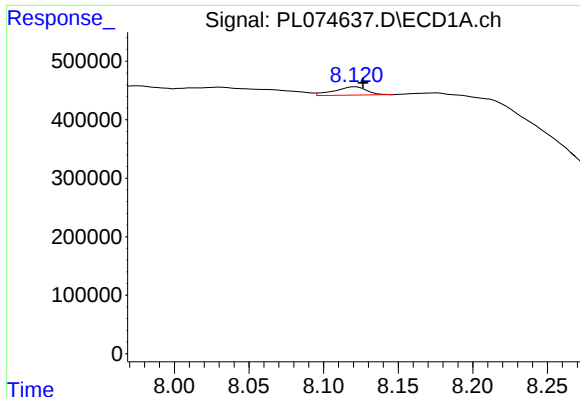

#8 Heptachlor epoxide


R.T.: 8.122 min
Delta R.T.: -0.005 min
Response: 217348
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

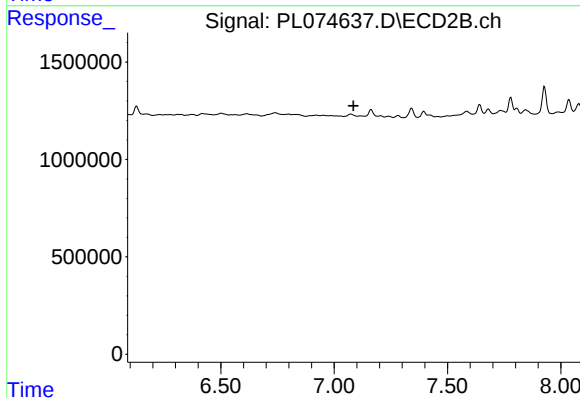


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.086 min
Response: 0
Conc: N.D.

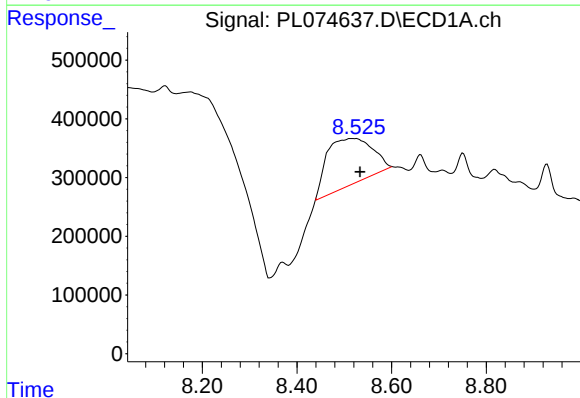


#9 Endosulfan I

R.T.: 8.526 min
Delta R.T.: -0.008 min
Response: 5377240
Conc: 9.33 ng/ml

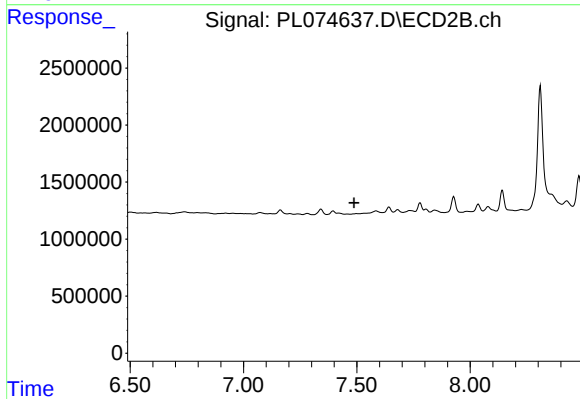

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.488 min
Response: 0
Conc: N.D.

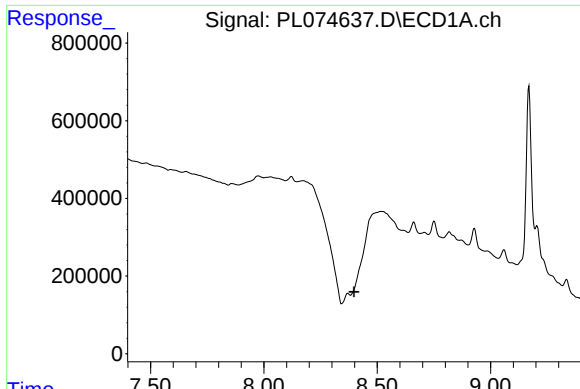

#10 gamma-Chlordane


R.T.: 8.370 min
Delta R.T.: -0.028 min
Response: -785239
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

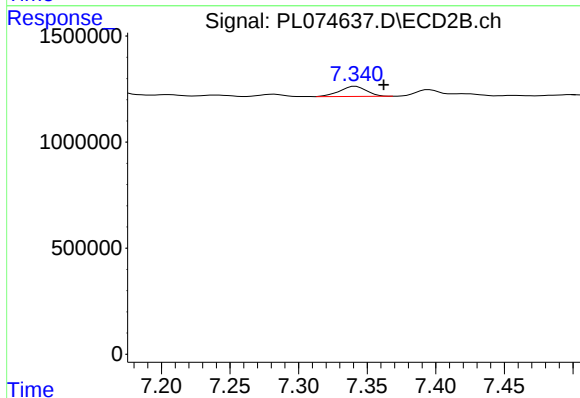


#10 gamma-Chlordane

R.T.: 7.342 min
Delta R.T.: -0.020 min
Response: 651001
Conc: 0.47 ng/ml

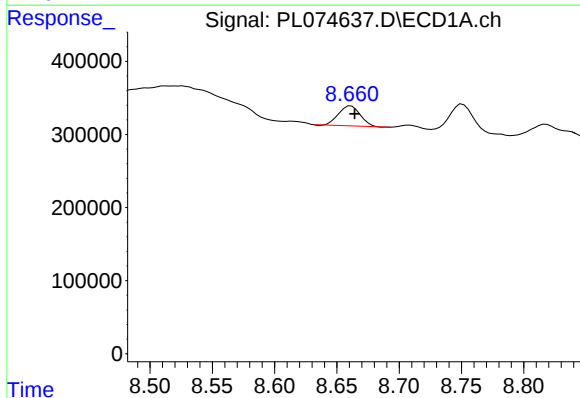


#12 4,4'-DDE

R.T.: 8.661 min
Delta R.T.: -0.003 min
Response: 331615
Conc: 0.72 ng/ml

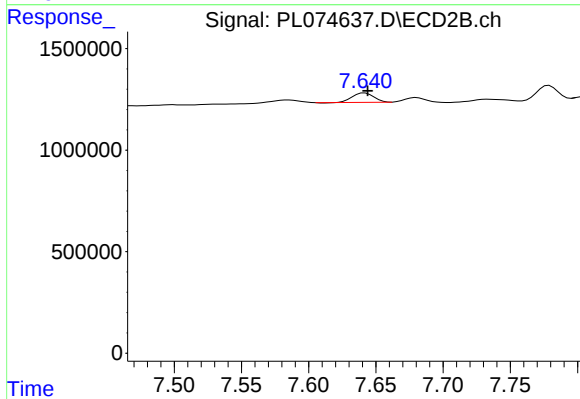

#12 4,4'-DDE


R.T.: 7.642 min
Delta R.T.: -0.002 min
Response: 502919
Conc: 0.43 ng/ml

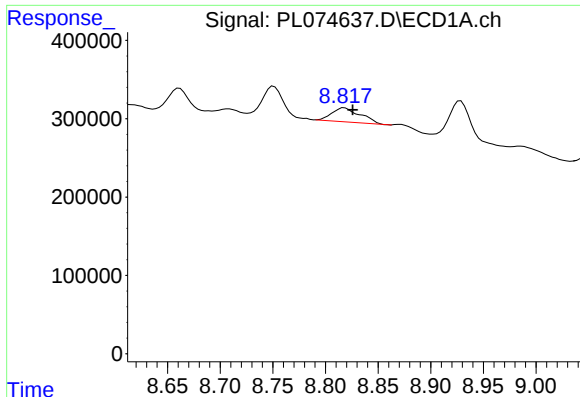

#13 Dieldrin


R.T.: 8.818 min
Delta R.T.: -0.008 min
Response: 339414
Conc: 0.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

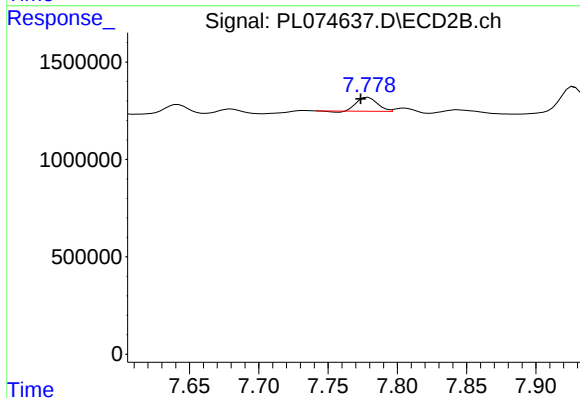


#13 Dieldrin

R.T.: 7.779 min
Delta R.T.: 0.005 min
Response: 730069
Conc: 0.57 ng/ml

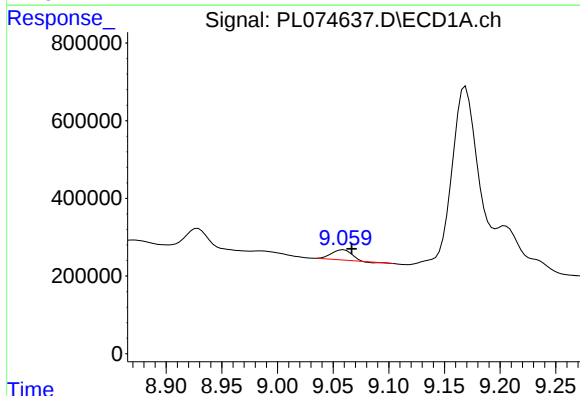


#14 Endrin

R.T.: 9.060 min
Delta R.T.: -0.007 min
Response: 307215
Conc: 0.74 ng/ml

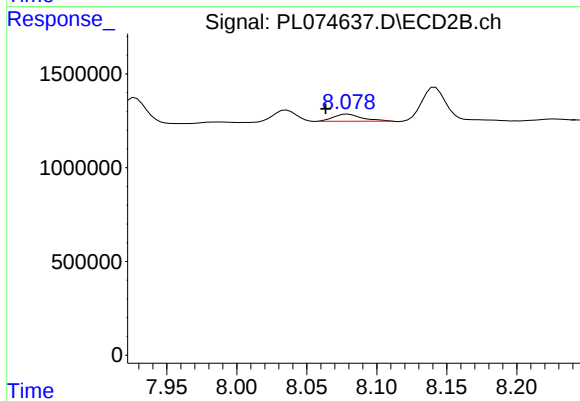

#14 Endrin


R.T.: 8.079 min
Delta R.T.: 0.016 min
Response: 515529
Conc: 0.49 ng/ml

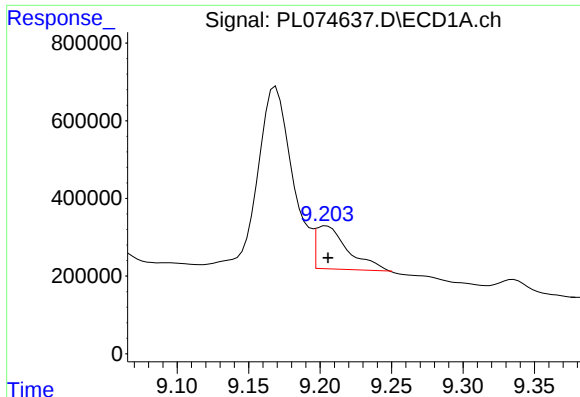

#16 4,4'-DDD


R.T.: 9.204 min
Delta R.T.: -0.001 min
Response: 1715971
Conc: 3.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

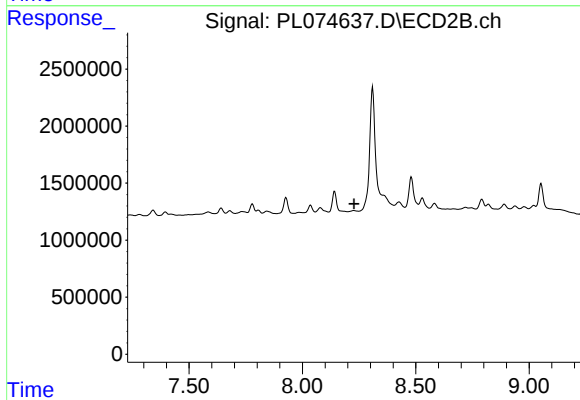


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.227 min
Response: 0
Conc: N.D.

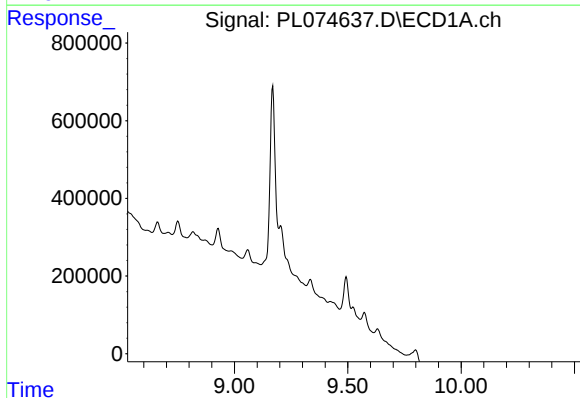


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.526 min
Response: 0
Conc: N.D.

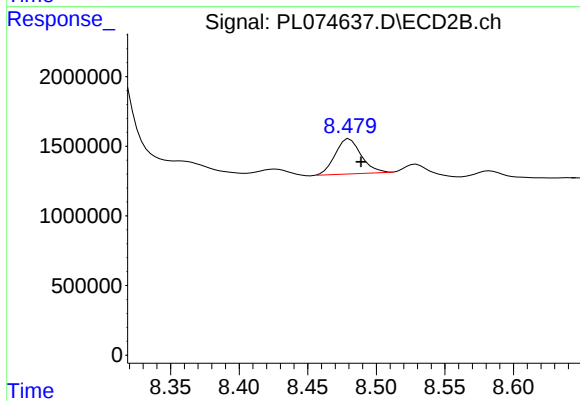

#17 4,4'-DDT


R.T.: 8.480 min
Delta R.T.: -0.008 min
Response: 3307578
Conc: 3.31 ng/ml

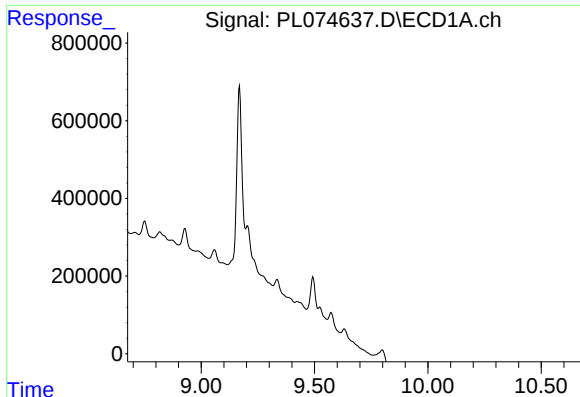

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

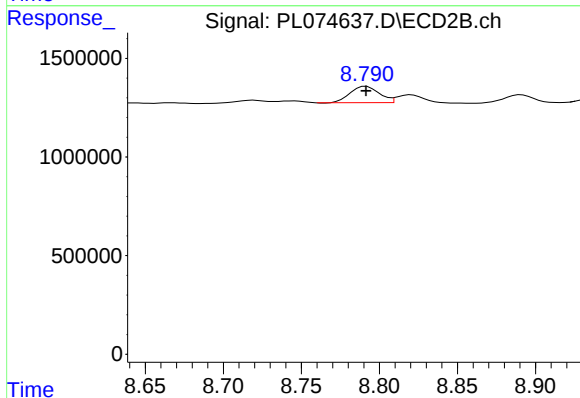


#19 Endosulfan Sulfate

R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 1083160
Conc: 1.00 ng/ml

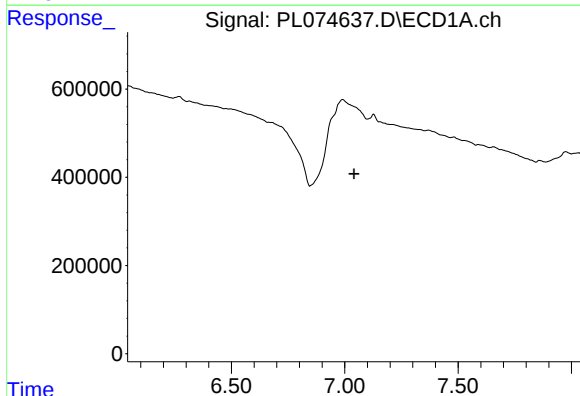


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

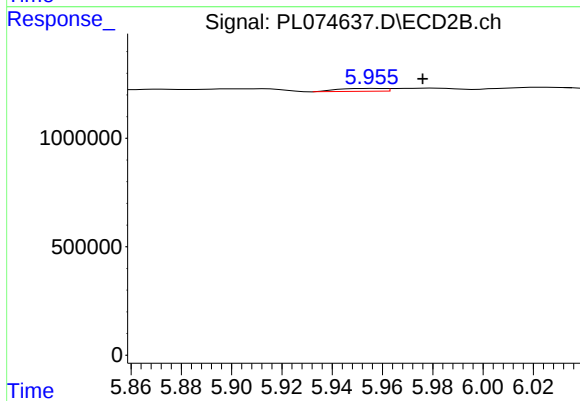

#23 Chlordane-1


R.T.: 5.956 min
Delta R.T.: -0.020 min
Response: 169165
Conc: 3.73 ng/ml

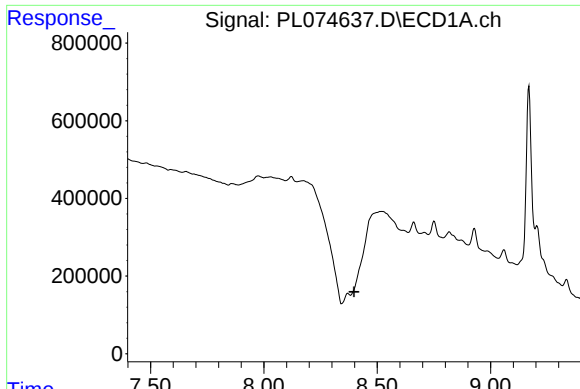

#25 Chlordane-3


R.T.: 8.370 min
Delta R.T.: -0.028 min
Response: -785239
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

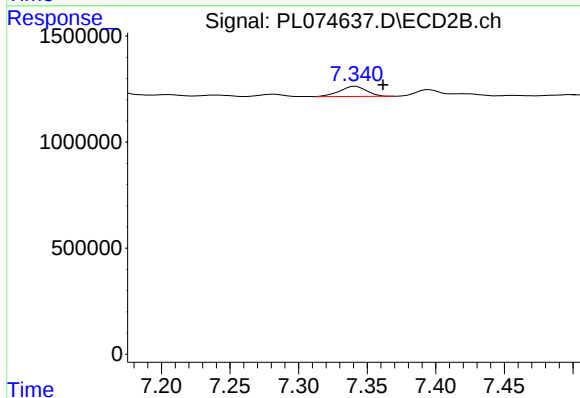


#25 Chlordane-3

R.T.: 7.342 min
Delta R.T.: -0.020 min
Response: 651001
Conc: 5.02 ng/ml

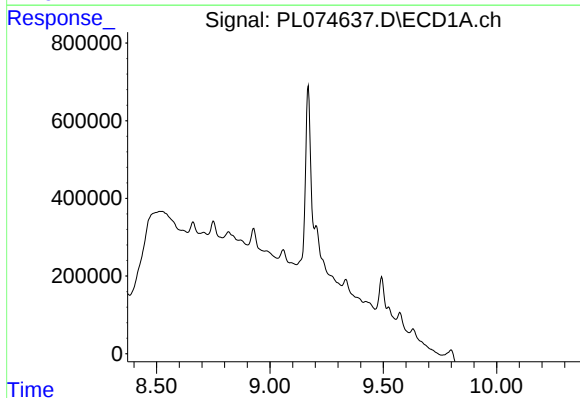


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.371 min
Response: 0
Conc: N.D.

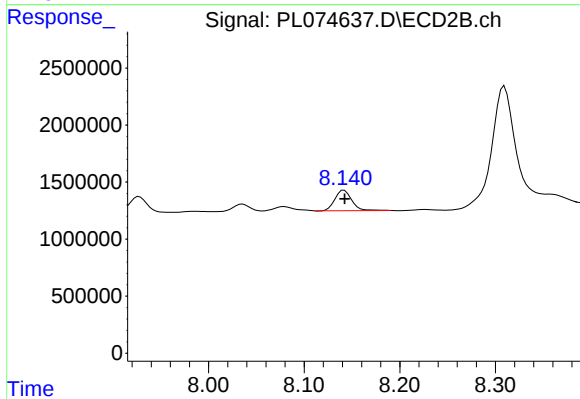

#27 Chlordane-5


R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 2191978
Conc: 59.28 ng/ml

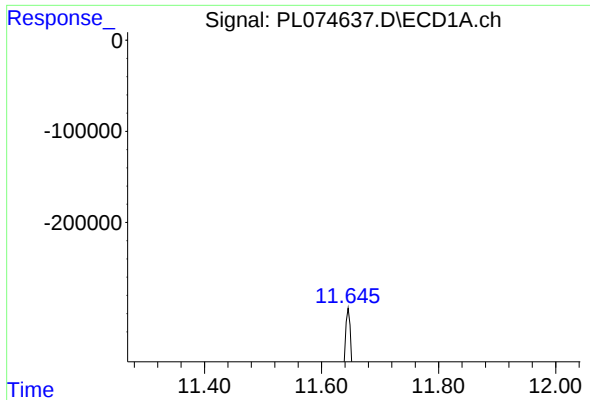

#28 Decachlorobiphenyl

R.T.: 11.647 min
Delta R.T.: -0.003 min
Response: 7909623
Conc: 17.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

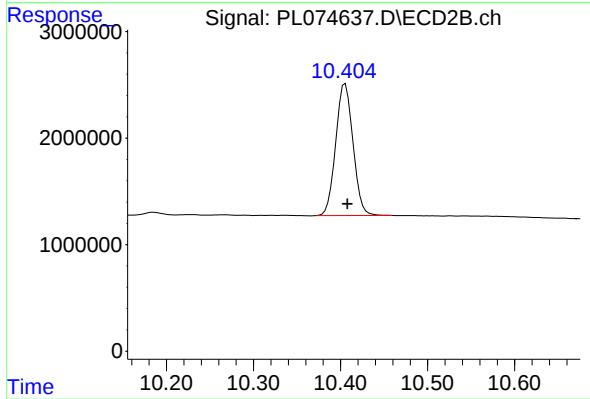

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.003 min
Response: 17073378
Conc: 16.63 ng/ml