

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
 Data File : PL074643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2022 00:30
 Operator : AR\AJ
 Sample : N2749-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 01:44:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:19:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.653	5991454	15163596	11.800	11.048
28)	SA Decachlor...	11.647	10.406	6532238	13798057	14.627	13.443
Target Compounds							
6)	B beta-BHC	0.000	6.129f	0	621042	N.D.	0.782 #
9)	A Endosulfan I	8.516f	7.503f	5228030	69418	9.069	0.055 #
10)	B gamma-Chl...	0.000	7.343f	0	578746	N.D.	0.418 #
12)	B 4,4'-DDE	8.660	7.643	246592	566415	0.533	0.481
13)	MA Dieldrin	0.000	7.779	0	896219	N.D.	0.704 #
14)	MA Endrin	9.060	8.083f	256669	568882	0.622	0.539
17)	MA 4,4'-DDT	0.000	8.481	0	2111176	N.D.	2.110 #
19)	B Endosulfa...	0.000	8.792	0	502436	N.D.	0.462 #
23)	Chlordane-1	0.000	5.954f	0	135105	N.D.	2.981 #
25)	Chlordane-3	0.000	7.343f	0	578746	N.D.	4.459 #
27)	Chlordane-5	0.000	8.142	0	1310851	N.D.	35.454 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
Data File : PL074643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2022 00:30
Operator : AR\AJ
Sample : N2749-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 01:44:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:19:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

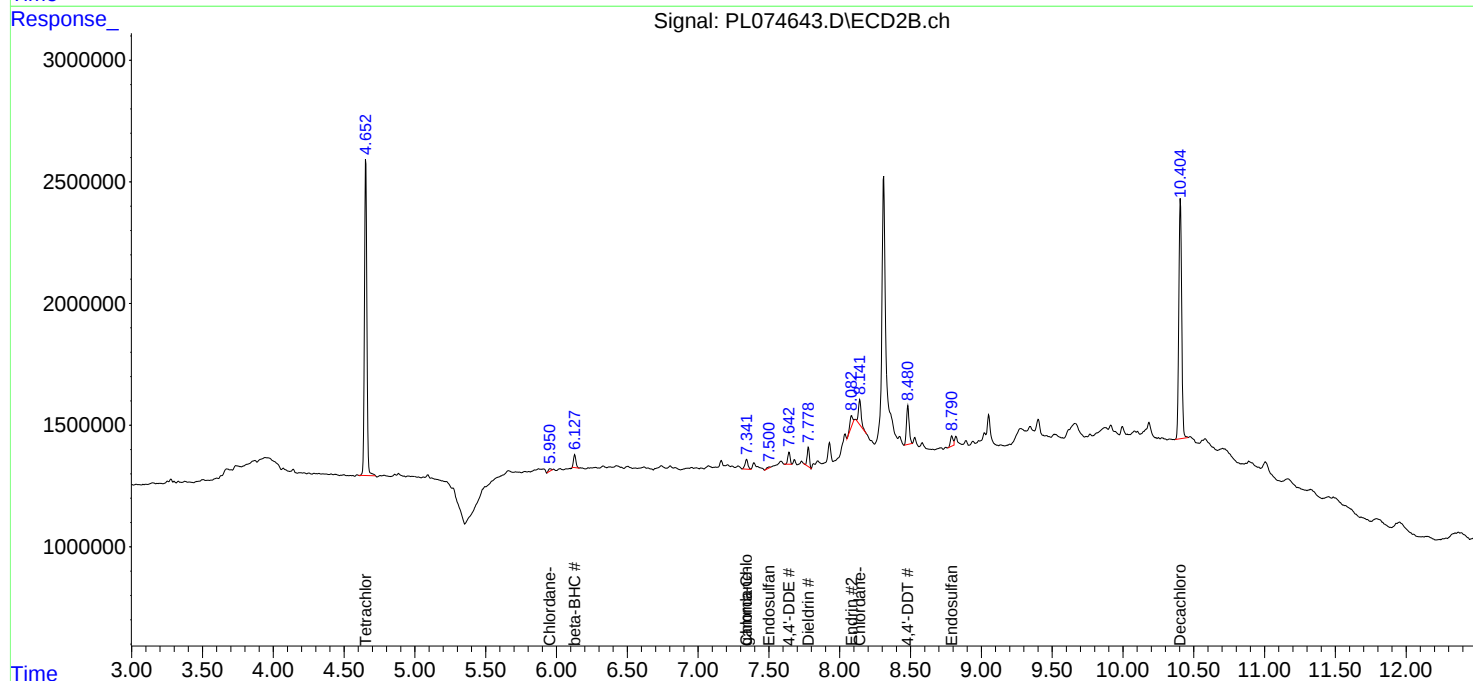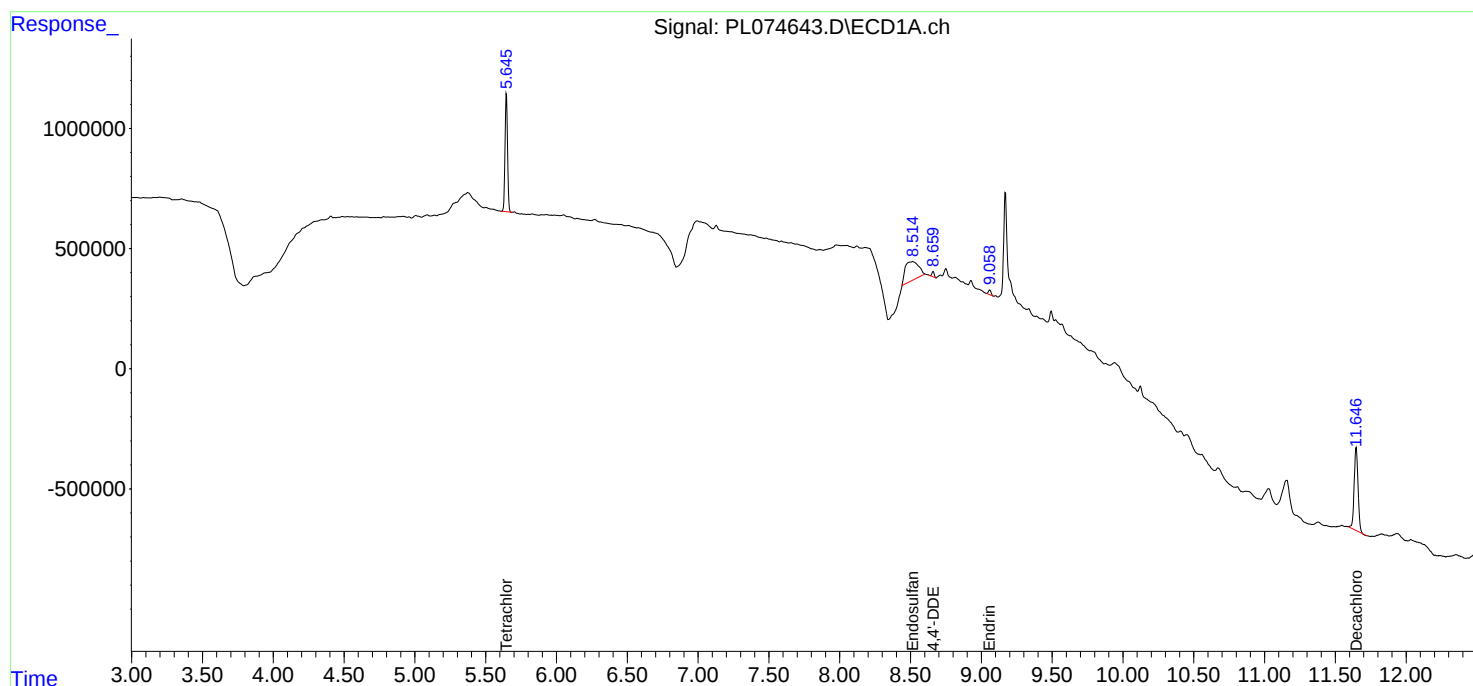


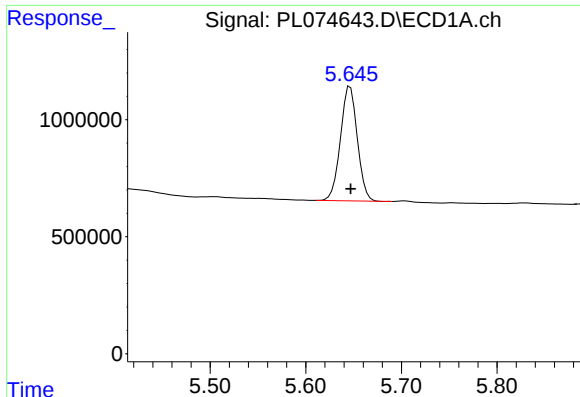

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 5991454
Conc: 11.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

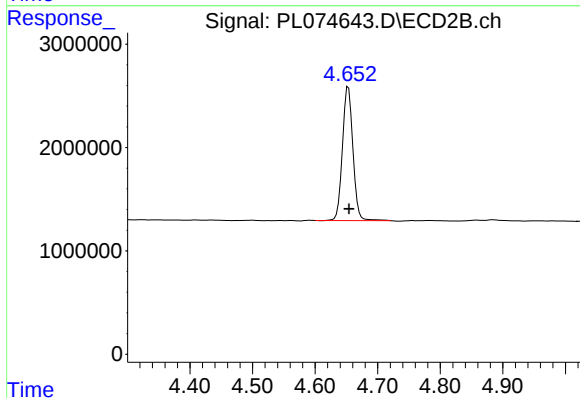


#1 Tetrachloro-m-xylene

R.T.: 4.653 min
Delta R.T.: -0.001 min
Response: 15163596
Conc: 11.05 ng/ml

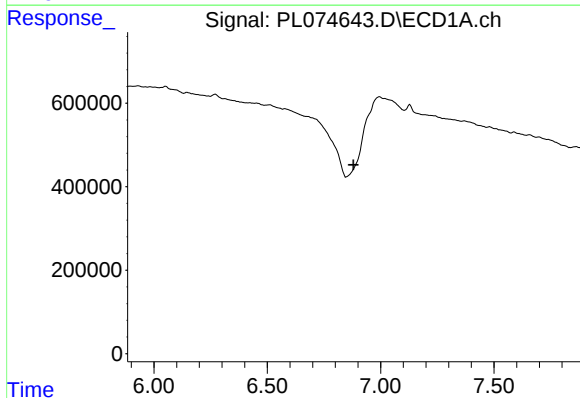


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.881 min
Response: 0
Conc: N.D.

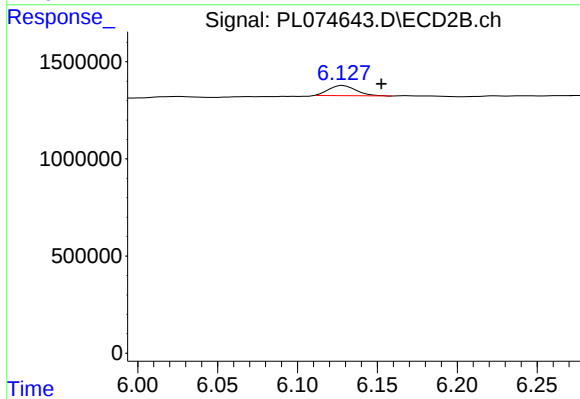

#6 beta-BHC


R.T.: 6.129 min
Delta R.T.: -0.024 min
Response: 621042
Conc: 0.78 ng/ml

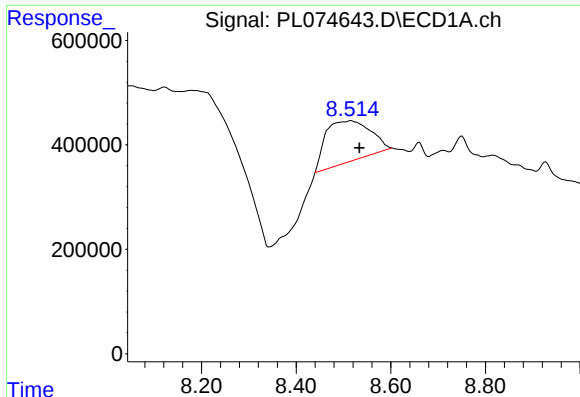

#9 Endosulfan I


R.T.: 8.516 min
Delta R.T.: -0.018 min
Response: 5228030
Conc: 9.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

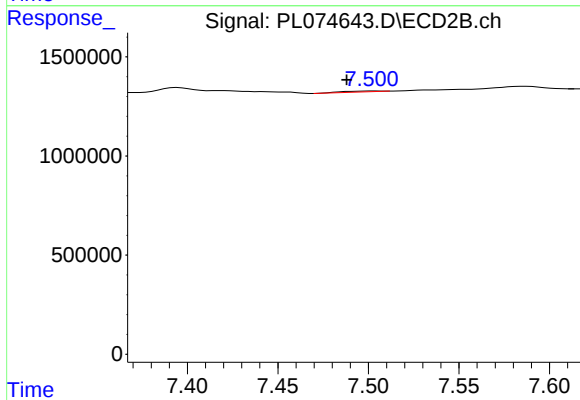


#9 Endosulfan I

R.T.: 7.503 min
Delta R.T.: 0.015 min
Response: 69418
Conc: 0.06 ng/ml

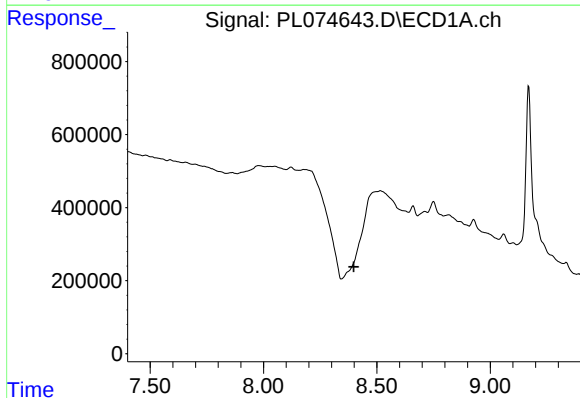


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

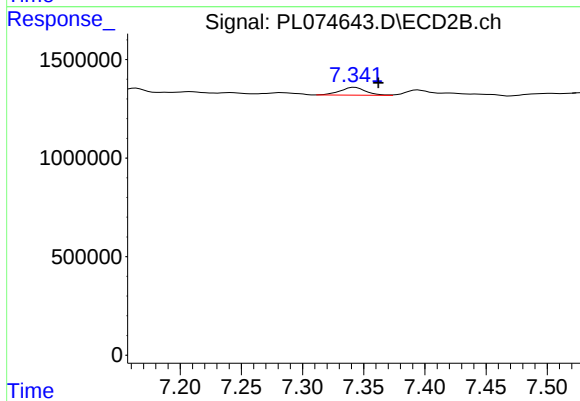

#10 gamma-Chlordane


R.T.: 7.343 min
Delta R.T.: -0.019 min
Response: 578746
Conc: 0.42 ng/ml

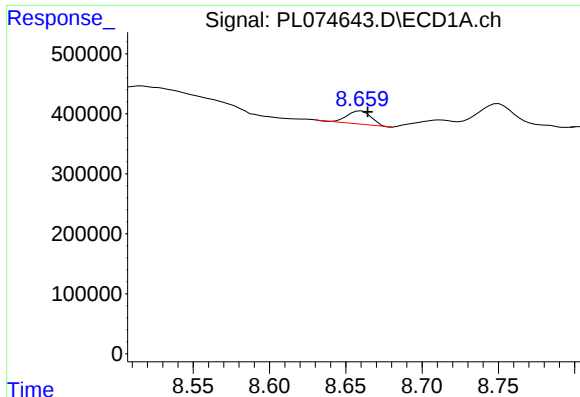

#12 4,4'-DDE


R.T.: 8.660 min
Delta R.T.: -0.004 min
Response: 246592
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

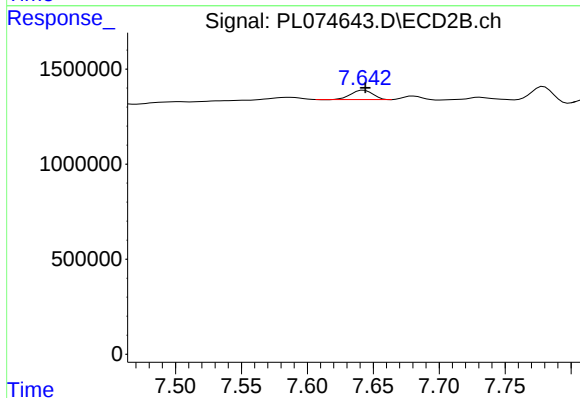


#12 4,4'-DDE

R.T.: 7.643 min
Delta R.T.: 0.000 min
Response: 566415
Conc: 0.48 ng/ml

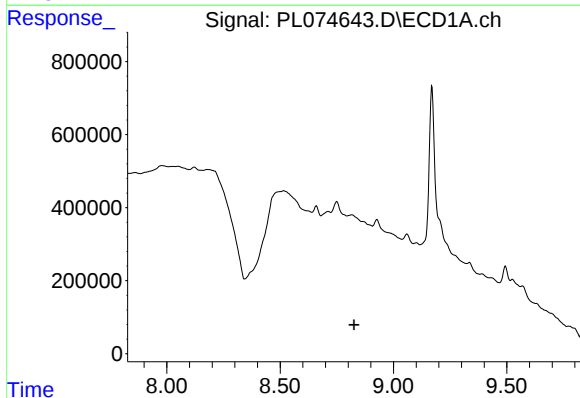


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.826 min
Response: 0
Conc: N.D.

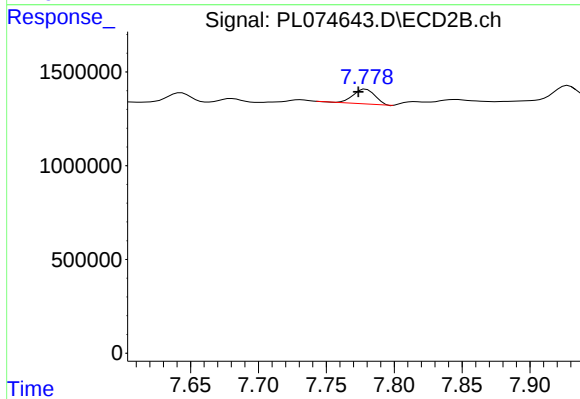

#13 Dieldrin


R.T.: 7.779 min
Delta R.T.: 0.006 min
Response: 896219
Conc: 0.70 ng/ml

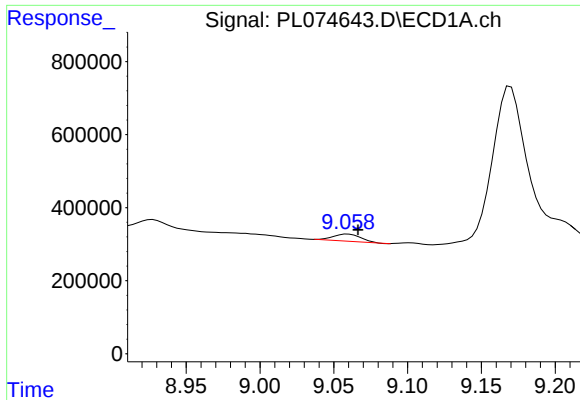

#14 Endrin


R.T.: 9.060 min
Delta R.T.: -0.007 min
Response: 256669
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

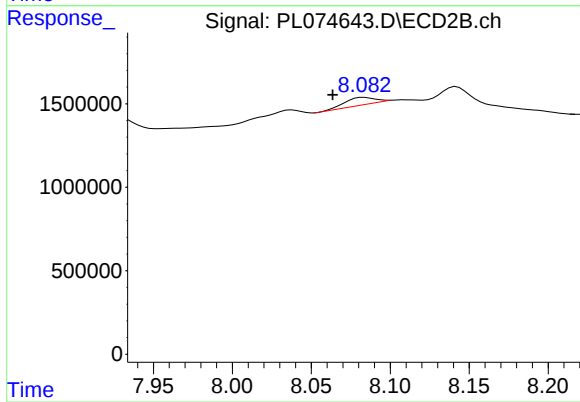


#14 Endrin

R.T.: 8.083 min
Delta R.T.: 0.020 min
Response: 568882
Conc: 0.54 ng/ml

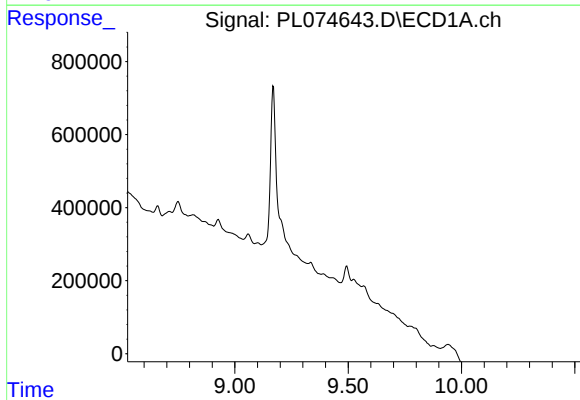


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.526 min
Response: 0
Conc: N.D.

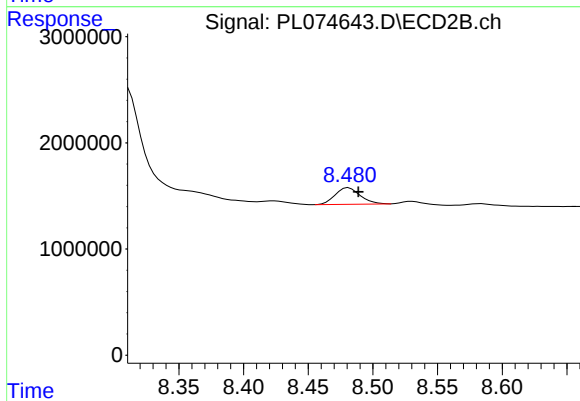

#17 4,4'-DDT


R.T.: 8.481 min
Delta R.T.: -0.007 min
Response: 2111176
Conc: 2.11 ng/ml

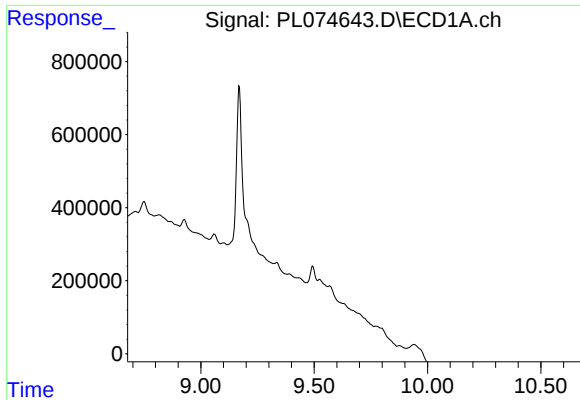

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

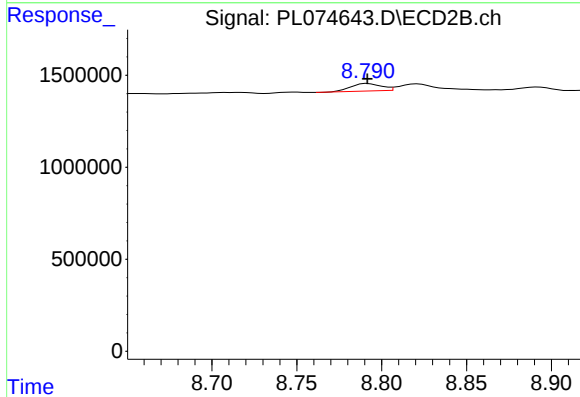


#19 Endosulfan Sulfate

R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 502436
Conc: 0.46 ng/ml

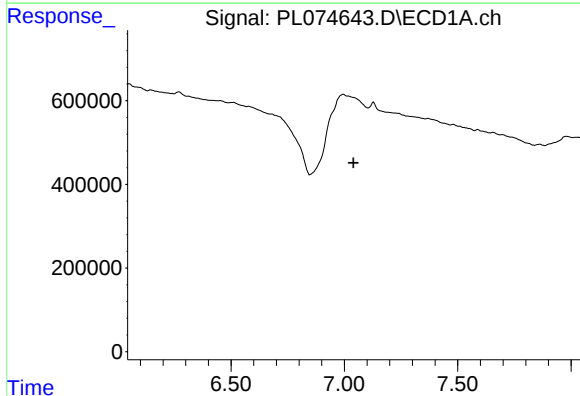


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

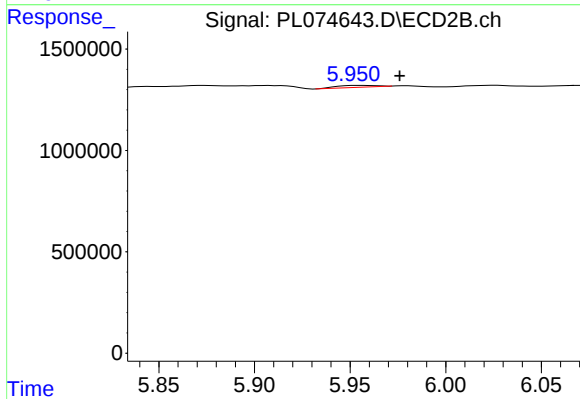

#23 Chlordane-1


R.T.: 5.954 min
Delta R.T.: -0.022 min
Response: 135105
Conc: 2.98 ng/ml

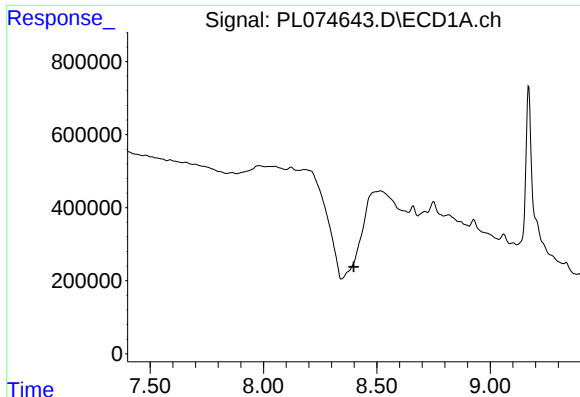

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

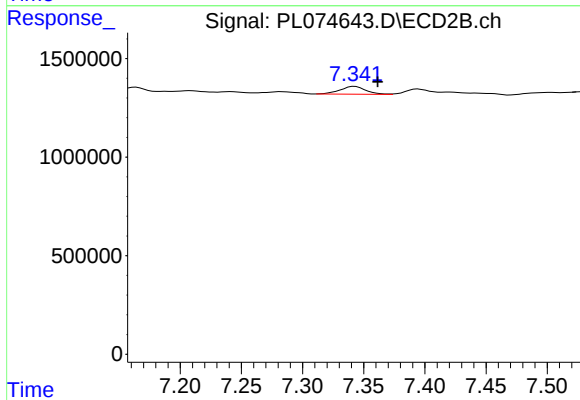


#25 Chlordane-3

R.T.: 7.343 min
Delta R.T.: -0.019 min
Response: 578746
Conc: 4.46 ng/ml

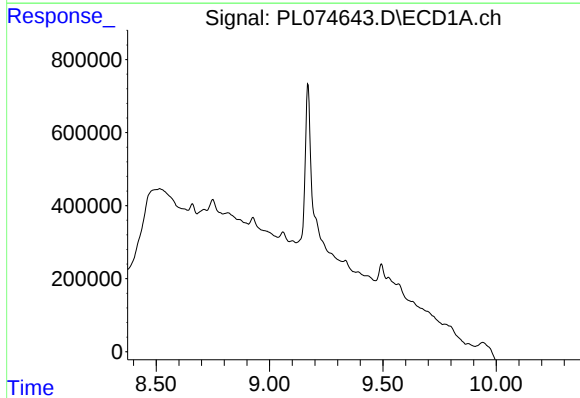


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

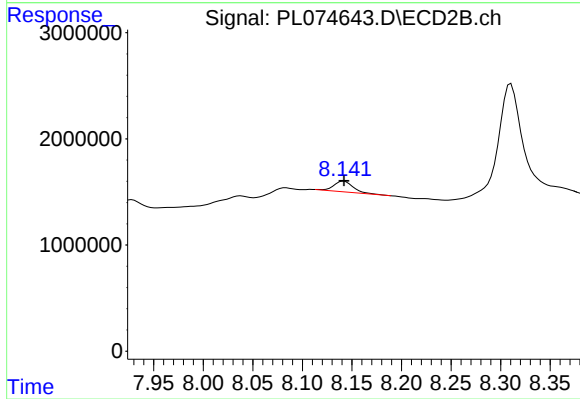

#27 Chlordane-5


R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 1310851
Conc: 35.45 ng/ml

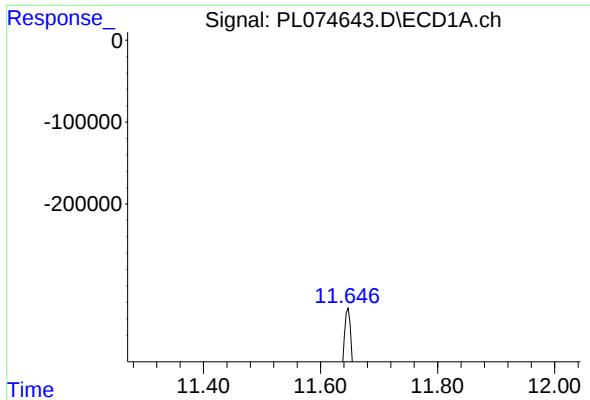

#28 Decachlorobiphenyl

R.T.: 11.647 min
Delta R.T.: -0.002 min
Response: 6532238
Conc: 14.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

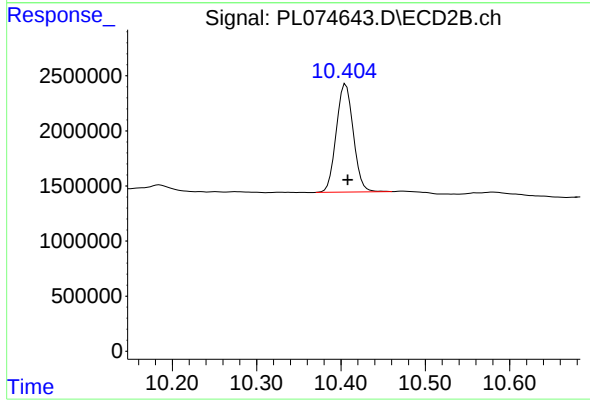

#28 Decachlorobiphenyl

R.T.: 10.406 min
Delta R.T.: -0.002 min
Response: 13798057
Conc: 13.44 ng/ml