

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
 Data File : PL074608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2022 12:08
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 15:17:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 15:16:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.653	51636678	157.3E6	99.973	97.931
28)	SA Decachlor...	11.650	10.408	43254312	96527493	94.681	93.337
Target Compounds							
23)	Chlordane-1	7.042	5.977	18425369	42283346	993.683	977.600
24)	Chlordane-2	7.636	6.663	20966785	49311830	981.688	935.090
25)	Chlordane-3	8.398	7.363	72456057	125.5E6	1046.827	991.026
26)	Chlordane-4	8.481	7.431	93399862	132.6E6	976.734	984.085
27)	Chlordane-5	9.375	8.143	15547090	34346465	1017.551	959.361



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
Data File : PL074608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2022 12:08
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 15:17:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 15:16:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

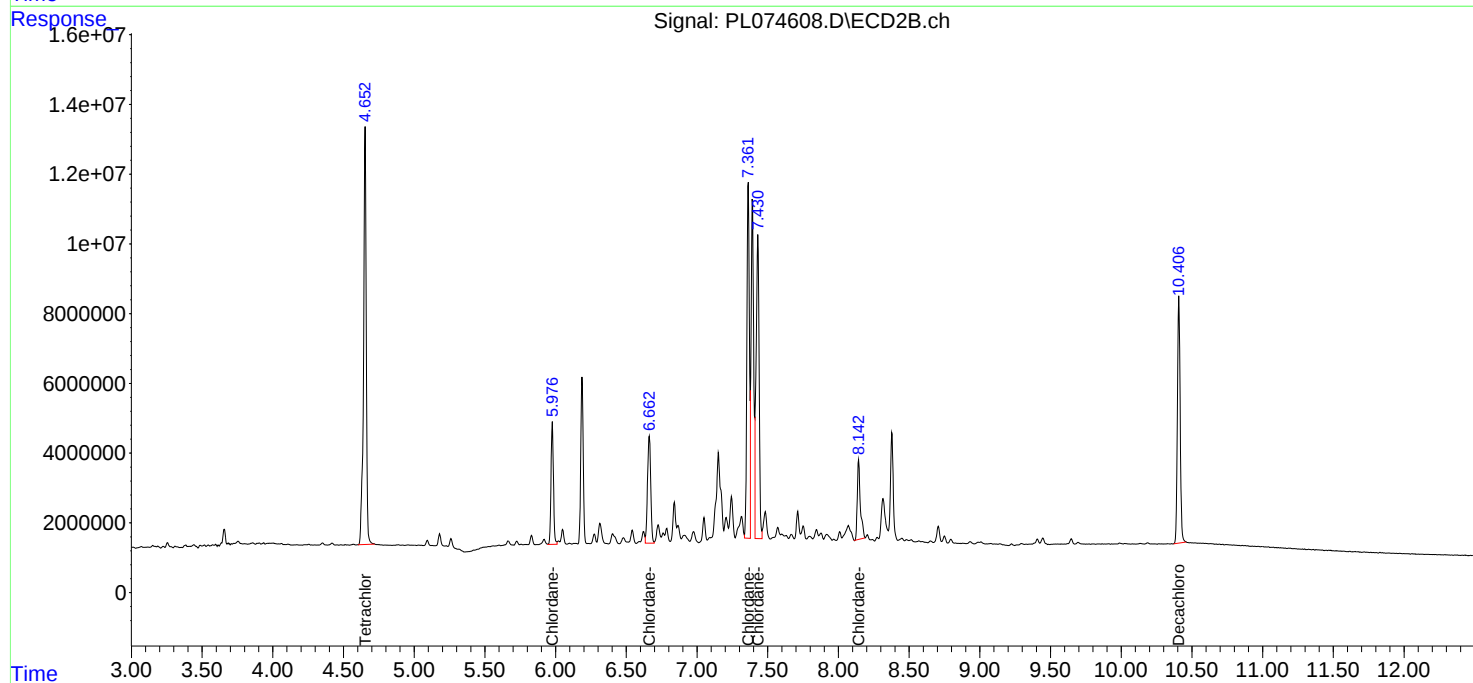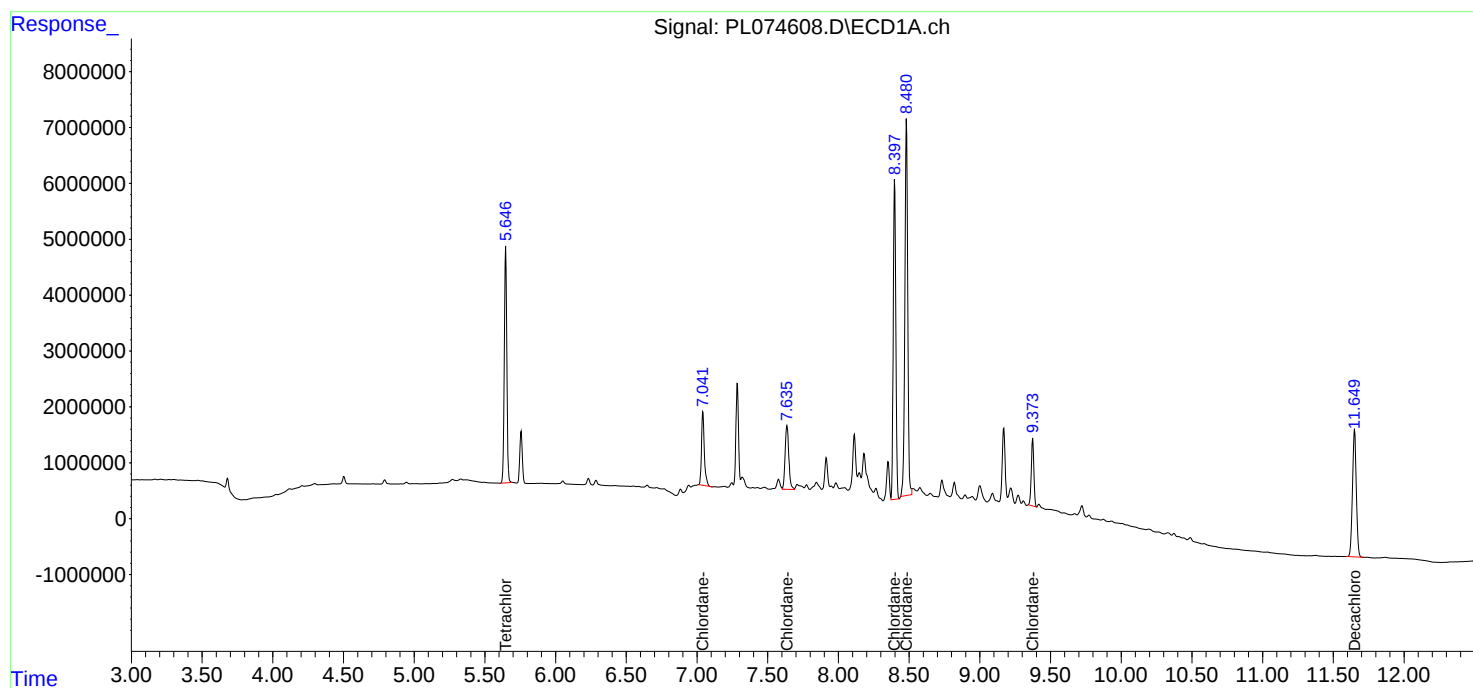


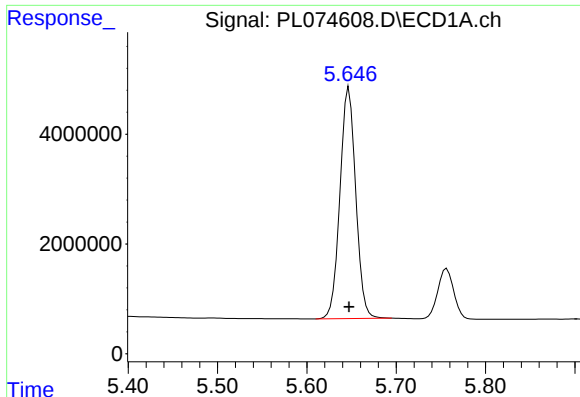

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 51636678
Conc: 99.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

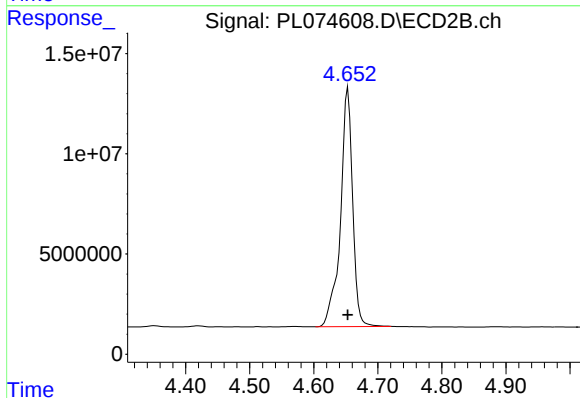


#1 Tetrachloro-m-xylene

R.T.: 4.653 min
Delta R.T.: 0.000 min
Response: 157290652
Conc: 97.93 ng/ml

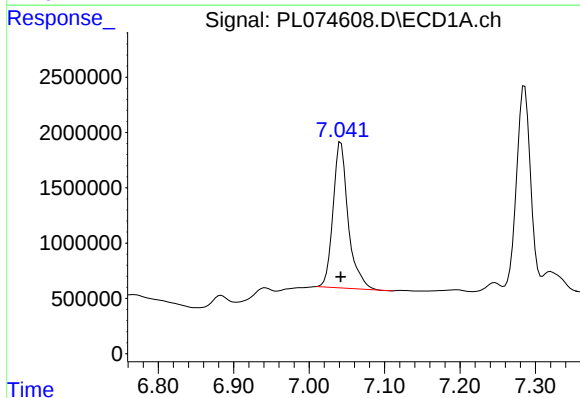


#23 Chlordane-1

R.T.: 7.042 min
Delta R.T.: 0.000 min
Response: 18425369
Conc: 993.68 ng/ml

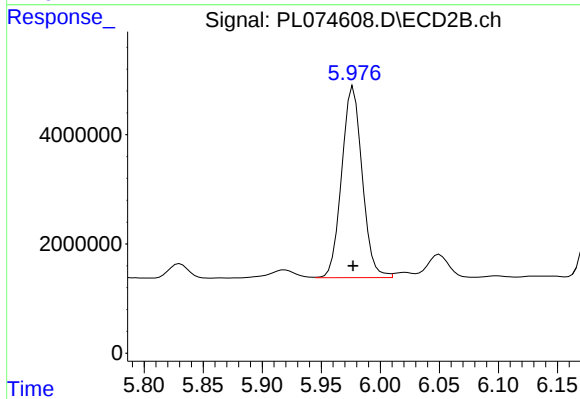

#23 Chlordane-1


R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 42283346
Conc: 977.60 ng/ml

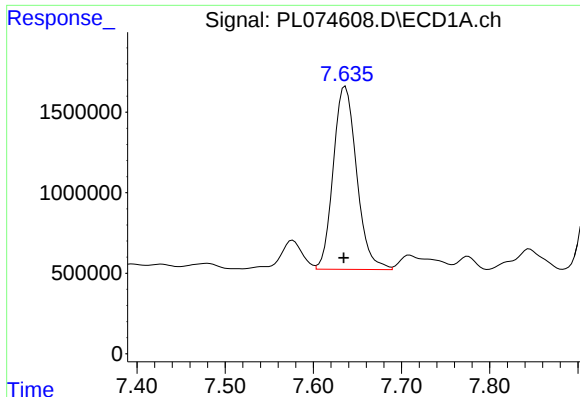

#24 Chlordane-2


R.T.: 7.636 min
Delta R.T.: 0.002 min
Response: 20966785
Conc: 981.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

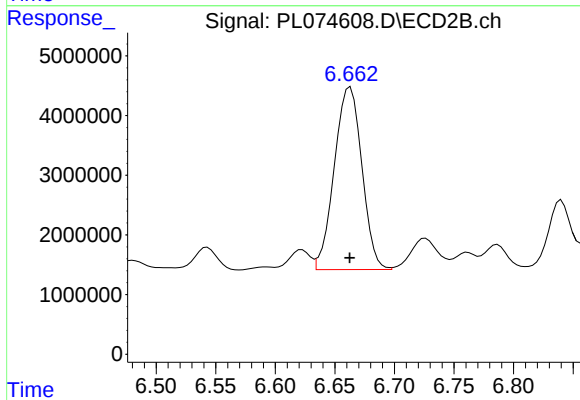


#24 Chlordane-2

R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 49311830
Conc: 935.09 ng/ml

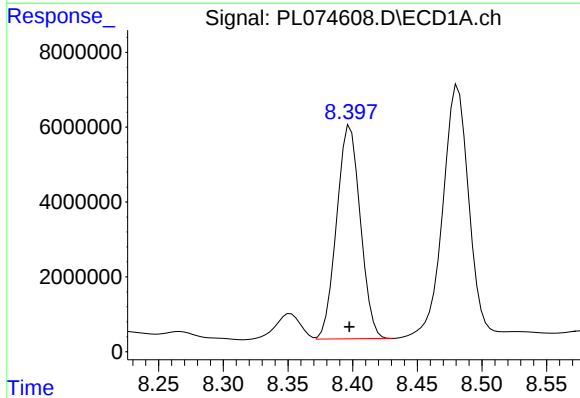


#25 Chlordane-3

R.T.: 8.398 min
Delta R.T.: 0.000 min
Response: 72456057
Conc: 1046.83 ng/ml

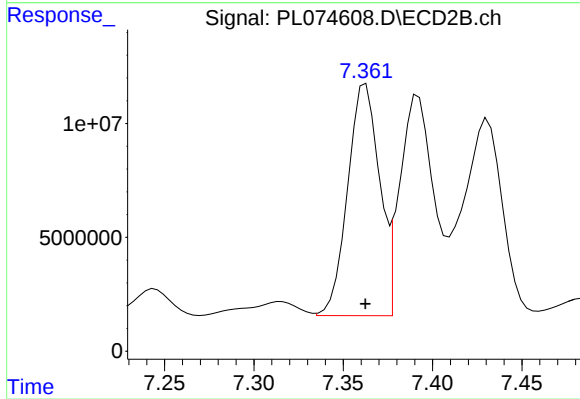

#25 Chlordane-3


R.T.: 7.363 min
Delta R.T.: 0.000 min
Response: 125519712
Conc: 991.03 ng/ml

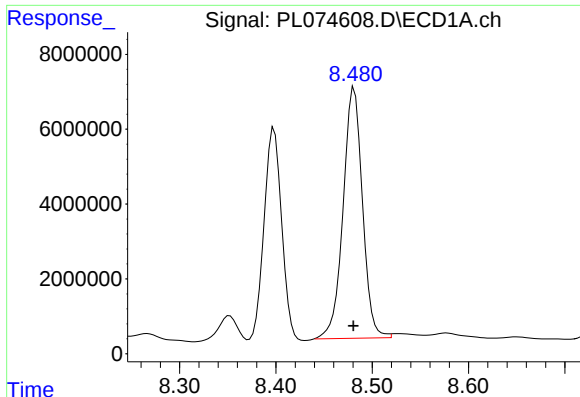

#26 Chlordane-4


R.T.: 8.481 min
Delta R.T.: 0.000 min
Response: 93399862
Conc: 976.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

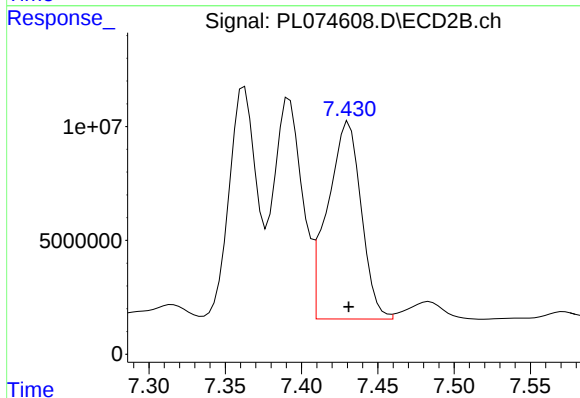


#26 Chlordane-4

R.T.: 7.431 min
Delta R.T.: 0.000 min
Response: 132604566
Conc: 984.08 ng/ml

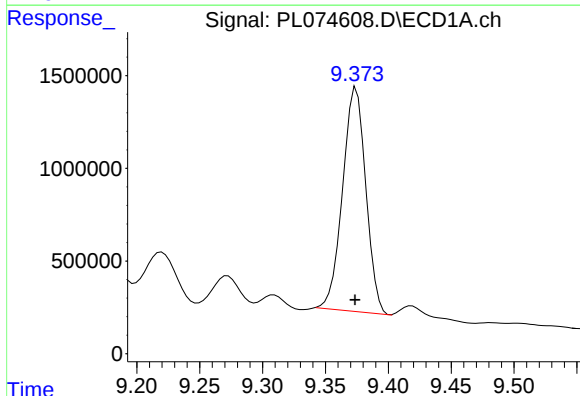


#27 Chlordane-5

R.T.: 9.375 min
Delta R.T.: 0.000 min
Response: 15547090
Conc: 1017.55 ng/ml

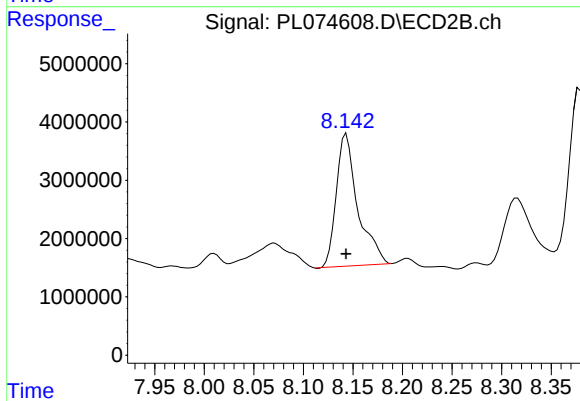

#27 Chlordane-5


R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 34346465
Conc: 959.36 ng/ml

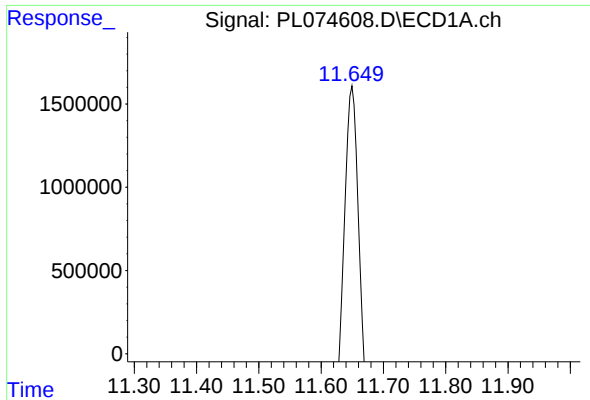

#28 Decachlorobiphenyl

R.T.: 11.650 min
Delta R.T.: 0.000 min
Response: 43254312
Conc: 94.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

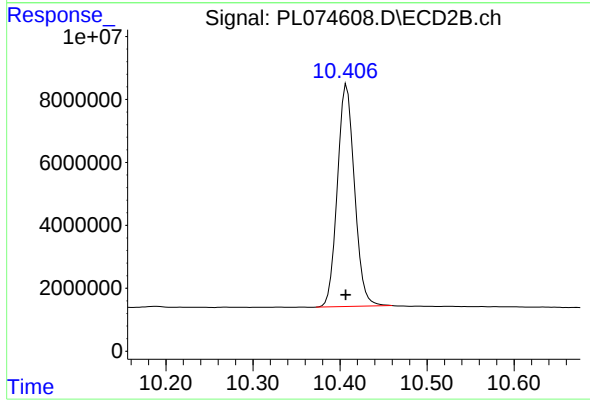

#28 Decachlorobiphenyl

R.T.: 10.408 min
Delta R.T.: 0.001 min
Response: 96527493
Conc: 93.34 ng/ml