

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
 Data File : PL074609.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2022 12:24
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 15:17:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 15:16:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.654	39147026	120.1E6	75.792	74.794
28)	SA Decachlor...	11.650	10.408	33282934	75271890	72.854	72.784
Target Compounds							
23)	Chlordane-1	7.042	5.977	13966499	32772694	753.216	757.712
24)	Chlordane-2	7.634	6.663	16084306	38597235	753.085	731.912
25)	Chlordane-3	8.398	7.363	53688372	96191856	775.676	759.472
26)	Chlordane-4	8.481	7.431	70596334	100.1E6	738.265	742.817
27)	Chlordane-5	9.374	8.143	11780588	26301069	771.035	734.638



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
Data File : PL074609.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2022 12:24
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 15:17:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 15:16:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

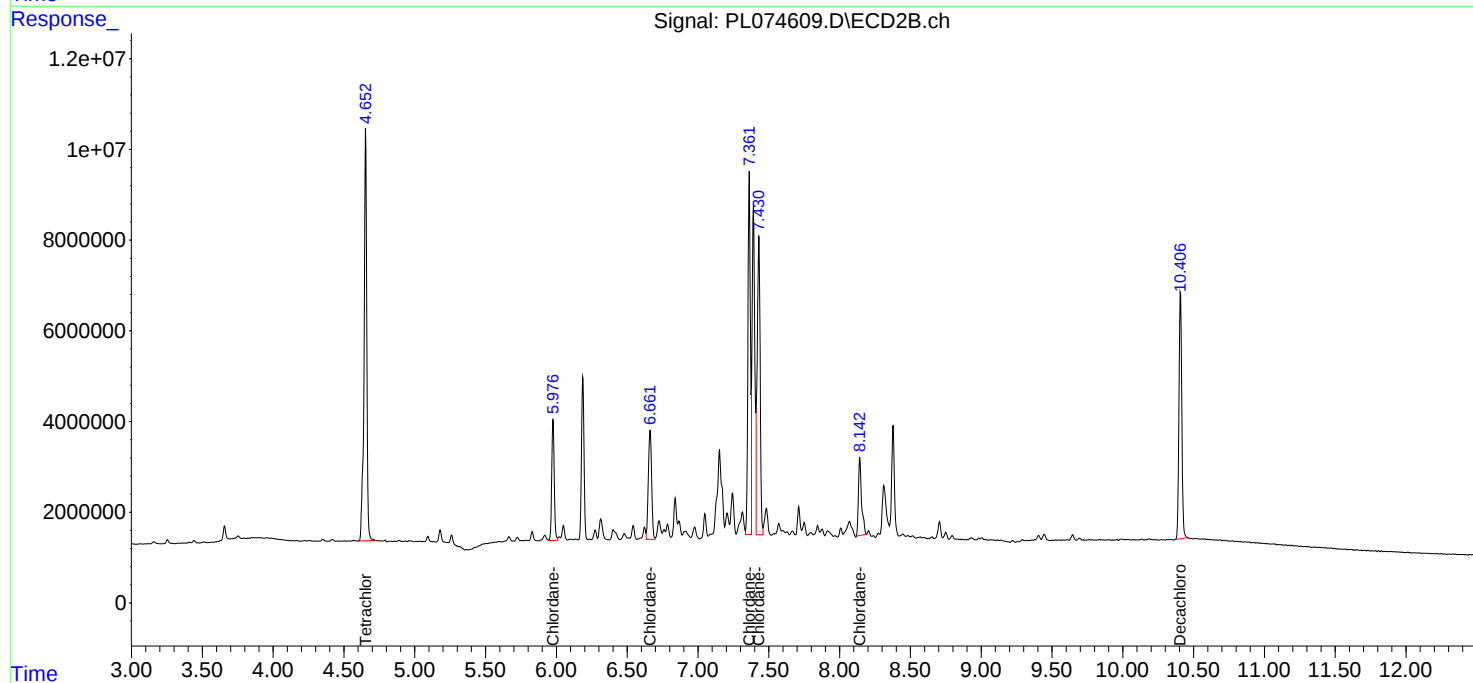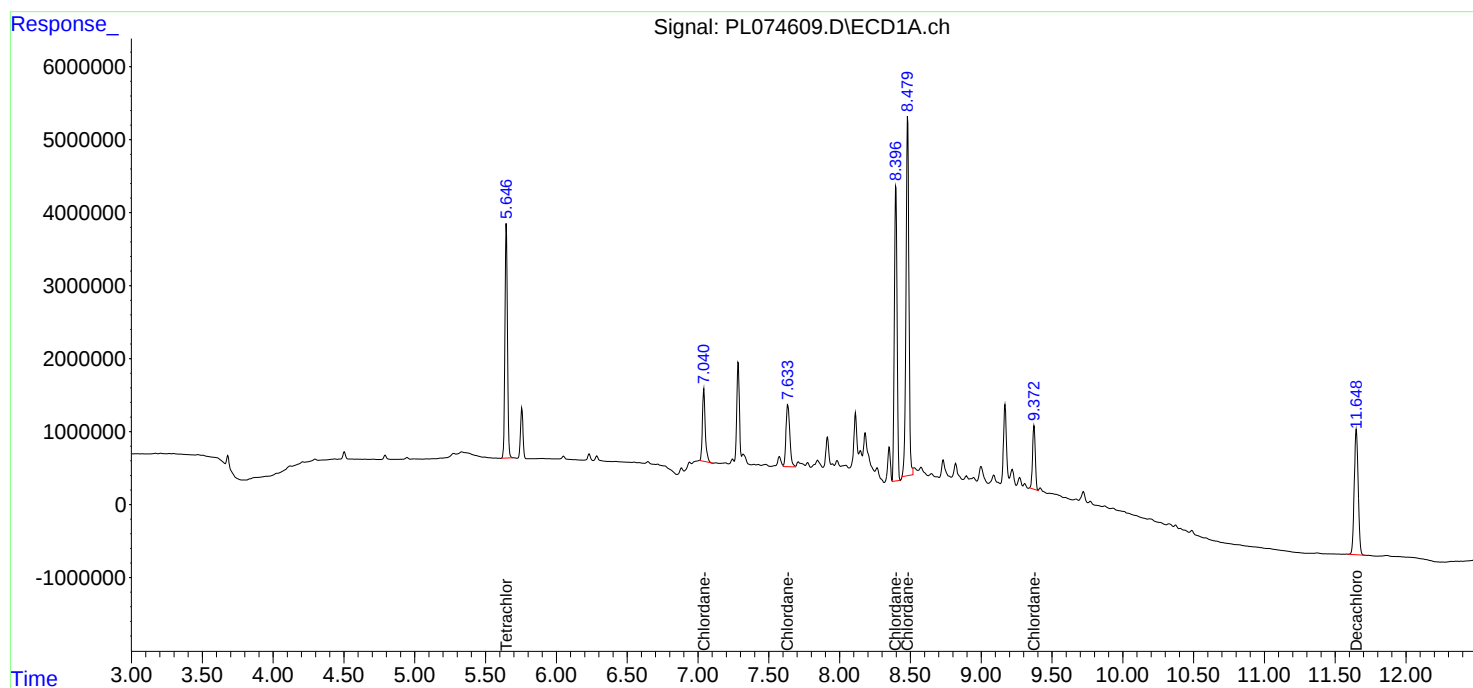


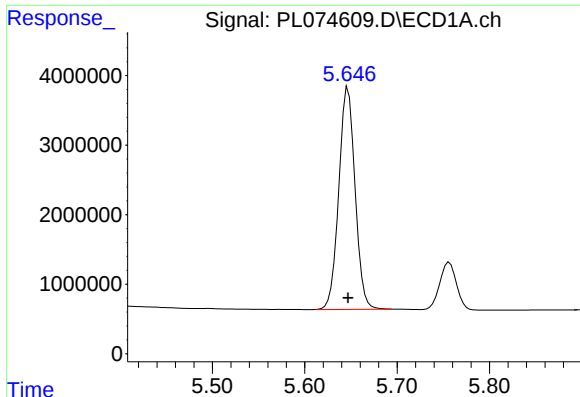

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 39147026
Conc: 75.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

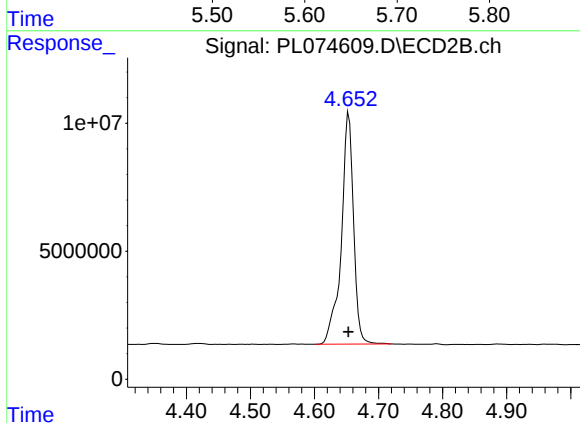


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 120130015
Conc: 74.79 ng/ml

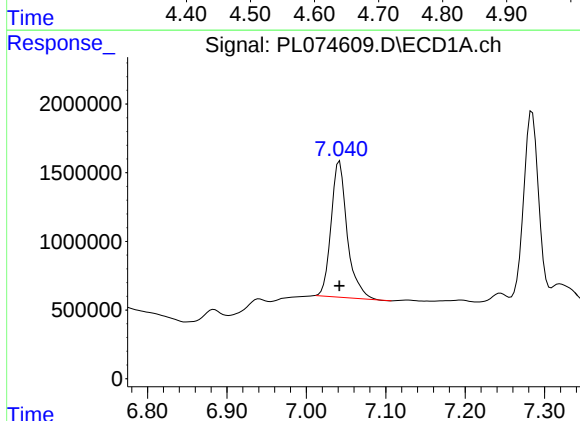


#23 Chlordane-1

R.T.: 7.042 min
Delta R.T.: 0.000 min
Response: 13966499
Conc: 753.22 ng/ml

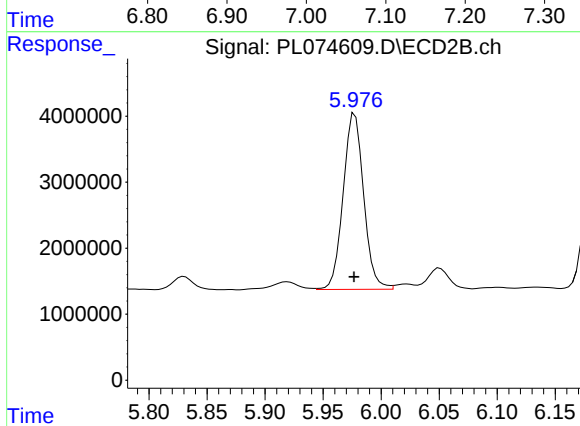

#23 Chlordane-1


R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 32772694
Conc: 757.71 ng/ml

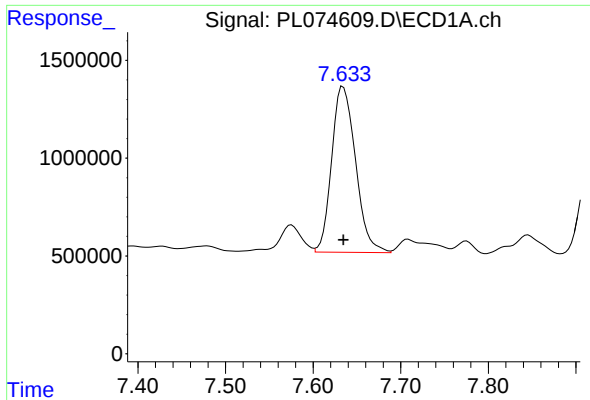

#24 Chlordane-2


R.T.: 7.634 min
Delta R.T.: 0.000 min
Response: 16084306
Conc: 753.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

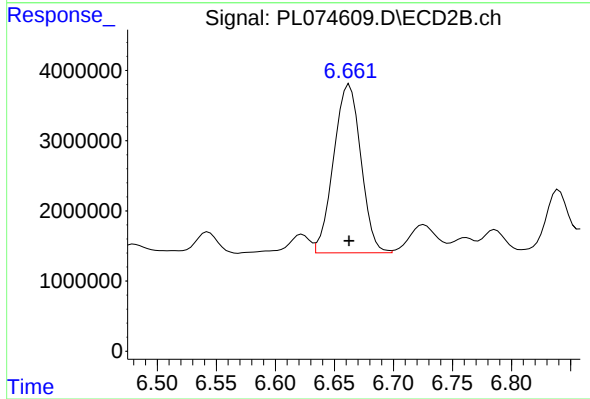


#24 Chlordane-2

R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 38597235
Conc: 731.91 ng/ml

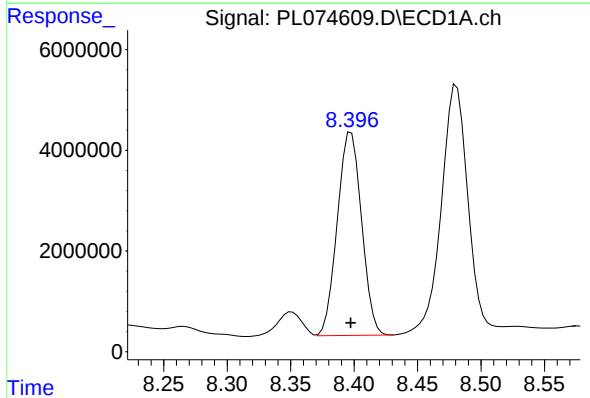


#25 Chlordane-3

R.T.: 8.398 min
Delta R.T.: 0.000 min
Response: 53688372
Conc: 775.68 ng/ml

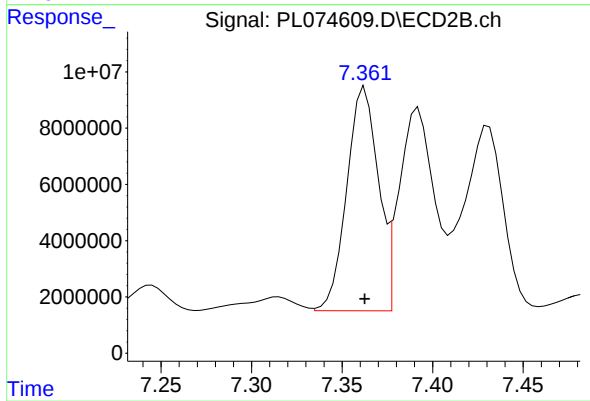

#25 Chlordane-3


R.T.: 7.363 min
Delta R.T.: 0.000 min
Response: 96191856
Conc: 759.47 ng/ml

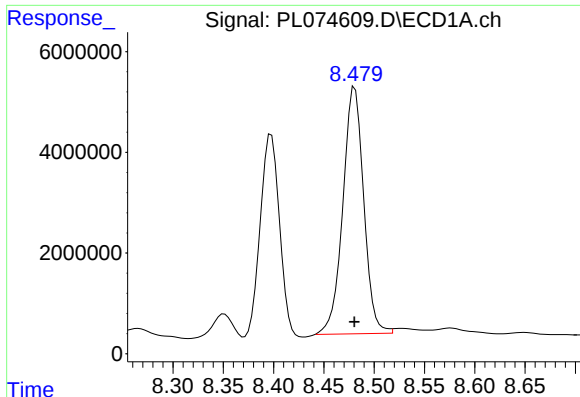

#26 Chlordane-4


R.T.: 8.481 min
Delta R.T.: 0.000 min
Response: 70596334
Conc: 738.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

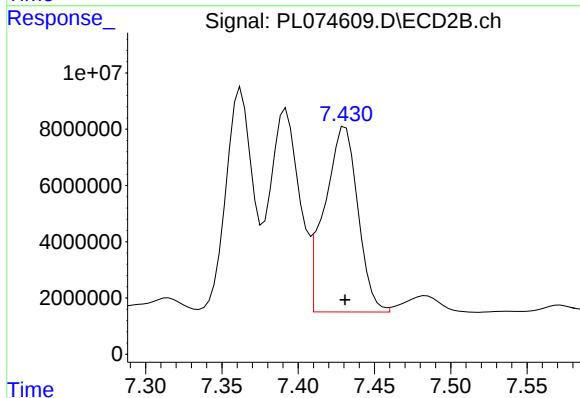


#26 Chlordane-4

R.T.: 7.431 min
Delta R.T.: 0.000 min
Response: 100093904
Conc: 742.82 ng/ml

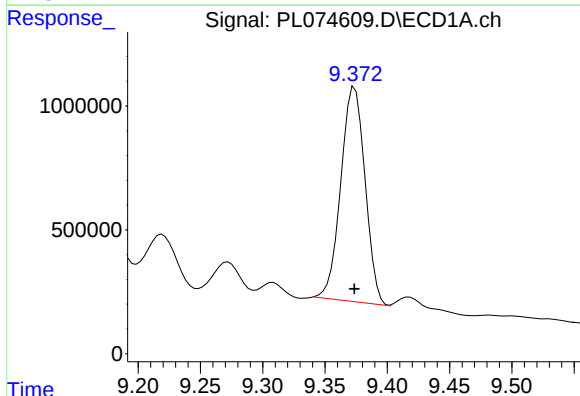


#27 Chlordane-5

R.T.: 9.374 min
Delta R.T.: 0.000 min
Response: 11780588
Conc: 771.03 ng/ml

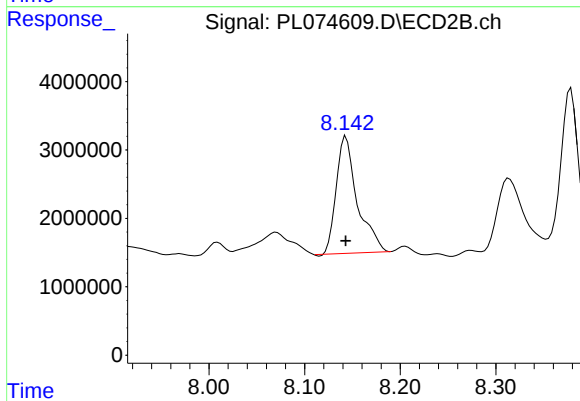

#27 Chlordane-5


R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 26301069
Conc: 734.64 ng/ml

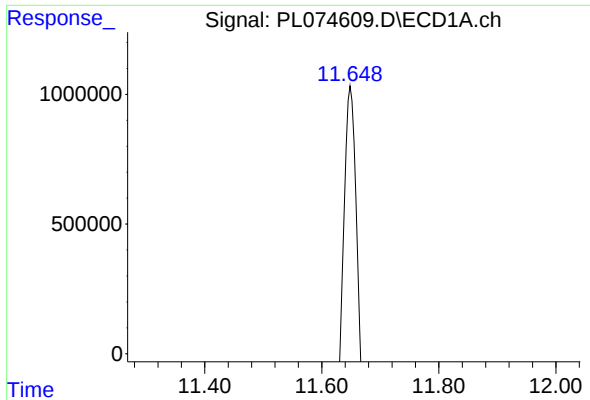

#28 Decachlorobiphenyl

R.T.: 11.650 min
Delta R.T.: 0.000 min
Response: 33282934
Conc: 72.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

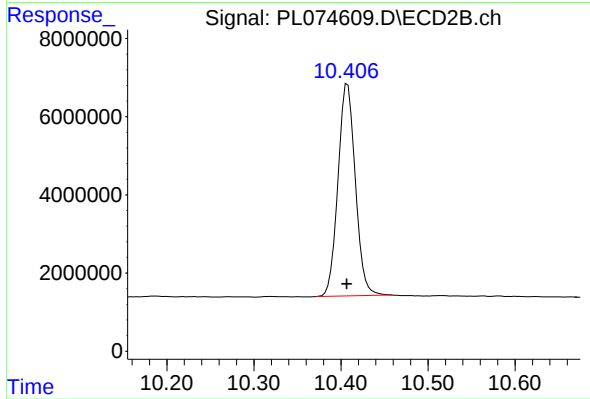

#28 Decachlorobiphenyl

R.T.: 10.408 min
Delta R.T.: 0.000 min
Response: 75271890
Conc: 72.78 ng/ml