

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
 Data File : PL074610.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2022 12:40
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 15:17:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 15:16:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.653	25825350	80307161	50.000	50.000
28)	SA Decachlor...	11.649	10.407	22842159	51708877	50.000	50.000
Target Compounds							
23)	Chlordane-1	7.042	5.977	9271249	21626102	500.000	500.000
24)	Chlordane-2	7.634	6.662	10678942	26367412	500.000	500.000
25)	Chlordane-3	8.397	7.362	34607451	63328131	500.000	500.000
26)	Chlordane-4	8.481	7.431	47812316	67374564	500.000	500.000
27)	Chlordane-5	9.374	8.143	7639468	17900707	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
Data File : PL074610.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2022 12:40
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 15:17:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 15:16:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

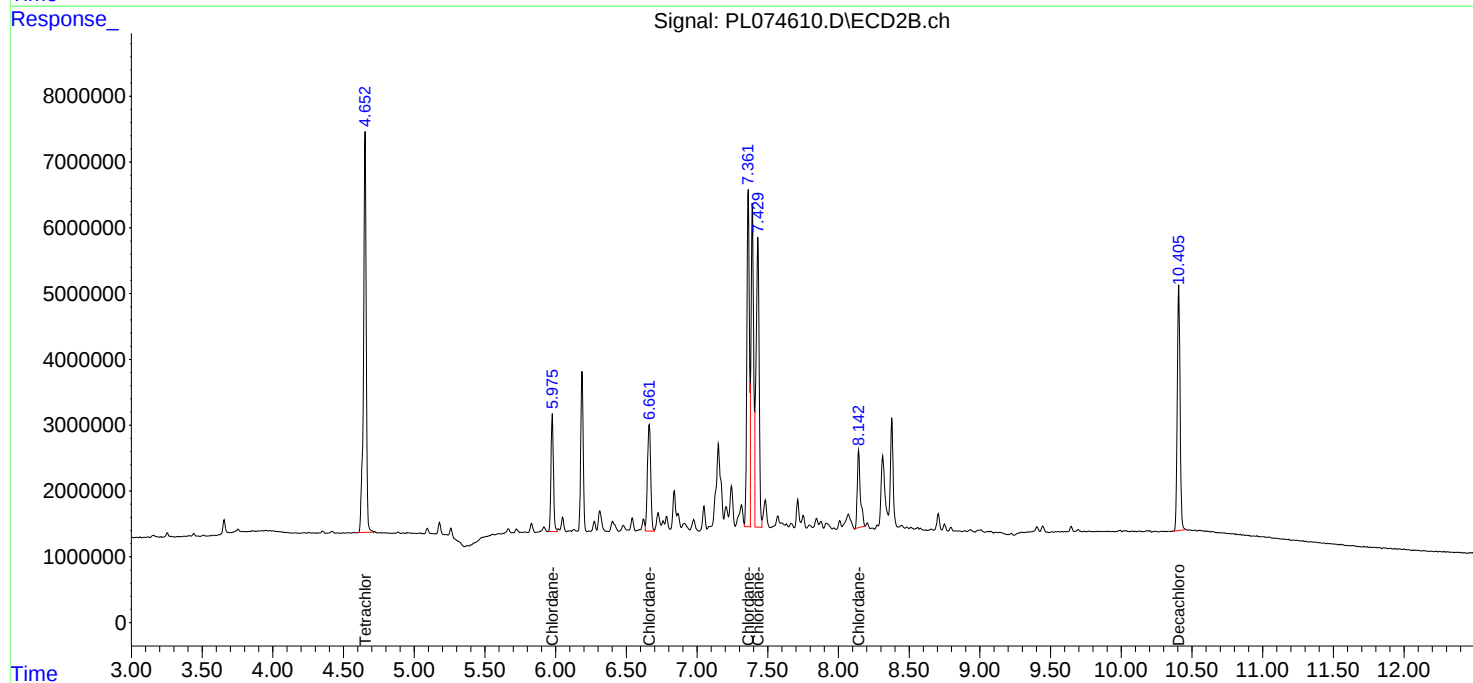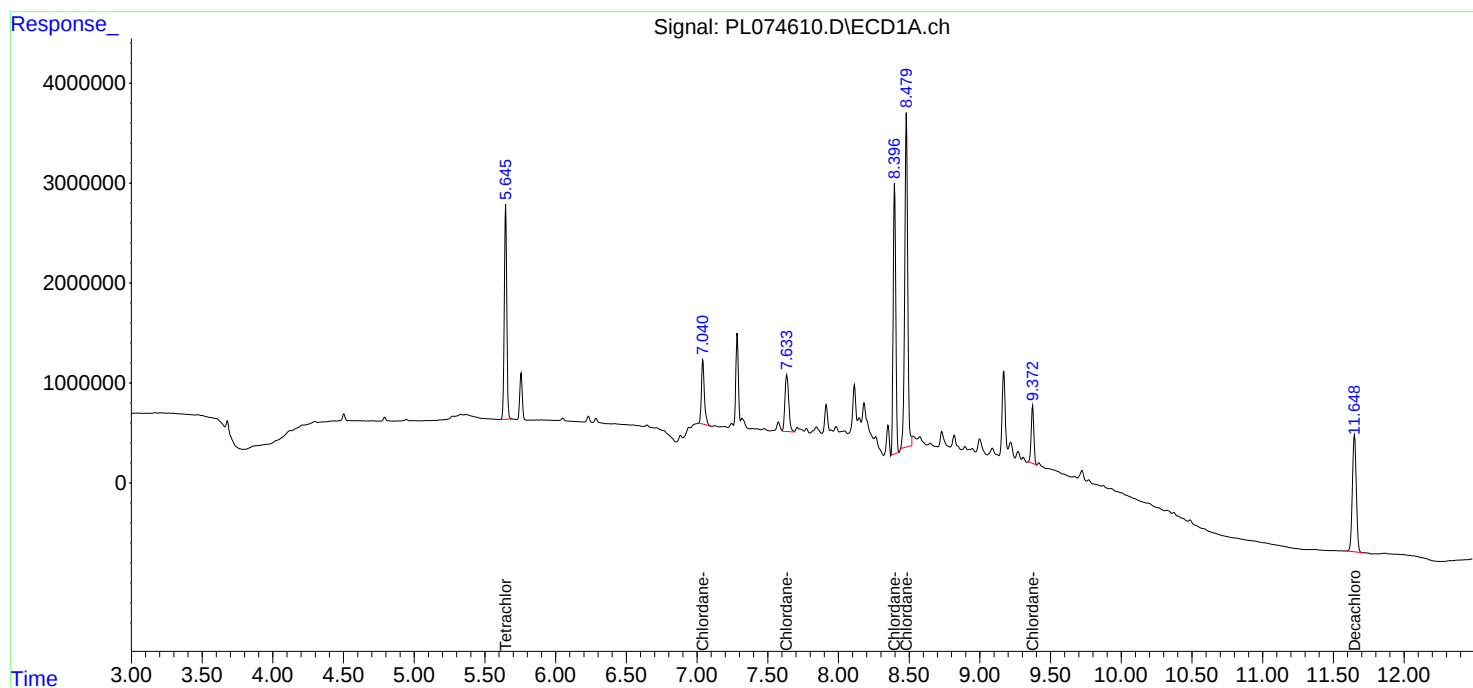


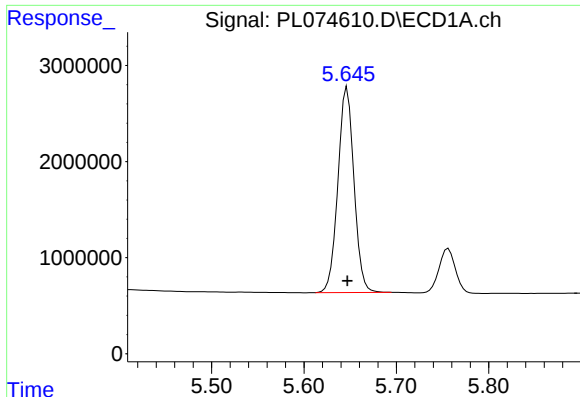

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 25825350
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

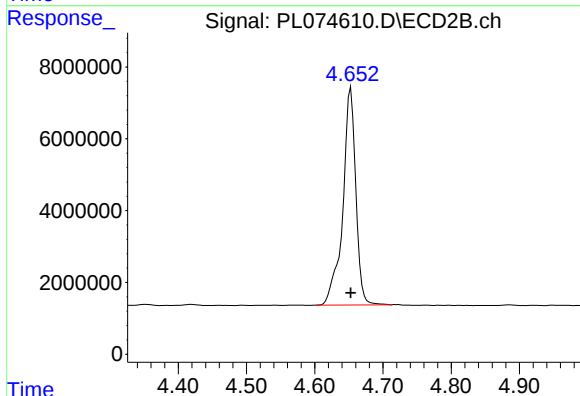


#1 Tetrachloro-m-xylene

R.T.: 4.653 min
Delta R.T.: 0.000 min
Response: 80307161
Conc: 50.00 ng/ml

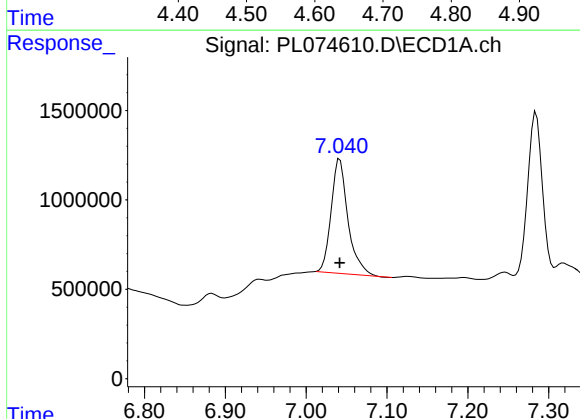


#23 Chlordane-1

R.T.: 7.042 min
Delta R.T.: 0.000 min
Response: 9271249
Conc: 500.00 ng/ml

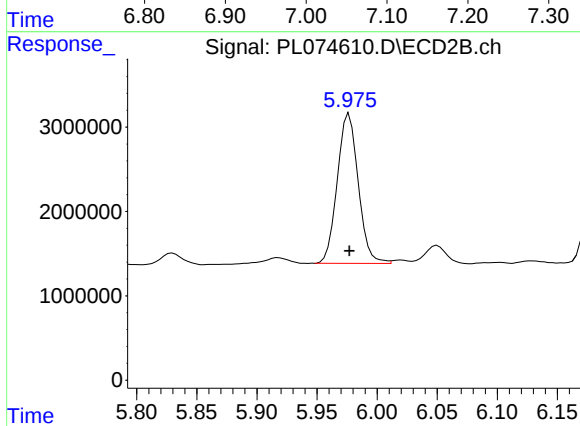

#23 Chlordane-1


R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 21626102
Conc: 500.00 ng/ml

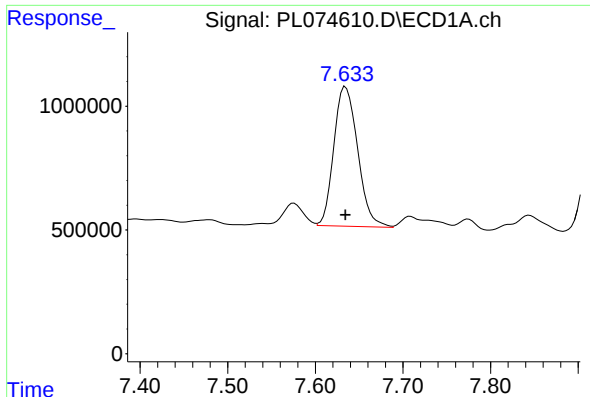

#24 Chlordane-2


R.T.: 7.634 min
Delta R.T.: 0.000 min
Response: 10678942
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

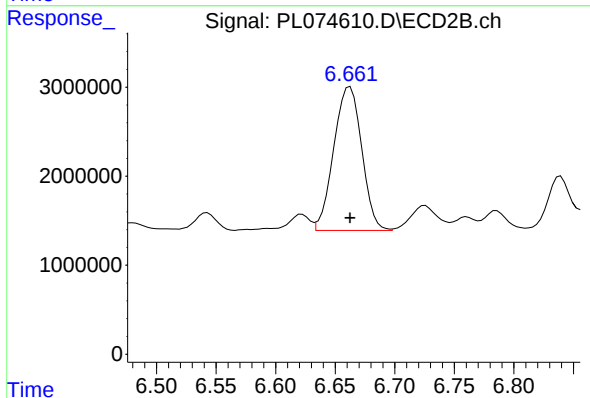


#24 Chlordane-2

R.T.: 6.662 min
Delta R.T.: 0.000 min
Response: 26367412
Conc: 500.00 ng/ml

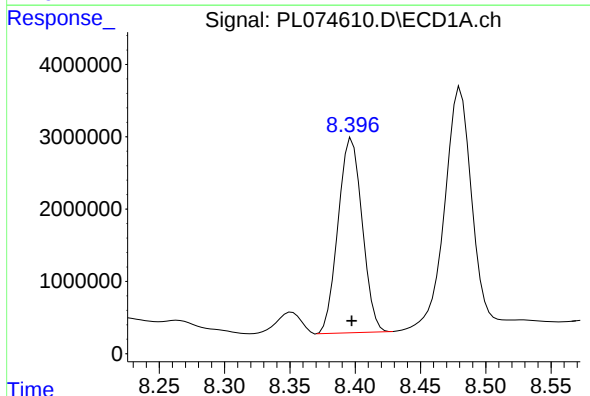


#25 Chlordane-3

R.T.: 8.397 min
Delta R.T.: 0.000 min
Response: 34607451
Conc: 500.00 ng/ml

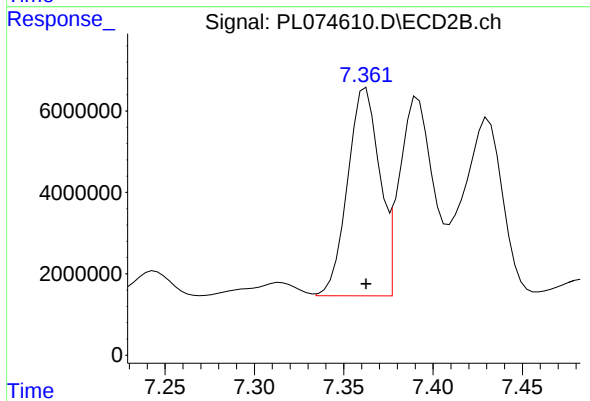

#25 Chlordane-3


R.T.: 7.362 min
Delta R.T.: 0.000 min
Response: 63328131
Conc: 500.00 ng/ml

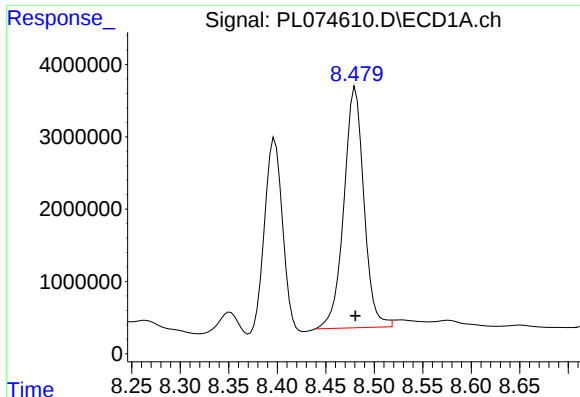

#26 Chlordane-4


R.T.: 8.481 min
Delta R.T.: 0.000 min
Response: 47812316
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

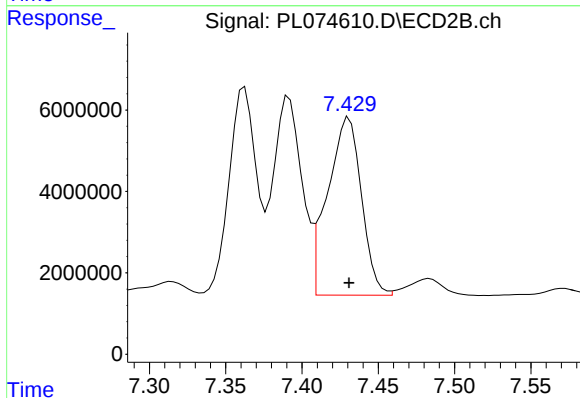


#26 Chlordane-4

R.T.: 7.431 min
Delta R.T.: 0.000 min
Response: 67374564
Conc: 500.00 ng/ml

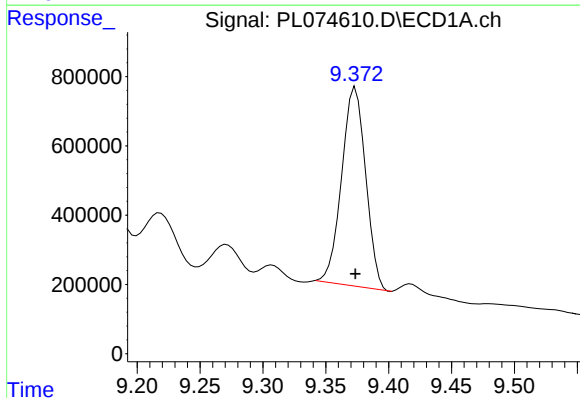


#27 Chlordane-5

R.T.: 9.374 min
Delta R.T.: 0.000 min
Response: 7639468
Conc: 500.00 ng/ml

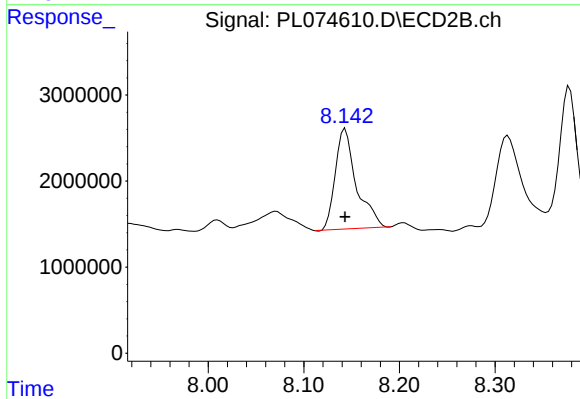

#27 Chlordane-5


R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 17900707
Conc: 500.00 ng/ml

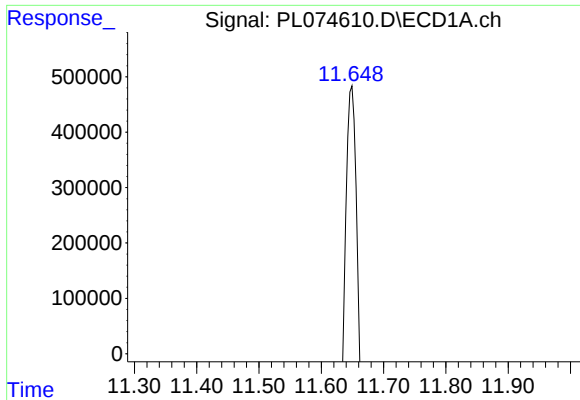

#28 Decachlorobiphenyl

R.T.: 11.649 min
Delta R.T.: 0.000 min
Response: 22842159
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

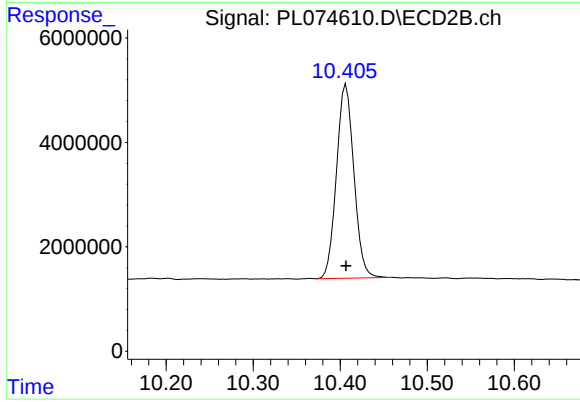

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: 0.000 min
Response: 51708877
Conc: 50.00 ng/ml