

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
 Data File : PL074611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2022 12:57
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 15:17:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 15:16:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.653	12533738	39106377	24.266	24.348
28)	SA Decachlor...	11.649	10.407	11505277	26581958	25.184	25.703
Target Compounds							
23)	Chlordane-1	7.041	5.977	4768638	11080150	257.173	256.175
24)	Chlordane-2	7.634	6.663	5522113	13786344	258.551	261.428
25)	Chlordane-3	8.397	7.362	16202747	31261700	234.093	246.823
26)	Chlordane-4	8.481	7.431	24428396	33370458	255.461	247.649
27)	Chlordane-5	9.374	8.143	3716822	9318892	243.264	260.294



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
Data File : PL074611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2022 12:57
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 15:17:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 15:16:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

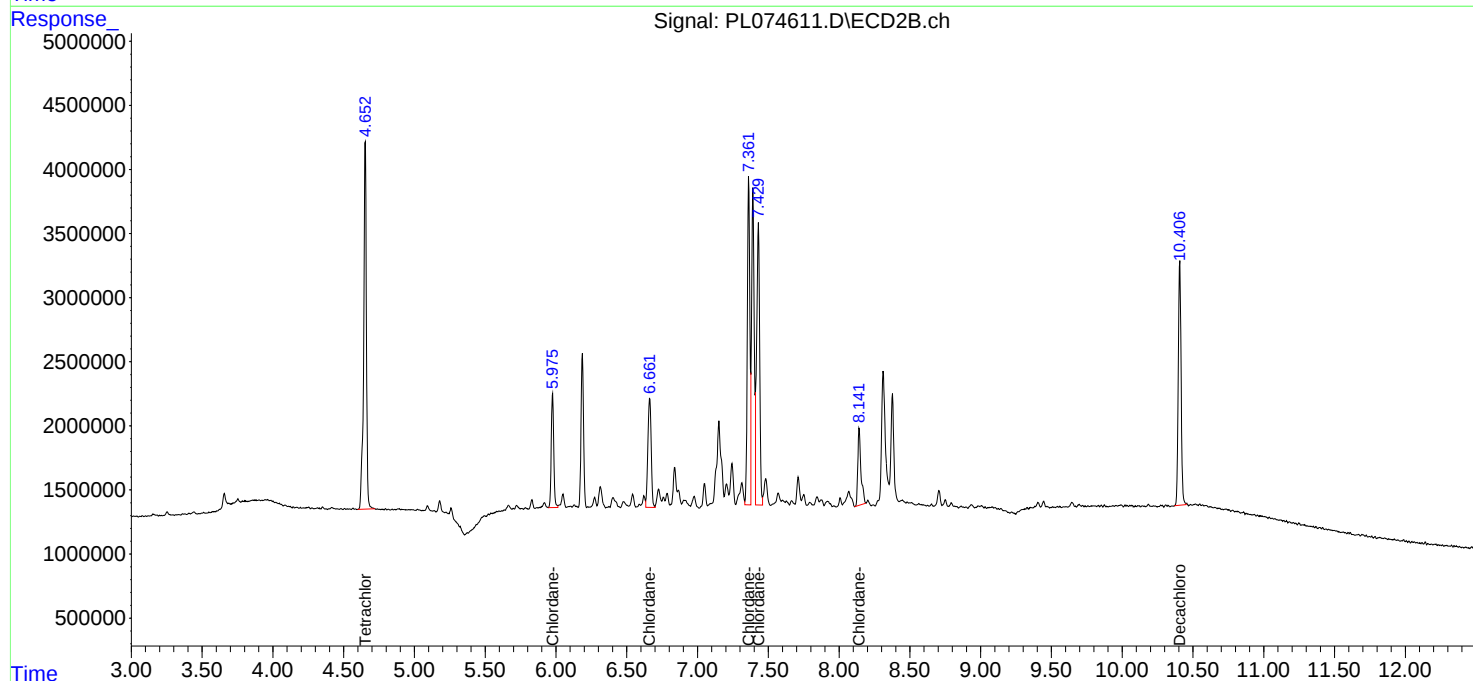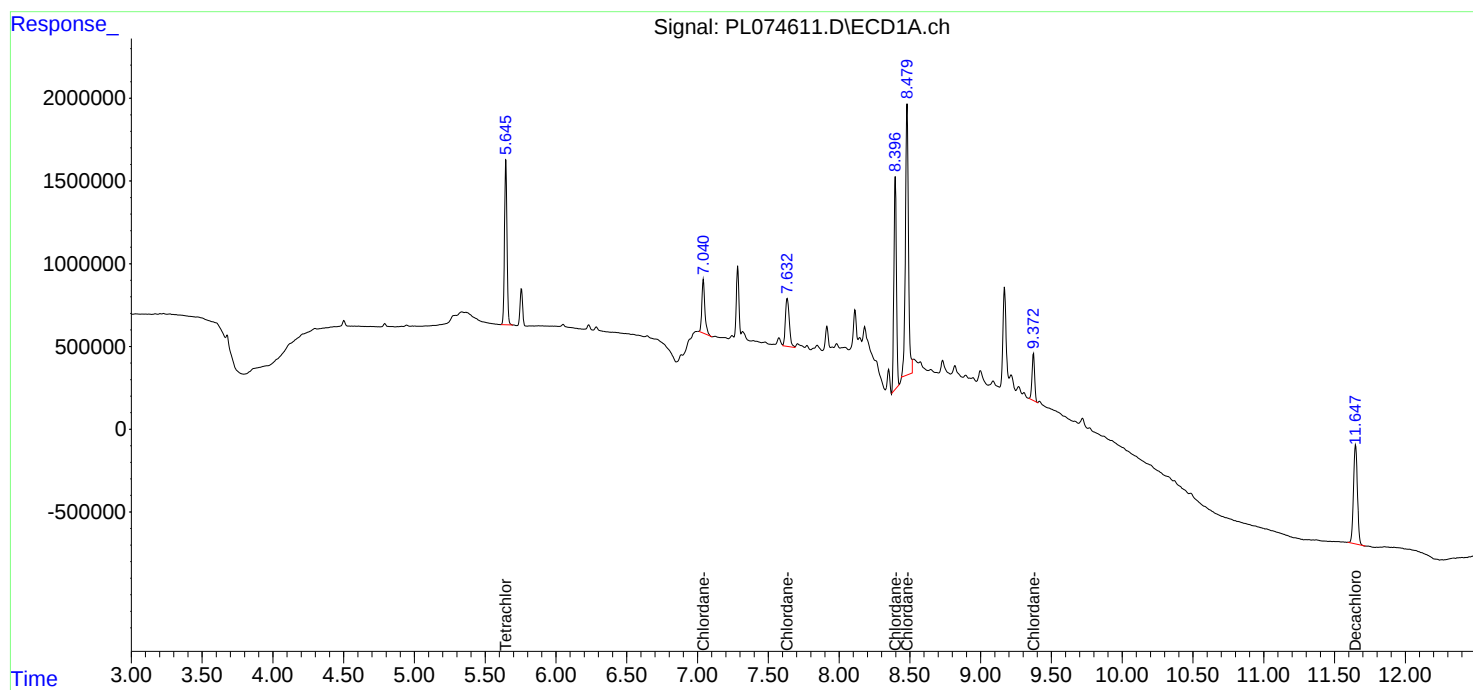


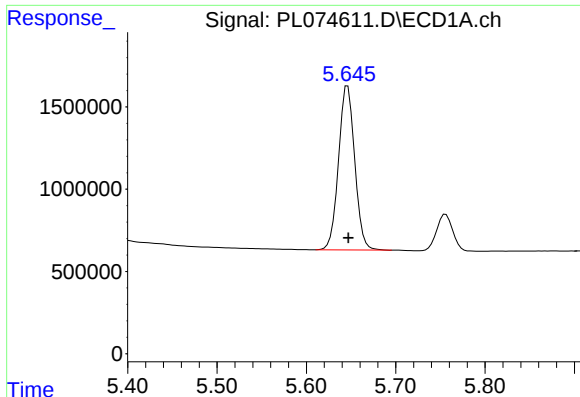

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 12533738
Conc: 24.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

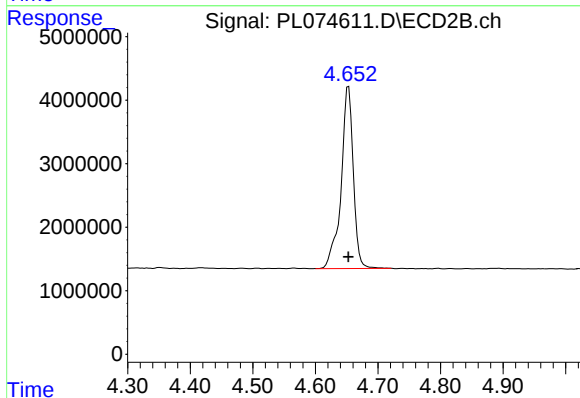


#1 Tetrachloro-m-xylene

R.T.: 4.653 min
Delta R.T.: 0.000 min
Response: 39106377
Conc: 24.35 ng/ml

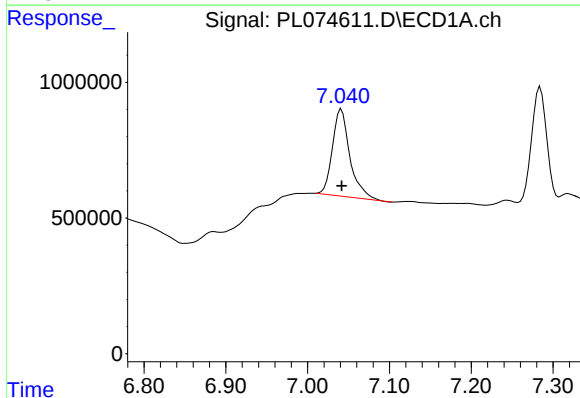


#23 Chlordane-1

R.T.: 7.041 min
Delta R.T.: 0.000 min
Response: 4768638
Conc: 257.17 ng/ml

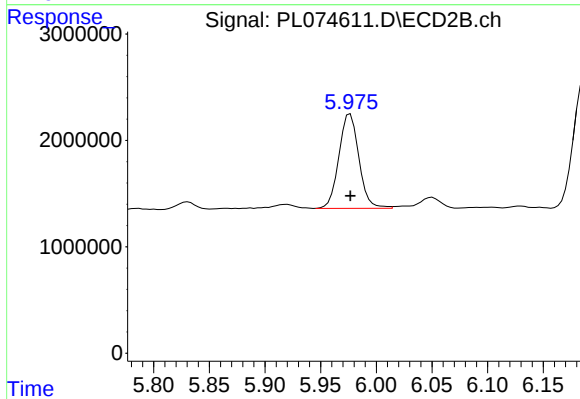

#23 Chlordane-1


R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 11080150
Conc: 256.18 ng/ml

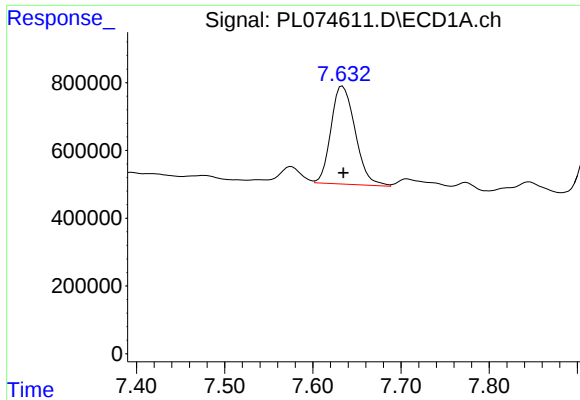

#24 Chlordane-2


R.T.: 7.634 min
Delta R.T.: 0.000 min
Response: 5522113
Conc: 258.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

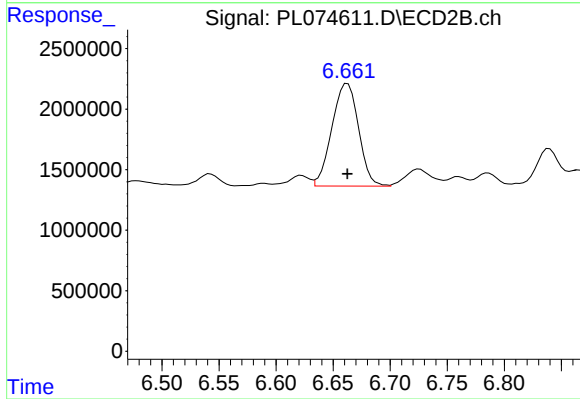


#24 Chlordane-2

R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 13786344
Conc: 261.43 ng/ml

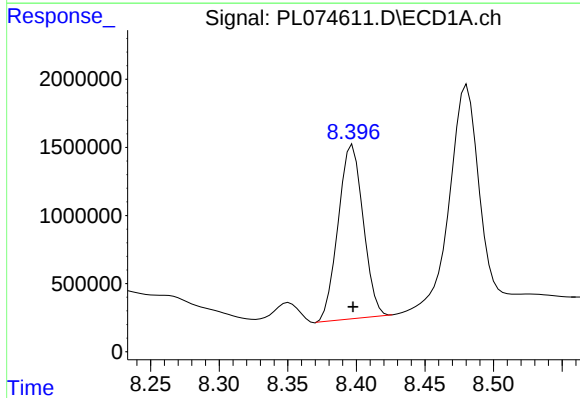


#25 Chlordane-3

R.T.: 8.397 min
Delta R.T.: 0.000 min
Response: 16202747
Conc: 234.09 ng/ml

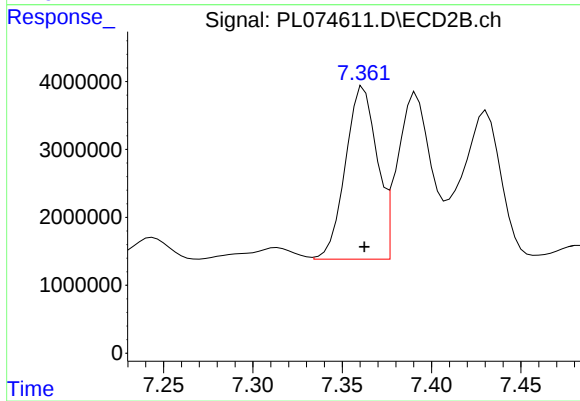

#25 Chlordane-3


R.T.: 7.362 min
Delta R.T.: 0.000 min
Response: 31261700
Conc: 246.82 ng/ml

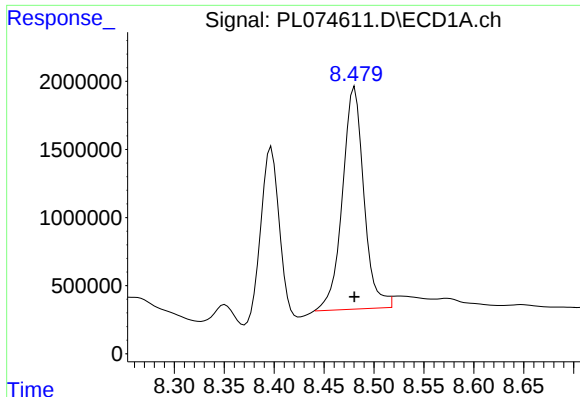

#26 Chlordane-4


R.T.: 8.481 min
Delta R.T.: 0.000 min
Response: 24428396
Conc: 255.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

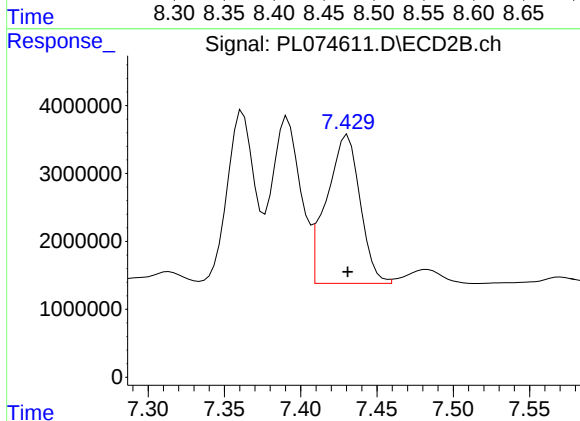


#26 Chlordane-4

R.T.: 7.431 min
Delta R.T.: 0.000 min
Response: 33370458
Conc: 247.65 ng/ml

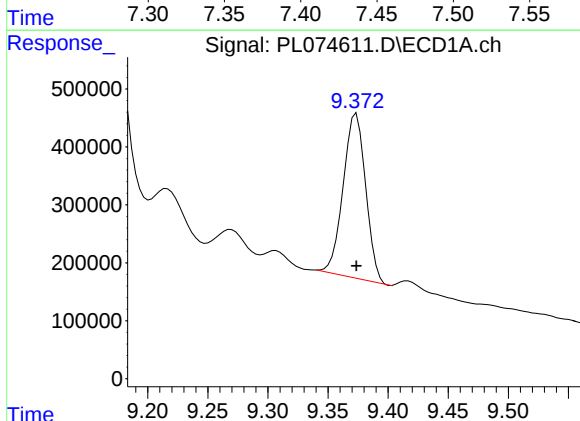


#27 Chlordane-5

R.T.: 9.374 min
Delta R.T.: 0.000 min
Response: 3716822
Conc: 243.26 ng/ml

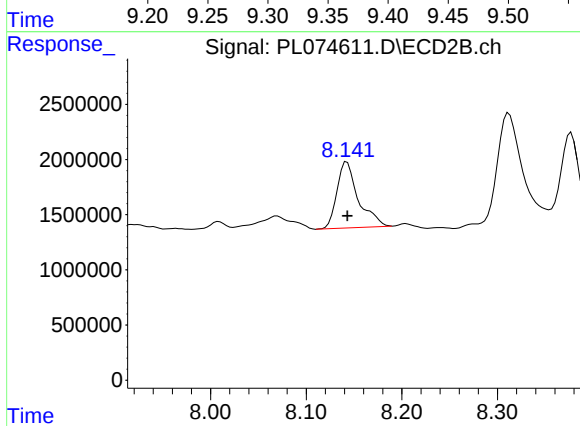

#27 Chlordane-5


R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 9318892
Conc: 260.29 ng/ml

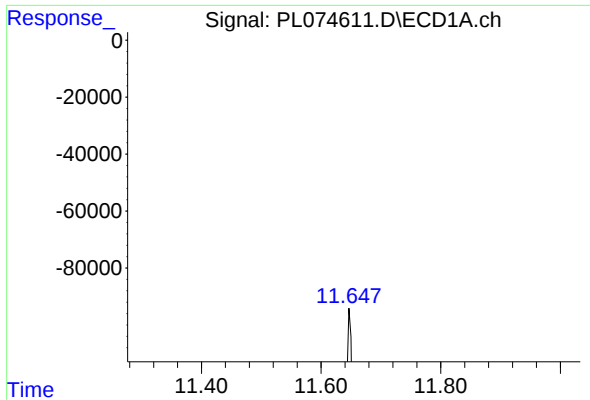

#28 Decachlorobiphenyl

R.T.: 11.649 min
Delta R.T.: 0.000 min
Response: 11505277
Conc: 25.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

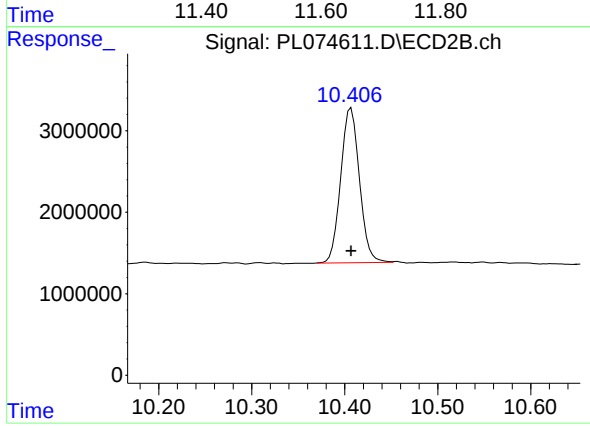

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: 0.000 min
Response: 26581958
Conc: 25.70 ng/ml