

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
 Data File : PL074619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2022 15:08
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL051122CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 16:17:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 16:15:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.653	28340229	83443543	54.222	51.324
28)	SA Decachlor...	11.649	10.407	25923783	56616329	55.984	53.039
Target Compounds							
23)	Chlordane-1	7.041	5.976	10255643	22881622	520.881	504.886
24)	Chlordane-2	7.635	6.662	11885030	27623910	536.230	497.501
25)	Chlordane-3	8.397	7.362	38989377	68031227	569.527	524.164
26)	Chlordane-4	8.481	7.430	52732916	71999926	547.362	525.212
27)	Chlordane-5	9.374	8.142	8610597	19293222	553.818	521.808



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051122\
Data File : PL074619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2022 15:08
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL051122CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 16:17:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Wed May 11 16:15:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

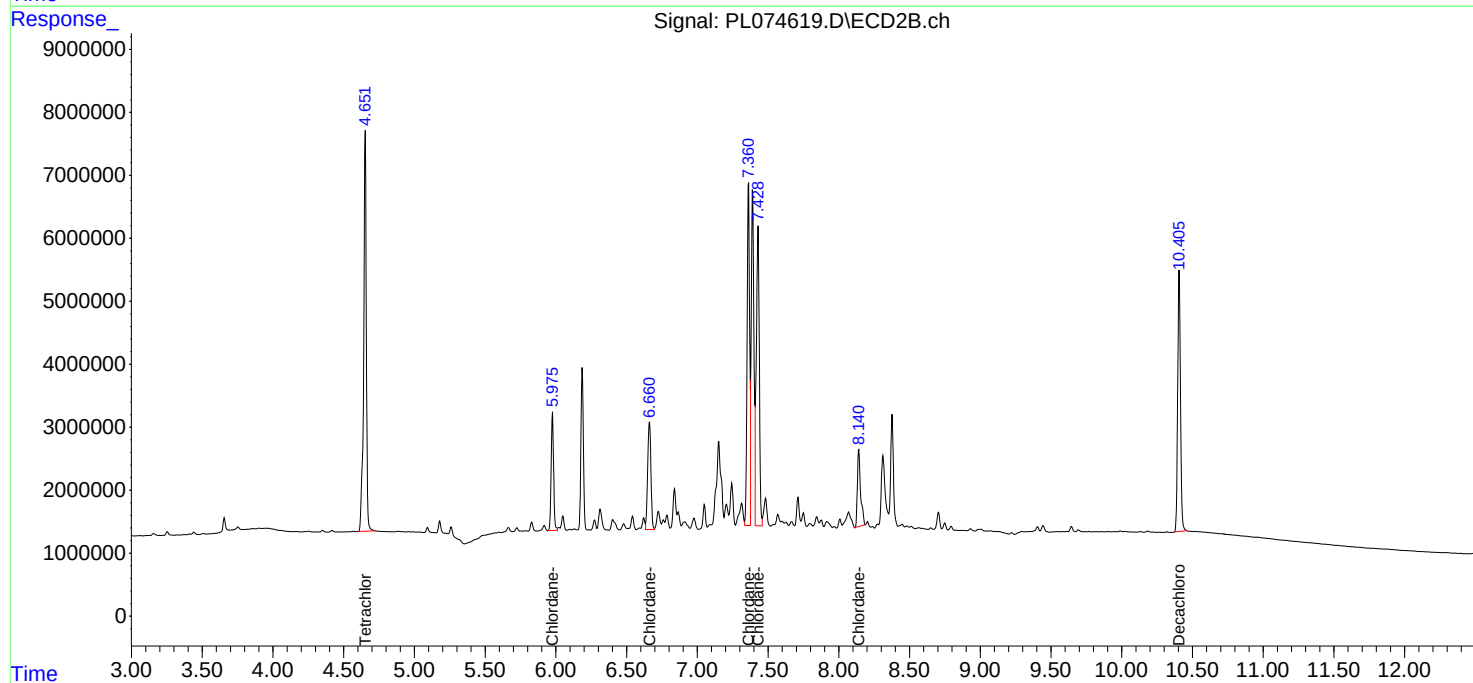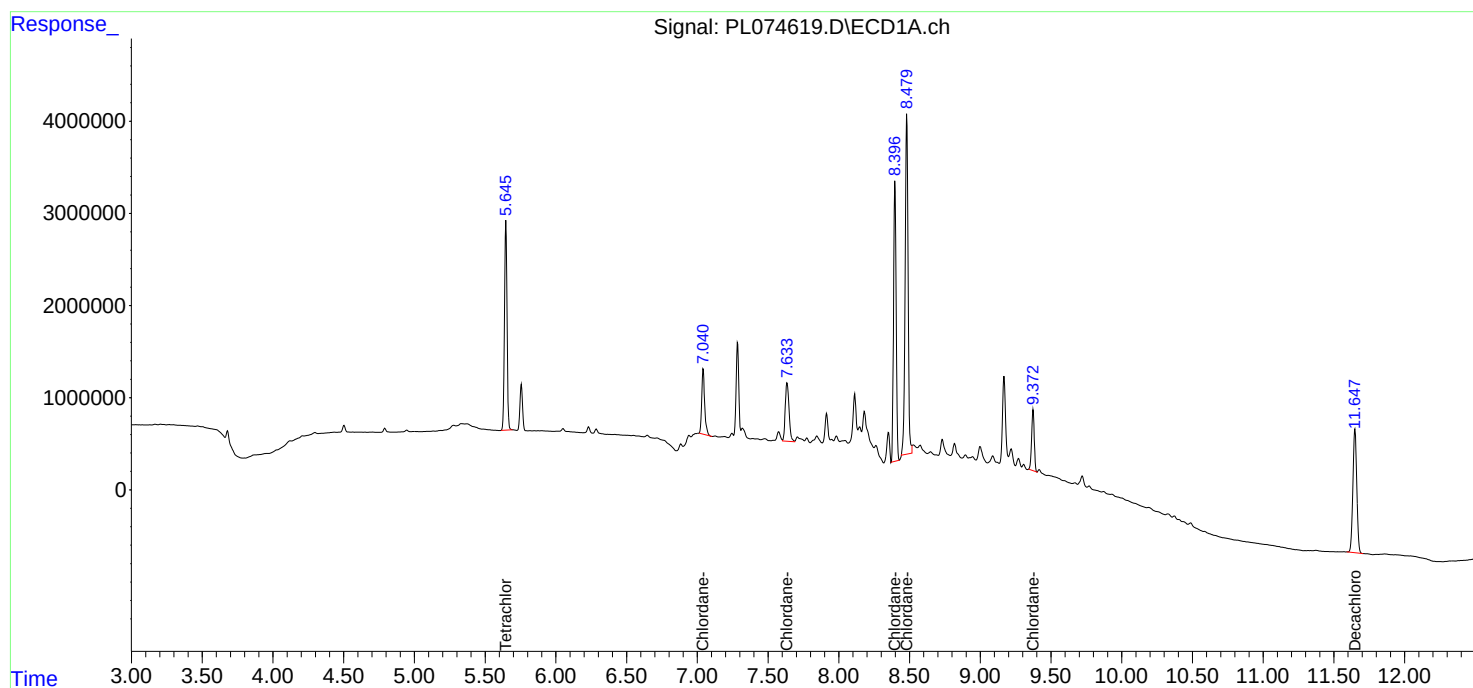


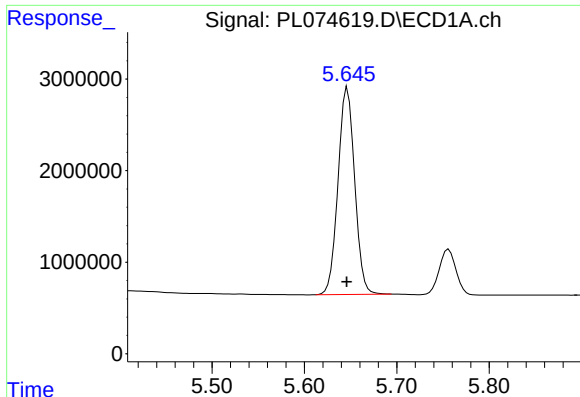

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 28340229
Conc: 54.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL051122CHLOR

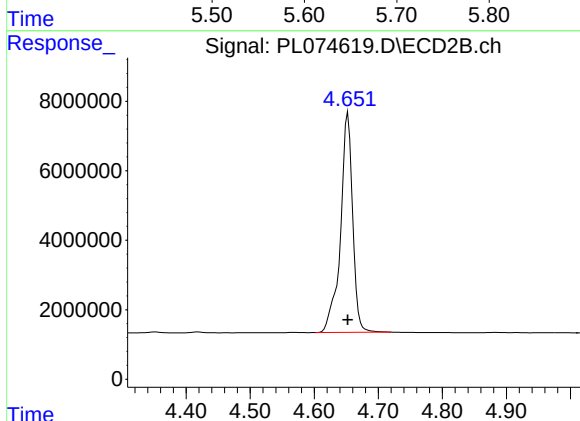


#1 Tetrachloro-m-xylene

R.T.: 4.653 min
Delta R.T.: 0.000 min
Response: 83443543
Conc: 51.32 ng/ml

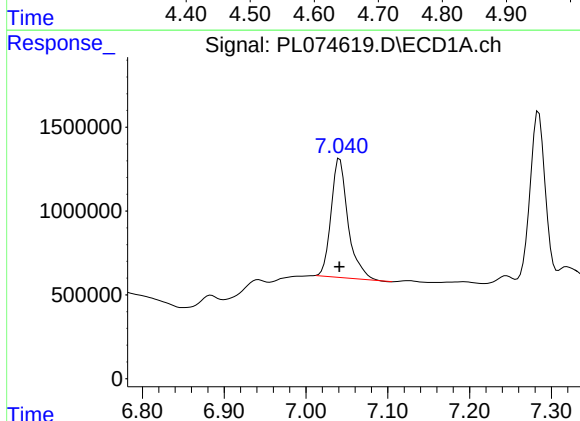


#23 Chlordane-1

R.T.: 7.041 min
Delta R.T.: 0.000 min
Response: 10255643
Conc: 520.88 ng/ml

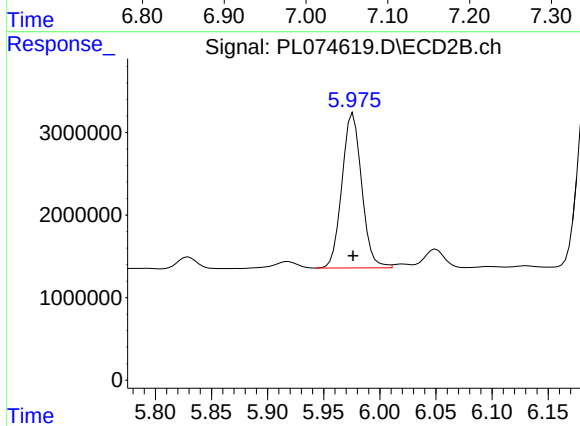

#23 Chlordane-1


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 22881622
Conc: 504.89 ng/ml

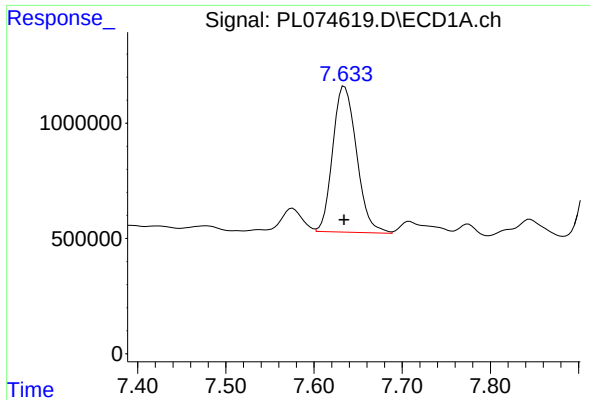

#24 Chlordane-2


R.T.: 7.635 min
Delta R.T.: 0.000 min
Response: 11885030
Conc: 536.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL051122CHLOR

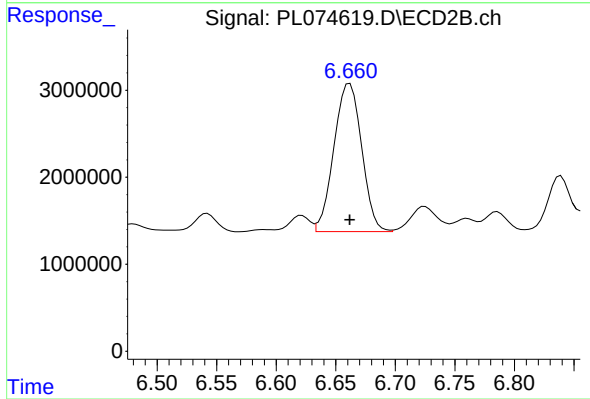


#24 Chlordane-2

R.T.: 6.662 min
Delta R.T.: 0.000 min
Response: 27623910
Conc: 497.50 ng/ml

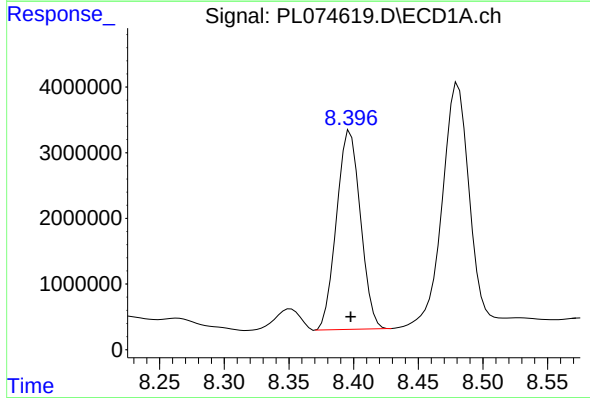


#25 Chlordane-3

R.T.: 8.397 min
Delta R.T.: 0.000 min
Response: 38989377
Conc: 569.53 ng/ml

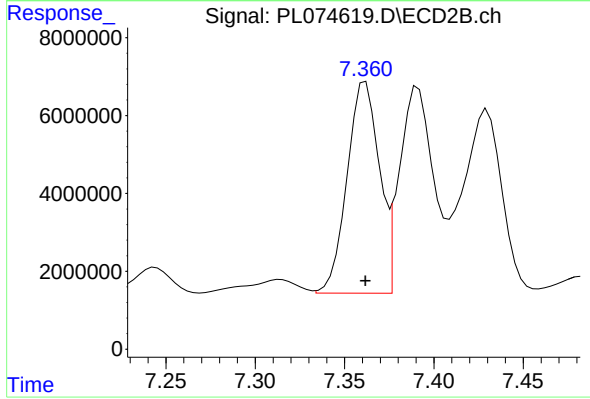

#25 Chlordane-3


R.T.: 7.362 min
Delta R.T.: 0.000 min
Response: 68031227
Conc: 524.16 ng/ml

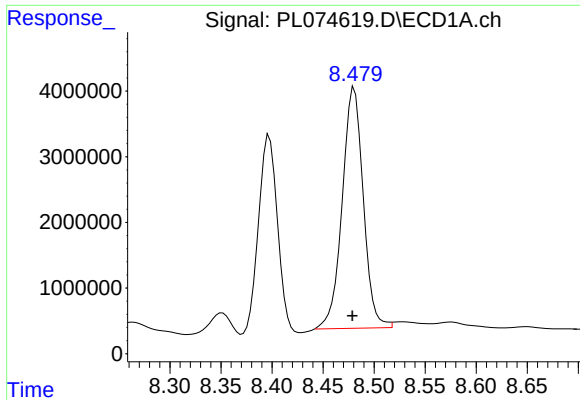

#26 Chlordane-4


R.T.: 8.481 min
Delta R.T.: 0.002 min
Response: 52732916
Conc: 547.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL051122CHLOR

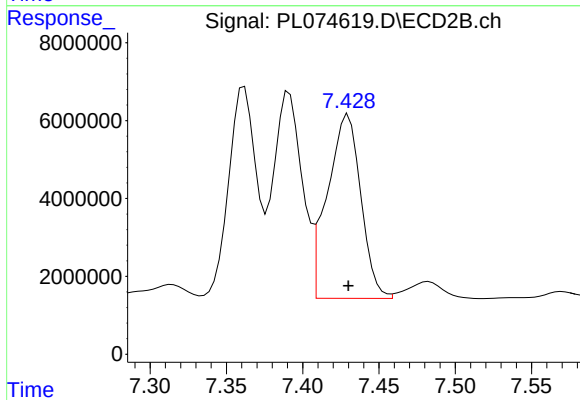


#26 Chlordane-4

R.T.: 7.430 min
Delta R.T.: 0.000 min
Response: 71999926
Conc: 525.21 ng/ml

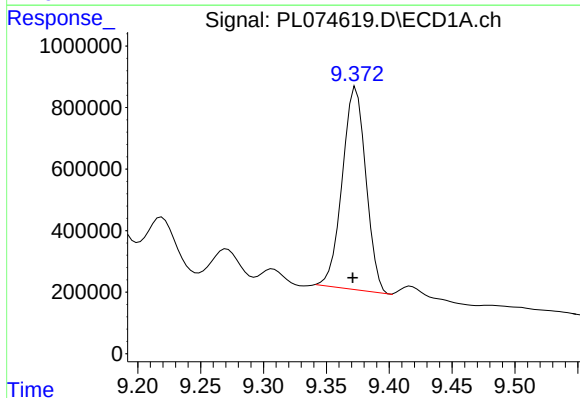


#27 Chlordane-5

R.T.: 9.374 min
Delta R.T.: 0.003 min
Response: 8610597
Conc: 553.82 ng/ml

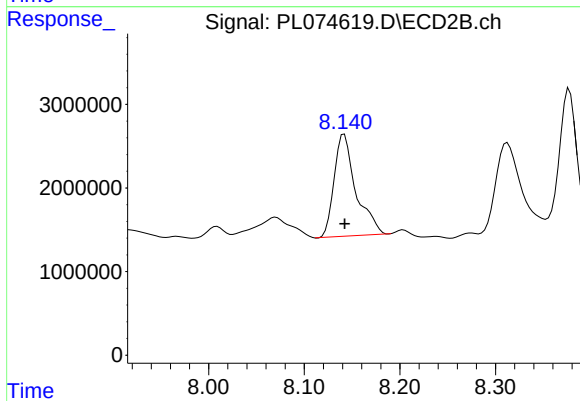

#27 Chlordane-5


R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 19293222
Conc: 521.81 ng/ml

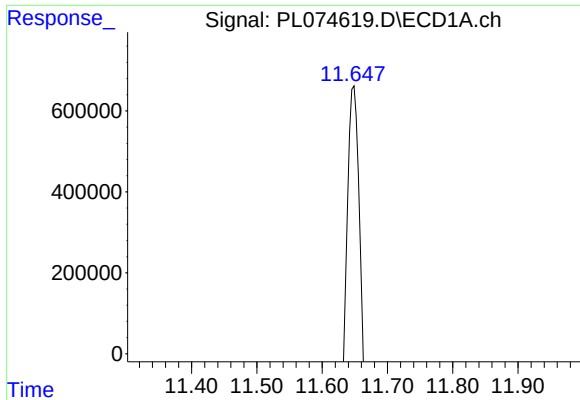

#28 Decachlorobiphenyl

R.T.: 11.649 min
Delta R.T.: 0.000 min
Response: 25923783
Conc: 55.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL051122CHLOR

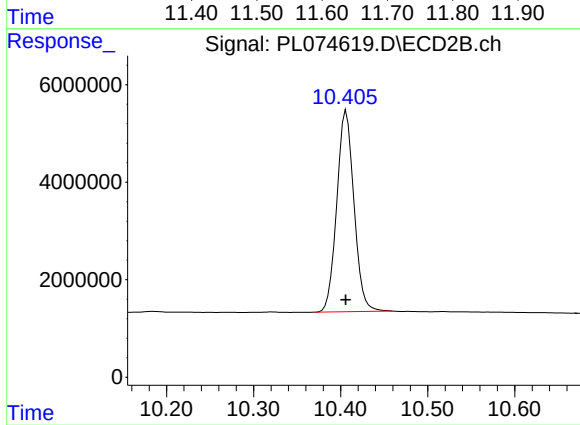

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: 0.000 min
Response: 56616329
Conc: 53.04 ng/ml