

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051123\
 Data File : PL082660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2023 17:27
 Operator : AR\AJ
 Sample : PB152710BS
 Misc : CH-BS
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB152710BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 21:37:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.640	50758406	56079560	19.002	24.206 #
28)	SA Decachlor...	8.735	7.749	40609036	45865257	21.272	20.094
Target Compounds							
23)	Chlordane-1	4.460	3.624	22880069	19671031	206.981	221.808
24)	Chlordane-2	4.987	4.197	26593802	25047893	223.379	223.357
25)	Chlordane-3	5.692	4.824	91974095	60549899	213.049	213.122
26)	Chlordane-4	5.773	4.884	112.8E6	64402142	216.948	215.820
27)	Chlordane-5	6.614	5.776	18607211	20149108	198.165	204.119



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051123\
Data File : PL082660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2023 17:27
Operator : AR\AJ
Sample : PB152710BS
Misc : CH-BS
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB152710BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 21:37:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

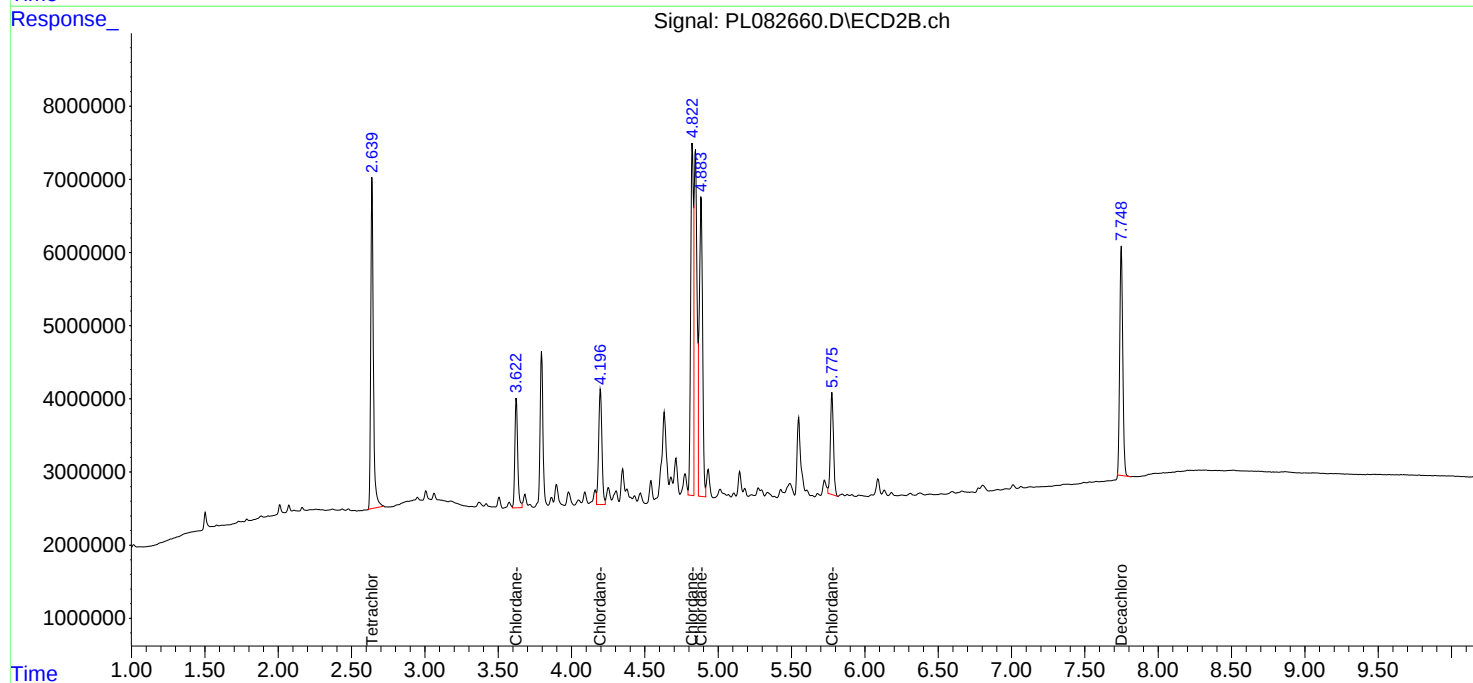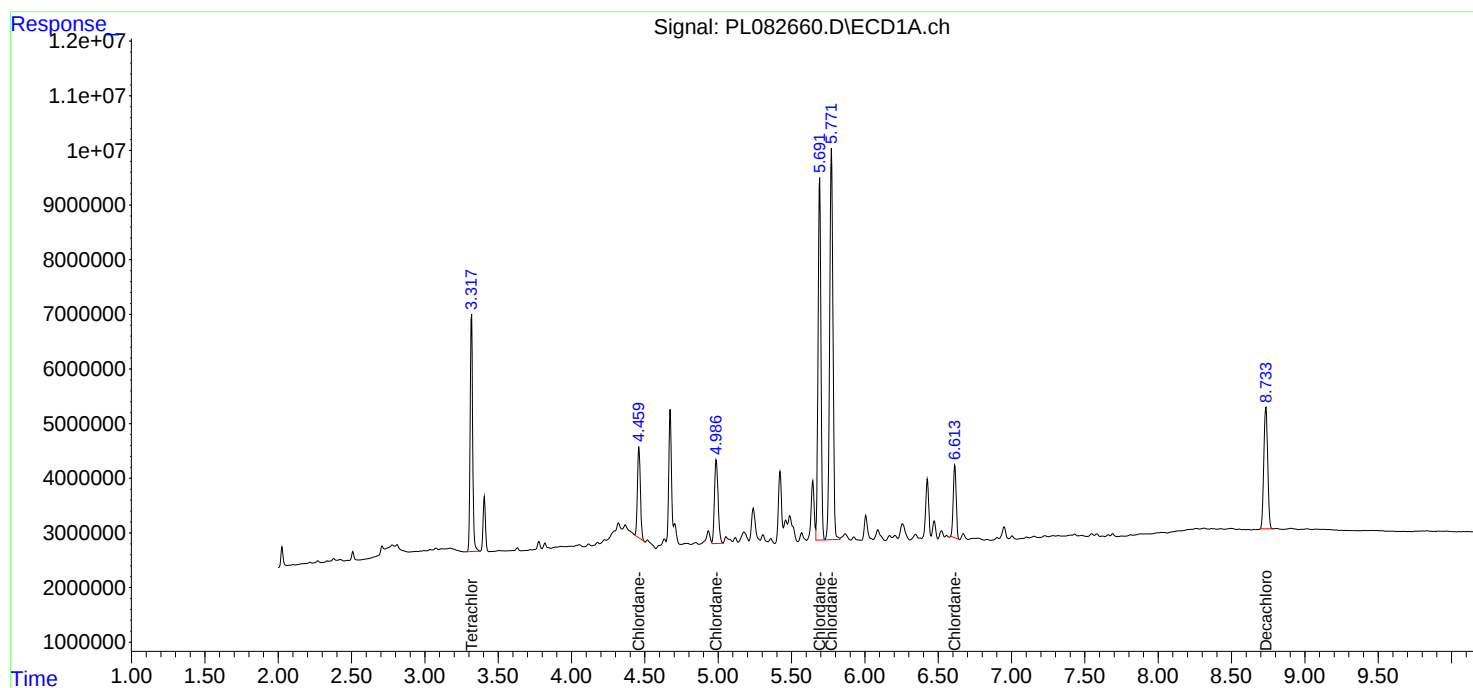


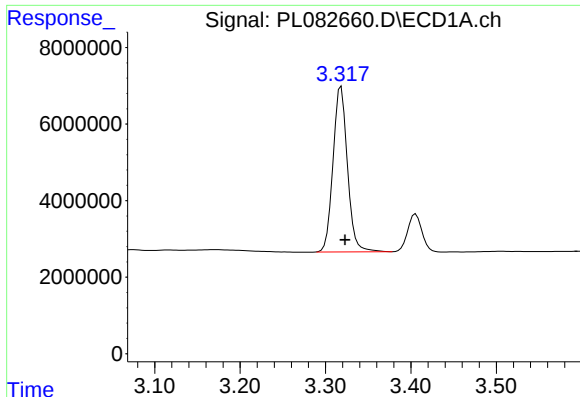

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: -0.005 min
Response: 50758406
Conc: 19.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152710BS

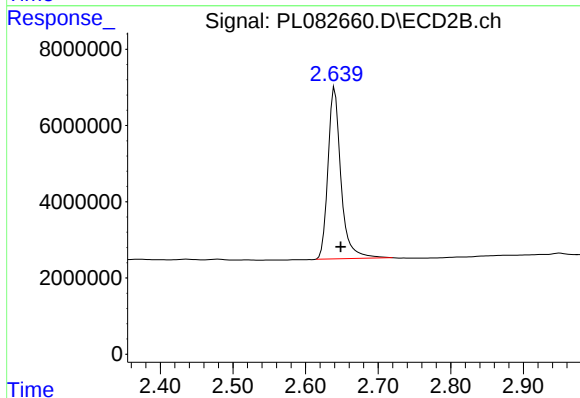


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: -0.008 min
Response: 56079560
Conc: 24.21 ng/ml

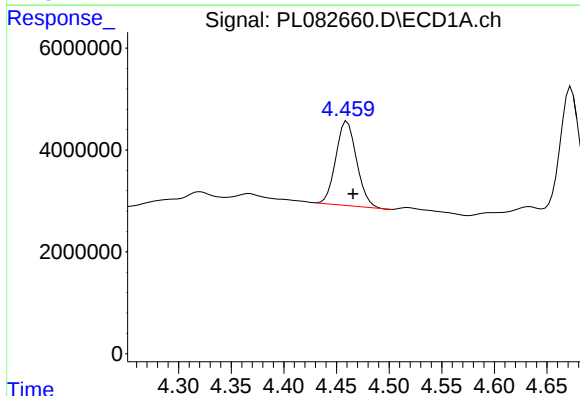


#23 Chlordane-1

R.T.: 4.460 min
Delta R.T.: -0.006 min
Response: 22880069
Conc: 206.98 ng/ml

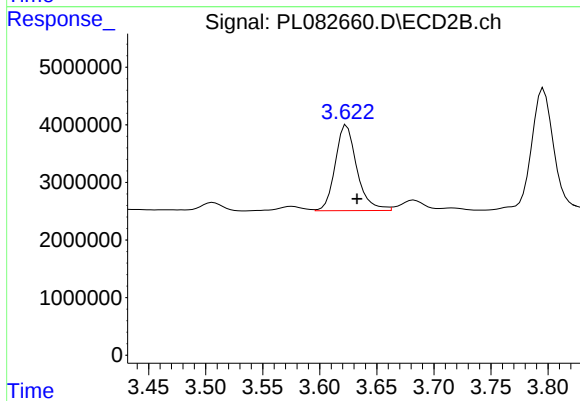

#23 Chlordane-1


R.T.: 3.624 min
Delta R.T.: -0.009 min
Response: 19671031
Conc: 221.81 ng/ml

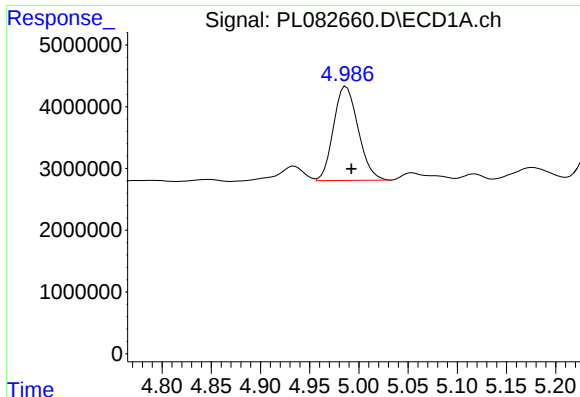

#24 Chlordane-2


R.T.: 4.987 min
Delta R.T.: -0.005 min
Response: 26593802
Conc: 223.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152710BS

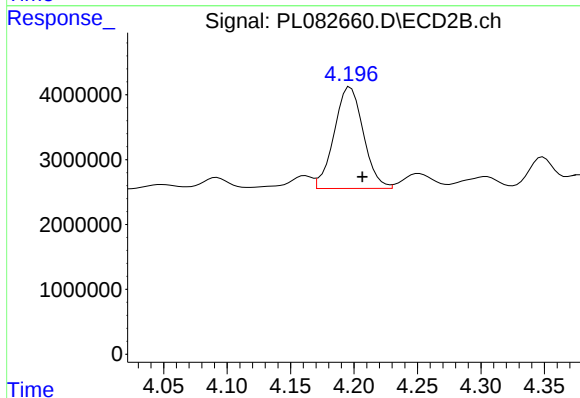


#24 Chlordane-2

R.T.: 4.197 min
Delta R.T.: -0.010 min
Response: 25047893
Conc: 223.36 ng/ml

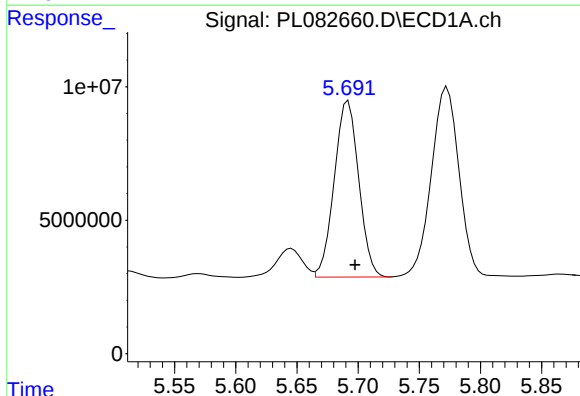


#25 Chlordane-3

R.T.: 5.692 min
Delta R.T.: -0.006 min
Response: 91974095
Conc: 213.05 ng/ml

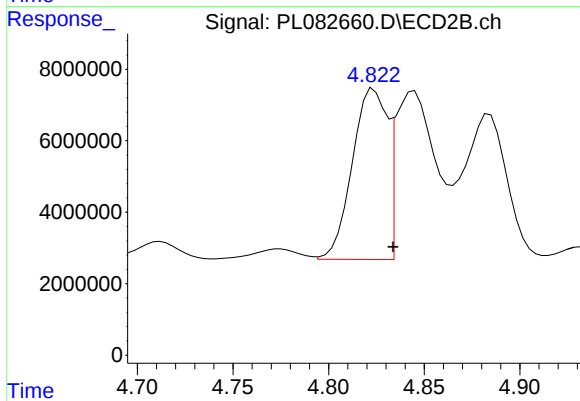

#25 Chlordane-3


R.T.: 4.824 min
Delta R.T.: -0.010 min
Response: 60549899
Conc: 213.12 ng/ml

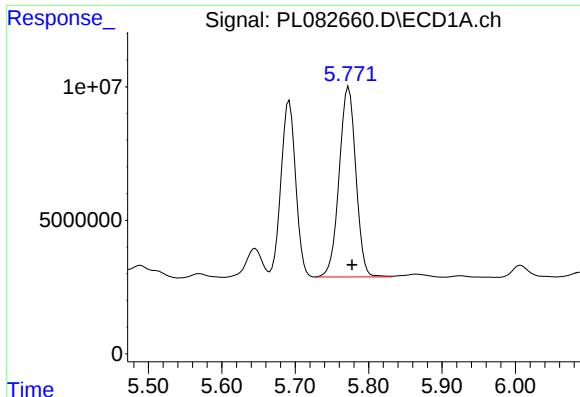

#26 Chlordane-4


R.T.: 5.773 min
Delta R.T.: -0.005 min
Response: 112794519
Conc: 216.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152710BS

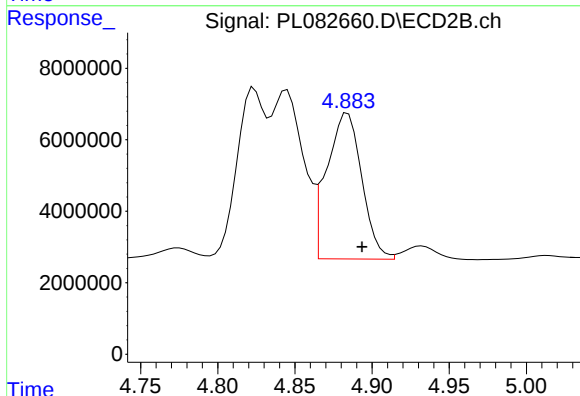


#26 Chlordane-4

R.T.: 4.884 min
Delta R.T.: -0.009 min
Response: 64402142
Conc: 215.82 ng/ml

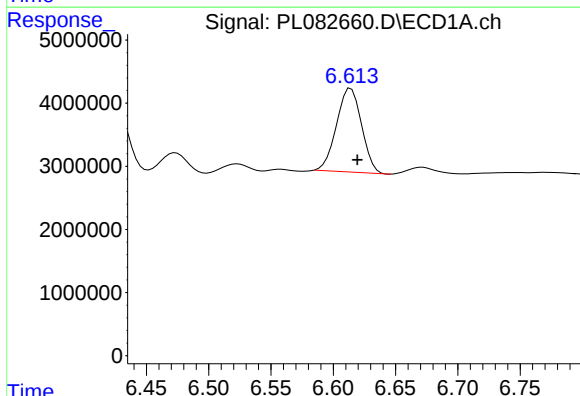


#27 Chlordane-5

R.T.: 6.614 min
Delta R.T.: -0.005 min
Response: 18607211
Conc: 198.16 ng/ml

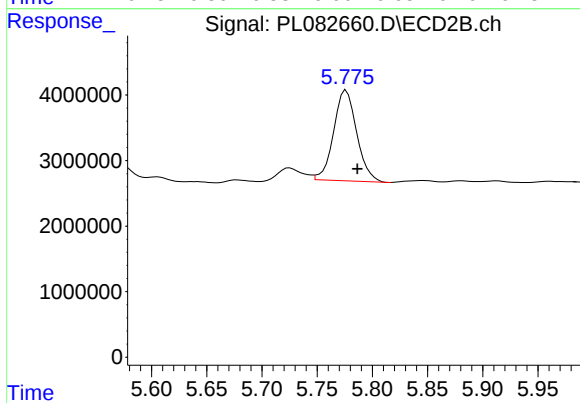

#27 Chlordane-5


R.T.: 5.776 min
Delta R.T.: -0.010 min
Response: 20149108
Conc: 204.12 ng/ml

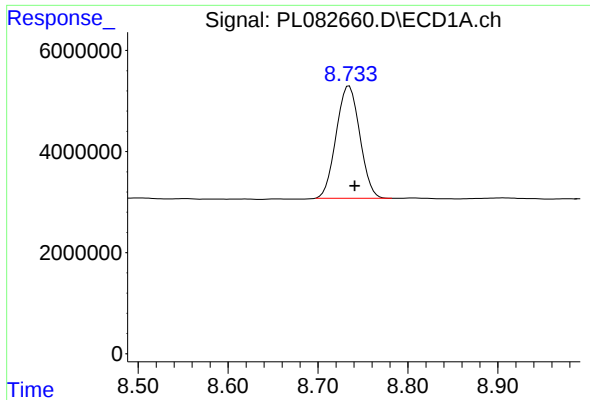

#28 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.006 min
Response: 40609036
Conc: 21.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB152710BS

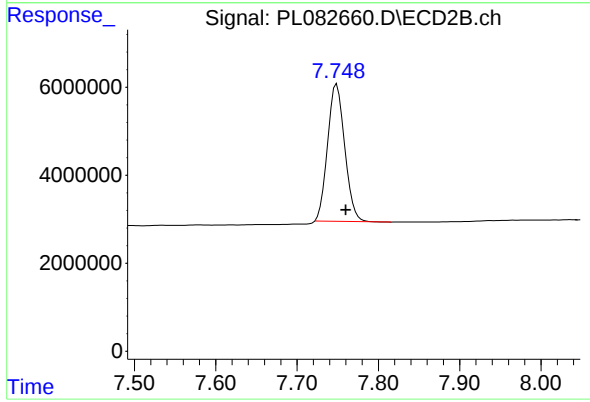

#28 Decachlorobiphenyl

R.T.: 7.749 min
Delta R.T.: -0.011 min
Response: 45865257
Conc: 20.09 ng/ml