

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051123\
 Data File : PL082662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2023 17:54
 Operator : AR\AJ
 Sample : 02643-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FSND-IDW-S-05042023

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/12/2023
 Supervised By : Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 11 21:38:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.318	2.641	48415274	42785768	18.125	18.468
28) SA Decachlor...	8.736	7.747	39337419	44634682	20.605	19.555m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051123\
Data File : PL082662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2023 17:54
Operator : AR\AJ
Sample : 02643-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FSND-IDW-S-05042023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/12/2023
Supervised By : Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 11 21:38:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

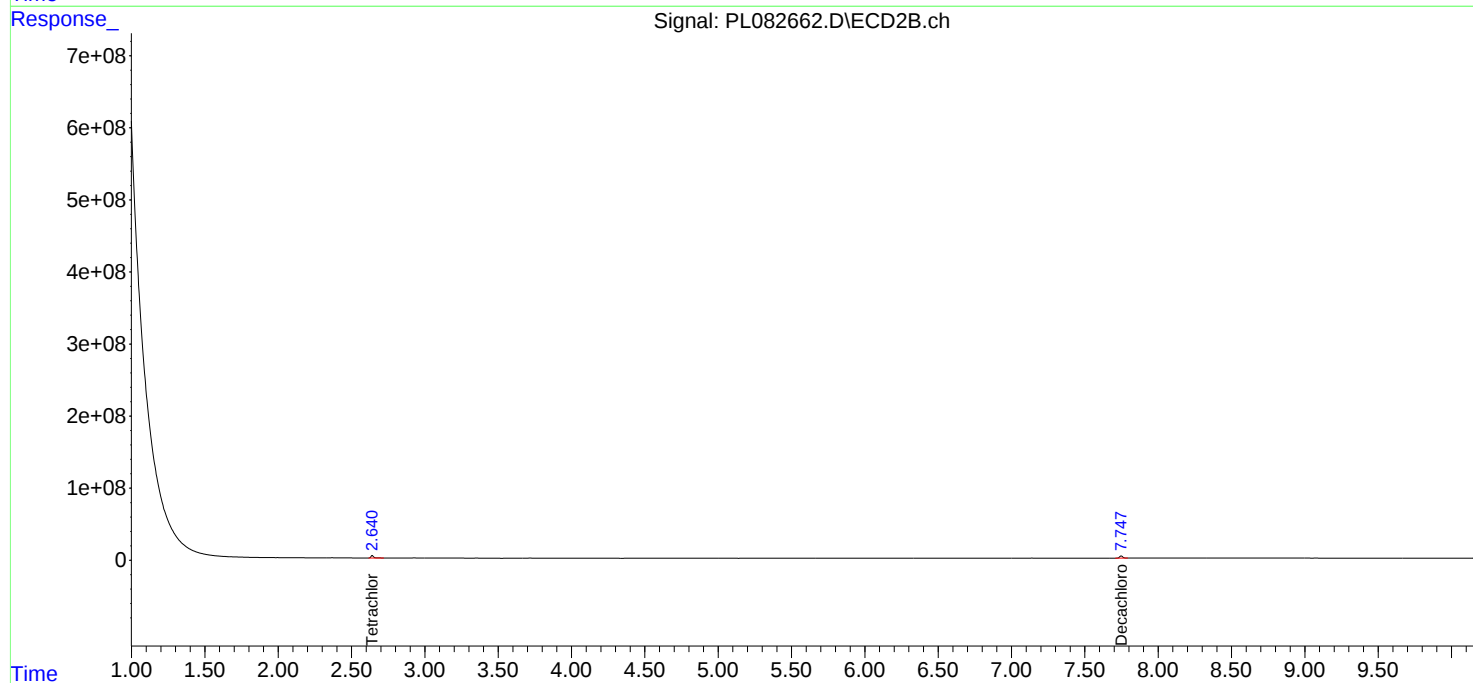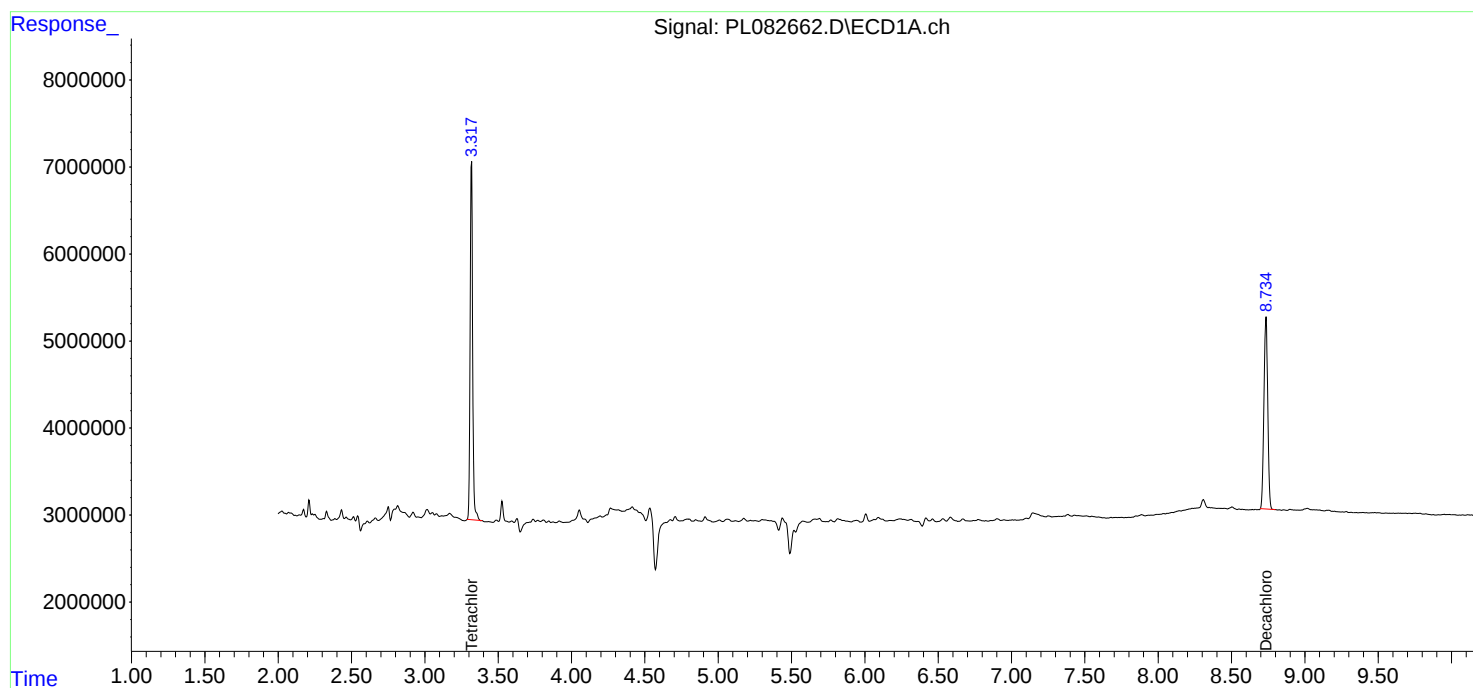

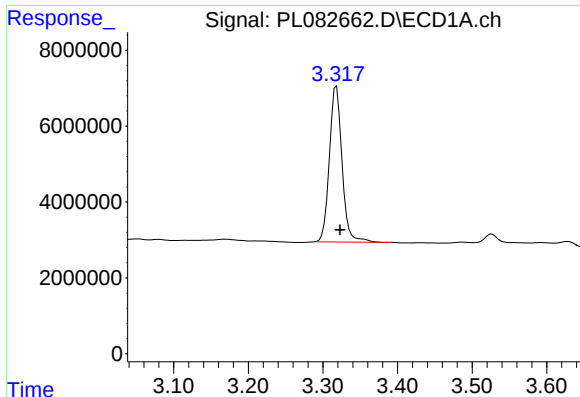


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: -0.005 min
Response: 48415274
Conc: 18.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
FSND-IDW-S-05042023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/12/2023
Supervised By :Ankita Jodhani 05/16/2023

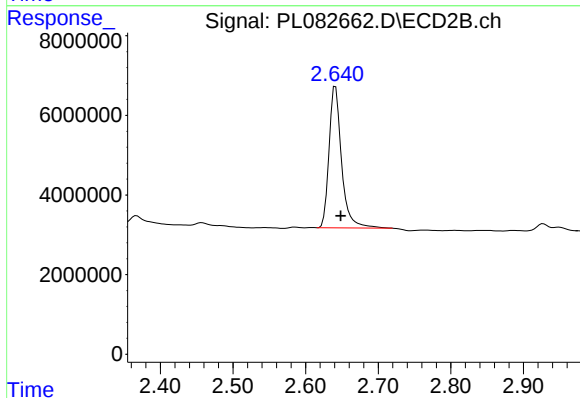


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: -0.007 min
Response: 42785768
Conc: 18.47 ng/ml

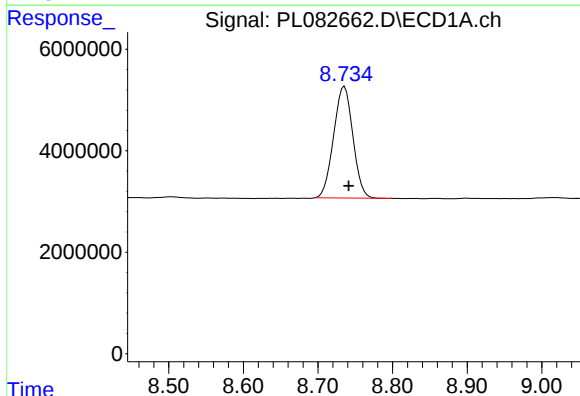

#28 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: -0.005 min
Response: 39337419
Conc: 20.61 ng/ml

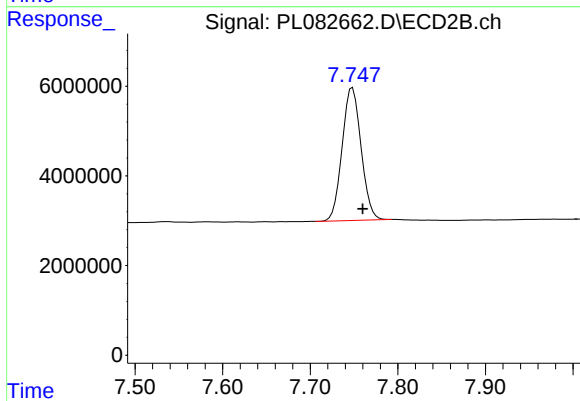

#28 Decachlorobiphenyl

R.T.: 7.747 min
Delta R.T.: -0.013 min
Response: 44634682
Conc: 19.56 ng/ml m