

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051123\
 Data File : PL082677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2023 21:25
 Operator : AR\AJ
 Sample : 02743-07 (Sig #1); 02743-01 (Sig #2)
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DRUM-A-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 05:50:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.319	2.641	42984555	38674326	16.092	16.693
28) SA Decachlor...	8.734	7.748	24417625	25969458	12.790	11.378

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051123\
Data File : PL082677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2023 21:25
Operator : AR\AJ
Sample : 02743-07 (Sig #1); 02743-01 (Sig #2)
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DRUM-A-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 05:50:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

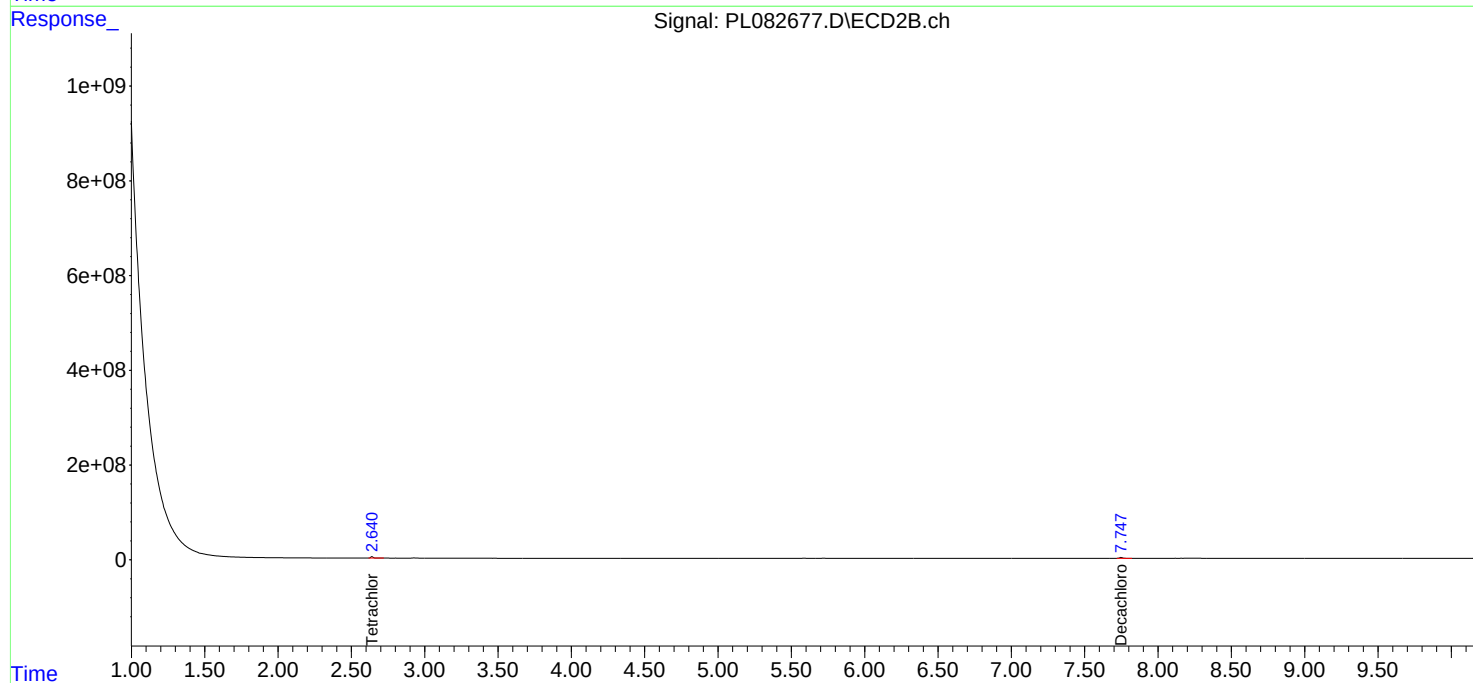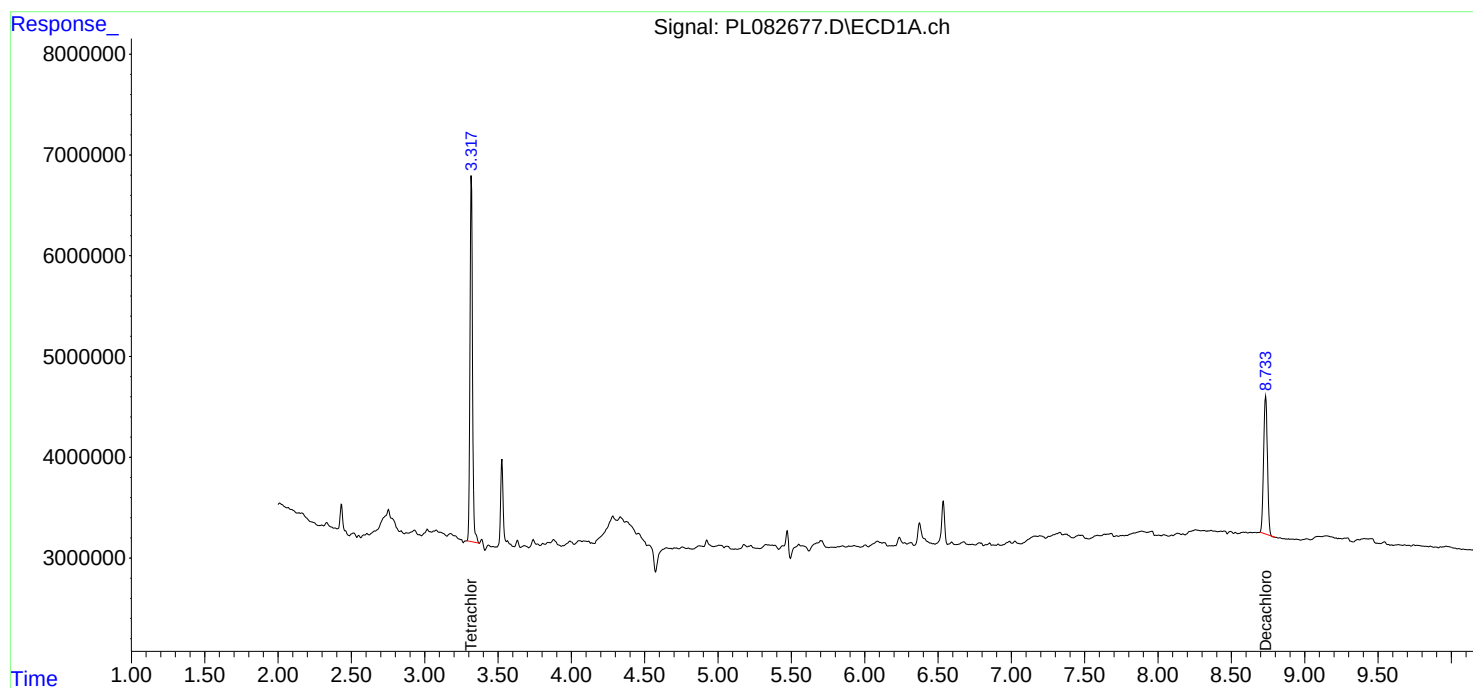


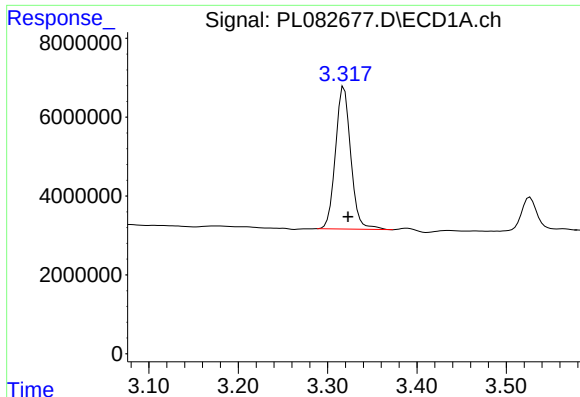

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: -0.004 min
Response: 42984555
Conc: 16.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
DRUM-A-WATER

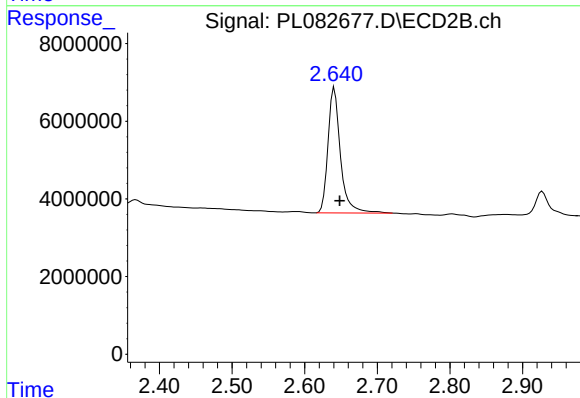


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: -0.007 min
Response: 38674326
Conc: 16.69 ng/ml

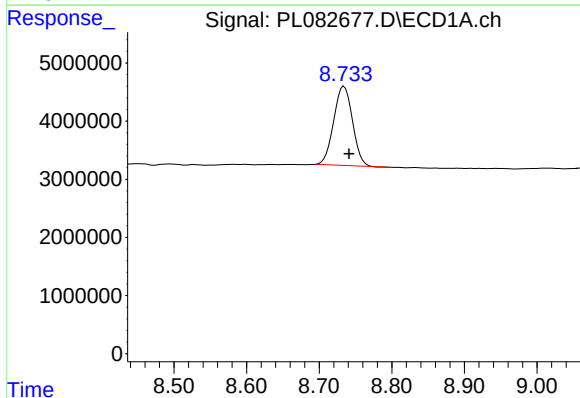

#28 Decachlorobiphenyl

R.T.: 8.734 min
Delta R.T.: -0.007 min
Response: 24417625
Conc: 12.79 ng/ml

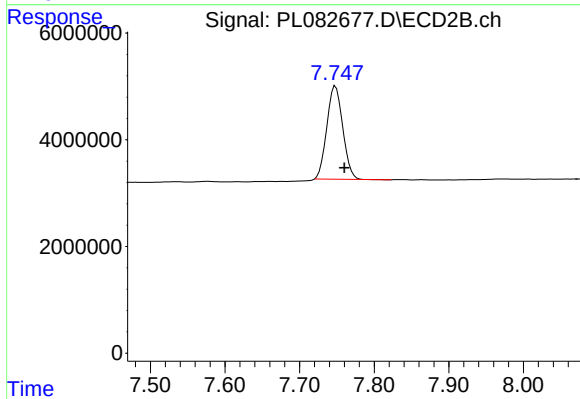

#28 Decachlorobiphenyl

R.T.: 7.748 min
Delta R.T.: -0.012 min
Response: 25969458
Conc: 11.38 ng/ml