

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
 Data File : PL058651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 01:59
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 09:05:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Wed May 13 09:01:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	4.078	103.2E6	113.7E6	52.503	53.704
28)	SA Decachlor...	8.323	9.193	67950082	92108347	53.194	53.163
Target Compounds							
23)	Chlordane-1	4.416	5.083	26292664	42812437	524.293	534.981
24)	Chlordane-2	4.922	5.553	28630297	45469361	527.076	532.084
25)	Chlordane-3	5.497	6.203	76104984	164.4E6	543.978	542.783
26)	Chlordane-4	5.555	6.279	62641668	197.4E6	545.787	541.643
27)	Chlordane-5	6.395	7.087	26227335	33706567	537.359	539.914


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
Data File : PL058651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 01:59
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 09:05:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Wed May 13 09:01:52 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

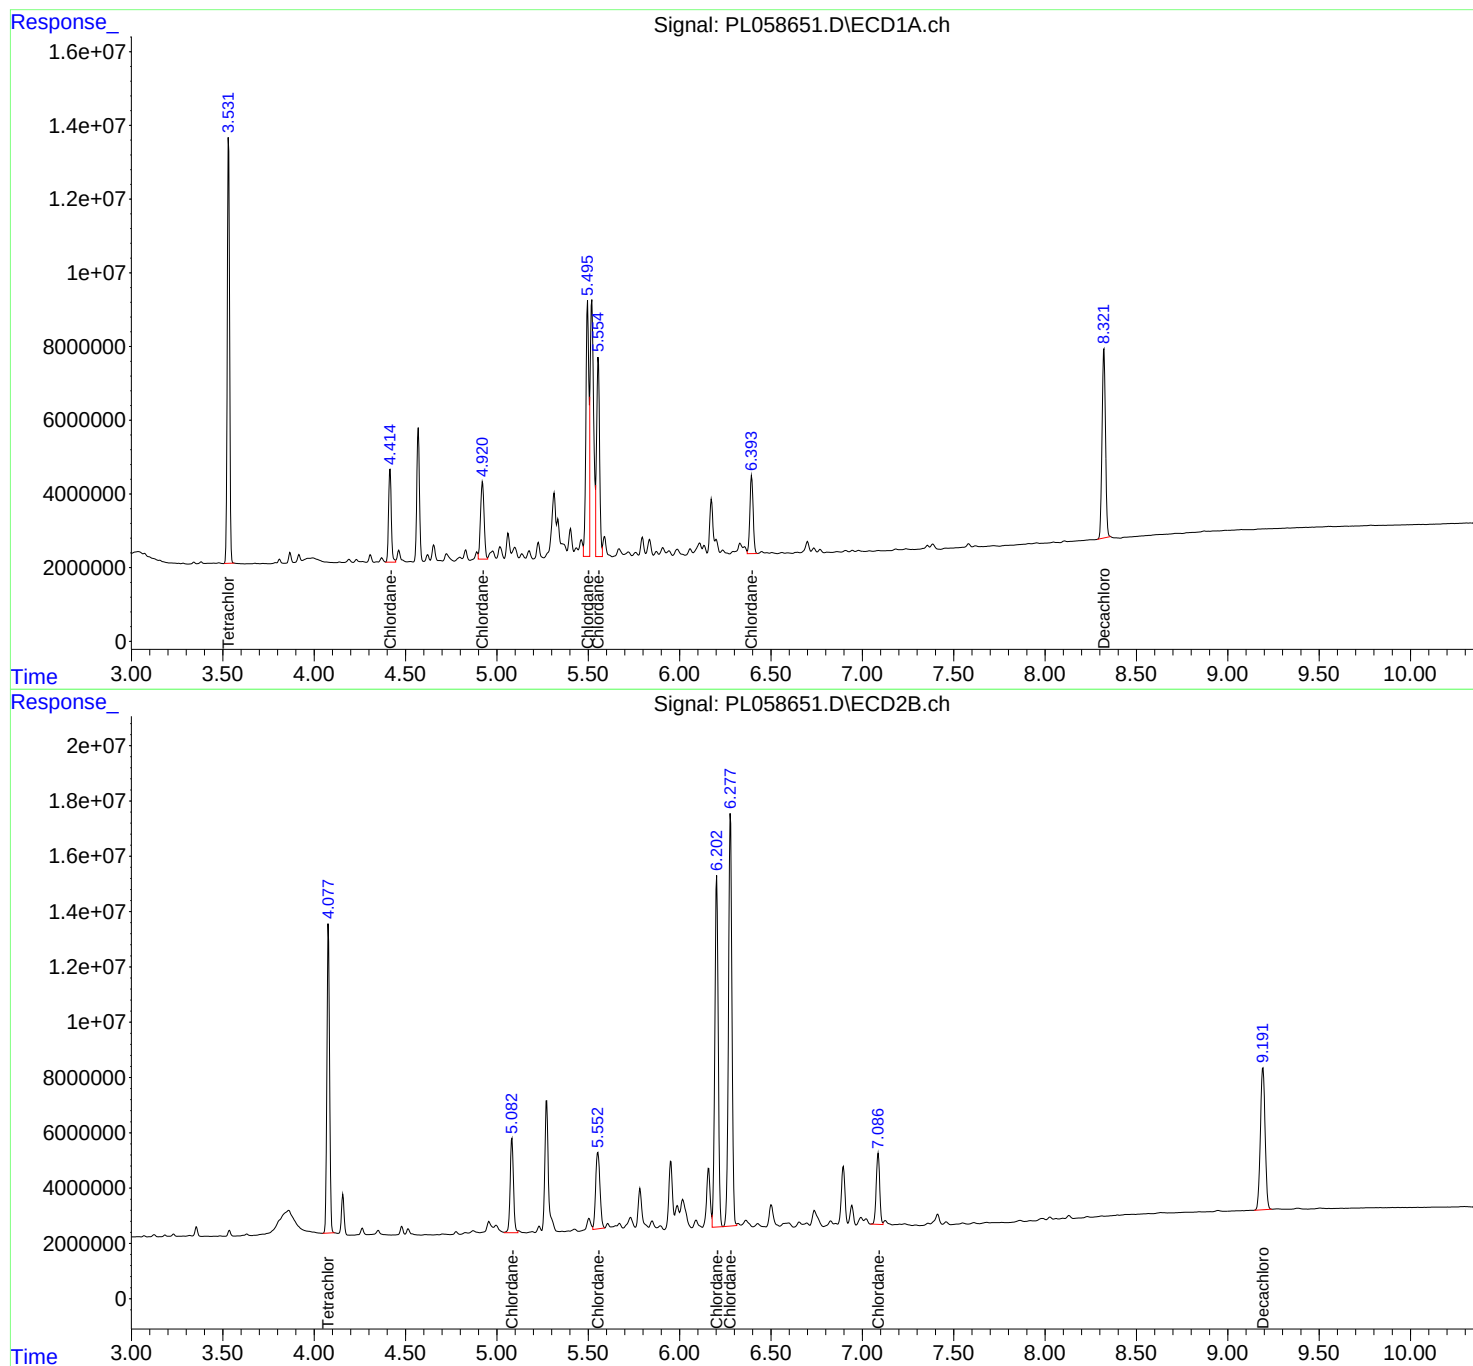

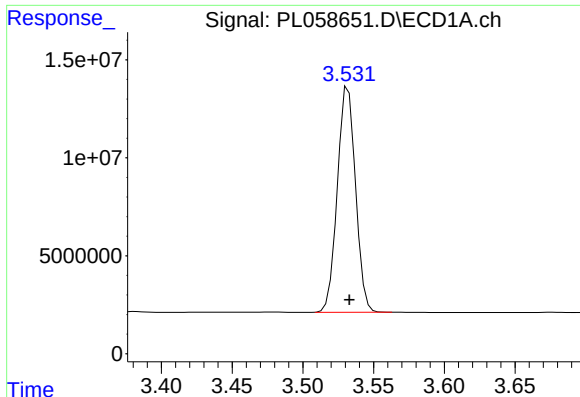


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: 0.000 min
Response: 103228202
Conc: 52.50 ng/ml

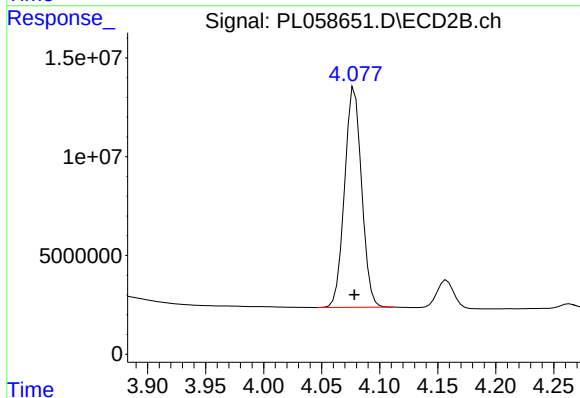


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 113741635
Conc: 53.70 ng/ml

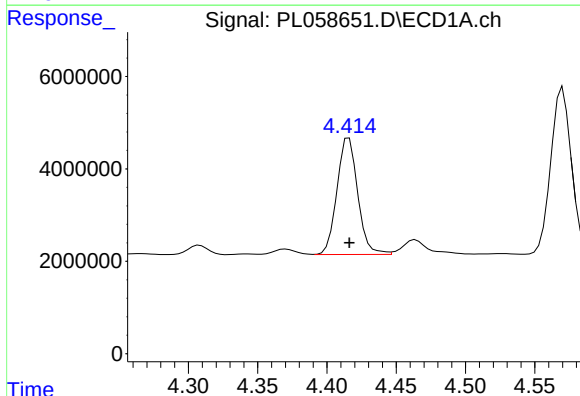


#23 Chlordane-1

R.T.: 4.416 min
Delta R.T.: 0.000 min
Response: 26292664
Conc: 524.29 ng/ml

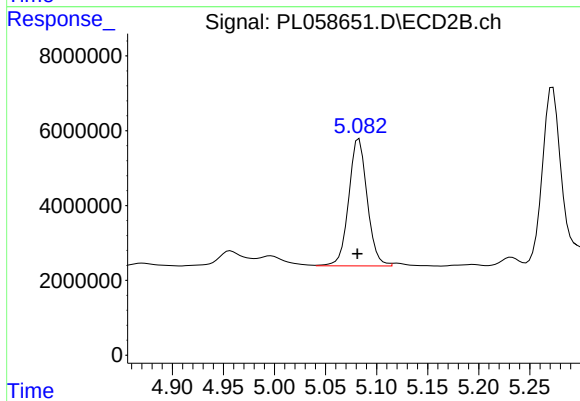


#23 Chlordane-1

R.T.: 5.083 min
Delta R.T.: 0.002 min
Response: 42812437
Conc: 534.98 ng/ml

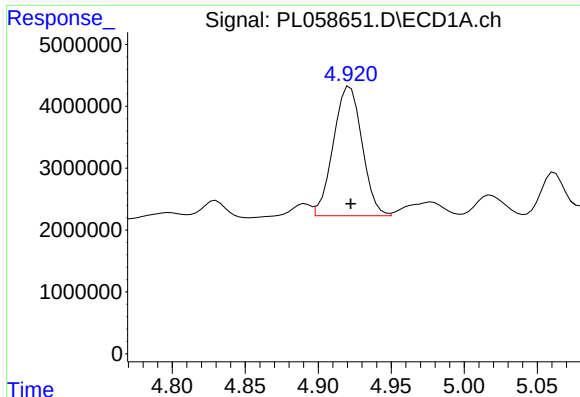


#24 Chlordane-2

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 28630297
Conc: 527.08 ng/ml

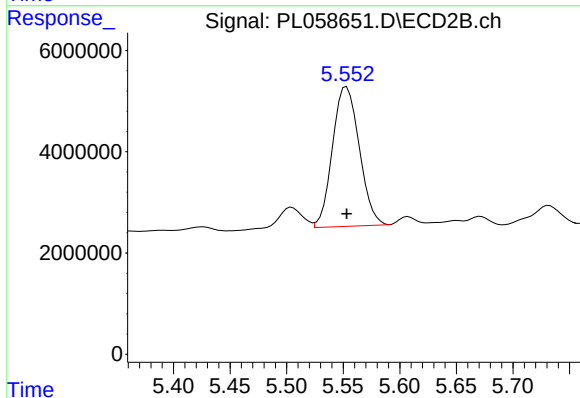


#24 Chlordane-2

R.T.: 5.553 min
Delta R.T.: 0.000 min
Response: 45469361
Conc: 532.08 ng/ml

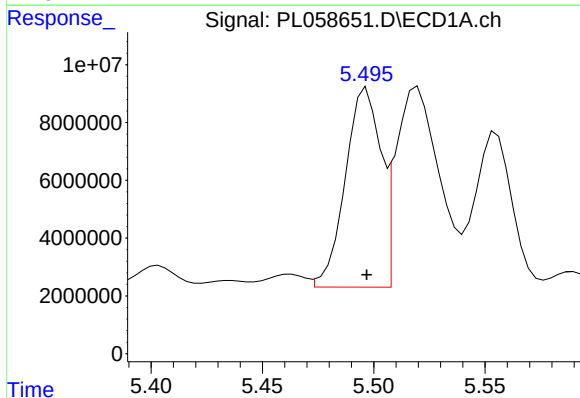


#25 Chlordane-3

R.T.: 5.497 min
Delta R.T.: 0.000 min
Response: 76104984
Conc: 543.98 ng/ml

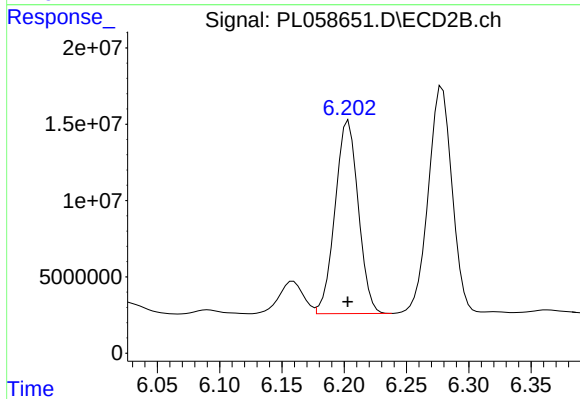


#25 Chlordane-3

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 164400718
Conc: 542.78 ng/ml

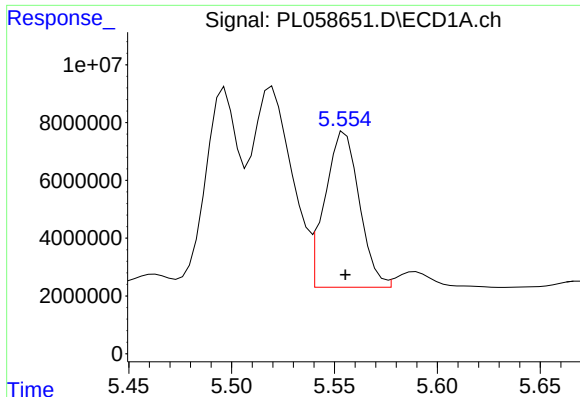


#26 Chlordane-4

R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 62641668
Conc: 545.79 ng/ml

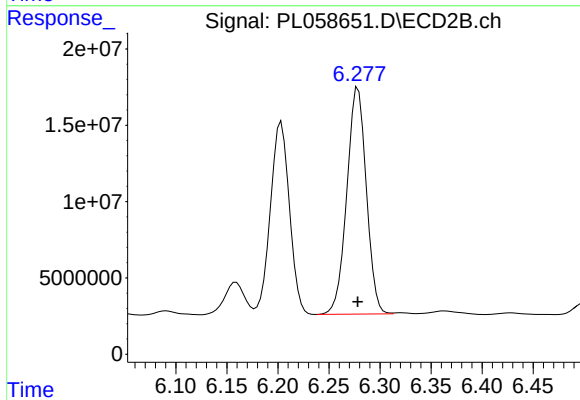


#26 Chlordane-4

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 197408227
Conc: 541.64 ng/ml

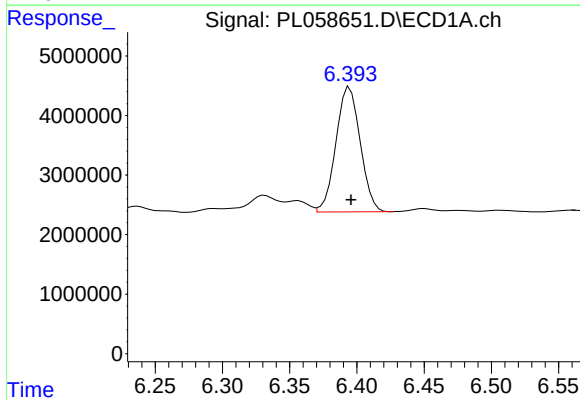


#27 Chlordane-5

R.T.: 6.395 min
Delta R.T.: 0.000 min
Response: 26227335
Conc: 537.36 ng/ml

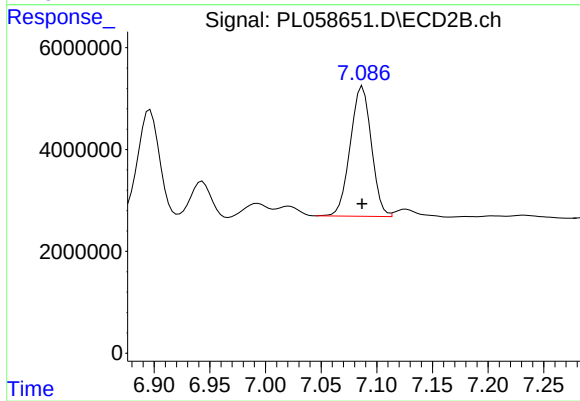


#27 Chlordane-5

R.T.: 7.087 min
Delta R.T.: 0.000 min
Response: 33706567
Conc: 539.91 ng/ml

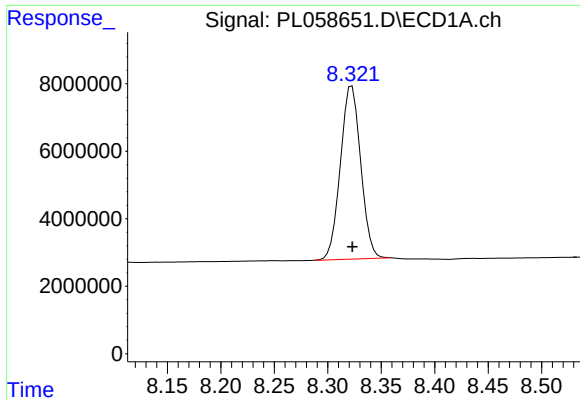

#28 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: 0.000 min
Response: 67950082
Conc: 53.19 ng/ml

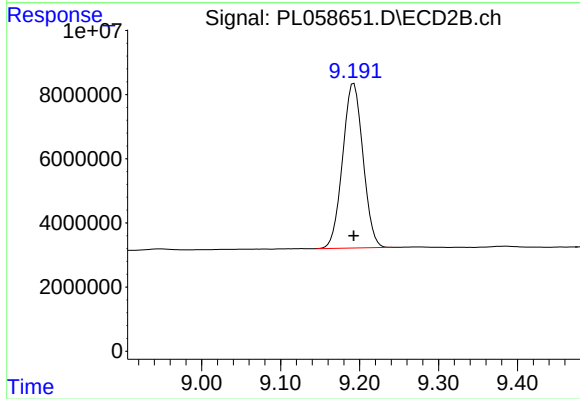

#28 Decachlorobiphenyl

R.T.: 9.193 min
Delta R.T.: 0.000 min
Response: 92108347
Conc: 53.16 ng/ml