

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
 Data File : PL058661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 04:19
 Operator : AJ\MA
 Sample : PB128678BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 09:09:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
 Quant Title : GC Extractables
 QLast Update : Wed May 13 09:01:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.533	4.078	37241856	49960302	18.941	23.589
28)	SA Decachlor...	8.321	9.192	31604409	43265058	24.741	24.972
Target Compounds							
25)	Chlordane-3	0.000	6.177f	0	571194	N.D.	1.886 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051220\
Data File : PL058661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 04:19
Operator : AJ\MA
Sample : PB128678BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 09:09:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051220.M
Quant Title : GC Extractables
QLast Update : Wed May 13 09:01:52 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

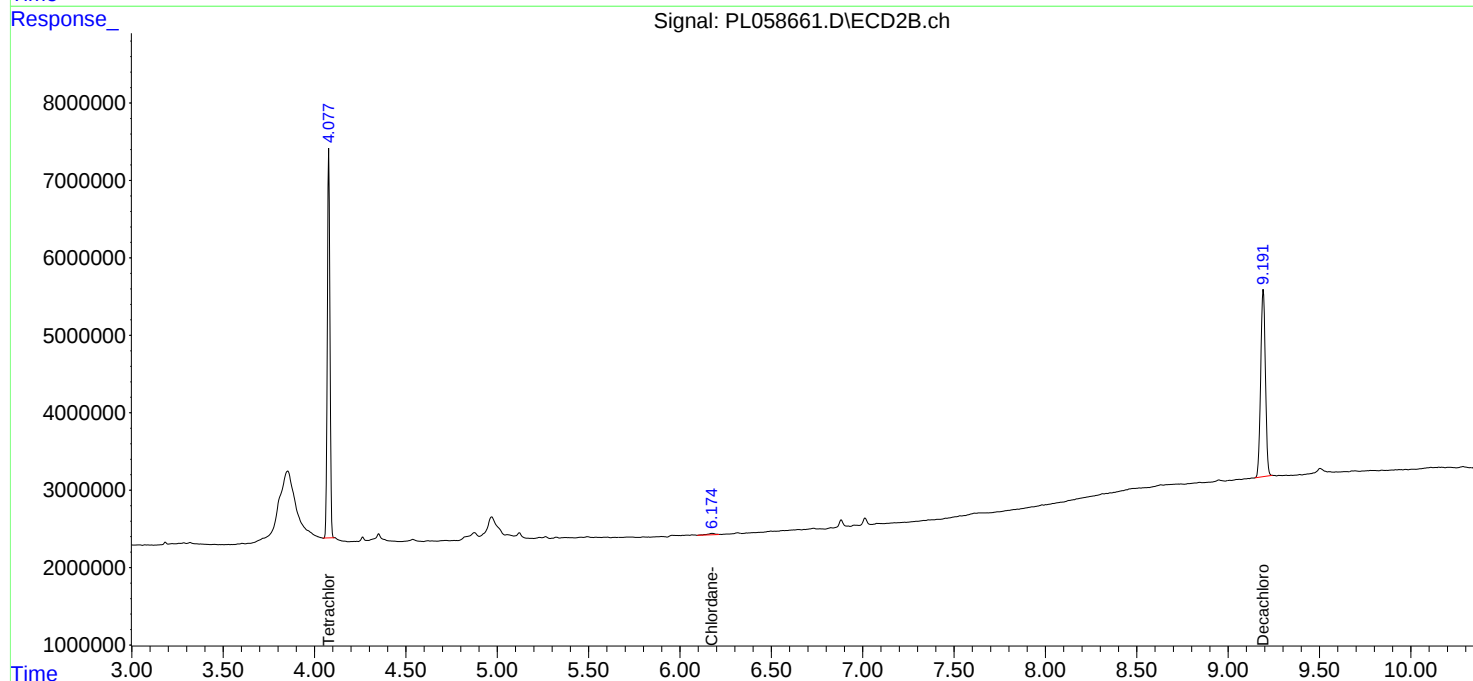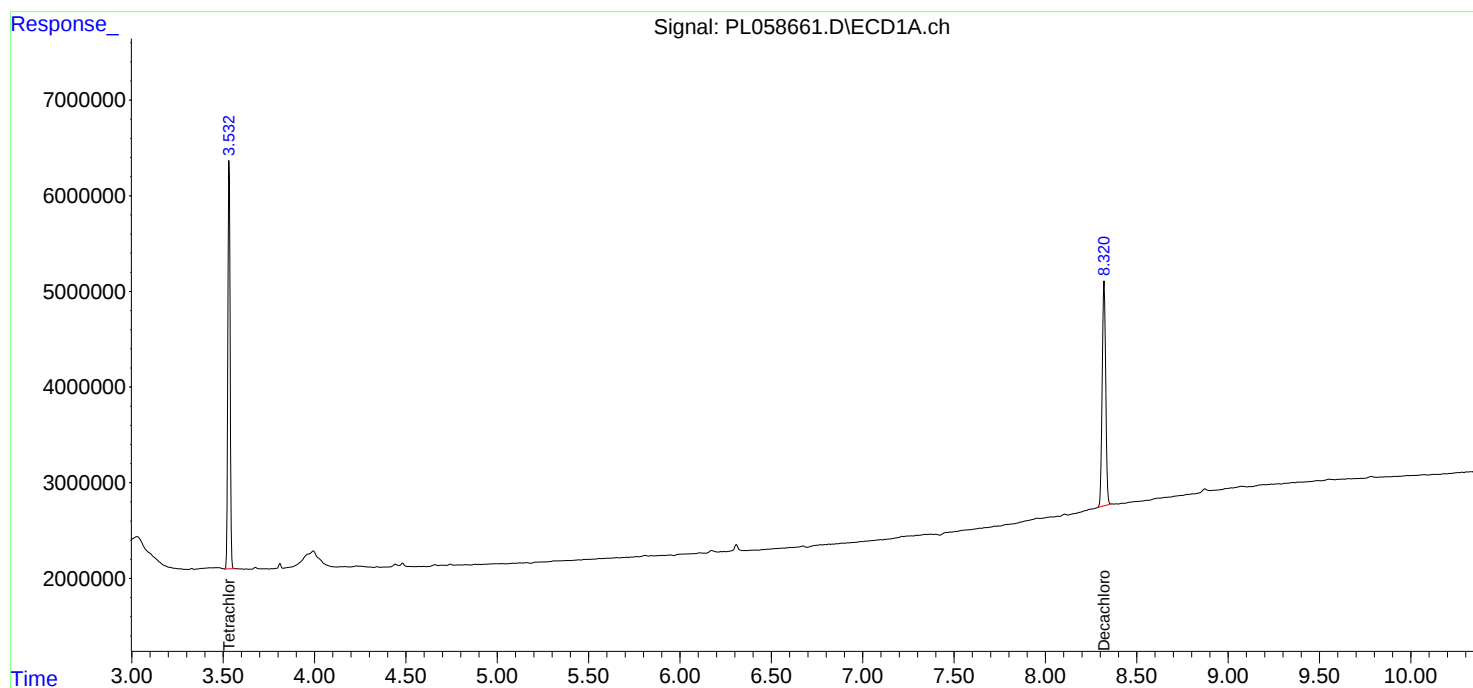

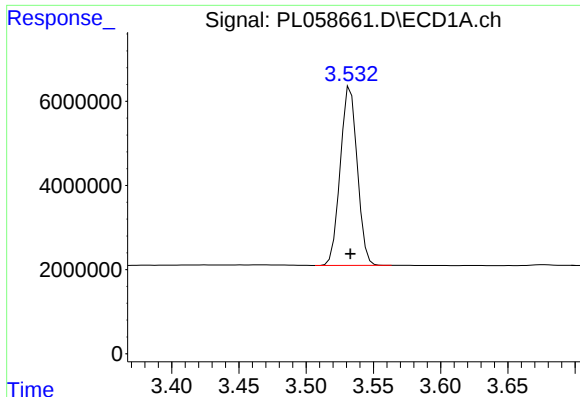


#1 Tetrachloro-m-xylene

R.T.: 3.533 min
Delta R.T.: 0.000 min
Response: 37241856
Conc: 18.94 ng/ml

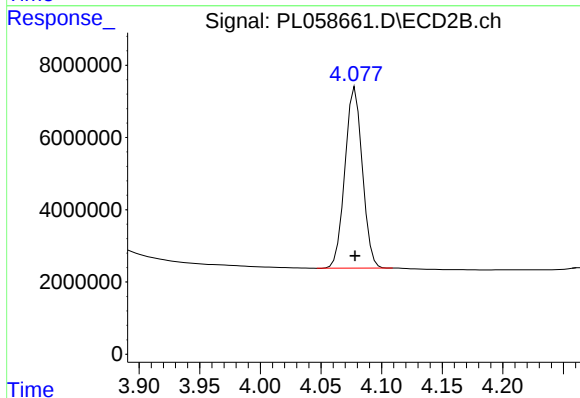


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 49960302
Conc: 23.59 ng/ml

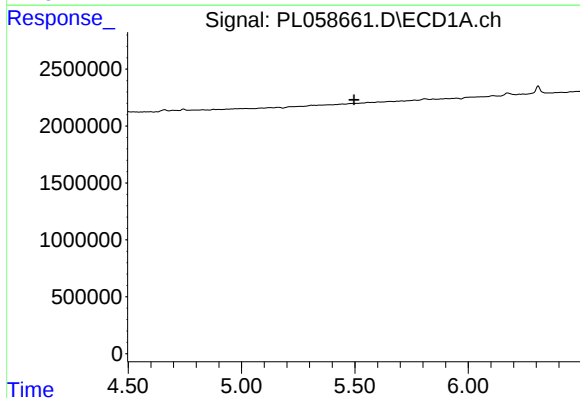


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.497 min
Response: 0
Conc: N.D.

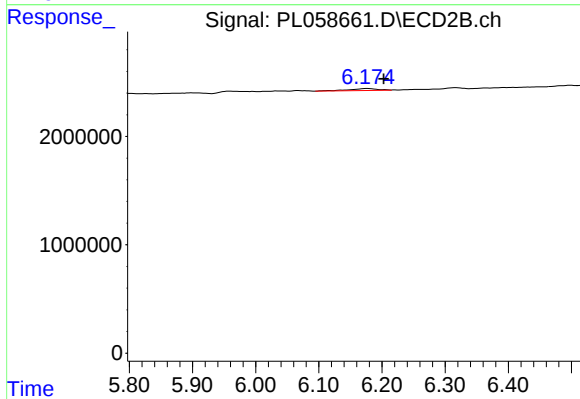


#25 Chlordane-3

R.T.: 6.177 min
Delta R.T.: -0.026 min
Response: 571194
Conc: 1.89 ng/ml

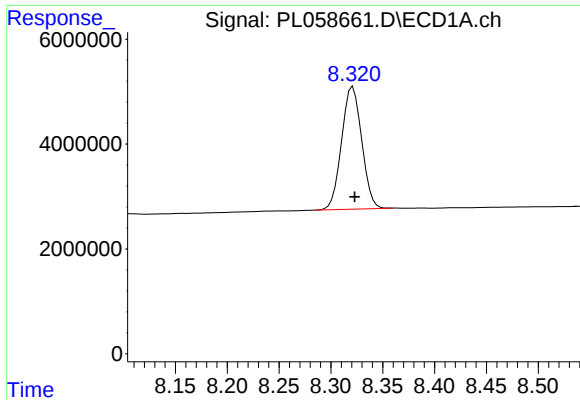

#28 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: -0.002 min
Response: 31604409
Conc: 24.74 ng/ml

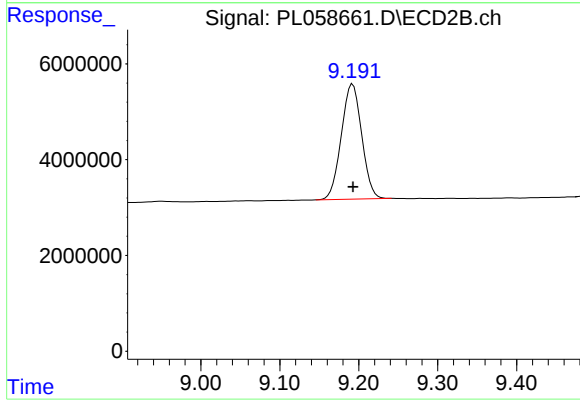

#28 Decachlorobiphenyl

R.T.: 9.192 min
Delta R.T.: 0.000 min
Response: 43265058
Conc: 24.97 ng/ml